


# ThermaCAM™ B2

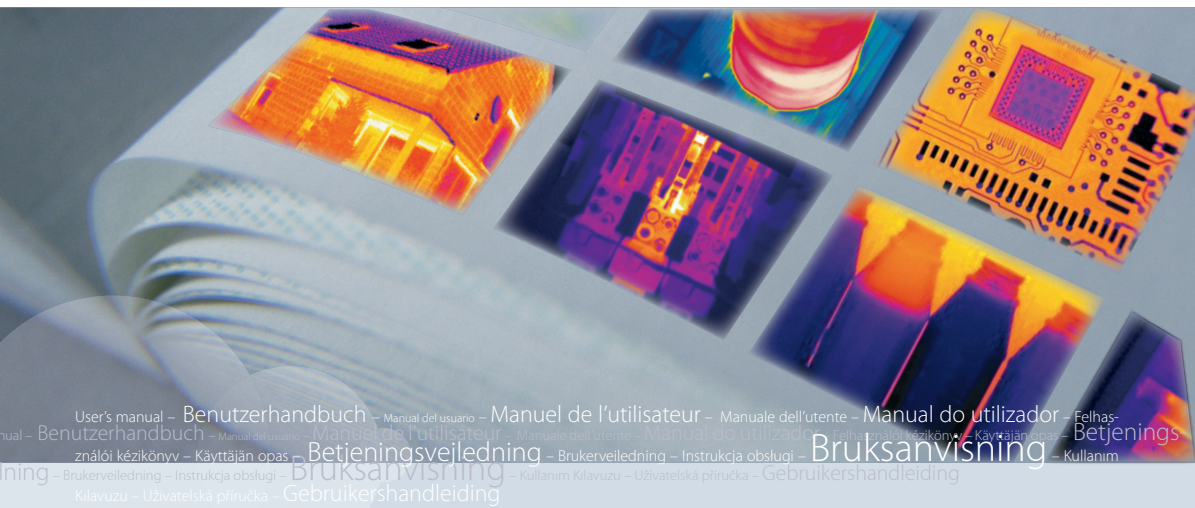

User's manual – Benutzerhandbuch – Manual del usuario – Manuel de l'utilisateur – Manuale dell'utente – Manual do utilizador – Felhasználói kézikönyv – Käyttöäjan opas – Betjeningsvejledning – Brukerveiledning – Instrukcja obsługi – Bruksanvisning – Kullanim – Brukerveiledning – Instrukcja obsługi – Bruksanvisning – Kullanim – Brukerveiledning – Instrukcja obsługi – Bruksanvisning – Kullanim

## User's manual

|            |                   |
|------------|-------------------|
| Publ. No.  | 1558073           |
| Revision   | a156              |
| Language   | English (EN)      |
| Issue date | February 28, 2006 |



|                                                            |           |
|------------------------------------------------------------|-----------|
| <b>Warnings &amp; cautions</b>                             | <b>1</b>  |
| <b>Important note about this manual</b>                    | <b>2</b>  |
| <b>Welcome!</b>                                            | <b>3</b>  |
| <b>Packing list</b>                                        | <b>4</b>  |
| <b>System overview</b>                                     | <b>5</b>  |
| <b>Connecting system components</b>                        | <b>6</b>  |
| <b>Introduction to building thermography</b>               | <b>7</b>  |
| <b>Tutorials</b>                                           | <b>8</b>  |
| <b>Camera overview</b>                                     | <b>9</b>  |
| <b>Camera program</b>                                      | <b>10</b> |
| <b>Electrical power system</b>                             | <b>11</b> |
| <b>Maintenance &amp; cleaning</b>                          | <b>12</b> |
| <b>Troubleshooting</b>                                     | <b>13</b> |
| <b>Technical specifications &amp; dimensional drawings</b> | <b>14</b> |
| <b>Glossary</b>                                            | <b>15</b> |



**Thermographic measurement techniques**

**16**

**History of infrared technology**

**17**

**Theory of thermography**

**18**

**Emissivity tables**

**19**



---

# ThermaCAM™ B2

*User's manual*



---

### Legal disclaimer

All products manufactured by FLIR Systems are warranted against defective materials and workmanship for a period of one (1) year from the delivery date of the original purchase, provided such products have been under normal storage, use and service, and in accordance with FLIR Systems instruction.

All products not manufactured by FLIR Systems included in systems delivered by FLIR Systems to the original purchaser carry the warranty, if any, of the particular supplier only and FLIR Systems has no responsibility whatsoever for such products.

The warranty extends only to the original purchaser and is not transferable. It is not applicable to any product which has been subjected to misuse, neglect, accident or abnormal conditions of operation. Expendable parts are excluded from the warranty.

In the case of a defect in a product covered by this warranty the product must not be further used in order to prevent additional damage. The purchaser shall promptly report any defect to FLIR Systems or this warranty will not apply.

FLIR Systems will, at its option, repair or replace any such defective product free of charge if, upon inspection, it proves to be defective in material or workmanship and provided that it is returned to FLIR Systems within the said one-year period.

FLIR Systems has no other obligation or liability for defects than those set forth above.

No other warranty is expressed or implied. FLIR Systems specifically disclaims the implied warranties of merchantability and fitness for a particular purpose.

FLIR Systems shall not be liable for any direct, indirect, special, incidental or consequential loss or damage, whether based on contract, tort or any other legal theory.

### Copyright

© FLIR Systems, 2006. All rights reserved worldwide. No parts of the software including source code may be reproduced, transmitted, transcribed or translated into any language or computer language in any form or by any means, electronic, magnetic, optical, manual or otherwise, without the prior written permission of FLIR Systems.

This manual must not, in whole or part, be copied, photocopied, reproduced, translated or transmitted to any electronic medium or machine readable form without prior consent, in writing, from FLIR Systems.

Names and marks appearing on the products herein are either registered trademarks or trademarks of FLIR Systems and/or its subsidiaries. All other trademarks, trade names or company names referenced herein are used for identification only and are the property of their respective owners.

### Quality assurance

The Quality Management System under which these products are developed and manufactured has been certified in accordance with the ISO 9001 standard.

FLIR Systems is committed to a policy of continuous development; therefore we reserve the right to make changes and improvements on any of the products described in this manual without prior notice.

### Patents

This product is protected by patents, design patents, patents pending, or design patents pending.

One or several of the following patents, design patents, patents pending, or design patents pending apply to the products and/or features described in this manual:

| Designation | Status        | Reg. No.       |
|-------------|---------------|----------------|
| China       | Application   | 00809178.1     |
| China       | Application   | 01823221.3     |
| China       | Application   | 01823226.4     |
| China       | Design Patent | 235308         |
| China       | Design Patent | ZL02331553.9   |
| China       | Design Patent | ZL02331554.7   |
| China       | Pending       | 200530018812.0 |
| EPC         | Patent        | 1188086        |
| EPO         | Application   | 01930377.5     |
| EPO         | Application   | 01934715.2     |
| EPO         | Application   | 27282912       |
| EU          | Design Patent | 000279476-0001 |
| France      | Patent        | 1188086        |

| Designation   | Status        | Reg. No.        |
|---------------|---------------|-----------------|
| Germany       | Patent        | 60004227.8      |
| Great Britain | Design Patent | 106017          |
| Great Britain | Design Patent | 3006596         |
| Great Britain | Design Patent | 3006597         |
| Great Britain | Patent        | 1188086         |
| International | Design Patent | DM/057692       |
| International | Design Patent | DM/061609       |
| Japan         | Application   | 2000-620406     |
| Japan         | Application   | 2002-588123     |
| Japan         | Application   | 2002-588070     |
| Japan         | Design Patent | 1144833         |
| Japan         | Design Patent | 1182246         |
| Japan         | Design Patent | 1182620         |
| Japan         | Pending       | 2005-020460     |
| PCT           | Application   | PCT/SE01/00983  |
| PCT           | Application   | PCT/SE01/00984  |
| PCT           | Application   | PCT/SE02/00857  |
| PCT           | Application   | PCT/SE03/00307  |
| PCT           | Application   | PCT/SE/00/00739 |
| Sweden        | Application   | 0302837-0       |
| Sweden        | Design Patent | 68657           |
| Sweden        | Design Patent | 75530           |
| Sweden        | Patent        | 518836          |
| Sweden        | Patent        | 522971          |
| Sweden        | Patent        | 524024          |
| U.S.          | Application   | 09/576266       |
| U.S.          | Application   | 10/476,217      |
| U.S.          | Application   | 10/476,760      |
| U.S.          | Design Patent | 466540          |
| U.S.          | Design Patent | 483782          |
| U.S.          | Design Patent | 484155          |
| U.S.          | Patent        | 5,386,117       |
| U.S.          | Patent        | 5,637,871       |
| U.S.          | Patent        | 5,756,999       |
| U.S.          | Patent        | 6,028,309       |
| U.S.          | Patent        | 6,707,044       |
| U.S.          | Patent        | 6,812,465       |

| Designation | Status  | Reg. No.   |
|-------------|---------|------------|
| U.S.        | Pending | 29/233,400 |

# Table of contents

|          |                                                                                |           |
|----------|--------------------------------------------------------------------------------|-----------|
| <b>1</b> | <b>Warnings &amp; cautions</b>                                                 | <b>1</b>  |
| <b>2</b> | <b>Important note about this manual</b>                                        | <b>3</b>  |
| <b>3</b> | <b>Welcome!</b>                                                                | <b>5</b>  |
| 3.1      | About FLIR Systems                                                             | 6         |
| 3.1.1    | A few images from our facilities                                               | 8         |
| 3.2      | Comments & questions                                                           | 10        |
| <b>4</b> | <b>Packing list</b>                                                            | <b>11</b> |
| <b>5</b> | <b>System overview</b>                                                         | <b>13</b> |
| <b>6</b> | <b>Connecting system components</b>                                            | <b>15</b> |
| <b>7</b> | <b>Introduction to building thermography</b>                                   | <b>17</b> |
| 7.1      | Important note                                                                 | 17        |
| 7.2      | Typical field investigations                                                   | 17        |
| 7.2.1    | Guidelines                                                                     | 17        |
| 7.2.1.1  | General guidelines                                                             | 17        |
| 7.2.1.2  | Guidelines for moisture detection, mold detection & detection of water damages | 18        |
| 7.2.1.3  | Guidelines for detection of air infiltration & insulation deficiencies         | 18        |
| 7.2.2    | About moisture detection                                                       | 19        |
| 7.2.3    | Moisture detection (1): Low-slope commercial roofs                             | 19        |
| 7.2.3.1  | General information                                                            | 19        |
| 7.2.3.2  | Safety precautions                                                             | 20        |
| 7.2.3.3  | Commented building structures                                                  | 21        |
| 7.2.3.4  | Commented infrared images                                                      | 22        |
| 7.2.4    | Moisture detection (2): Commercial & residential façades                       | 24        |
| 7.2.4.1  | General information                                                            | 24        |
| 7.2.4.2  | Commented building structures                                                  | 24        |
| 7.2.4.3  | Commented infrared images                                                      | 26        |
| 7.2.5    | Moisture detection (3): Decks & balconies                                      | 26        |
| 7.2.5.1  | General information                                                            | 26        |
| 7.2.5.2  | Commented building structures                                                  | 27        |
| 7.2.5.3  | Commented infrared images                                                      | 29        |
| 7.2.6    | Moisture detection (4): Plumbing breaks & leaks                                | 29        |
| 7.2.6.1  | General information                                                            | 29        |
| 7.2.6.2  | Commented infrared images                                                      | 30        |
| 7.2.7    | Air infiltration                                                               | 32        |
| 7.2.7.1  | General information                                                            | 32        |
| 7.2.7.2  | Commented building structures                                                  | 32        |
| 7.2.7.3  | Commented infrared images                                                      | 34        |
| 7.2.8    | Insulation deficiencies                                                        | 35        |
| 7.2.8.1  | General information                                                            | 35        |
| 7.2.8.2  | Commented building structures                                                  | 35        |
| 7.2.8.3  | Commented infrared images                                                      | 37        |
| 7.3      | Theory of building science                                                     | 39        |
| 7.3.1    | General information                                                            | 39        |
| 7.3.2    | The effects of testing and checking                                            | 40        |

|          |                                                              |           |
|----------|--------------------------------------------------------------|-----------|
| 7.3.3    | Sources of disruption in thermography .....                  | 41        |
| 7.3.4    | Surface temperature and air leaks .....                      | 43        |
| 7.3.4.1  | Pressure conditions in a building .....                      | 43        |
| 7.3.5    | Measuring conditions & measuring season .....                | 49        |
| 7.3.6    | Interpretation of infrared images .....                      | 49        |
| 7.3.7    | Humidity & dew point .....                                   | 51        |
| 7.3.7.1  | Relative & absolute humidity .....                           | 51        |
| 7.3.7.2  | Definition of dew point .....                                | 52        |
| 7.4      | Disclaimer .....                                             | 53        |
| 7.4.1    | Copyright notice .....                                       | 53        |
| 7.4.2    | Training & certification .....                               | 53        |
| 7.4.3    | National or regional building codes .....                    | 53        |
| <b>8</b> | <b>Tutorials .....</b>                                       | <b>55</b> |
| 8.1      | Switching on & switching off the camera .....                | 55        |
| 8.1.1    | Switching on the camera .....                                | 55        |
| 8.1.2    | Switching off the camera .....                               | 55        |
| 8.2      | Working with images .....                                    | 56        |
| 8.2.1    | Acquiring an image .....                                     | 56        |
| 8.2.2    | Freezing an image .....                                      | 56        |
| 8.2.3    | Saving an image .....                                        | 56        |
| 8.2.4    | Deleting one or several images .....                         | 57        |
| 8.2.5    | Opening an image .....                                       | 57        |
| 8.3      | Working with measurements .....                              | 58        |
| 8.3.1    | Laying out a spot .....                                      | 58        |
| 8.3.2    | Laying out a measurement area .....                          | 58        |
| 8.4      | Working with alarms .....                                    | 59        |
| 8.4.1    | Setting the reference temperature .....                      | 59        |
| 8.4.2    | Setting up a color alarm .....                               | 60        |
| 8.4.2.1  | Setting up a color alarm using the menu system .....         | 60        |
| 8.4.2.2  | Setting up a color alarm without using the menu system ..... | 60        |
| 8.4.3    | Setting up a silent alarm (i.e. a visual alarm) .....        | 61        |
| 8.4.4    | Setting up an audible alarm .....                            | 61        |
| 8.5      | Creating files for image descriptions .....                  | 62        |
| 8.6      | Changing level & span .....                                  | 63        |
| 8.6.1    | Changing level .....                                         | 63        |
| 8.6.2    | Changing span .....                                          | 63        |
| 8.7      | Changing system settings .....                               | 64        |
| 8.7.1    | Changing language .....                                      | 64        |
| 8.7.2    | Changing temperature unit .....                              | 64        |
| 8.7.3    | Changing date format .....                                   | 64        |
| 8.7.4    | Changing time format .....                                   | 64        |
| 8.7.5    | Changing date & time .....                                   | 65        |
| 8.8      | Working with the camera .....                                | 66        |
| 8.8.1    | Removing the lens .....                                      | 66        |
| 8.8.2    | Adjusting the focus .....                                    | 67        |
| 8.8.3    | Inserting & removing the battery .....                       | 67        |
| 8.8.3.1  | Inserting the battery .....                                  | 68        |
| 8.8.3.2  | Removing the battery .....                                   | 68        |
| <b>9</b> | <b>Camera overview .....</b>                                 | <b>71</b> |
| 9.1      | Camera parts .....                                           | 71        |
| 9.2      | Keypad buttons & functions .....                             | 75        |
| 9.3      | Laser LocatIR .....                                          | 77        |

|           |                                                                  |            |
|-----------|------------------------------------------------------------------|------------|
| 9.4       | LED indicator on keypad .....                                    | 78         |
| <b>10</b> | <b>Camera program .....</b>                                      | <b>79</b>  |
| 10.1      | Result table .....                                               | 79         |
| 10.2      | System messages .....                                            | 80         |
| 10.2.1    | Status messages .....                                            | 80         |
| 10.2.2    | Warning messages .....                                           | 80         |
| 10.3      | Selecting screen objects .....                                   | 81         |
| 10.3.1    | Selecting screen objects .....                                   | 81         |
| 10.3.2    | Examples of selected screen objects .....                        | 81         |
| 10.4      | Menu system .....                                                | 83         |
| 10.4.1    | Navigating the menu system .....                                 | 83         |
| 10.4.2    | Meas. mode .....                                                 | 83         |
| 10.4.3    | Manual adjust/Automatic adjust .....                             | 84         |
| 10.4.4    | Emissivity .....                                                 | 85         |
| 10.4.5    | Palette .....                                                    | 86         |
| 10.4.6    | Hide graphics / Show graphics .....                              | 86         |
| 10.4.7    | File .....                                                       | 87         |
| 10.4.8    | Setup .....                                                      | 88         |
| 10.4.8.1  | Settings .....                                                   | 88         |
| 10.4.8.2  | Date/time .....                                                  | 90         |
| 10.4.8.3  | Local settings .....                                             | 91         |
| 10.4.8.4  | Camera info .....                                                | 91         |
| 10.4.8.5  | Factory default .....                                            | 91         |
| <b>11</b> | <b>Electrical power system .....</b>                             | <b>93</b>  |
| 11.1      | Internal battery charging .....                                  | 95         |
| 11.2      | External battery charging .....                                  | 96         |
| 11.3      | Battery safety warnings .....                                    | 97         |
| <b>12</b> | <b>Maintenance &amp; cleaning .....</b>                          | <b>99</b>  |
| 12.1      | Camera body, cables & accessories .....                          | 99         |
| 12.2      | Lenses .....                                                     | 99         |
| <b>13</b> | <b>Troubleshooting .....</b>                                     | <b>101</b> |
| <b>14</b> | <b>Technical specifications &amp; dimensional drawings .....</b> | <b>103</b> |
| 14.1      | Imaging performance .....                                        | 103        |
| 14.2      | Image presentation .....                                         | 103        |
| 14.3      | Laser LocatIR .....                                              | 103        |
| 14.4      | Electrical power system .....                                    | 103        |
| 14.5      | Environmental specifications .....                               | 104        |
| 14.6      | Physical specifications .....                                    | 104        |
| 14.7      | Communications interfaces .....                                  | 104        |
| 14.8      | Pin configurations .....                                         | 105        |
| 14.8.1    | RS-232/USB connector .....                                       | 105        |
| 14.8.2    | Power connector .....                                            | 105        |
| 14.8.3    | CVBS connector .....                                             | 106        |
| 14.9      | Relationship between fields of view and distance .....           | 107        |
| 14.10     | Camera – dimensional drawings .....                              | 125        |
| 14.11     | Battery charger – dimensional drawing .....                      | 128        |
| 14.12     | Battery – dimensional drawing .....                              | 129        |
| <b>15</b> | <b>Glossary .....</b>                                            | <b>131</b> |

---

|                                                                   |            |
|-------------------------------------------------------------------|------------|
| <b>16 Thermographic measurement techniques .....</b>              | <b>135</b> |
| 16.1 Introduction .....                                           | 135        |
| 16.2 Emissivity .....                                             | 135        |
| 16.2.1 Finding the emissivity of a sample .....                   | 136        |
| 16.2.1.1 Step 1: Determining reflected apparent temperature ..... | 136        |
| 16.2.1.2 Step 2: Determining the emissivity .....                 | 138        |
| 16.3 Reflected apparent temperature .....                         | 139        |
| <b>17 History of infrared technology .....</b>                    | <b>141</b> |
| <b>18 Theory of thermography .....</b>                            | <b>145</b> |
| 18.1 Introduction .....                                           | 145        |
| 18.2 The electromagnetic spectrum .....                           | 145        |
| 18.3 Blackbody radiation .....                                    | 146        |
| 18.3.1 Planck's law .....                                         | 147        |
| 18.3.2 Wien's displacement law .....                              | 148        |
| 18.3.3 Stefan-Boltzmann's law .....                               | 150        |
| 18.3.4 Non-blackbody emitters .....                               | 150        |
| 18.4 Infrared semi-transparent materials .....                    | 153        |
| <b>19 Emissivity tables .....</b>                                 | <b>155</b> |
| 19.1 References .....                                             | 155        |
| 19.2 Important note about the emissivity tables .....             | 155        |
| 19.3 Tables .....                                                 | 155        |
| <b>Index .....</b>                                                | <b>171</b> |

10474103.a1



- This equipment generates, uses, and can radiate radio frequency energy and if not installed and used in accordance with the instruction manual, may cause interference to radio communications. It has been tested and found to comply with the limits for a Class A computing device pursuant to Subpart J of Part 15 of FCC Rules, which are designed to provide reasonable protection against such interference when operated in a commercial environment. Operation of this equipment in a residential area is likely to cause interference in which case the user at his own expense will be required to take whatever measures may be required to correct the interference.
- An infrared camera is a precision instrument and uses a very sensitive IR detector. Pointing the camera towards highly intensive energy sources – such as devices emitting laser radiation, or reflections from such devices – may affect the accuracy of the camera readings, or even harm – or irreparably damage – the detector. Note that this sensitivity is also present when the camera is switched off and the lens cap is mounted on the lens.
- Each camera from FLIR Systems is calibrated prior to shipping. It is advisable that the camera is sent in for calibration once a year.
- For protective reasons, the LCD (where applicable) will be switched off if the detector temperature exceeds +60 °C (+149 °F) and the camera will be switched off if the detector temperature exceeds +68 °C (+154.4 °F).
- The camera requires a warm-up time of 5 minutes before accurate measurements (where applicable) can be expected.

INTENTIONALLY LEFT BLANK

---

## 2 Important note about this manual

2

As far as it is practically possible, FLIR Systems configures each manual to reflect each customer's particular camera configuration. However, please note the following exceptions:

- The packing list is subject to specific customer configuration and may contain more or less items
- FLIR Systems reserves the right to discontinue models, parts and accessories, and other items, or change specifications at any time without prior notice
- In some cases, the manual may describe features that are not available in your particular camera configuration

INTENTIONALLY LEFT BLANK

---

# 3 Welcome!

Thank you for choosing the ThermaCAM™ B2 infrared camera – the industry-standard tool for carrying out building thermography inspections!

The ThermaCAM™ B2 IR camera measures and images the emitted infrared radiation from an object. The fact that radiation is a function of object surface temperature makes it possible for the camera to calculate and display this temperature. The camera system also features a laser pointer, a 2.5" color LCD, an IR lens, a removable battery and a range of accessories.

The camera is very easy to use. It is operated by using a few buttons which are conveniently placed on the camera, allowing fingertip control of major functions. A built-in menu system also gives easy access to an advanced, simple-to-use camera software for increased functionality.

To document the object under inspection it is possible to capture and store images to the camera's internal memory. The images can be analyzed either in the field by using the real-time measurement functions built into the camera, or in a PC using FLIR Systems ThermaCAM Reporter software by downloading the images from the camera using ThermaCAM™ QuickView.

## 3.1 About FLIR Systems

With over 40 years experience in IR systems and applications development, and over 30 000 infrared cameras in use worldwide, FLIR Systems is the undisputed global commercial IR industry leader.



**Figure 3.1** FLIR Systems, Boston, USA, FLIR Systems, Danderyd, Sweden, and FLIR Systems, Portland, USA.



**Figure 3.2** Indigo Operations, Niceville, USA, and Indigo Operations, Santa Barbara, USA. Indigo Operations is a division of FLIR Systems.

As pioneers in the IR industry, FLIR Systems has a long list of 'firsts' the world of infrared thermography:

- 1965: 1st thermal imaging system for predictive maintenance (Model 650).
- 1973: 1st battery-operated portable IR scanner for industrial applications predictive maintenance (Model 750).
- 1975: 1st TV compatible system (Model 525).
- 1978: 1st dual-wavelength scanning system capable of real-time analog recording of thermal events (Model 780). Instrumental in R & D market development.
- 1983: 1st thermal imaging and measurement system with on-screen temperature measurement.
- 1986: 1st TE (thermo-electrically) cooled system.
- 1989: 1st single-piece infrared camera system for PM (predictive maintenance) and R & D (research & development) with on-board digital storage.
- 1991: 1st Windows-based thermographic analysis and reporting system.
- 1993: 1st Focal Plane Array (FPA) system for PM and R & D applications.
- 1995: 1st full-featured camcorder style FPA infrared system (ThermaCAM).
- 1997: 1st: uncooled microbolometer-based PM/R & D system.

- 2000: 1st thermography system with both thermal and visual imaging.
- 2000: 1st thermography system to incorporate thermal/visual/voice and text data logging.
- 2002: 1st automated thermography system (model P60) to feature detachable remotely controllable LCD, JPEG image storage, enhanced connectivity including USB and IrDA wireless, thermal/visual/voice and text data logging.
- 2002: 1st low-cost ultra-compact hand-held thermography camera (E series). Revolutionary, ergonomic design, lightest IR measurement camera available.
- 2003: 1st low-cost, ultra-compact infrared camera for fixed installation intended for automation and security applications. Exceptionally user-friendly due to standard interfaces and extensive built-in functionality.
- 2004: 1st camera models specially designed for building thermography (B1, B2 and B20)

3

10401603.a3





**Figure 3.3 LEFT:** FLIR Systems Thermovision® Model 661. The photo is taken on May 30th, 1969 at the distribution plant near Beckomberga, in Stockholm, Sweden. The camera weighed approx. 25 kg (55 lb), the oscilloscope 20 kg (44 lb), the tripod 15 kg (33 lb). The operator also needed a 220 VAC generator set, and a 10 L (2.6 US gallon) jar with liquid nitrogen. To the left of the oscilloscope the Polaroid attachment (6 kg/13 lb) can be seen. **RIGHT:** FLIR Systems ThermoCAM Model E2 from 2002 – weight: 0.7 kg (1.54 lb), including battery.

With this tradition of unparalleled technical excellence and innovative achievements, FLIR Systems continues to develop new infrared products, educational venues and applications expertise to meet the diverse demands of thermographers worldwide.


### 3.1.1 A few images from our facilities

10401303.a1

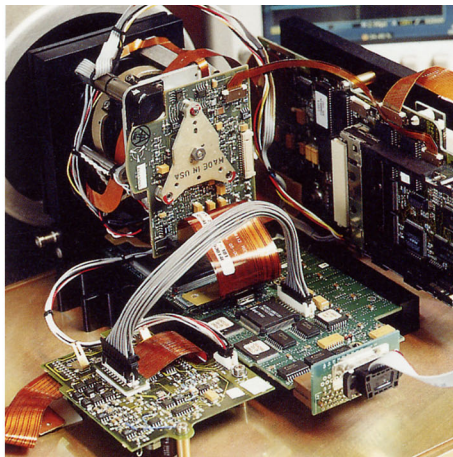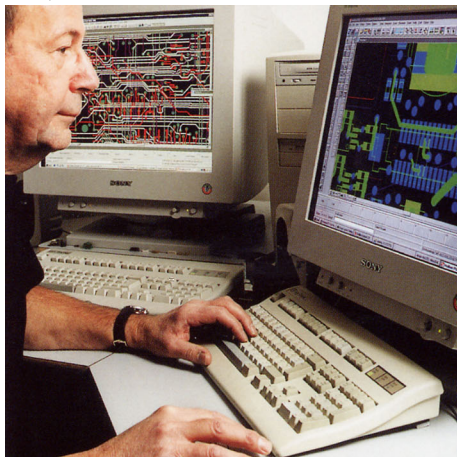

**Figure 3.4 LEFT:** Development of system electronics; **RIGHT:** Testing of an FPA detector

10401403.a1

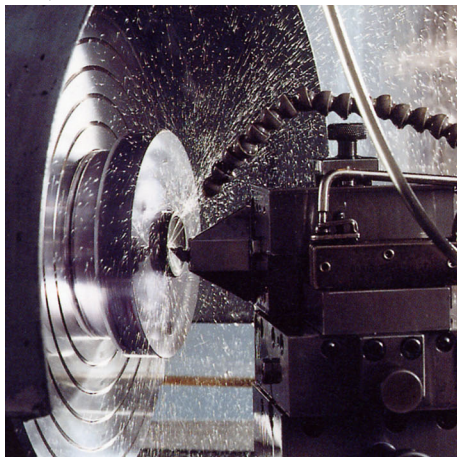

**Figure 3.5 LEFT:** Diamond turning machine; **RIGHT:** Lens polishing

10401503.a1



3

**Figure 3.6** LEFT: Testing of IR cameras in the climatic chamber; RIGHT: Robot for camera testing and calibration

## 3.2 *Comments & questions*

FLIR Systems is committed to a policy of continuous development, and although we have tested and verified the information in this manual to the best of our ability, you may find that features and specifications have changed since the time of printing. Please let us know about any errors you find, as well as your suggestions for future editions, by sending an e-mail to:

*documentation@flir.se*

☛ Do not use this e-mail address for technical support questions. Technical support is handled by FLIR Systems local sales offices.

---

## 4 Packing list

The ThermaCAM™ B2 and its accessories are delivered in a hard transport case which typically contains the items below. On receipt of the transport case, inspect all items and check them against the delivery note. Any damaged items must be reported to the local FLIR Systems representative immediately.


| Description                             | Part Number             | Qty. |
|-----------------------------------------|-------------------------|------|
| Battery                                 | 1 195 106               | 2    |
| Hand strap                              | 1 195 221               | 1    |
| Lens cap for camera body                | 1 120 987               | 1    |
| Operator's manual                       | 1558073                 | 1    |
| Power supply                            | 1 909 528               | 1    |
| ThermaCAM™ B2 infrared camera with lens | Configuration-dependent | 1    |
| TrainIR CD                              | 1 195 494               | 1    |
| USB cable                               | 1 195 128               | 1    |
| Video cable                             | 1 909 775               | 1    |

INTENTIONALLY LEFT BLANK

## 5 System overview

This system overview shows all accessories that are possible to order for a ThermoCAM™ B2.

10396703,a4

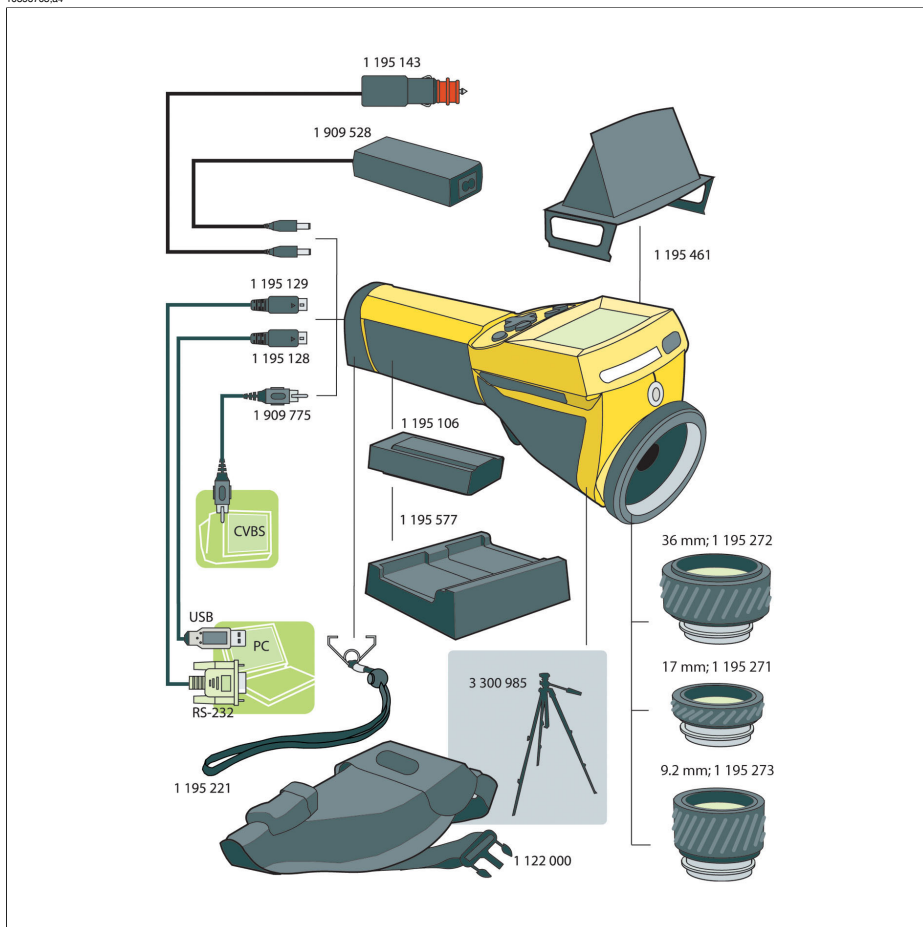


**Figure 5.1** System overview

INTENTIONALLY LEFT BLANK

## 6 Connecting system components

10438303.a2

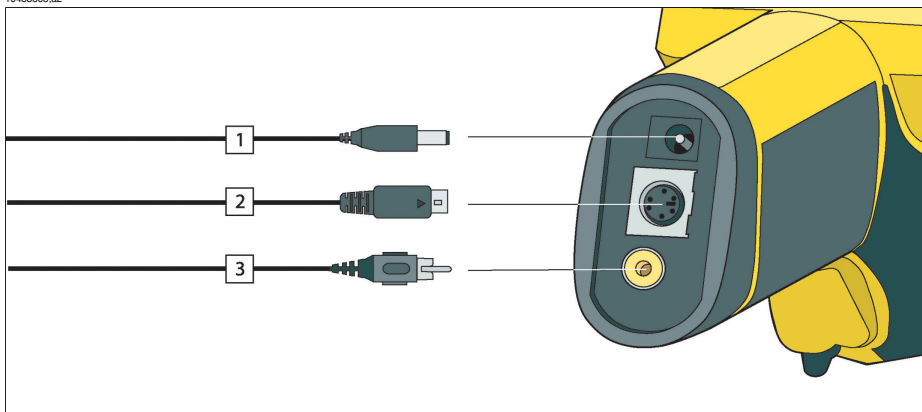

**Figure 6.1** How to connect system components

**Figure 6.2** Explanations of callouts

| Callout | Explanation                              |
|---------|------------------------------------------|
| 1       | Power supply cable (11–16 VDC)           |
| 2       | USB / RS-232 cable                       |
| 3       | Video cable (CVBS, i.e. composite video) |

INTENTIONALLY LEFT BLANK

---

# 7 Introduction to building thermography

## 7.1 *Important note*

All camera functions and features that are described in this section may not be supported by your particular camera configuration.


## 7.2 *Typical field investigations*

### 7.2.1 Guidelines

As will be noted in subsequent sections there are a number of general guidelines the user should take heed of when carrying out building thermography inspection. This section gives a summary of these guidelines.

#### 7.2.1.1 *General guidelines*

- The emissivity of the majority of building materials fall between 0.85 and 0.95. Setting the emissivity value in the camera to 0.90 can be regarded as a good starting point.
- An infrared inspection alone should never be used as a decision point for further actions. Always verify suspicions and findings using other methods, such as construction drawings, moisture meters, humidity & temperature datalogging, tracer gas testing etc.
- Change level and span to thermally tune the infrared image and reveal more details. The figure below shows the difference between a thermally untuned and a thermally tuned infrared image.

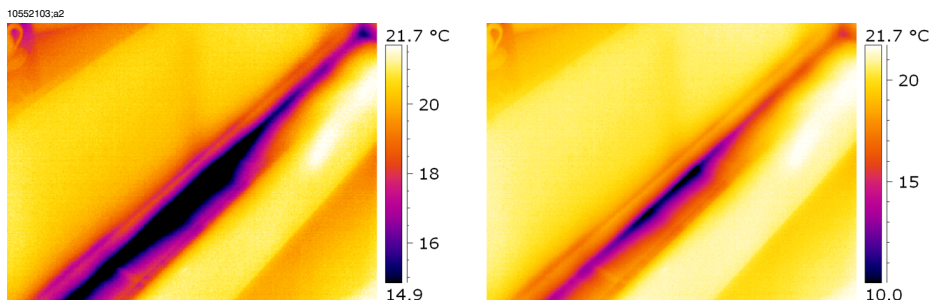


**Figure 7.1** LEFT: A thermally untuned infrared image; RIGHT: A thermally tuned infrared image, after having changed level and span.

### 7.2.1.2 *Guidelines for moisture detection, mold detection & detection of water damages*

- Building defects related to moisture and water damages may only show up when heat has been applied to the surface, e.g. from the sun.
- The presence of water changes the thermal conductivity and the thermal mass of the building material. It may also change the surface temperature of building material due to evaporative cooling. Thermal conductivity is a material's ability to conduct heat, while thermal mass is its ability to store heat.
- Infrared inspection does not directly detect the presence of mold, rather it may be used to find moisture where mold may develop or has already developed. Mold requires temperatures between +4°C to +38°C (+40°F to +100°F), nutrients and moisture to grow. Humidity levels above 50% can provide sufficient moisture to enable mold to grow.

10556003.a1

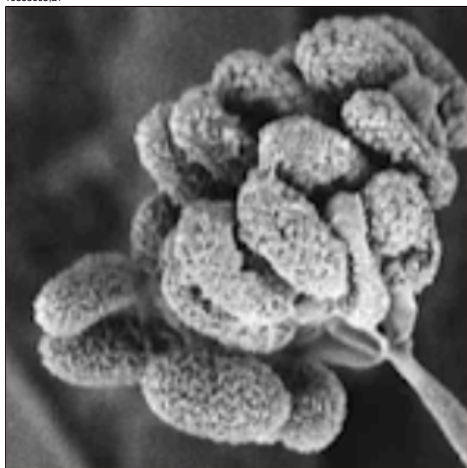

**Figure 7.2** Microscopic view of mold spore

### 7.2.1.3 *Guidelines for detection of air infiltration & insulation deficiencies*

- For very accurate camera measurements, take measurements of the temperature and enter this value in the camera.
- It is recommended that there is a difference in pressure between the outside and the inside of the building structure. This facilitates the analysis of the infrared images and reveals deficiencies that would not be visible otherwise. Although a negative pressure of between 10 and 50 Pa is recommended, carrying out the inspection at a lower negative pressure may be acceptable. To do this, close all windows, doors and ventilation ducts and then run the kitchen exhaust fan for some time to reach a negative pressure of 5–10 Pa (applies to residential houses only).

- A difference in temperature between the inside and the outside of 10–15°C (18–27°F) is recommended. Inspections can be carried out at a lower temperature difference, but will make the analysis of the infrared images somewhat more difficult.
- Avoid direct sunlight on a part of a building structure—e.g. a façade—that is to be inspected from the inside. The sunlight will heat the façade which will equalize the temperature differences on the inside and mask deficiencies in the building structure. Spring seasons with low nighttime temperatures ( $\pm 0^{\circ}\text{C}$  ( $+32^{\circ}\text{F}$ )) and high daytime temperatures ( $+14^{\circ}\text{C}$  ( $+57^{\circ}\text{F}$ )) are especially risky.

### 7.2.2 About moisture detection

Moisture in a building structure can originate from several different sources, e.g.:

- External leaks, such as floods, leaking fire hydrants etc.
- Internal leaks, such as freshwater piping, waste water piping etc.
- Condensation, which is humidity in the air falling out as liquid water due to condensation on cold surfaces.
- Building moisture, which is any moisture in the building material prior to erecting the building structure.
- Water remaining from firefighting.

As a non-destructive detection method, using an infrared camera has a number of advantages over other methods, and a few disadvantages:

| Advantage                                                                                                                                                                                                                                                                                                                                                                 | Disadvantage                                                                                                                                                                                                                         |
|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <ul style="list-style-type: none"> <li>■ The method is quick.</li> <li>■ The method is a non-intrusive means of investigation.</li> <li>■ The method does not require relocation of the occupants.</li> <li>■ The method features an illustrative visual presentation of findings.</li> <li>■ The method confirms failure points and moisture migration paths.</li> </ul> | <ul style="list-style-type: none"> <li>■ The method only detects surface temperature differentials and can not see through walls.</li> <li>■ The method can not detect subsurface damage, i.e. mold or structural damage.</li> </ul> |

### 7.2.3 Moisture detection (1): Low-slope commercial roofs

#### 7.2.3.1 General information

Low-slope commercial roofing is one of the most common roof types for industrial building, such as warehouses, industrial plants, machinery shops etc. Its major advantages over a pitched roof is the lower cost in material and building. However, due to its design where snow and ice will not fall off by itself—as is the case for the majority of pitched roofs—it must be strongly built to support the accumulated weight of both roof structure and any snow, ice and rain.

Although a basic understanding of the construction of low-slope commercial roofs is desirable when carrying out a roof thermography inspection, expert knowledge is not necessary. There is a large number of different design principles for low-slope commercial roofs—both when it comes to material and design—and it would be impossible for the infrared inspection person to know them all. If additional information about a certain roof is needed, the architect or contractor of the building can usually supply the relevant information.

Common causes of roof failure are outlined in the table below (from SPIE Thermosense Proceedings Vol. 371 (1982), p. 177).

| Cause            | %    |
|------------------|------|
| Poor workmanship | 47.6 |
| Roof traffic     | 2.6  |
| Poor design      | 16.7 |
| Trapped moisture | 7.8  |
| Materials        | 8.0  |
| Age & weathering | 8.4  |

Potential leak locations include the following:



- Flashing
- Drains
- Penetrations
- Seams
- Blisters



#### 7.2.3.2 Safety precautions

- Recommend a minimum of two people on a roof, preferably three or more.
- Inspect the underside of the roof for structural integrity prior to walking on it.
- Avoid stepping on blisters that are common on built up bitumen and gravel roofs.
- Have a cell phone or radio available in case of emergency.
- Inform local police and plant security prior to doing nighttime roof survey.

### 7.2.3.3 Commented building structures

This section includes a few typical examples of moisture problems on low-slope commercial roofs.
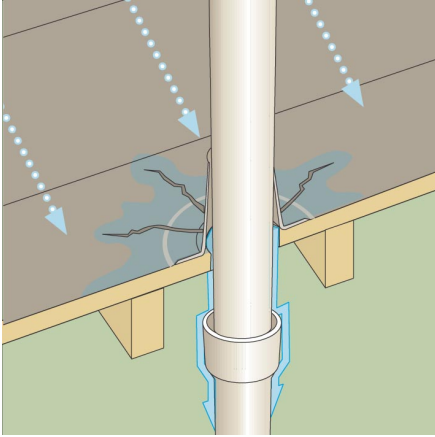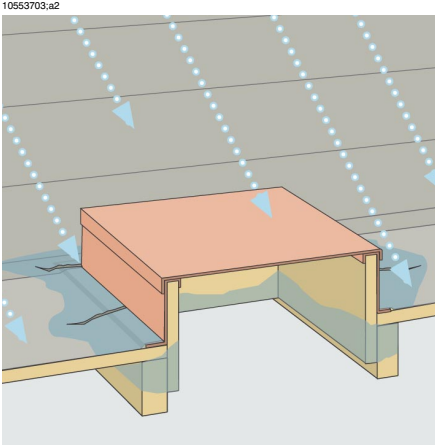
| Structural drawing                                                                                    | Comment                                                                                                                              |
|-------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------|
| <p>10553603;a2</p>   | <p>Inadequate sealing of roof membrane around conduit and ventilation ducts leading to local leakage around the conduit or duct.</p> |
| <p>10553703;a2</p>  | <p>Roof membrane inadequately sealed around roof access hatch.</p>                                                                   |
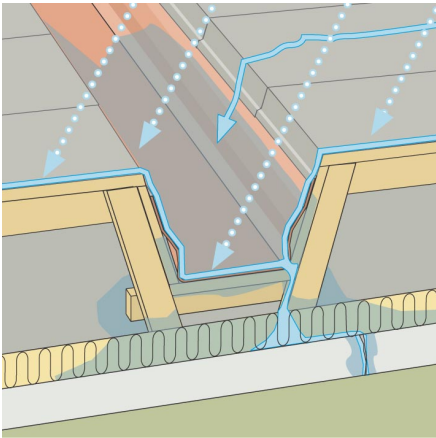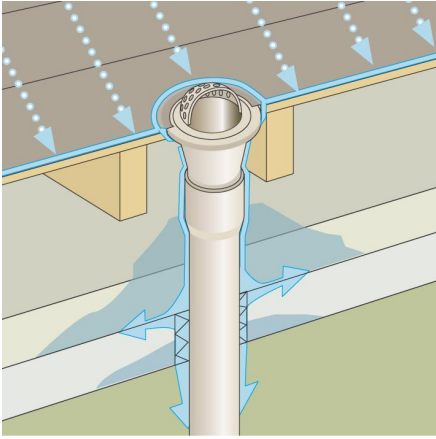
| Structural drawing                                                                                        | Comment                                                                                                                                                                            |
|-----------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <div>10553803;a2</div>   | Drainage channels located too high and with too low an inclination. Some water will remain in the drainage channel after rain, which may lead to local leakage around the channel. |
| <div>10553803;a2</div>  | Inadequate sealing between roof membrane and roof outlet leading to local leakage around the roof outlet.                                                                          |



7

7.2.3.4      *Commented infrared images*

How do you find wet insulation below the surface of the roof? When the surface itself is dry, including any gravel or ballast, a sunny day will warm the entire roof. Early in the evening, if the sky is clear, the roof will begin to cool down by radiation. Because of its higher thermal capacity the wet insulation will stay warmer longer than the dry and will be visible in the infrared imager (see photos below). The technique is particularly effective on roofs having absorbent insulation—such as wood fiber, fiberglass, and perlite—where thermal patterns correlate almost perfectly with moisture.

Infrared inspections of roofs with nonabsorbent insulations, common in many single-ply systems, are more difficult to diagnose because patterns are more diffuse.

This section includes a few typical infrared images of moisture problems on low-slope commercial roofs:
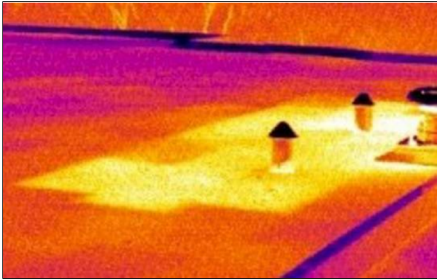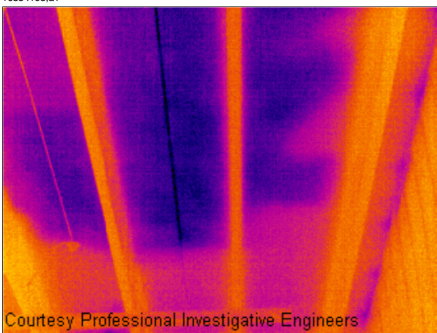
| Infrared image                                                                                                                                             | Comment                                                                                                                                                                                                                                                                                |
|------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <p>10554003.a1</p>                                                        | <p>Moisture detection on a roof, recorded during the evening.</p> <p>Since the building material affected by moisture has a higher thermal mass, its temperature decreases slower than surrounding areas.</p>                                                                          |
| <p>10554103.a1</p>  <p>Courtesy Professional Investigative Engineers</p> | <p>Water-damaged roofing components and insulation identified from infrared scan from the underside of the built-up roof on a structural concrete tee deck.</p> <p>Affected areas are cooler than the surrounding sound areas, due to conductive and/or thermal capacitive effect.</p> |
| <p>10554203.a1</p>                                                      | <p>Daytime survey of built-up low-slope commercial roof.</p> <p>Affected areas are cooler than the surrounding dry areas, due to conductive and/or thermal capacitive effect.</p>                                                                                                      |



7.2.4                    **Moisture detection (2): Commercial & residential façades**



7.2.4.1                **General information**

Thermography has proven to be invaluable in the assessment of moisture infiltration into commercial and residential façades. Being able to provide a physical illustration of the moisture migration paths is more conclusive than extrapolating moisture meter probe locations and more cost-effective than large intrusive test cuts.

7.2.4.2                **Commented building structures**


This section includes a few typical examples of moisture problems on commercial and residential façades.
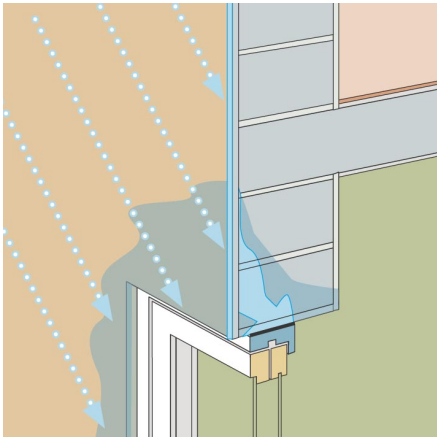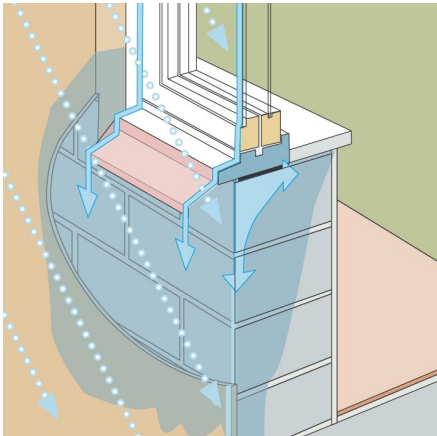
| Structural drawing                                                                                         | Comment                                                                                                                                                                                     |
|------------------------------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <div>10554303;a2</div>   | Pelting rain penetrates the façade due to badly executed bed joints. Moisture builds up in the masonry above the window.                                                                    |
| <div>10554403;a2</div>  | Pelting rain hits the window at an angle. Most of the rain runs off the window edge flashing but some finds its way into the masonry where the plaster meets the underside of the flashing. |
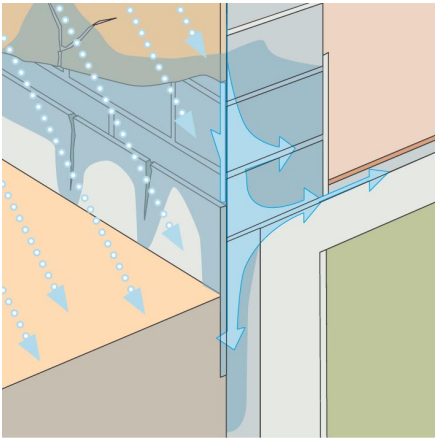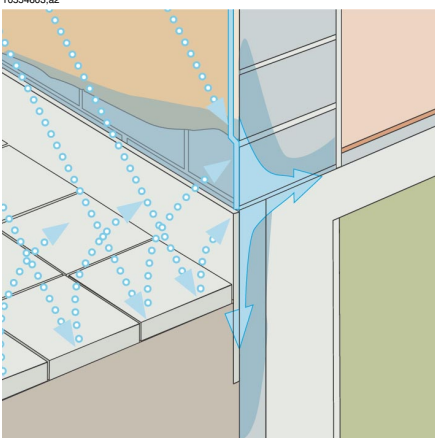
| Structural drawing                                                                                    | Comment                                                                                                                                                         |
|-------------------------------------------------------------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <p>10554503,a2</p>   | <p>Rain hits the façade at an angle and penetrates the plaster through cracks. The water then follows the inside of the plaster and leads to frost erosion.</p> |
| <p>10554603,a2</p>  | <p>Rain splashes on the façade and penetrates the plaster and masonry by absorption, which eventually leads to frost erosion.</p>                               |

7.2.4.3                      *Commented infrared images*

This section includes a few typical infrared images of moisture problems on commercial & residential façades.
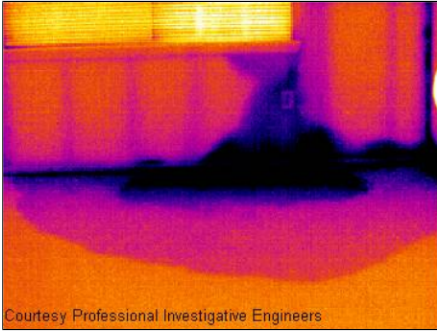
| Infrared image                                                                                                                                                     | Comment                                                                                                                                                                            |
|--------------------------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <div>10554703.a1</div>  <div>Courtesy Professional Investigative Engineers</div>  | Improperly terminated and sealed stone veneer to window frame and missing flashings has resulted in moisture infiltration into the wall cavity and interior living space.          |
| <div>10554803.a1</div>  <div>Courtesy Professional Investigative Engineers</div> | Moisture migration into drywall from capillary drive and interior finish components from inadequate clearance and slope of grade from vinyl siding façade on an apartment complex. |

7.2.5                      **Moisture detection (3): Decks & balconies**



7.2.5.1                      *General information*



Although there are differences in design, materials and construction, decks—plaza decks, courtyard decks etc—suffer from the same moisture and leaking problems as low-slope commercial roofs. Improper flashing, inadequately sealed membranes, and insufficient drainage may lead to substantial damage in the building structures below.

Balconies, although smaller in size, require the same care in design, choice of material, and workmanship as any other building structure. Since balconies are usually supported on one side only, moisture leading to corrosion of struts and concrete reinforcement can cause problems and lead to hazardous situations.

### 7.2.5.2 Commented building structures



This section includes a few typical examples of moisture problems on decks and balconies.
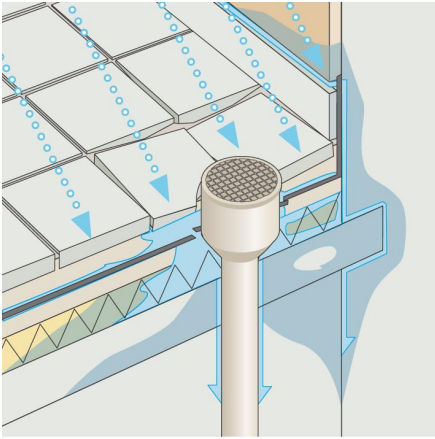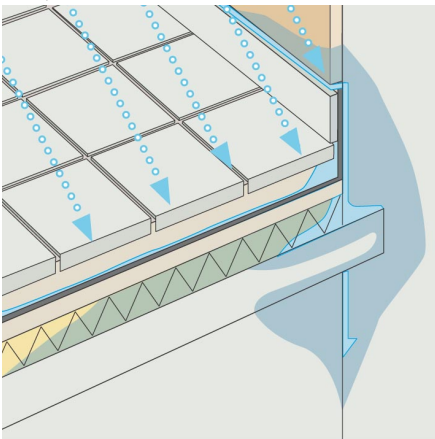
| Structural drawing                                                                                    | Comment                                                                                                 |
|-------------------------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------|
| <p>10555203:a2</p>   | <p>Improper sealing of paving and membrane to roof outlet, leading to leakage during rain.</p>          |
| <p>10555103:a2</p>  | <p>No flashing at deck-to-wall connection, leading to rain penetrating the concrete and insulation.</p> |
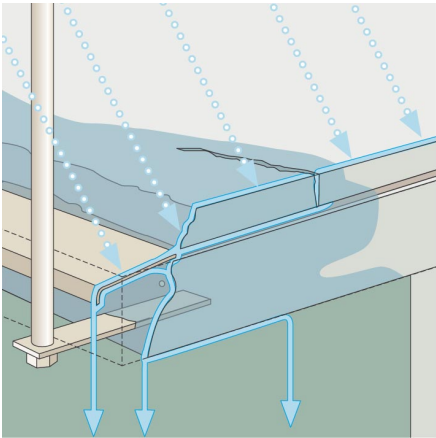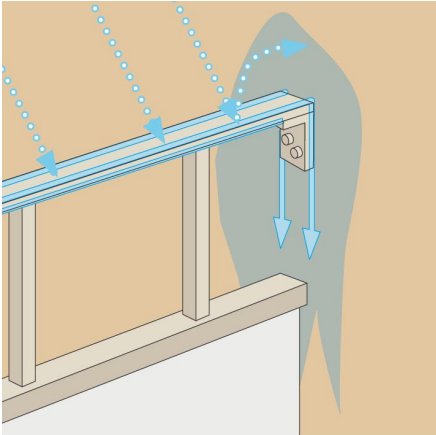
| Structural drawing                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              | Comment                                                                                                                                                                           |
|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <div>10555003.a2</div>  <p>The drawing shows a cross-section of a concrete structure. A vertical pipe is on the left. A horizontal concrete slab (drop apron) is shown with a crack. Dotted blue arrows represent water droplets falling from above. Solid blue arrows show water penetrating through the crack in the concrete and flowing downwards. The concrete is shown with a jagged, broken texture where the water is penetrating.</p> | <p>Water has penetrated the concrete due to inadequately sized drop apron and has led to concrete disintegration and corrosion of reinforcement.</p> <p><b>SECURITY RISK!</b></p> |
| <div>10554903.a2</div>  <p>The drawing shows a cross-section of a wall and a handrail. A metal bracket is used to fasten the handrail to the wall. Dotted blue arrows represent water droplets falling from above. Solid blue arrows show water penetrating through the bracket and the wall, flowing downwards. The wall is shown with a jagged, broken texture where the water is penetrating.</p>                                          | <p>Water has penetrated the plaster and underlying masonry at the point where the handrail is fastened to the wall.</p> <p><b>SECURITY RISK!</b></p>                              |

### 7.2.5.3 Commented infrared images

This section includes a few typical infrared images of moisture problems on decks and balconies.
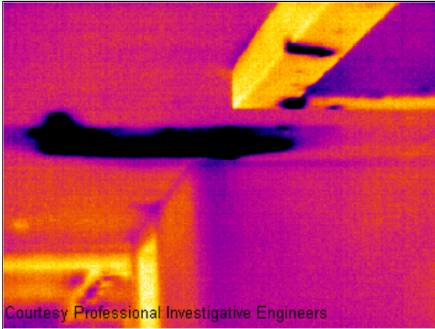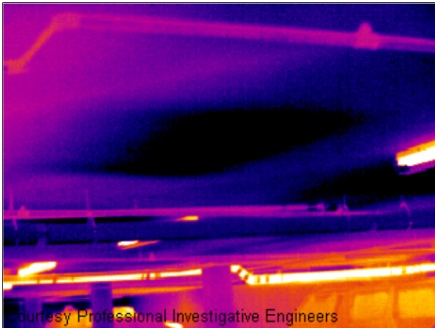
| Infrared image                                                                                                                                             | Comment                                                                                                                                                                                                                 |
|------------------------------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <p>10555303.a1</p>  <p>Courtesy Professional Investigative Engineers</p>  | <p>Improper flashing at balcony-to-wall connections and missing perimeter drainage system resulted in moisture intrusion into the wood framing support structure of the exterior walkway balcony of a loft complex.</p> |
| <p>10555403.a1</p>  <p>Courtesy Professional Investigative Engineers</p> | <p>A missing composite drainage plane or medium on a below-grade parking garage plaza deck structure resulted in standing water between the structural concrete deck and the plaza wearing surface.</p>                 |

## 7.2.6 Moisture detection (4): Plumbing breaks & leaks



### 7.2.6.1 General information



Water from plumbing leaks can often lead to severe damage on a building structure. Small leaks may be difficult to detect, but can—over the years—penetrate structural walls and foundations to a degree where the building structure is beyond repair.

Using building thermography at an early stage when plumbing breaks and leaks are suspected can lead to substantial savings on material and labor.

7.2.6.2                      *Commented infrared images*

This section includes a few typical infrared images of plumbing breaks & leaks.
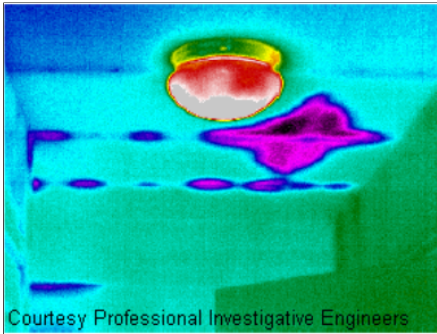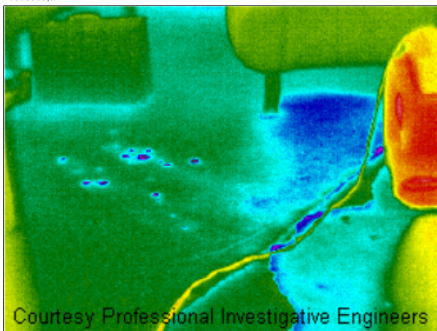
| Infrared image                                                                                                                                                 | Comment                                                                                                                                                                                      |
|----------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <div>10555503.a1</div>  <p>Courtesy Professional Investigative Engineers</p>  | Moisture migration tracking along steel joist channels inside ceiling of a single family home where a plumbing line had ruptured.                                                            |
| <div>10555603.a1</div>  <p>Courtesy Professional Investigative Engineers</p> | Water from plumbing leak was found to have migrated farther than originally anticipated by the contractor during remediation techniques of cutting back carpet and installing dehumidifiers. |
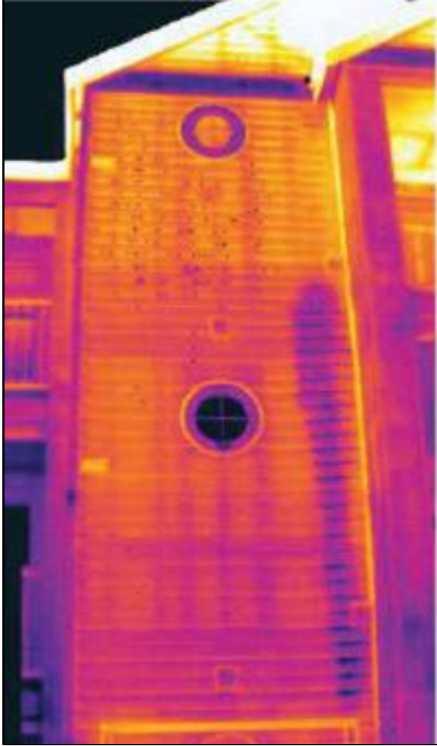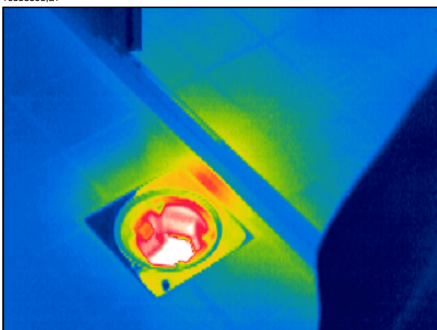
| Infrared image                                                                                                                    | Comment                                                                                                                                                                                                                            |
|-----------------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <p data-bbox="150 199 210 211">10555703.a1</p>   | <p data-bbox="611 199 1054 302">The infrared image of this vinyl-sided 3-floor apartment house clearly shows the path of a serious leak from a washing machine on the third floor, which is completely hidden within the wall.</p> |
| <p data-bbox="150 976 210 987">10555803.a1</p>  | <p data-bbox="611 976 1054 1032">Water leak due to improper sealing between floor drain and tiles.</p>                                                                                                                             |

7.2.7 Air infiltration

7.2.7.1 General information


Due to the wind pressure on a building, temperature differences between the inside and the outside of the building, and the fact that most buildings use exhaust air terminal devices to extract used air from the building, a negative pressure of 2–5 Pa can be expected. When this negative pressure leads to cold air entering the building structure due to deficiencies in building insulation and/or building sealing, we have what is called *air infiltration*. Air infiltration can be expected at joints and seams in the building structure.



Due to the fact that air infiltration creates an air flow of cool air into e.g. a room, it can lead to substantial deterioration of the indoor climate. Air flows as small as 0.15 m/s (0.49 ft./s) are usually noticed by inhabitants, although these air flows may be difficult to detect using ordinary measurement devices.

On an infrared image air infiltration can be identified by its typical ray pattern, which emanates from the point of exit in the building structure—e.g. from behind a skirting strip. Furthermore, areas of air infiltration typically have a lower detected temperature than areas where there is only an insulation deficiency. This is due to the chill factor of the air flow.

7.2.7.2 Commented building structures




This section includes a few typical examples of details of building structures where air infiltration may occur.
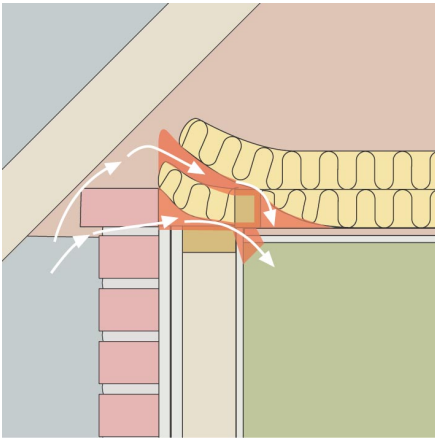
| Structural drawing                                                                                                                                                                                                                                                                                                                                                                                                               | Comment                                                                                                                                                                                        |
|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|  <p>10552503.a2</p> <p>The diagram shows a cross-section of a brick wall and roofline. A yellow fiberglass insulation batt is shown improperly installed, with a gap between it and the wall. Red arrows indicate air infiltration entering the room from behind the cornice. The drawing is labeled '10552503.a2' in the top left corner.</p> | <p>Insulation deficiencies at the eaves of a brickwall house due to improperly installed fiberglass insulation batts.</p> <p>The air infiltration enters the room from behind the cornice.</p> |
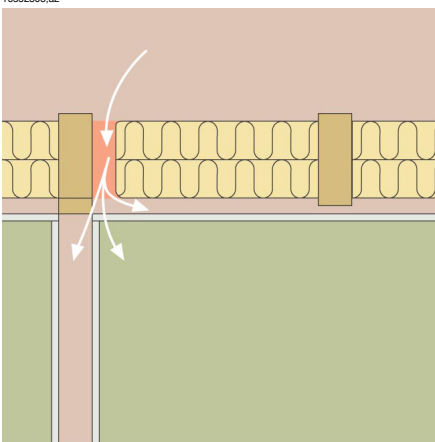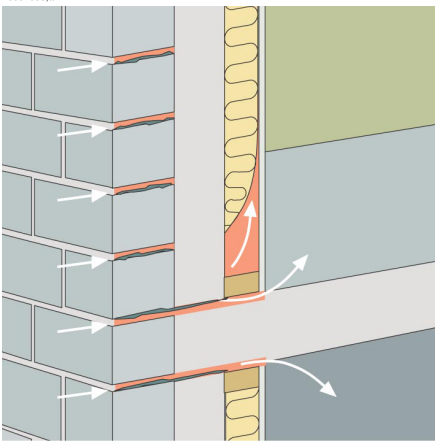
| Structural drawing                                                                                    | Comment                                                                                                                                                                               |
|-------------------------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <p>10552303;a2</p>   | <p>Insulation deficiencies in an intermediate floor due to improperly installed fiberglass insulation batts.</p> <p>The air infiltration enters the room from behind the cornice.</p> |
| <p>10552603;a2</p>  | <p>Air infiltration in a concrete floor-over-crawl-space due to cracks in the brick wall façade.</p> <p>The air infiltration enters the room beneath the skirting strip.</p>          |

7.2.7.3            *Commented infrared images*

This section includes a few typical infrared images of details of building structures where air infiltration has occurred.
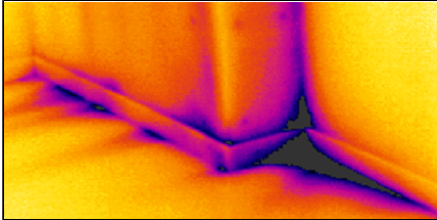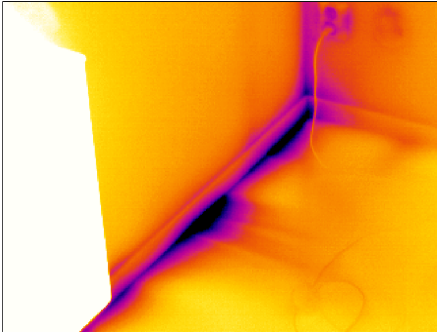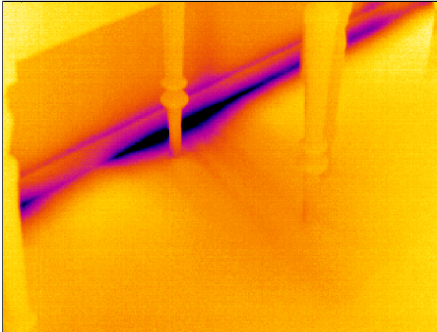
| Infrared image                                                                                            | Comment                                                                                                                       |
|-----------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------|
| <div>10552703.a1</div>   | Air infiltration from behind a skirting strip. Note the typical ray pattern.                                                  |
| <div>10552803.a1</div>   | Air infiltration from behind a skirting strip. Note the typical ray pattern.<br><br>The white area to the left is a radiator. |
| <div>10552903.a1</div>  | Air infiltration from behind a skirting strip. Note the typical ray pattern.                                                  |

## 7.2.8 Insulation deficiencies

### 7.2.8.1 General information

Insulation deficiencies do not necessarily lead to air infiltration. If fiberglass insulation batts are improperly installed air pockets will form in the building structure. Since these air pockets have a different thermal conductivity than areas where the insulation batts are properly installed, the air pockets can be detected during a building thermography inspection.


As a rule of thumb, areas with insulation deficiencies typically have higher temperatures than where there is only an air infiltration.



When carrying out building thermography inspections aimed at detecting insulation deficiencies, be aware of the following parts in a building structure, which may look like insulation deficiencies on the infrared image:

- Wooden joists, studs, rafter, beams
- Steel girders and steel beams
- Water piping inside walls, ceilings, floors
- Electrical installations inside walls, ceilings, floors—such as trunking, piping etc.
- Concrete columns inside timber framed walls
- Ventilation ducts & air ducts

### 7.2.8.2 Commented building structures



This section includes a few typical examples of details of building structures with insulation deficiencies:

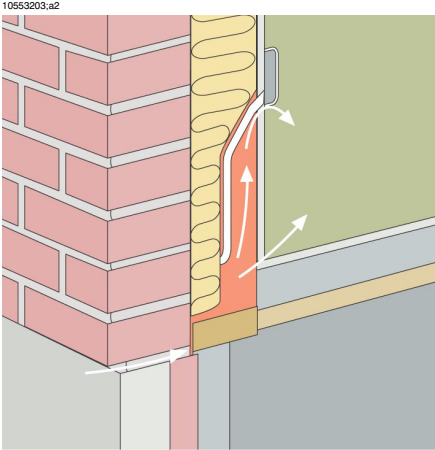
| Structural drawing                                                                 | Comment                                                                                                                                                                                                                              |
|------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|  | <p>Insulation deficiencies (and air infiltration) due to improper installation of insulation batts around an electrical mains supply.</p> <p>This kind of insulation deficiency will show up as dark areas on an infrared image.</p> |
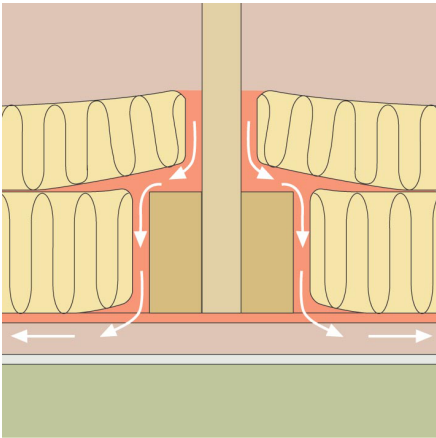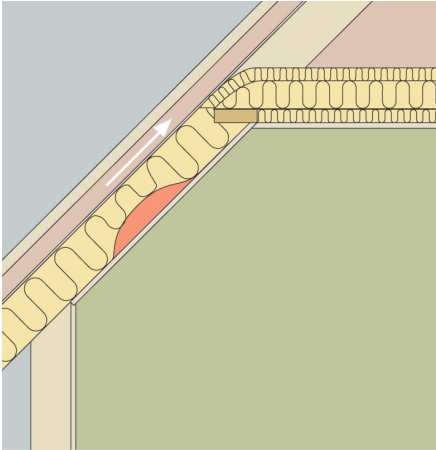
| Structural drawing                                                                                    | Comment                                                                                                                                                                                                                                                                             |
|-------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <p>10553103;a2</p>   | <p>Insulation deficiencies due to improper installation of insulation batts around an attic floor beam. Cool air infiltrates the structure and cools down the inside of the ceiling.</p> <p>This kind of insulation deficiency will show up as dark areas on an infrared image.</p> |
| <p>10553003;a2</p>  | <p>Insulation deficiencies due to improper installation of insulation batts creating an air pocket on the outside of an inclined ceiling.</p> <p>This kind of insulation deficiency will show up as dark areas on an infrared image.</p>                                            |

### 7.2.8.3 Commented infrared images

This section includes a few typical infrared images of insulation deficiencies.
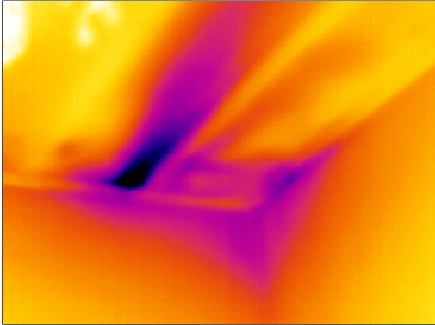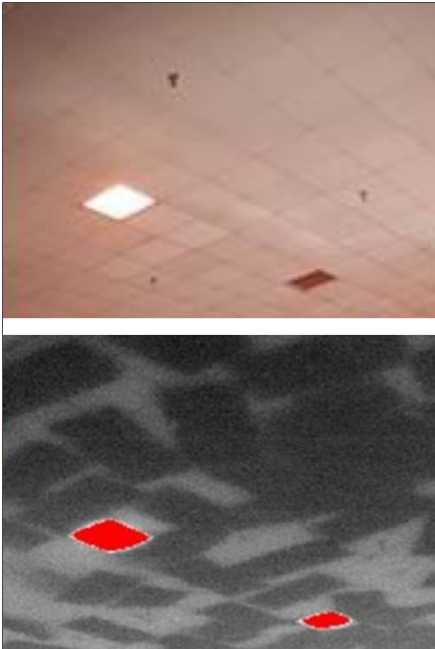
| Infrared image                                                                                        | Comment                                                                                                                                                                                  |
|-------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <p>10553303.a1</p>   | <p>Insulation deficiencies in an intermediate floor structure. The deficiency may be due to either missing insulation batts or improperly installed insulations batts (air pockets).</p> |
| <p>10553403.a1</p>  | <p>Improperly installed fiberglass batts in a suspended ceiling.</p>                                                                                                                     |
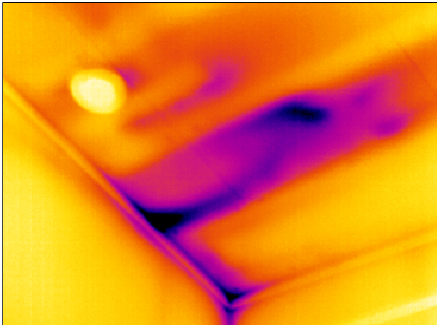
| Infrared image                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           | Comment                                                                                                                                                                           |
|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <div>10553503.a1</div>  An infrared thermography image of a floor structure. The image shows a corner where two walls meet the floor. The floor surface is predominantly yellow and orange, indicating higher temperatures. There are several dark, irregular patches of purple and blue, particularly along the edges and in the center, which represent areas of lower temperature. These cooler areas suggest insulation deficiencies, such as missing insulation batts or air pockets, which are causing heat loss. | Insulation deficiencies in an intermediate floor structure. The deficiency may be due to either missing insulation batts or improperly installed insulations batts (air pockets). |

## 7.3 *Theory of building science*

### 7.3.1 General information

The demand for energy-efficient constructions has increased significantly in recent times. Developments in the field of energy, together with the demand for pleasant indoor environments, have resulted in ever-greater significance having to be attached to both the function of a building's thermal insulation and airtightness and the efficiency of its heating and ventilation systems.

Defective insulation and tightness in highly insulated and airtight structures can have a great impact on energy losses. Defects in a building's thermal insulation and airtightness do not merely entail risk of excessive heating and maintenance costs, they also create the conditions for a poor indoor climate.

A building's degree of insulation is often stated in the form of a thermal resistance or a coefficient of thermal transmittance (U value) for the various parts of the building. However, the stated thermal resistance values rarely provide a measure of the actual energy losses in a building. Air leakage from joints and connections that are not airtight and insufficiently filled with insulation often gives rise to considerable deviations from the designed and expected values.

Verification that individual materials and building elements have the promised properties is provided by means of laboratory tests. Completed buildings have to be checked and inspected in order to ensure that their intended insulation and airtightness functions are actually achieved.

In its structural engineering application, thermography is used to study temperature variations over the surfaces of a structure. Variations in the structure's thermal resistance can, under certain conditions, produce temperature variations on its surfaces. Leakage of cold (or warm) air through the structure also affects the variation in surface temperature. This means that insulation defects, thermal bridges and air leaks in a building's enclosing structural components can be located and surveyed.

Thermography itself does not directly show the structure's thermal resistance or airtightness. Where quantification of thermal resistance or airtightness is required, additional measurements have also to be taken. Thermographic analysis of buildings relies on certain prerequisites in terms of temperature and pressure conditions across the structure.

Details, shapes and contrasts in the thermal image can vary quite clearly with changes in any of these parameters. The in-depth analysis and interpretation of thermal images therefore requires thorough knowledge of such aspects as material and structural properties, the effects of climate and the latest measuring techniques. For assessing

the results of measurements, there are special requirements in terms of the skills and experience of those taking the measurements, e.g. by means of authorization by a national or regional standardization body.

### 7.3.2 The effects of testing and checking

It can be difficult to anticipate how well the thermal insulation and airtightness of a completed building will work. There are certain factors involved in assembling the various components and building elements that can have a considerable impact on the final result. The effects of transport, handling and storage at the site and the way the work is done cannot be calculated in advance. To ensure that the intended function is actually achieved, verification by testing and checking the completed building is required.

Modern insulation technology has reduced the theoretical heat requirement. This does mean, however, that defects that are relatively minor, but at important locations, e.g. leaking joints or incorrectly installed insulation, can have considerable consequences in terms both of heat and comfort. Verification tests, e.g. by means of thermography, have proved their value, from the point of view both of the designer and the contractor and of the developer, the property manager and the user.

- For the designer, the important thing is to find out about the function of various types of structures, so that they can be designed to take into account both working methods and functional requirements. The designer must also know how different materials and combinations of materials function in practice. Effective testing and checking, as well as experiential feedback, can be used to achieve the required development in this area.
- The contractor is keen on more testing and inspection in order to ensure that the structures keep to an expected function that corresponds to established requirements in the regulations issued by authorities and in contractual documents. The contractor wants to know at an early stage of construction about any changes that may be necessary so that systematic defects can be prevented. During construction, a check should therefore be carried out on the first apartments completed in a mass production project. Similar checking then follows as production continues. In this way systematic defects can be prevented and unnecessary costs and future problems can be avoided. This check is of benefit both to manufacturers and to users.
- For the developer and the property manager it is essential that buildings are checked with reference to heat economy, maintenance (damage from moisture or moisture infiltration) and comfort for the occupants (e.g. cooled surfaces and air movements in occupied zones).

- For the user the important thing is that the finished product fulfills the promised requirements in terms of the building's thermal insulation and airtightness. For the individual, buying a house involves a considerable financial commitment, and the purchaser therefore wants to know that any defects in the construction will not involve serious financial consequences or hygiene problems.

The effects of testing and checking a building's insulation and airtightness are partly physiological and partly financial.

The physiological experience of an indoor climatic environment is very subjective, varying according to the particular human body's heat balance and the way the individual experiences temperature. The experience of climate depends on both the indoor air temperature and that of the surrounding surfaces. The speed of movement and moisture content of indoor air are also of some significance. Physiologically, a draft produces the sensation of local cooling of the body's surface caused by

- excessive air movements in the occupied zone with normal air temperature;
- normal air movements in the occupied zone but a room temperature that is too low;
- substantial radiated heat exchange with a cold surface.

It is difficult to assess the quantitative effects of testing and checking a building's thermal insulation.

Investigations have shown that defects found in the thermal insulation and airtightness of buildings cause heat losses that are about 20–30% more than was expected. Monitoring energy consumption before and after remedial measures in relatively large complexes of small houses and in multi-dwelling blocks has also demonstrated this. The figures quoted are probably not representative of buildings in general, since the investigation data cannot be said to be significant for the entire building stock. A cautious assessment however would be that effectively testing and checking a building's thermal insulation and airtightness can result in a reduction in energy consumption of about 10%.

Research has also shown that increased energy consumption associated with defects is often caused by occupants increasing the indoor temperature by one or a few degrees above normal to compensate for the effect of annoying thermal radiation towards cooled surfaces or a sensation of disturbing air movements in a room.

### 7.3.3 Sources of disruption in thermography

During thermography, the risk of confusing temperature variations caused by insulation defects with those associated with the natural variation in U values along warm surfaces of a structure is considered slight under normal conditions.

The temperature changes associated with variations in the U value are generally gradual and symmetrically distributed across the surface. Variations of this kind do of course occur at the angles formed by roofs and floors and at the corners of walls.

Temperature changes associated with air leaks or insulation defects are in most cases more evident with characteristically shaped sharp contours. The temperature pattern is usually asymmetrical.

During thermography and when interpreting an infrared image, comparison infrared images can provide valuable information for assessment.

The sources of disruption in thermography that occur most commonly in practice are

- the effect of the sun on the surface being thermographed (sunlight shining in through a window);
- hot radiators with pipes;
- lights directed at, or placed near, the surface being measured;
- air flows (e.g. from air intakes) directed at the surface;
- the effect of moisture deposits on the surface.

**7** Surfaces on which the sun is shining should not be subjected to thermography. If there is a risk of an effect by sunlight, windows should be covered up (closing Venetian blinds). However, be aware that there are building defects or problems (typically moisture problems) that only show up when heat has been applied to the surface, e.g. from the sun.

For more information about moisture detection, see section 7.2.2 – About moisture detection on page 19.

A hot radiator appears as a bright light surface in an infrared image. The surface temperature of a wall next to a radiator is raised, which may conceal any defects present.

For maximum prevention of disruptive effects from hot radiators, these may be shut off a short while before the measurement is taken. However, depending on the construction of the building (low or high mass), these may need to be shut off several hours before a thermographic survey. The room air temperature must not fall so much as to affect the surface temperature distribution on the structure's surfaces. There is little timelag with electric radiators, so they cool down relatively quickly once they have been switched off (20–30 minutes).

Lights placed against walls should be switched off when the infrared image is taken.

During thermography there should not be any disruptive air flows (e.g. open windows, open valves, fans directed at the surface being measured) that could affect the surfaces being thermographed.

Any wet surfaces, e.g. as a result of surface condensation, have a definite effect on heat transfer at the surface and the surface temperature. Where there is moisture on a surface, there is usually some evaporation which draws off heat, thus lowering the temperature of the surface by several degrees. There is risk of surface condensation at major thermal bridges and insulation defects.

Significant disruptions of the kind described here can normally be detected and eliminated before measuring.

If during thermography it is not possible to shield surfaces being measured from disruptive factors, these must be taken into account when interpreting and evaluating the results. The conditions in which the thermography was carried out should be recorded in detail when each measurement is taken.

### 7.3.4 Surface temperature and air leaks

Defects in building airtightness due to small gaps in the structure can be detected by measuring the surface temperature. If there is a negative pressure in the building under investigation, air flows into the space through leaks in the building. Cold air flowing in through small gaps in a wall usually lowers the temperature in adjacent areas of the wall. The result is that a cooled surface area with a characteristic shape develops on the inside surface of the wall. Thermography can be used to detect cooled surface areas. Air movements at the wall surface can be measured using an air velocity indicator. If there is a positive pressure inside the building being investigated, warm room air will leak out through gaps in the wall, resulting in locally warm surface areas around the locations of the leaks.

The amount of leakage depends partly on gaps and partly on the differential pressure across the structure.

#### 7.3.4.1 *Pressure conditions in a building*

The most important causes of differential pressure across a structural element in a building are

- wind conditions around the building;
- the effects of the ventilation system;
- temperature differences between air inside and outside (thermal differential pressure).

The actual pressure conditions inside a building are usually caused by a combination of these factors.

The resultant pressure gradient across the various structural elements can be illustrated by the figure on page 45. The irregular effects of wind on a building means that in practice the pressure conditions may be relatively variable and complicated.

In a steady wind flow, Bernoulli's Law applies:

$$\frac{\rho v^2}{2} + p = \text{constant}$$

where:

|        |                                  |
|--------|----------------------------------|
| $\rho$ | Air density in kg/m <sup>3</sup> |
| $v$    | Wind velocity in m/s             |
| $p$    | Static pressure in Pa            |

and where:

$$\frac{\rho v^2}{2} + p$$

denotes the dynamic pressure and  $p$  the static pressure. The total of these pressures gives the total pressure.

7

Wind load against a surface makes the dynamic pressure become a static pressure against the surface. The magnitude of this static pressure is determined by, amongst other things, the shape of the surface and its angle to the wind direction.


The portion of the dynamic pressure that becomes a static pressure on the surface ( $p_{\text{stat}}$ ) is determined by what is known as a stress concentration factor:

$$C = \frac{p_{\text{stat}}}{\frac{\rho v^2}{2}}$$

If  $\rho$  is 1.23 kg/m<sup>3</sup> (density of air at +15°C (+59°F)), this gives the following local pressures in the wind flow:

$$p_{\text{stat}} = C \times \frac{\rho v^2}{2} = C \times \frac{v^2}{1.63} \text{ Pa}$$

10551803.a1

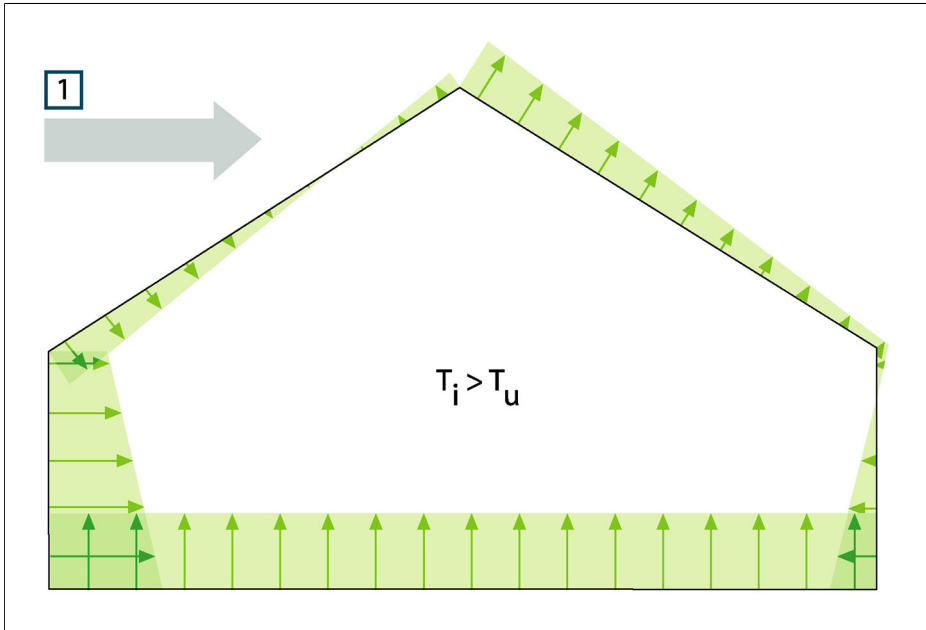


7

**Figure 7.3** Distribution of resultant pressures on a building's enclosing surfaces depending on wind effects, ventilation and internal/external temperature difference. 1: Wind direction;  $T_u$ : Thermodynamic air temperature outdoors in K;  $T_i$ : Thermodynamic air temperature indoors in K.

If the whole of the dynamic pressure becomes static pressure, then  $C = 1$ . Examples of stress concentration factor distributions for a building with various wind directions are shown in the figure on page 46.

The wind therefore causes an internal negative pressure on the windward side and an internal positive pressure on the leeward side. The air pressure indoors depends on the wind conditions, leaks in the building and how these are distributed in relation to the wind direction. If the leaks in the building are evenly distributed, the internal pressure may vary by  $\pm 0.2 p_{\text{stat}}$ . If most of the leaks are on the windward side, the internal pressure increases somewhat. In the opposite case, with most of the leaks on the leeward side, the internal pressure falls.

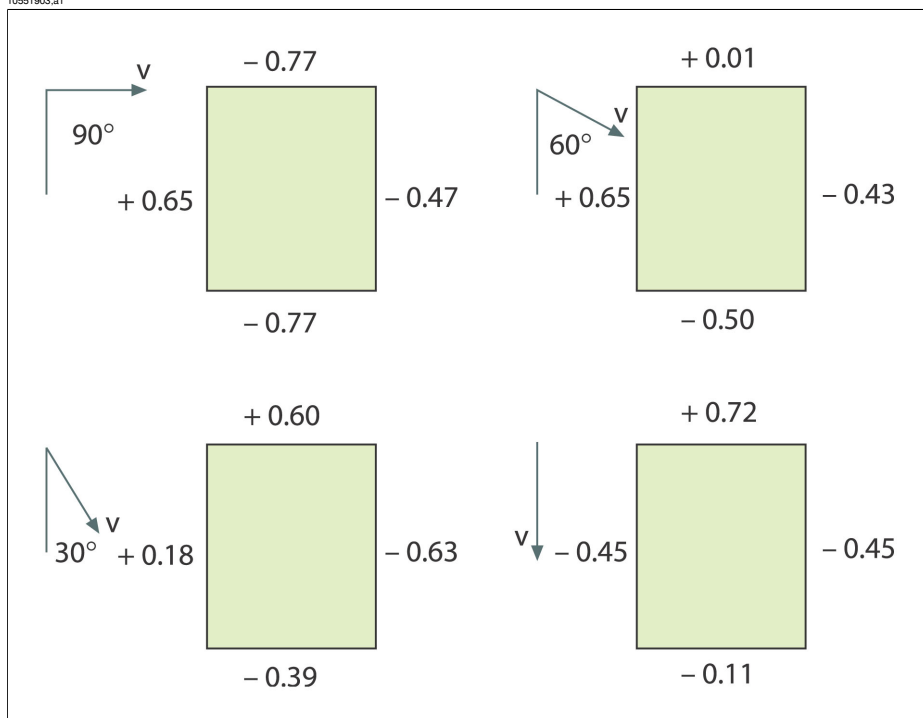

**Figure 7.4** Stress concentration factor (C) distributions for various wind directions and wind velocities (v) relative to a building.

Wind conditions can vary substantially over time and between relatively closely situated locations. In thermography, such variations can have a clear effect on the measurement results.

It has been demonstrated experimentally that the differential pressure on a façade exposed to an average wind force of about 5 m/s (16.3 ft/s) will be about 10 Pa.

Mechanical ventilation results in a constant internal negative or positive pressure (depending on the direction of the ventilation). Research has showed that the negative pressure caused by mechanical extraction (kitchen fans) in small houses is usually between 5 and 10 Pa. Where there is mechanical extraction of ventilation air, e.g. in multi-dwelling blocks, the negative pressure is somewhat greater, 10–50 Pa. Where there is so-called balanced ventilation (mechanically controlled supply and extract air), this is normally adjusted to produce a slight negative pressure inside (3–5 Pa).

The differential pressure caused by temperature differences, the so-called chimney effect (airtightness differences of air at different temperatures) means that there is a negative pressure in the building's lower part and a positive pressure in the upper

part. At a certain height there is a neutral zone where the pressures on the inside and outside are the same, see the figure on page 48. This differential pressure may be described by the relationship:


$$\Delta p = g \times \rho_u \times h \left( 1 - \frac{T_u}{T_i} \right) \text{ Pa}$$

|            |                                                      |
|------------|------------------------------------------------------|
| $\Delta p$ | Air pressure differential within the structure in Pa |
| $g$        | 9.81 m/s <sup>2</sup>                                |
| $\rho_u$   | Air density in kg/m <sup>3</sup>                     |
| $T_u$      | Thermodynamic air temperature outdoors in K          |
| $T_i$      | Thermodynamic air temperature indoors in K           |
| $h$        | Distance from the neutral zone in meters             |

If  $\rho_u = 1.29 \text{ kg/m}^3$  (density of air at a temperature of 273 K and  $\approx 100 \text{ kPa}$ ), this produces:

$$\Delta p \approx 13 \times h \left( 1 - \frac{T_u}{T_i} \right)$$

With a difference of  $+25^\circ\text{C}$  ( $+77^\circ\text{F}$ ) between the ambient internal and external temperatures, the result is a differential pressure difference within the structure of about 1 Pa/m difference in height ( $= 3.28 \text{ Pa/ft.}$ ).

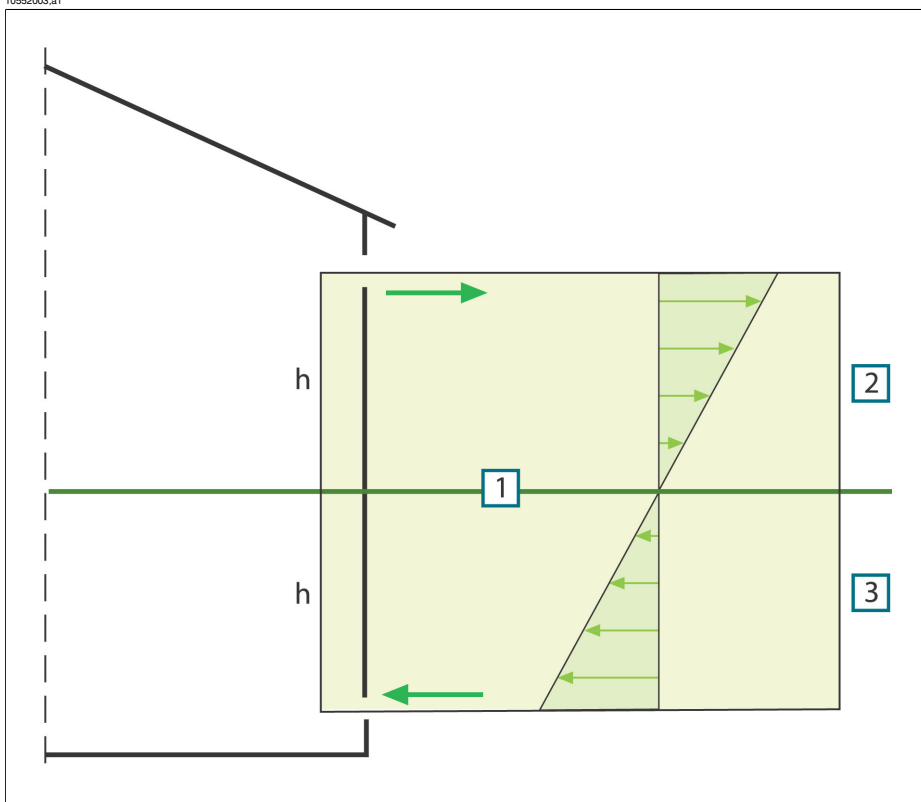

**Figure 7.5** Distribution of pressures on a building with two openings and where the external temperature is lower than the internal temperature. 1: Neutral zone; 2: Positive pressure; 3: Negative pressure; **h**: Distance from the neutral zone in meters.

The position of the neutral zone may vary, depending on any leaks in the building. If the leaks are evenly distributed vertically, this zone will be about halfway up the building. If more of the leaks are in the lower part of the building, the neutral zone will move downwards. If more of the leaks are in the upper part, it will move upwards. Where a chimney opens above the roof, this has a considerable effect on the position of the neutral zone, and the result may be a negative pressure throughout the building. This situation most commonly occurs in small buildings.

In a larger building, such as a tall industrial building, with leaks at doors and any windows in the lower part of the building, the neutral zone is about one-third of the way up the building.

### 7.3.5 Measuring conditions & measuring season

The foregoing may be summarized as follows as to the requirements with regard to measuring conditions when carrying out thermographic imaging of buildings.

Thermographic imaging is done in such a way that the disruptive influence from external climatic factors is as slight as possible. The imaging process is therefore carried out indoors, i.e. where a building is heated, the structure's warm surfaces are examined.

Outdoor thermography is only used to obtain reference measurements of larger façade surfaces. In certain cases, e.g. where the thermal insulation is very bad or where there is an internal positive pressure, outdoor measurements may be useful. Even when investigating the effects of installations located within the building's climatic envelope, there may be justification for thermographic imaging from outside the building.

The following conditions are recommended:

- The air temperature difference within the relevant part of the building must be at least  $+10^{\circ}\text{C}$  ( $+18^{\circ}\text{F}$ ) for a number of hours before thermographic imaging and for as long as the procedure takes. For the same period, the ambient temperature difference must not vary by more than  $\pm 30\%$  of the difference when the thermographic imaging starts. During the thermographic imaging, the indoor ambient temperature should not change by more than  $\pm 2^{\circ}\text{C}$  ( $\pm 3.6^{\circ}\text{F}$ ).
- For a number of hours prior before thermographic imaging and as long as it continues, no influencing sunlight may fall upon the relevant part of the building.
- Negative pressure within the structure  $\approx 10\text{--}50$  Pa.
- When conducting thermographic imaging in order to locate only air leaks in the building's enclosing sections, the requirements in terms of measuring conditions may be lower. A difference of  $5^{\circ}\text{C}$  ( $9^{\circ}\text{F}$ ) between the inside and outside ambient temperatures ought to be sufficient for detecting such defects. To be able to detect air leaks, certain requirements must however be made with regard to the differential pressure; about 10 Pa should be sufficient.

### 7.3.6 Interpretation of infrared images

The main purpose of thermography is to locate faults and defects in thermal insulation in exterior walls and floor structures and to determine their nature and extent. The measuring task can also be formulated in such a way that the aim of the thermography is to confirm whether or not the wall examined has the promised insulation and airtightness characteristics. The 'promised thermal insulation characteristics' for the wall according to the design can be converted into an expected surface temperature distribution for the surface under investigation if the measuring conditions at the time when the measurements are taken are known.

In practice the method involves the following:

Laboratory or field tests are used to produce an expected temperature distribution in the form of typical or comparative infrared images for common wall structures, comprising both defect-free structures and structures with in-built defects. Examples of typical infrared images are shown in section 7.2 – Typical field investigations beginning on page 17.

If infrared images of structural sections taken during field measurements are intended for use as comparison infrared images, then the structure's composition, the way it was built, and the measurement conditions at the time the infrared image was taken must be known in detail and documented.

In order, during thermography, to be able to comment on the causes of deviations from the expected results, the physical, metrological and structural engineering prerequisites must be known.

The interpretation of infrared images taken during field measurements may be described in brief as follows:

7

A comparison infrared image for a defect-free structure is selected on the basis of the wall structure under investigation and the conditions under which the field measurement was taken. An infrared image of the building element under investigation is then compared with the selected infrared image. Any deviation that cannot be explained by the design of the structure or the measurement conditions is noted as a suspected insulation defect. The nature and extent of the defect is normally determined using comparison infrared images showing various defects.

If no suitable comparison infrared image is available, evaluation and assessment are done on the basis of experience. This requires more precise reasoning during the analysis.

When assessing an infrared image, the following should be looked at:

- Uniformity of brightness in infrared images of surface areas where there are no thermal bridges
- Regularity and occurrence of cooled surface areas, e.g. at studding and corners
- Contours and characteristic shapes in the cooled surface area
- Measured temperature differences between the structure's normal surface temperature and the selected cooled surface area
- Continuity and uniformity of the isotherm curve on the surface of the structure. In the camera software the isotherm function is called **Isotherm** or **Color alarm**, depending on camera model.

Deviations and irregularities in the appearance of the infrared image often indicate insulation defects. There may obviously be considerable variations in the appearance of infrared images of structures with insulation defects. Certain types of insulation defects have a characteristic shape on the infrared image. Section 7.2 – Typical field investigations beginning on page 17 shows examples of interpretations of infrared images.

When taking infrared images of the same building, the infrared images from different areas should be taken with the same settings on the infrared camera, as this makes comparison of the various surface areas easier.

### 7.3.7 Humidity & dew point

#### 7.3.7.1 Relative & absolute humidity

Humidity can be expressed in two different ways—either as *relative humidity* or as *absolute humidity*. Relative humidity is expressed in percent of how much water a certain volume of air can hold at a certain temperature, while absolute humidity is expressed in percent water by weight of material. The latter way to express humidity is common when measuring humidity in wood and other building materials.

The higher the temperature of air, the larger the amount of water this certain volume of air can hold. The following table specifies the maximum amounts of water in air at different temperatures.

**Figure 7.6** **A:** Temperature in degrees Celsius; **B:** Maximum amount of water expressed in g/m<sup>3</sup> (at sea level)

| A    | B     | A    | B     | A    | B    | A    | B    |
|------|-------|------|-------|------|------|------|------|
| 30.0 | 30.44 | 20.0 | 17.33 | 10.0 | 9.42 | 0.0  | 4.86 |
| 29.0 | 28.83 | 19.0 | 16.34 | 9.0  | 8.84 | -1.0 | 4.49 |
| 28.0 | 27.29 | 18.0 | 15.40 | 8.0  | 8.29 | -2.0 | 4.15 |
| 27.0 | 25.83 | 17.0 | 14.51 | 7.0  | 7.77 | -3.0 | 3.83 |
| 26.0 | 24.43 | 16.0 | 13.66 | 6.0  | 7.28 | -4.0 | 3.53 |
| 25.0 | 23.10 | 15.0 | 12.86 | 5.0  | 6.81 | -5.0 | 3.26 |
| 24.0 | 21.83 | 14.0 | 12.09 | 4.0  | 6.38 | -6.0 | 3.00 |
| 23.0 | 20.62 | 13.0 | 11.37 | 3.0  | 5.96 | -7.0 | 2.76 |
| 22.0 | 19.47 | 12.0 | 10.69 | 2.0  | 5.57 | -8.0 | 2.54 |
| 21.0 | 18.38 | 11.0 | 10.04 | 1.0  | 5.21 | -9.0 | 2.34 |

**Figure 7.7 A:** Temperature in degrees Fahrenheit; **B:** Maximum amount of water in gr/ft<sup>3</sup> (at sea level)

| A    | B     | A    | B    | A    | B    | A    | B    |
|------|-------|------|------|------|------|------|------|
| 86.0 | 13.30 | 68.0 | 7.58 | 50.0 | 4.12 | 32.0 | 2.12 |
| 84.2 | 12.60 | 66.2 | 7.14 | 48.2 | 3.86 | 30.2 | 1.96 |
| 82.4 | 11.93 | 64.4 | 6.73 | 46.4 | 3.62 | 28.4 | 1.81 |
| 80.6 | 11.29 | 62.6 | 6.34 | 44.6 | 3.40 | 26.6 | 1.67 |
| 78.8 | 10.68 | 60.8 | 5.97 | 42.8 | 3.18 | 24.8 | 1.54 |
| 77.0 | 10.10 | 59.0 | 5.62 | 41.0 | 2.98 | 23.0 | 1.42 |
| 75.2 | 9.54  | 57.2 | 5.29 | 39.2 | 2.79 | 21.2 | 1.31 |
| 73.4 | 9.01  | 55.4 | 4.97 | 37.4 | 2.61 | 19.4 | 1.21 |
| 71.6 | 8.51  | 53.6 | 4.67 | 35.6 | 2.44 | 17.6 | 1.11 |
| 69.8 | 8.03  | 51.8 | 4.39 | 33.8 | 2.28 | 15.8 | 1.02 |

7

*Example:*

The relative humidity of a certain volume of air at a temperature of +30°C (+86°F) is 40 % RH. Amount of water in 1 m<sup>3</sup> (35.31 ft<sup>3</sup>) of air at +30°C = 30.44 × Rel Humidity = 30.44 × 0.40 = 12.18 g (187.96 gr).

### 7.3.7.2 Definition of dew point

Dew point can be regarded as the temperature at which the humidity in a certain volume of air will condense as liquid water.

*Example:*

The relative humidity of a certain volume of air at a temperature of +30°C (+86°F) is 40 % RH. Amount of water in 1 m<sup>3</sup> (35.31 ft<sup>3</sup>) of air at +30°C = 30.44 × Rel Humidity = 30.44 × 0.40 = 12.18 g (187.96 gr). In the table above, look up the temperature for which the amount of water in air is closest to 12.18 g. This would be +14.0°C (+57.2°F), which is the approximate dew point.

## 7.4 *Disclaimer*

### 7.4.1 Copyright notice

Some sections and/or images appearing in this chapter are copyrighted to the following organizations and companies:

- FORMAS—The Swedish Research Council for Environment, Agricultural Sciences and Spatial Planning, Stockholm, Sweden
- ITC—Infrared Training Center, Boston, MA, United States
- Stockton Infrared Thermographic Services, Inc., Randleman, NC, United States
- Professional Investigative Engineers, Westminster, CO, United States

### 7.4.2 Training & certification

**Carrying out building thermography inspections requires substantial training and experience, and may require certification from a national or regional standardization body. This section is provided only as an introduction to building thermography. The user is strongly recommended to attend relevant training courses.**

**For more information about infrared training, visit the following website:**

**<http://www.infraredtraining.com>**

### 7.4.3 National or regional building codes

The commented building structures in this chapter may differ in construction from country to country. For more information about construction details and standards of procedure, always consult national or regional building codes.

INTENTIONALLY LEFT BLANK

---

## 8 Tutorials

### 8.1 *Switching on & switching off the camera*

#### 8.1.1 Switching on the camera

| Step | Action                                           |
|------|--------------------------------------------------|
| 1    | Insert the battery into the battery compartment. |
| 2    | Press PWR/NO to switch on the camera.            |

#### 8.1.2 Switching off the camera

| Step | Action                                                                                                                                                                                       |
|------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 1    | To switch off the camera, press and hold down PWR/NO until the message <b>Shutting down...</b> appears. Briefly pressing PWR/NO when the camera is in menu mode will cancel menu selections. |

## 8.2 Working with images

### 8.2.1 Acquiring an image

| Step | Action                                                                                                                                                                                                                                            |
|------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 1    | Point the camera at a warm object, like a face or a hand.                                                                                                                                                                                         |
| 2    | Adjust the focus by turning the focus ring at the front of the lens.<br>☛ Please note what is the locking ring and what is the focus ring in the figure on page 66. Trying to adjust the focus by rotating the locking ring will remove the lens. |
| 3    | If the camera is in manual adjust mode, press and hold down SEL for more than one second to autoadjust the camera.                                                                                                                                |

### 8.2.2 Freezing an image

| Step | Action                                                                                                                                                                                                                                        |
|------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 1    | Adjust focus by turning the focus ring at the front of the lens.<br>☛ Please note what is the locking ring and what is the focus ring in the figure on page 66. Trying to adjust the focus by rotating the locking ring will remove the lens. |
| 2    | If the camera is in manual adjust mode, press and hold down SEL for more than one second to autoadjust the camera.                                                                                                                            |
| 3    | Briefly pressing SAVE/FRZ will display a confirmation box. <ul style="list-style-type: none"> <li>■ To save the image, press YES</li> <li>■ To leave the confirmation box without saving the image, press NO</li> </ul>                       |

### 8.2.3 Saving an image

| Step | Action                                                                                                                                                                                                                                            |
|------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 1    | Adjust the focus by turning the focus ring at the front of the lens.<br>☛ Please note what is the locking ring and what is the focus ring in the figure on page 66. Trying to adjust the focus by rotating the locking ring will remove the lens. |
| 2    | If the camera is in manual adjust mode, press and hold down SEL for more than one second to autoadjust the camera.                                                                                                                                |
| 3    | Briefly press SAVE/FRZ to freeze the image. This will display a confirmation box where you will be prompted to accept or cancel the image. Accepting the image will save it to the internal memory.                                               |
| 4    | To save an image directly (without freezing the image first), press SAVE/FRZ for more than 1 second.                                                                                                                                              |

### 8.2.4 Deleting one or several images

| Step | Action                                                                                                       |
|------|--------------------------------------------------------------------------------------------------------------|
| 1    | Press MENU/YES to display the vertical menu bar.                                                             |
| 2    | Point to <b>File</b> on the vertical menu bar and press the MENU/YES.                                        |
| 3    | Point to <b>Delete image</b> or <b>Delete all images</b> and press MENU/YES to delete one or several images. |

### 8.2.5 Opening an image

| Step | Action                                                                                                           |
|------|------------------------------------------------------------------------------------------------------------------|
| 1    | Press MENU/YES to display the vertical menu bar.                                                                 |
| 2    | Point to <b>File</b> on the vertical menu bar and press MENU/YES.                                                |
| 3    | Point to <b>Images</b> to display thumbnails of the most recently saved images.                                  |
| 4    | To open an image, select the image by pressing the navigation pad left/right or up/down and then press MENU/YES. |

## 8.3 Working with measurements

### 8.3.1 Laying out a spot

➡ The camera requires a warm-up time of 5 minutes before accurate measurements can be expected.

| Step | Action                                                                                                                                 |
|------|----------------------------------------------------------------------------------------------------------------------------------------|
| 1    | Press MENU/YES to display the vertical menu bar.                                                                                       |
| 2    | Point to <b>Meas. mode</b> on the vertical menu bar and press MENU/YES.                                                                |
| 3    | Select <b>Spot</b> in the <b>Meas. mode</b> dialog box and press MENU/YES.                                                             |
| 4    | Press SEL until small brackets appear around the spot. You can now move the spot by pressing the navigation pad left/right or up/down. |
| 5    | The temperature will be displayed in the top right corner of the LCD.                                                                  |

### 8.3.2 Laying out a measurement area

➡ The camera needs a warm-up time of 5 minutes before accurate measurements can be expected.

| Step | Action                                                                                                              |
|------|---------------------------------------------------------------------------------------------------------------------|
| 1    | Press MENU/YES to display the vertical menu bar.                                                                    |
| 2    | Point to <b>Meas. mode</b> on the vertical menu bar and press MENU/YES.                                             |
| 3    | Select <b>Area max</b> , <b>Area min</b> or <b>Area avg</b> in the <b>Meas. mode</b> dialog box and press MENU/YES. |
| 4    | The temperature will be displayed in the top right corner of the LCD.                                               |

## 8.4 Working with alarms

You can choose between the following alarm outputs:

- a color alarm, which will assign a color to all pixels above or below a preset temperature level
- a silent alarm, which, compared to the color alarm, will make the font of the temperature result increase in size and its background turn red
- an audible alarm, which, compared to the visual alarm, also triggers a 'beep'.

A settings can also be made in the camera so that an alarm output takes into account the reference temperature. A typical application when you would want to use an alarm that takes into account the reference temperature is screening of people for face temperature detection.

Firstly, the reference temperature is set by screening 10 persons with normal face temperature. The camera puts each of these 10 results in an internal camera buffer and calculates the average temperature value after having discarded the two highest and two lowest values in the event of erroneous samples. Every time a new sample is saved to the internal buffer, the oldest sample will be discarded and a new reference temperature will be calculated 'on the fly'.

Using an alarm that takes into account the reference temperature means that an alarm output will only be triggered if the temperature value exceeds the sum of the average temperature value in the buffer + the user-defined delta alarm offset value.

8

### 8.4.1 Setting the reference temperature

| Step | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                             |
|------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 1    | Press YES to display the vertical menu bar.                                                                                                                                                                                                                                                                                                                                                                                                                        |
| 2    | Point to <b>Settings</b> on the <b>Setup</b> menu and press YES.                                                                                                                                                                                                                                                                                                                                                                                                   |
| 3    | In the <b>Settings</b> dialog box, press the navigation pad up/down to go to <b>Trigger button</b> .                                                                                                                                                                                                                                                                                                                                                               |
| 4    | Press the navigation pad left/right to select <b>Update ref temp</b> .                                                                                                                                                                                                                                                                                                                                                                                             |
| 5    | Press the navigation pad up/down to go to <b>Shutter period</b> .                                                                                                                                                                                                                                                                                                                                                                                                  |
| 6    | <p>Press the navigation pad left/right to select shutter period.</p> <p>Although the shutter period works independently of other functions described in this document, FLIR Systems recommends that <b>Short</b> is selected when using the camera for detection of face temperature.</p> <p>☛ Selecting <b>Normal</b> will calibrate the camera at least every 15th minute, while selecting <b>Short</b> will calibrate the camera at least every 3rd minute.</p> |

| Step | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
|------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 7    | Pointing the camera to the first person with a normal face temperature and pulling the trigger will display the message <b>Sampled nn.n °C</b> .                                                                                                                                                                                                                                                                                                            |
| 8    | After having carried out the same procedure on the following 9 persons, you can do one of the following: <ul style="list-style-type: none"> <li>■ Actively continue to sample every new person by pulling the trigger button, and let camera update the reference temperature</li> <li>■ Stop sampling and let the camera trigger an alarm as soon as the alarm conditions are met (<math>&gt;</math> reference temperature + delta alarm value)</li> </ul> |

### 8.4.2 Setting up a color alarm

#### 8.4.2.1 Setting up a color alarm using the menu system

| Step | Action                                                                                                                                                                                                                                                                                                                                                                                                                                          |
|------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 1    | Press MENU/YES to display the vertical menu bar.                                                                                                                                                                                                                                                                                                                                                                                                |
| 2    | Point to <b>Meas. mode</b> and press YES to display the <b>Meas. mode</b> dialog box.                                                                                                                                                                                                                                                                                                                                                           |
| 3    | Select <b>Meas. mode</b> by pressing the navigation pad left/right. The alarm function is typically used together with <b>Area max</b> .                                                                                                                                                                                                                                                                                                        |
| 4    | For <b>Alarm</b> , select one of the following by pressing the navigation pad left/right: <ul style="list-style-type: none"> <li>■ Above</li> <li>■ Below</li> </ul>                                                                                                                                                                                                                                                                            |
| 5    | For <b>Alarm output</b> , select <b>Color only</b> by pressing the navigation pad left/right.                                                                                                                                                                                                                                                                                                                                                   |
| 6    | Specify the <b>Alarm temp</b> by pressing the navigation pad left/right. You can also change the color alarm without using the menu system by pressing the navigation pad up/down after having selected the temperature result by pressing SEL. A selected temperature result is highlighted in yellow.<br>☛ <b>Alarm temp</b> will only be available if <b>Update ref temp</b> has been previously selected in the <b>Settings</b> dialog box. |
| 7    | Specify <b>Delta alarm</b> by pressing the navigation pad left/right.<br>☛ <b>Delta alarm</b> will only be available if <b>Update ref temp</b> has been previously selected in the <b>Settings</b> dialog box.                                                                                                                                                                                                                                  |

#### 8.4.2.2 Setting up a color alarm without using the menu system

| Step | Action                                                                                                                                                                                                  |
|------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 1    | Press SEL until the color alarm symbol and the color alarm temperature in the top right hand corner of the screen is selected.<br><br>The color alarm symbol is an arrow pointing upwards or downwards. |
| 2    | Press the navigation pad up/down to change the color alarm temperature.                                                                                                                                 |

### 8.4.3 Setting up a silent alarm (i.e. a visual alarm)

| Step | Action                                                                                                                                                                                                           |
|------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 1    | Press MENU/YES to display the vertical menu bar.                                                                                                                                                                 |
| 2    | Point to <b>Meas. mode</b> and press YES to display the <b>Meas. mode</b> dialog box.                                                                                                                            |
| 3    | Select <b>Meas. mode</b> by pressing the navigation pad left/right. The alarm function is typically used together with <b>Area max</b> .                                                                         |
| 4    | For <b>Alarm</b> , select one of the following by pressing the navigation pad left/right: <ul style="list-style-type: none"> <li>■ Above</li> <li>■ Below</li> </ul>                                             |
| 5    | For <b>Alarm output</b> , select <b>Silent</b> by pressing the navigation pad left/right.                                                                                                                        |
| 6    | Specify the <b>Alarm temp</b> by pressing the navigation pad left/right.<br>☛ <b>Alarm temp</b> will only be available if <b>Update ref temp</b> has been previously selected in the <b>Settings</b> dialog box. |
| 7    | Specify <b>Delta alarm</b> by pressing the navigation pad left/right.<br>☛ <b>Delta alarm</b> will only be available if <b>Update ref temp</b> has been previously selected in the <b>Settings</b> dialog box.   |

### 8.4.4 Setting up an audible alarm

| Step | Action                                                                                                                                                                                                           |
|------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 1    | Press MENU/YES to display the vertical menu bar.                                                                                                                                                                 |
| 2    | Point to <b>Meas. mode</b> and press YES to display the <b>Meas. mode</b> dialog box.                                                                                                                            |
| 3    | Select <b>Meas. mode</b> by pressing the navigation pad left/right. The alarm function is typically used together with <b>Area max</b> .                                                                         |
| 4    | For <b>Alarm</b> , select one of the following by pressing the navigation pad left/right: <ul style="list-style-type: none"> <li>■ Above</li> <li>■ Below</li> </ul>                                             |
| 5    | For <b>Alarm output</b> , select <b>Beep</b> by pressing the navigation pad left/right.                                                                                                                          |
| 6    | Specify the <b>Alarm temp</b> by pressing the navigation pad left/right.<br>☛ <b>Alarm temp</b> will only be available if <b>Update ref temp</b> has been previously selected in the <b>Settings</b> dialog box. |
| 7    | Specify <b>Delta alarm</b> by pressing the navigation pad left/right.<br>☛ <b>Delta alarm</b> will only be available if <b>Update ref temp</b> has been previously selected in the <b>Settings</b> dialog box.   |

## 8.5 *Creating files for image descriptions*

Follow this procedure to create a text file where any value of the first label will be used as an image description:

| Step | Action                                                                                                                                                           |
|------|------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 1    | Using any ASCII text editor (Notepad, Wordpad etc), type the first label within brackets:<br><br><Recommendation>                                                |
| 2    | On the next lines, type the values you want to use, but this time without brackets:<br><br>Check connections<br>Check cables<br>Check gaskets<br>Check mountings |
| 3    | The final result should look like this:<br><br><Recommendation><br>Check connections<br>Check cables<br>Check gaskets<br>Check mountings                         |
| 4    | Save the file to Desktop, using any file name you want.                                                                                                          |
|      | Rename the file name extension to .tcf.                                                                                                                          |
| 5    | Connect the camera to your computer using ThermaCAM™ QuickView. This makes your camera appear as a hard disk drive in Windows® Explorer.                         |
| 6    | Move the file from Desktop to your camera using a drag-and-drop operation.                                                                                       |

☞ For information about how to connect the camera to your computer, see the ThermaCAM™ QuickView user's manual.

## 8.6 *Changing level & span*

### 8.6.1 Changing level

| Step | Action                                                                                                          |
|------|-----------------------------------------------------------------------------------------------------------------|
| 1    | Press MENU/YES to display the vertical menu bar.                                                                |
| 2    | Point to <b>Manual adjust</b> on the vertical menu bar and press MENU/YES.                                      |
| 3    | Press the navigation pad up/down to change the level. An arrow pointing upwards or downwards will be displayed. |

For more information about level, see section 10.4.3 – Manual adjust/Automatic adjust on page 84.

### 8.6.2 Changing span

| Step | Action                                                                                                                                    |
|------|-------------------------------------------------------------------------------------------------------------------------------------------|
| 1    | Press MENU/YES to display the vertical menu bar.                                                                                          |
| 2    | Point to <b>Manual adjust</b> on the vertical menu bar and press MENU/YES.                                                                |
| 3    | Press the navigation pad left/right to change the span. Two arrows pointing away from each other or towards each other will be displayed. |

For more information about span, see section 10.4.3 – Manual adjust/Automatic adjust on page 84.

## 8.7 *Changing system settings*

### 8.7.1 Changing language

| Step | Action                                                                      |
|------|-----------------------------------------------------------------------------|
| 1    | Press MENU/YES to display the vertical menu bar.                            |
| 2    | Point to <b>Local Settings</b> on the <b>Setup</b> menu and press MENU/YES. |
| 3    | Press the navigation pad up/down to select <b>Language</b> .                |
| 4    | Press the navigation pad left/right to change the language.                 |
| 5    | Press MENU/YES to confirm your changes and leave the dialog box.            |

### 8.7.2 Changing temperature unit

| Step | Action                                                                      |
|------|-----------------------------------------------------------------------------|
| 1    | Press MENU/YES to display the vertical menu bar.                            |
| 2    | Point to <b>Local Settings</b> on the <b>Setup</b> menu and press MENU/YES. |
| 3    | Press the navigation pad up/down to select <b>Temp unit</b> .               |
| 4    | Press the navigation pad left/right to change the temperature unit.         |
| 5    | Press MENU/YES to confirm your changes and leave the dialog box.            |

### 8.7.3 Changing date format

| Step | Action                                                                      |
|------|-----------------------------------------------------------------------------|
| 1    | Press MENU/YES to display the vertical menu bar.                            |
| 2    | Point to <b>Local Settings</b> on the <b>Setup</b> menu and press MENU/YES. |
| 3    | Press the navigation pad up/down to select <b>Date format</b> .             |
| 4    | Press the navigation pad left/right to change the date format.              |
| 5    | Press MENU/YES to confirm your changes and leave the dialog box.            |

### 8.7.4 Changing time format

| Step | Action                                                                      |
|------|-----------------------------------------------------------------------------|
| 1    | Press MENU/YES to display the vertical menu bar.                            |
| 2    | Point to <b>Local Settings</b> on the <b>Setup</b> menu and press MENU/YES. |
| 3    | Press the navigation pad up/down to select <b>Time format</b> .             |
| 4    | Press the navigation pad left/right to change the time format.              |

| Step | Action                                                           |
|------|------------------------------------------------------------------|
| 5    | Press MENU/YES to confirm your changes and leave the dialog box. |

### 8.7.5 Changing date & time

| Step | Action                                                                                |
|------|---------------------------------------------------------------------------------------|
| 1    | Press MENU/YES to display the vertical menu bar.                                      |
| 2    | Point to <b>Date/time</b> on the <b>Setup</b> menu and press MENU/YES.                |
| 3    | Press the navigation pad up/down to select year, month, day, hour, minute and second. |
| 4    | Press the navigation pad left/right to change each parameter.                         |
| 5    | Press MENU/YES to confirm your changes and leave the dialog box.                      |


## 8.8 Working with the camera

### 8.8.1 Removing the lens

➡ Please note the following:


- Before trying to remove fingerprints or other marks on the lens elements, see section 12.2 – Lenses on page 99.
- Removing an IR lens will expose very sensitive camera parts. Do not touch any exposed parts.
- Please note what is the locking ring and what is the focus ring in the figure below. Trying to remove the lens by rotating the focus ring may damage the lens.

10374803.a4

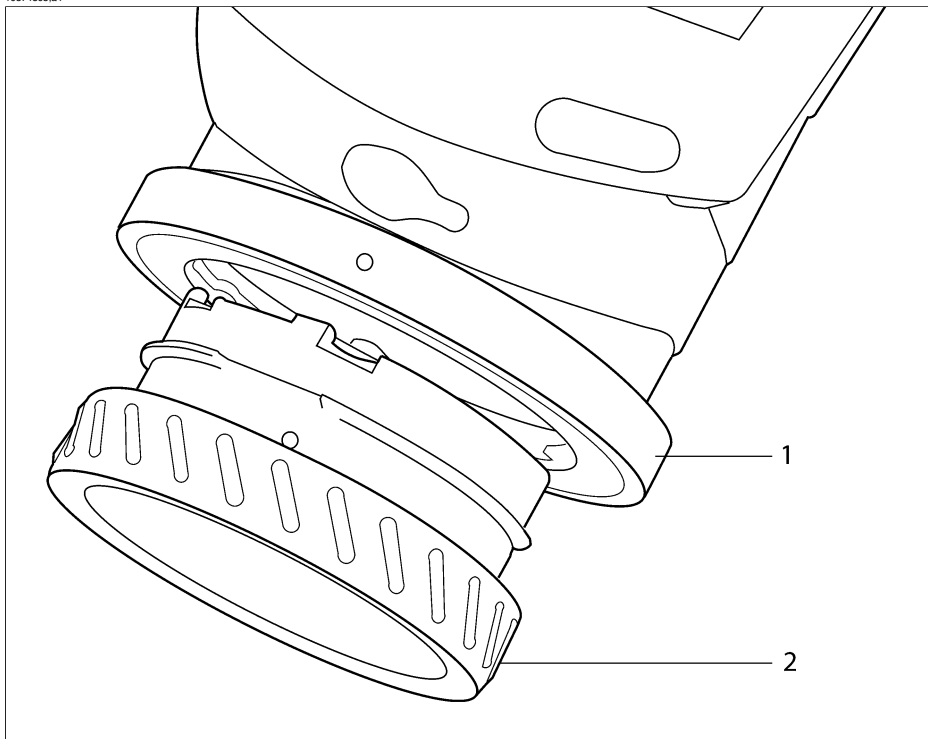

**Figure 8.1** Removing a lens. 1: Locking ring; 2: Focus ring

10396303.a3

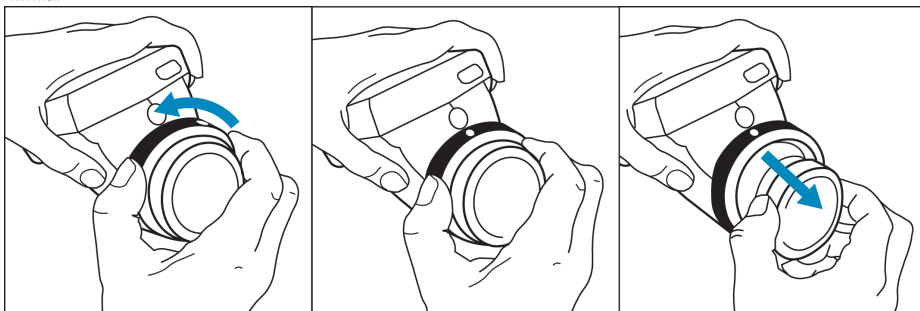**Figure 8.2** Removing a lens

| Step | Action                                                                                                               |
|------|----------------------------------------------------------------------------------------------------------------------|
| 1    | Rotate the locking ring on the camera 30° counter-clock-wise until the index mark is lined up with the laser window. |
| 2    | Carefully pull out the lens. Do not use excessive force.                                                             |

### 8.8.2 Adjusting the focus

☛ Please note what is the locking ring and what is the focus ring in figure 8.1 on page 66. Trying to adjust the focus by rotating the locking ring will remove the lens.


| Step | Action                                                                       |
|------|------------------------------------------------------------------------------|
| 1    | To adjust the focus, rotate the focus ring clock-wise or counter-clock-wise. |

### 8.8.3 Inserting & removing the battery

☛ The camera is shipped with charged batteries. To increase the battery life, the battery should be fully discharged and charged a couple of times. You can do this by using the camera until the battery is fully depleted.

8.8.3.1                    *Inserting the battery*

10396403.a2

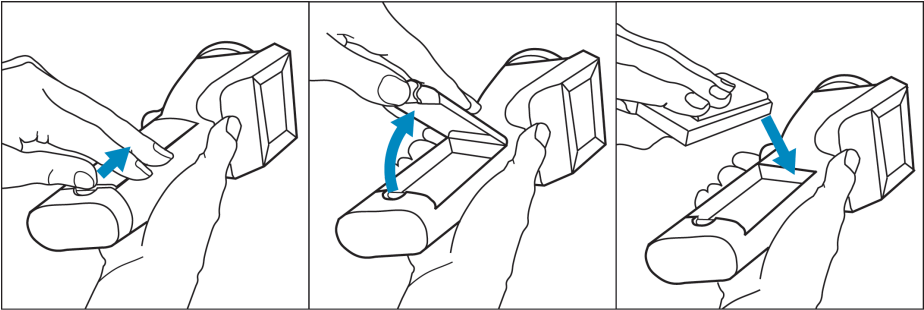


**Figure 8.3** Inserting the battery

| Step | Action                                                                                                                            |
|------|-----------------------------------------------------------------------------------------------------------------------------------|
| 1    | Remove lid of the battery compartment by pressing the locking mechanism.                                                          |
| 2    | Insert the battery with the connectors facing the rear end of the camera and the arrow symbol facing the front end of the camera. |
| 3    | Replace the lid of the battery compartment.                                                                                       |

8.8.3.2                    *Removing the battery*

10396503.a2

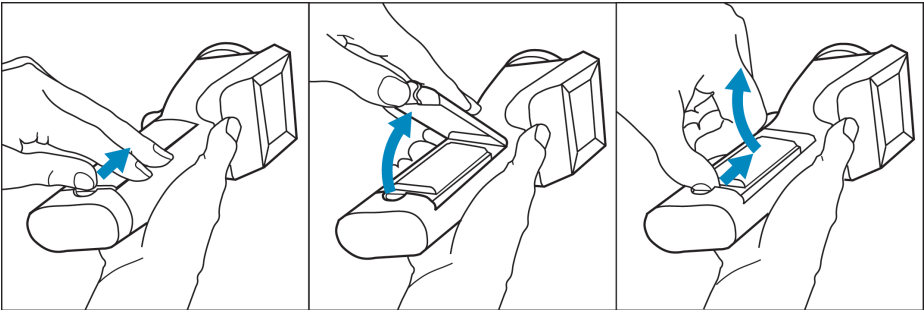

**Figure 8.4** Removing the battery

| Step | Action                                                                                                        |
|------|---------------------------------------------------------------------------------------------------------------|
| 1    | Remove the lid of the battery compartment by pressing the locking mechanism.                                  |
| 2    | Remove the battery by firmly grabbing its rear end and carefully lifting it out from the battery compartment. |
| 3    | Replace the lid of the battery compartment.                                                                   |


For more information about the battery system, see section 11 – Electrical power system on page 93.

INTENTIONALLY LEFT BLANK

## 9 Camera overview

### 9.1 Camera parts

10308903.a5

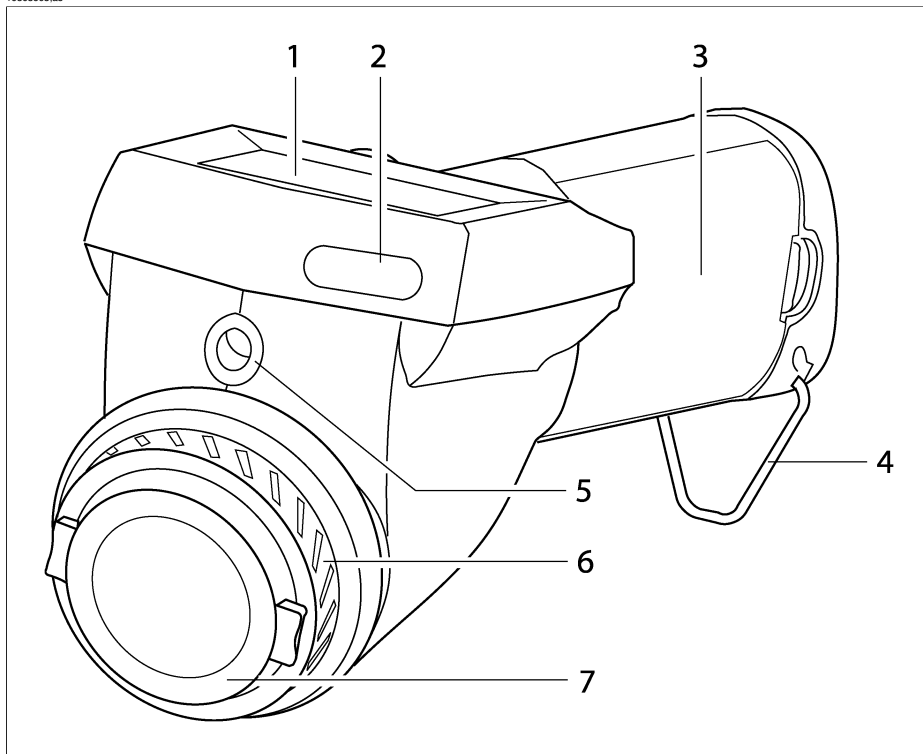


**Figure 9.1** Camera parts – front view

| Callout | Description of part              |
|---------|----------------------------------|
| 1       | LCD                              |
| 2       | IrDA infrared communication link |
| 3       | Lid of the battery compartment   |
| 4       | Ring for hand strap              |

| Callout | Description of part                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
|---------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 5       | <p>Laser LocatIR with lens cap</p> <p>☛ Please note the following:</p> <ul style="list-style-type: none"><li>■ A laser icon appears on the screen when the Laser LocatIR is switched on.</li><li>■ Since the distance between the laser beam and the image center will vary by the target distance, Laser LocatIR should only be used as an aiming aid. Always check the LCD to make sure the camera captures the desired target.</li><li>■ Do not look directly into the laser beam.</li><li>■ When not in use, the Laser LocatIR should always be protected by the lens cap.</li></ul> |
| 6       | Focus ring                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |
| 7       | Lens cap                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |

10315803.a4

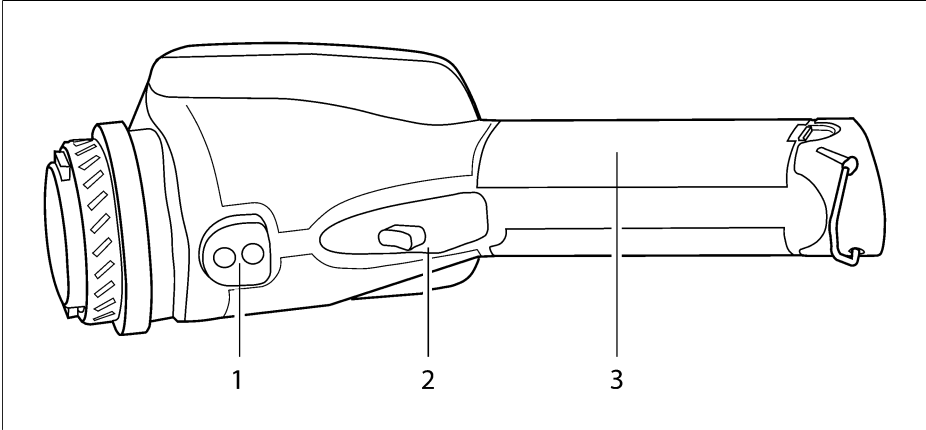

**Figure 9.2** Camera parts – view from below

| Callout | Description of part            |
|---------|--------------------------------|
| 1       | Tripod mount                   |
| 2       | Trigger                        |
| 3       | Lid of the battery compartment |

10310603.a5

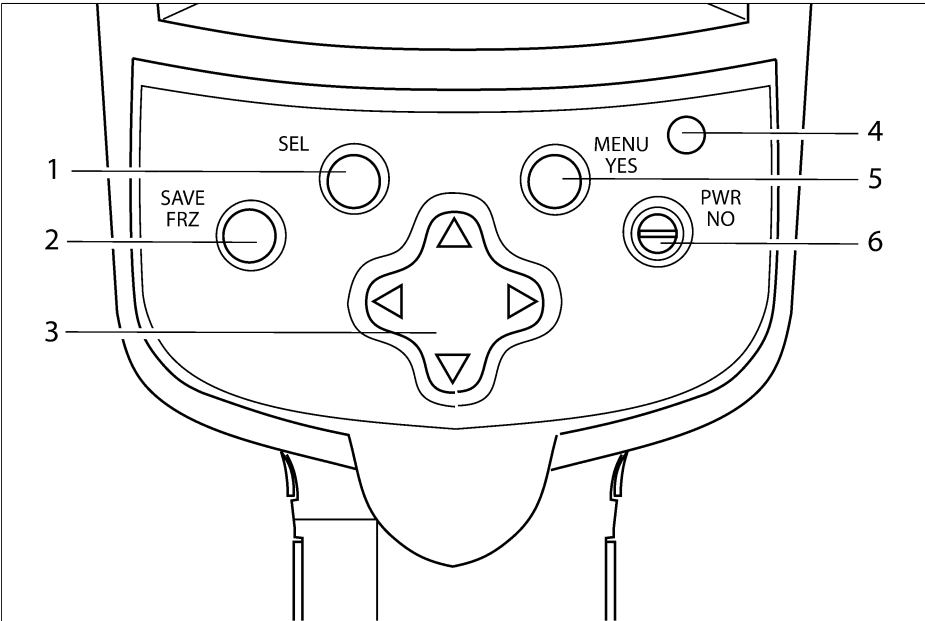


Figure 9.3 Camera parts – view from above

| Callout | Description of part                                                                                                                                          |
|---------|--------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 1       | <p>SEL button</p> <p>For more information about the functionality of this button, see section 9.2 – Keypad buttons &amp; functions on page 75</p>            |
| 2       | <p>SAVE/FRZ button</p> <p>For more information about the functionality of this button, see section 9.2 – Keypad buttons &amp; functions on page 75</p>       |
| 3       | <p>Navigation pad</p> <p>For more information about the functionality of the navigation pad, see section 9.2 – Keypad buttons &amp; functions on page 75</p> |
| 4       | <p>LED indicator</p>                                                                                                                                         |
| 5       | <p>MENU/YES button</p> <p>For more information about the functionality of this button, see section 9.2 – Keypad buttons &amp; functions on page 75</p>       |
| 6       | <p>PWR/NO button</p> <p>For more information about the functionality of this button, see section 9.2 – Keypad buttons &amp; functions on page 75</p>         |

## 9.2 Keypad buttons & functions

| Button          | Comments                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |
|-----------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| SAVE/FRZ button | <ul style="list-style-type: none"> <li>■ Briefly press SAVE/FRZ to freeze the current image and display a dialog box where you can choose to save or cancel the image</li> <li>■ Press and hold down SAVE/FRZ for more than one second to save the current image without previewing</li> </ul> <p>☛ The image will be saved according to the syntax <i>/Rnnnn.jpg</i> where <i>nnnn</i> is a unique counter. The counter can be reset by pointing to <b>Factory default</b> on the <b>Setup</b> menu.</p> <p>☛ Approx. 200 JPG images can be saved.</p>                                                                                      |
| SEL button      | <ul style="list-style-type: none"> <li>■ Press and hold down SEL for more than one second to autoadjust the camera</li> <li>■ Briefly press SEL to show current navigation pad focus, i.e. which screen object you can change or move by using the navigation pad.</li> <li>■ Press SEL repeatedly to switch between different screen objects</li> </ul>                                                                                                                                                                                                                                                                                     |
| MENU/YES button | <ul style="list-style-type: none"> <li>■ Press MENU/YES to display the vertical menu bar</li> <li>■ Press MENU/YES to confirm selections in dialog boxes</li> <li>■ Press MENU/YES to display the graphics if you have previously selected <b>Hide graphics</b> on the vertical menu bar</li> </ul>                                                                                                                                                                                                                                                                                                                                          |
| PWR/NO button   | <ul style="list-style-type: none"> <li>■ Press PWR/NO when the camera is switched off to switch on the camera</li> <li>■ Press PWR/NO to cancel selections in dialog boxes</li> <li>■ Press and hold down PWR/NO for more than two seconds to switch off the camera</li> <li>■ Press PWR/NO to leave freeze and recall mode</li> <li>■ Press PWR/NO to display the graphics if you have previously selected <b>Hide graphics</b> on the vertical menu bar.</li> </ul>                                                                                                                                                                        |
| Navigation pad  | <p>In menu mode:</p> <ul style="list-style-type: none"> <li>■ Press left/right or up/down to navigate in menus and dialog boxes</li> <li>■ Press left/right or up/down to change or move a screen object previously selected by using SEL</li> </ul> <p>In manual adjust mode:</p> <ul style="list-style-type: none"> <li>■ Press up/down to change the level (after having selected the scale by pressing SEL)</li> <li>■ Press left/right to change the span (after having selected the scale by pressing SEL)</li> </ul> <p>For more information about level and span, see section 10.4.3 – Manual adjust/Automatic adjust on page 84</p> |

| Button  | Comments                                                                                                                                                                                                                                                                                                                                                                                                                          |
|---------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Trigger | <p>Pull the trigger to do one of the following:</p> <ul style="list-style-type: none"><li>■ Save the image</li><li>■ Switch on or switch off the Laser LocatIR</li><li>■ Autoadjust the camera</li><li>■ Update ref. temp</li></ul> <p>The function of the trigger depends on the trigger settings in the <b>Settings</b> dialog box. For more information about trigger settings, see section 10.4.8.1 – Settings on page 88</p> |

### 9.3 Laser LocatIR

By pulling the trigger on the bottom side of the camera body, a laser dot appears approx. 40 mm/1.57" above the target.

➡ Please note the following:

- A laser icon appears on the screen when the Laser LocatIR is switched on.
- Since the distance between the laser beam and the image center will vary by the target distance, Laser LocatIR should only be used as an aiming aid. Always check the LCD to make sure the camera captures the desired target.
- Do not look directly into the laser beam.
- When not in use, the Laser LocatIR should always be protected by the lens cap.


For more information about trigger settings, see section 10.4.8.1 – Settings on page 88.

10376403.a2



**Figure 9.4** Wavelength: 635 nm. Max. output power: 1 mW. This product complies with 21 CFR 1040.10 and 1040.11 except for deviations pursuant to Laser Notice No. 50, dated July 26th, 2001

10311303.a4

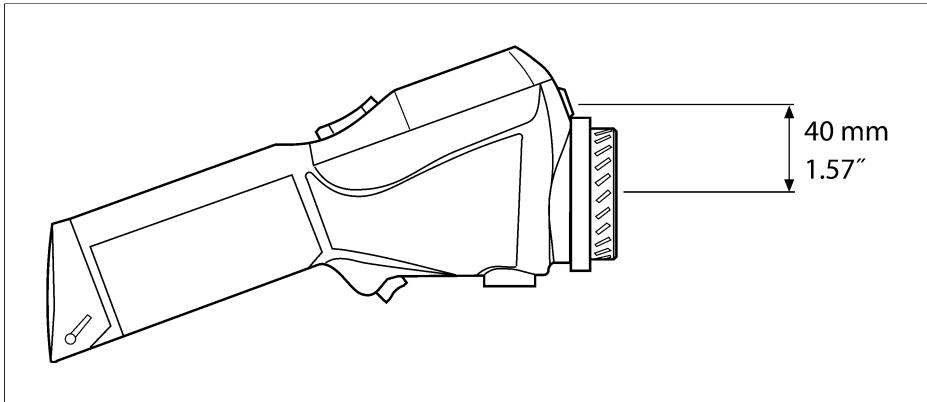

**Figure 9.5** Distance between the laser beam and the image center

## 9.4 LED indicator on keypad

**Figure 9.6** Explanations of the LED indicator on the keypad

| Indicator mode                                                           | Explanation                                                         |
|--------------------------------------------------------------------------|---------------------------------------------------------------------|
| Continuous green light                                                   | Powering up or operating.                                           |
| Flashing green light<br>(0.25 sec. switched on + 0.25 sec. switched off) | Battery charging in standby mode.                                   |
| Flashing green light<br>(3 sec. switched on + 0.06 sec. switched off)    | Battery charging in power-on mode.                                  |
| No light                                                                 | The camera is switched off, or the LCD is temporarily switched off. |

# 10 Camera program

## 10.1 Result table

The results of measurement markers are displayed in a result table in the top right-hand corner of the screen.

**Figure 10.1** Explanation of measurement markers appearing in the result table

| Icon                                                                              | Explanation                                                                                                                                                                          |
|-----------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|  | Spot                                                                                                                                                                                 |
| Max                                                                               | Area, maximum temperature                                                                                                                                                            |
| Min                                                                               | Area, minimum temperature                                                                                                                                                            |
|  | Area, average temperature                                                                                                                                                            |
|  | Color alarm above                                                                                                                                                                    |
|  | Color alarm below                                                                                                                                                                    |
| *                                                                                 | The * symbol indicates uncertain result due to an internal updating process after the range has been changed or the camera has been started. The symbol disappears after 15 seconds. |

## 10.2 System messages

### 10.2.1 Status messages

Status messages are displayed at the bottom of the screen, or in the top left part of the screen. Here you will find information about the current status of the camera.

**Figure 10.2** Status messages – a few examples

| Message     | Explanation                                                                                     |
|-------------|-------------------------------------------------------------------------------------------------|
| Frozen      | Message is displayed when the image is frozen.                                                  |
| Manual      | Message is displayed when the camera is currently in manual adjust mode.                        |
| Please wait | Message is displayed during operations that take some time.                                     |
| Restarting  | Message is displayed when the software is restarted, <i>i.e.</i> after <b>Factory default</b> . |
| Saving as   | Message is displayed while an image is being saved.                                             |

### 10.2.2 Warning messages

Warning messages are displayed in the center of the screen. Here you will find important information about battery status, for example.

**Figure 10.3** Critical camera information – a few examples

| Message                    | Explanation                                   |
|----------------------------|-----------------------------------------------|
| Battery low                | The battery level is below a critical level.  |
| Shutting down              | The camera will be switched off immediately.  |
| Shutting down in 2 seconds | The camera will be switched off in 2 seconds. |


## 10.3 Selecting screen objects

### 10.3.1 Selecting screen objects


Some screen objects – e.g. the scale, the information field, a spot *etc.* – can be selected by pressing SEL repeatedly until the object is either highlighted or surrounded by small brackets. After three seconds the cursor will automatically be hidden. Pressing SEL or the navigation pad will display the cursor again.

When an object is selected you can use the navigation pad to change its value or, where applicable, change its position.

### 10.3.2 Examples of selected screen objects

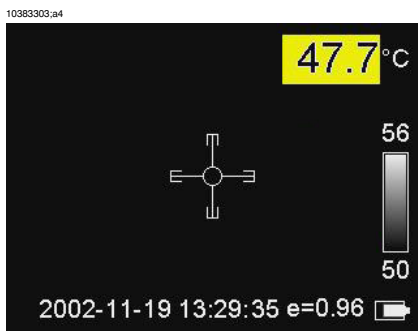

**Figure 10.4** A selected measurement marker (spot). Press the navigation pad at this stage to move the spot.

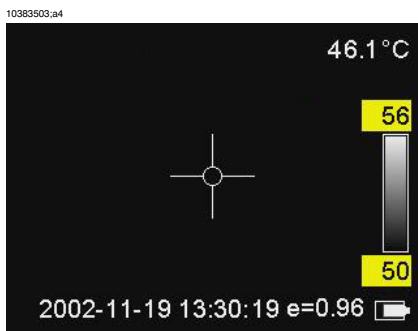


**Figure 10.5** A selected temperature scale. Press the navigation pad up/down at this stage to increase/decrease the *level*, and left/right to increase/decrease the *span*.

10383403.a3



**Figure 10.6** A selected color alarm. Press the navigation pad up/down at this stage to increase/decrease the color alarm temperature.

10383803.a3

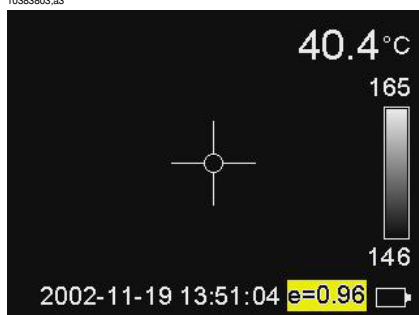

**Figure 10.7** A selected emissivity field. Press the navigation pad up/down at this stage to increase/decrease the emissivity.

## 10.4 Menu system

### 10.4.1 Navigating the menu system

- Press MENU/YES to display the vertical menu bar
- Press MENU/YES to confirm selections in menus and dialog boxes
- Press PWR/NO to exit the menu system
- Press PWR/NO to cancel selections in menus and dialog boxes
- Press the navigation pad up/down to move up/down in menus, submenus and dialog boxes
- Press the navigation pad right/left to move right/left in menus and submenus, and to change values in dialog boxes

### 10.4.2 Meas. mode

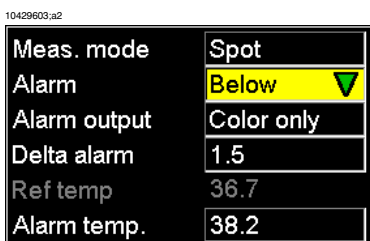


Figure 10.8 Meas. mode dialog box

Figure 10.9 Explanations of the Meas. mode dialog box


| Label      | Value                                                                                                                                                      | Explanation                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |
|------------|------------------------------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Meas. mode | <ul style="list-style-type: none"> <li>■ None</li> <li>■ Spot</li> <li>■ Area max</li> <li>■ Area min</li> <li>■ Area avg</li> <li>■ Diff spots</li> </ul> | <ul style="list-style-type: none"> <li>■ Select <b>None</b> to disable the measurement mode.</li> <li>■ Select <b>Spot</b> to lay out a spot, where the temperature of the spot will be displayed in the result table.</li> <li>■ Select <b>Area max</b> to lay out an area on the screen, where the maximum temperature in the area will be displayed in the result table.</li> <li>■ Select <b>Area min</b> to lay out an area on the screen, where the minimum temperature in the area will be displayed in the result table.</li> <li>■ Select <b>Area avg</b> to lay out an area on the screen, where the average temperature in the area will be displayed in the result table.</li> <li>■ Select <b>Diff spots</b> to calculate the difference between two spots and display this difference in the result table.</li> </ul> |

| Label        | Value                                                                                                  | Explanation                                                                                                                                                                                                                                                                                                                                                                                                                                                |
|--------------|--------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Alarm        | <ul style="list-style-type: none"> <li>Off</li> <li>Dew point</li> <li>Above</li> <li>Below</li> </ul> | <ul style="list-style-type: none"> <li>Select <b>Off</b> to disable the alarm</li> <li>Select <b>Dew point</b> to trigger an alarm when a measurement marker detects a cold surface where there is risk of humidity falling out as liquid water</li> <li>Select <b>Above</b> to assign an alarm color to all pixels above the alarm temperature</li> <li>Select <b>Below</b> to assign an alarm color to all pixels below the alarm temperature</li> </ul> |
| Alarm output | <ul style="list-style-type: none"> <li>Color only</li> <li>Silent</li> <li>Beep</li> </ul>             | <ul style="list-style-type: none"> <li>Select <b>Color only</b> to assign only a color to the pixels when an alarm is triggered.</li> <li>Select <b>Silent</b> to additionally make the font of the temperature result increase in size and be displayed against a red background (<i>i.e.</i> a visual alarm)</li> <li>Select <b>Beep</b> to additionally make the camera trigger a beep when an alarm is triggered.</li> </ul>                           |
| Delta alarm  | N/A                                                                                                    | <p>Enter an delta alarm value by pressing the navigation pad left/right.</p> <p>☞ This label is only available if <b>Update ref temp</b> has been previously selected in the <b>Settings</b> dialog box.</p>                                                                                                                                                                                                                                               |
| Ref temp     | User-defined                                                                                           | <p>For information purposes only.</p> <p>The reference temperature is calculated and updated 'on the fly'.</p> <p>☞ This label is only available if <b>Update ref temp</b> has been previously selected in the <b>Settings</b> dialog box.</p>                                                                                                                                                                                                             |
| Alarm temp   | User-defined                                                                                           | <p>Enter a temperature value by pressing the navigation pad left/right.</p>                                                                                                                                                                                                                                                                                                                                                                                |

#### 10.4.3 Manual adjust/Automatic adjust

Point to **Manual adjust** and press MENU/YES to manually select *level* and *span* settings. The level command can be regarded as the *brightness*, while the span command can be regarded as the *contrast*.


- Press the navigation pad up/down to change the level (indicated by an arrow pointing upwards or downwards in the temperature scale)
- Press the navigation pad left/right to change the span (indicated by two arrows pointing away from each other or towards each other)

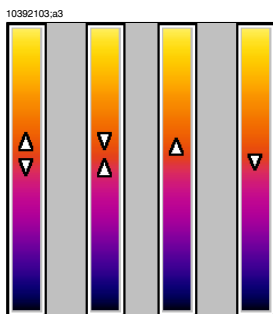

**Figure 10.10** Symbols in the temperature scale, indicating (1) increasing span; (2) decreasing span; (3) increasing level, and (4) decreasing level

Point to **Automatic adjust** and press MENU/YES to put the camera in automatic mode, continuously optimizing the image for best level and span.

#### 10.4.4 Emissivity



**Figure 10.11** Emissivity dialog box

Point to **Emissivity** on the vertical menu bar and press MENU/YES to display the **Emissivity** dialog box.

- To change the emissivity, press the navigation pad right/left
- To display an emissivity table and select a value from the table, press **Emissivity table**
- To change the parameters for the dew point alarm, enter a value for atmospheric temperature (**T Atmosphere**) and relative humidity (**Rel. Humidity**)
- To confirm the choice, press MENU/YES
- To cancel any changes, press PWR/NO
- To change **T Refl** (reflected ambient temperature), press the navigation pad right/left
- To confirm the choice, press MENU/YES
- To cancel any changes, press PWR/NO

For more information about emissivity and reflected ambient temperature, see section 16 – Thermographic measurement techniques on page 135 and section 18 – Theory of thermography on page 145

➡ Please note the following:

- When the scale is selected, you can change the emissivity directly by using the navigation pad.
- If you enter an emissivity value less than 0.30 the emissivity box will begin flashing to remind you that this value is unusually low.

#### 10.4.5 Palette

10382603.a4



**Figure 10.12** Palette dialog box

Point to **Palette** on the vertical menu bar and press MENU/YES to display the **Palette** dialog box.

- To select another palette, press the navigation pad left/right
- To confirm the choice, press MENU/YES
- To cancel any changes, press PWR/NO

#### 10.4.6 Hide graphics / Show graphics

Point to **Hide graphics** on the vertical menu bar and press MENU/YES to hide all graphics currently displayed on the screen. To display the graphics again, either:

- Point to **Show graphics** on the menu, *or*
- Briefly press SEL, *or*
- Briefly press MENU/YES, *or*
- Briefly press PWR/NO

⚡ The laser icon overrides the **Hide graphics** menu selection. This means that even though **Hide graphics** is selected when the Laser LocatIR is lit, the laser icon will still be displayed on the screen.

10.4.7 File


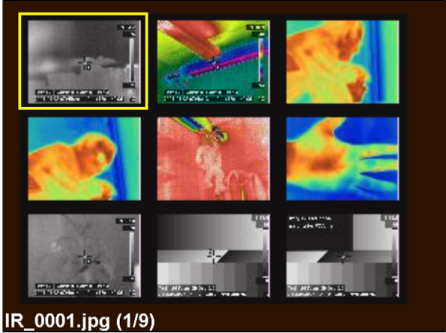


Figure 10.13 File menu

Figure 10.14 Explanations of the File menu

| Command           | Explanation                                                                                                                                                                                                                                                                                                                                  |
|-------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Images            | <p>Point to <b>Images</b> and press the joystick to display a thumbnail view of the images in the internal camera memory. Open an image by selecting the image using the joystick, then pressing MENU/YES.</p> <p>10568903.a1</p>  <p>IR_0001.jpg (1/9)</p> |
| Delete image      | <p>Point to <b>Delete image</b> and press MENU/YES to delete a recalled image.</p> <p>This choice will display a confirmation box where you can either confirm or cancel the deletion.</p>                                                                                                                                                   |
| Delete all images | <p>Point to <b>Delete all images</b> and press MENU/YES to delete all images.</p> <p>This choice will display a confirmation box where you can either confirm or cancel the deletion.</p>                                                                                                                                                    |

| Command           | Explanation                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |
|-------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Image description | <p>Point to <b>Image description</b> and press MENU/YES to display the <b>Image description</b> dialog box. Using this feature, you can add a brief description to an image one of the following ways:</p> <ul style="list-style-type: none"> <li>■ By sending a Pocket Word file (*.psw) from a PDA to the camera, using the IrDA infrared communication link</li> <li>■ By letting the camera read any value of the first label in a standard FLIR Systems *.tcf file (text comment file) located in the camera file system, and use this value as the image description</li> </ul> <p>The image description can be read out by other software – e.g. ThermoCAM™ QuickView.</p> <p>➡ For information about how to create files for image descriptions, see section 8.5 – Creating files for image descriptions on page 62</p> |

➡ Approx. 200 radiometric JPG images can be saved.

## 10.4.8 Setup

10383003.a4




Figure 10.15 Setup menu

### 10.4.8.1 Settings

10567203.a2

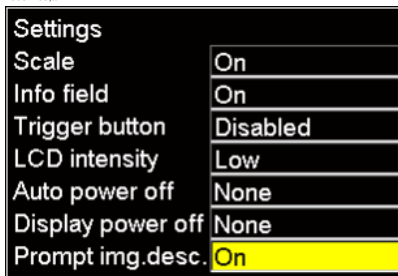


Figure 10.16 Settings dialog box

Figure 10.17 Explanations of the Settings dialog box

| Label | Value                                                                 | Explanation                                                                                                                              |
|-------|-----------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------|
| Scale | <ul style="list-style-type: none"> <li>■ On</li> <li>■ Off</li> </ul> | <ul style="list-style-type: none"> <li>■ Select On to display the scale on the screen</li> <li>■ Select Off to hide the scale</li> </ul> |

| Label             | Value                                                                                                                                                     | Explanation                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
|-------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Info field        | <ul style="list-style-type: none"> <li>■ On</li> <li>■ Off</li> <li>■ On + TRefl</li> </ul>                                                               | <ul style="list-style-type: none"> <li>■ Select <b>On</b> to display the information field at the bottom of the screen</li> <li>■ Select <b>Off</b> to hide the information field</li> <li>■ Select <b>On + TRefl</b> to display the information field and the reflected ambient temperature</li> </ul>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                          |
| Trigger           | <ul style="list-style-type: none"> <li>■ Laser</li> <li>■ Save</li> <li>■ Disabled</li> <li>■ One-shot autoadjust</li> <li>■ Update ref. temp.</li> </ul> | <ul style="list-style-type: none"> <li>■ Select <b>Laser</b> to activate the laser when pulling the trigger</li> <li>■ Select <b>Save</b> to save the current image when pulling the trigger</li> <li>■ Select <b>Disabled</b> to disable the trigger</li> <li>■ Select <b>One-shot autoadjust</b> to autoadjust the camera when pulling the trigger</li> <li>■ Select <b>Update ref. temp</b> to update the reference temperature when pulling the trigger</li> </ul> <p>If <b>Update ref. temp.</b> is selected:</p> <p>By pulling the trigger for more than 1 second, a dialog displaying the message <b>Restart ref temp at nn.n °C?</b> will appear.</p> <p>Do one of the following:</p> <ul style="list-style-type: none"> <li>■ Select <b>OK</b> to purge the internal camera buffer and begin a new sampling sequence</li> <li>■ Select <b>Cancel</b> to leave the dialog box</li> </ul> |
| LCD intensity     | <ul style="list-style-type: none"> <li>■ Low intensity of the LCD</li> <li>■ Medium</li> <li>■ High</li> </ul>                                            | <ul style="list-style-type: none"> <li>■ Select <b>Low</b> to set the LCD intensity to the lowest level</li> <li>■ Select <b>Medium</b> to set the LCD intensity to medium level</li> <li>■ Select <b>High</b> to set the LCD intensity to the highest level</li> </ul>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                          |
| Auto power off    | <ul style="list-style-type: none"> <li>■ None</li> <li>■ 2 min</li> <li>■ 5 min</li> <li>■ 10 min</li> </ul>                                              | <p>If the camera is switched on but currently not used, it will automatically be switched off after a specified time.</p> <p>Set the time by pressing the navigation pad left/right.</p>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |
| Display power off | <ul style="list-style-type: none"> <li>■ None</li> <li>■ 30 sec.</li> <li>■ 60 sec.</li> <li>■ 2 min.</li> </ul>                                          | <p>If the camera is switched on but currently not used, the display will automatically be switched off after a specified time.</p> <p>Set the time by pressing the navigation pad left/right.</p>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |
| Prompt img. desc. | <ul style="list-style-type: none"> <li>■ On</li> <li>■ Off</li> </ul>                                                                                     | <p>If you want to be prompted for adding an image description when saving an infrared image, select <b>On</b>.</p>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |

➡ For protective reasons, the LCD will be switched off if the detector temperature exceeds +60 °C (+149 °F) and the camera will be switched off if the detector temperature exceeds +68 °C (+154.4 °F)

#### 10.4.8.2 *Date/time*

10382103.a3

| Date/time |      |
|-----------|------|
| Year      | 2002 |
| Month     | 11   |
| Day       | 19   |
| Hour      | 10   |
| Minute    | 37   |
| Second    | 5    |


**Figure 10.18** Date/time dialog box

**Figure 10.19** Explanations of the Date/time dialog box

| Label  | Explanation                                                                                                                                                            |
|--------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Year   | 1970–2036                                                                                                                                                              |
| Month  | 1–12                                                                                                                                                                   |
| Day    | 1–31                                                                                                                                                                   |
| Hour   | <ul style="list-style-type: none"> <li>■ 12 a.m.–12 p.m.</li> <li>■ 1–24</li> </ul> <p>The format depends on the settings in the <b>Local Settings</b> dialog box.</p> |
| Minute | 00–59                                                                                                                                                                  |
| Second | 00–59                                                                                                                                                                  |

### 10.4.8.3 Local settings

10567103.a2

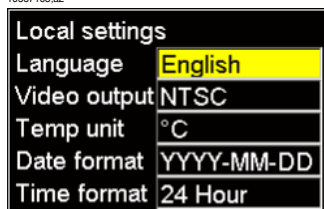

**Figure 10.20** Local settings dialog box

**Figure 10.21** Explanations of the Local settings dialog box

| Label        | Explanation                                                                                                                |
|--------------|----------------------------------------------------------------------------------------------------------------------------|
| Language     | Configuration-dependent                                                                                                    |
| Video output | <ul style="list-style-type: none"> <li>■ NTSC</li> <li>■ PAL</li> </ul>                                                    |
| Temp unit    | <ul style="list-style-type: none"> <li>■ °C – degrees Celsius or</li> <li>■ °F – degrees Fahrenheit</li> </ul>             |
| Date format  | <ul style="list-style-type: none"> <li>■ YYYY-MM-DD</li> <li>■ YY-MM-DD</li> <li>■ MM/DD/YY</li> <li>■ DD/MM/YY</li> </ul> |
| Time format  | <ul style="list-style-type: none"> <li>■ 24 hour</li> <li>■ AM/PM</li> </ul>                                               |

### 10.4.8.4 Camera info

The camera info panel shows information about memory usage, battery status, serial numbers, software revisions, etc.

No changes can be made.

### 10.4.8.5 Factory default

Point to **Factory default** and press MENU/YES to reset all camera settings to factory settings.

INTENTIONALLY LEFT BLANK

---

# 11 Electrical power system


The camera's electrical power system consists of the following parts:

- a removable battery
- a power supply
- an internal battery charger

The camera may powered either by using the battery, or by using the power supply. When using the power supply, the battery will – if it's inserted in the battery compartment – automatically be charged. You can still use the camera during charging.

🔔 Please note the following:

- The camera is shipped with charged batteries. To increase the battery life, the battery should be fully discharged and charged a couple of times by using the camera or leaving the camera on, until the camera says **Battery low**.
- The same power supply can be used for both the internal battery charger and the external battery charger.

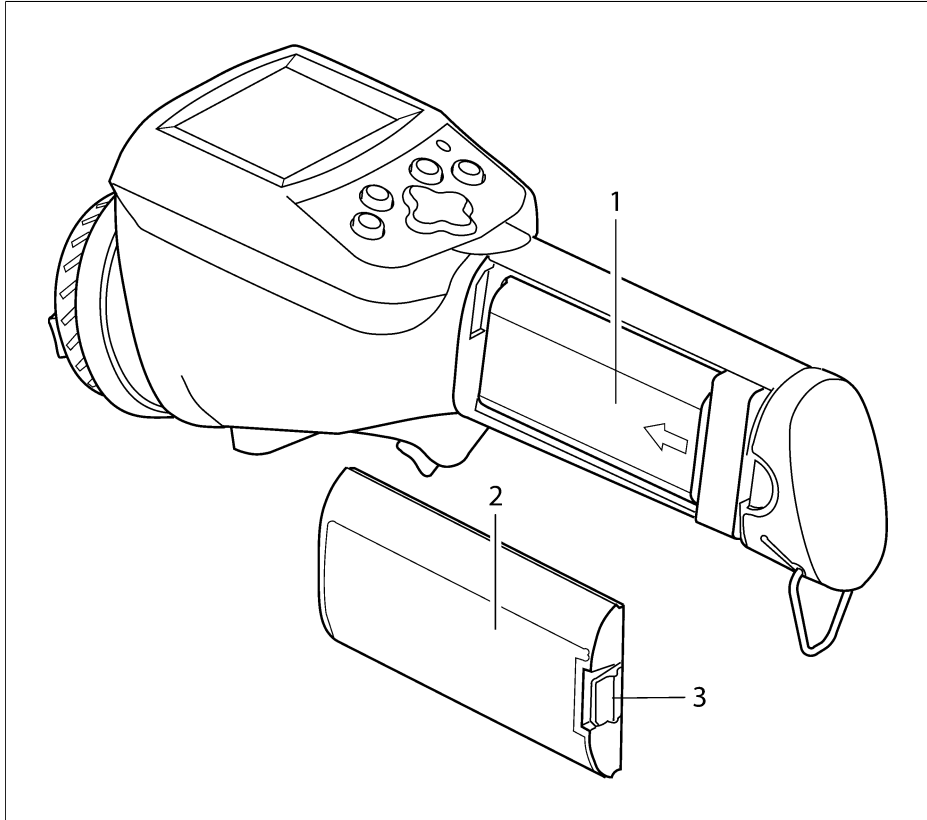

**Figure 11.1** Battery and battery compartment

| Callout | Description of part |
|---------|---------------------|
| 1       | Battery             |
| 2       | Battery cover       |
| 3       | Release button      |

The removable battery gives an operation time of approx. 1.5–2 hours. When **Battery low** is displayed on the screen it is time to charge the battery.

☛ The operation time of the camera when run on a battery is substantially shorter in low temperatures.

## 11.1 Internal battery charging

To charge the battery using the internal battery charger, follow the instructions below:

| Step | Action                                                                                                                                                                                    |
|------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 1    | Make sure that the battery is correctly inserted into the camera.                                                                                                                         |
| 2    | Connect the power cable to the camera.                                                                                                                                                    |
| 3    | While charging, the battery status symbol will pulse until the battery is fully charged. When the battery is fully charged the battery symbol will stop pulsing and be completely filled. |

10305803.a2



**Figure 11.2** Battery full symbol

## 11.2 External battery charging

➡ External battery charger is an extra option.

You can also charge the battery by using the external battery charger. The battery status during charging is indicated by a number of LEDs.

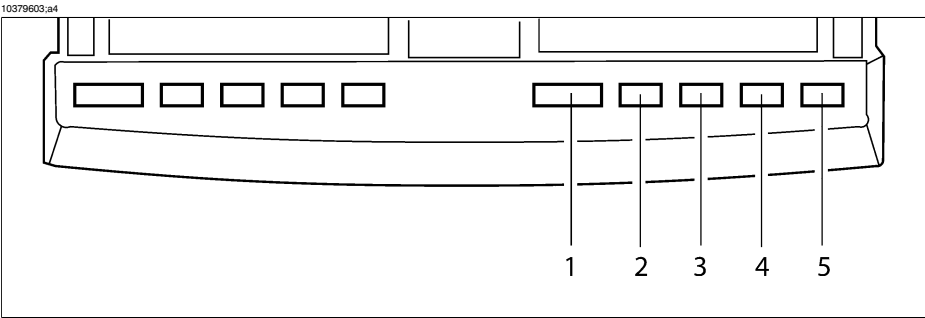


Figure 11.3 LED indicators on the external battery charger

Figure 11.4 LED indicators – explanations of callouts

| Situation                                              | LED indicator no. | Color & mode                                                                                                                  |
|--------------------------------------------------------|-------------------|-------------------------------------------------------------------------------------------------------------------------------|
| The charger is under power, but no battery is inserted | 1                 | Fixed red light                                                                                                               |
| The charger is under power, and a battery is inserted  | 1                 | Fixed green light                                                                                                             |
| The battery is too cold or too warm                    | 1                 | Flashing green light                                                                                                          |
| The battery is out of order                            | 1                 | Flashing red light                                                                                                            |
| The battery is now being charged                       | 5-2               | Pulsing green light from LED no. 5 to LED no. 2<br><br>Each LED represents 25 % battery capacity and will be lit accordingly. |

### 11.3 *Battery safety warnings*

- Do not place the battery in fire or heat the battery.
- Do not install the battery backwards so that the polarity is reversed.
- Do not connect the positive terminal and the negative terminal of the battery to each other with any metal object (such as wire).
- Do not pierce the battery with nails, strike the battery with a hammer, step on the battery, or otherwise subject it to strong impacts or shocks.
- Do not solder directly onto the battery.
- Do not expose the battery to water or salt water, or allow the battery to get wet.
- Do not disassemble or modify the battery. The battery contains safety and protection devices which, if damaged, may cause the battery to generate heat, explode or ignite.
- Do not place the battery on or near fires, stoves, or other high-temperature locations.
- When the battery is worn out, insulate the terminals with adhesive tape or similar materials before disposal.
- Immediately discontinue use of the battery if, while using, charging, or storing the battery, the battery emits an unusual smell, feels hot, changes color, changes shape, or appears abnormal in any other way. Contact your sales location if any of these problems are observed.
- In the event that the battery leaks and the fluid gets into one's eye, do not rub the eye. Rinse well with water and immediately seek medical care. If left untreated the battery fluid could cause damage to the eye.
- When charging the battery, only use a specified battery charger.
- Do not attach the batteries to a power supply plug or directly to a car's cigarette lighter.
- Do not place the batteries in or near fire, or into direct sunlight. When the battery becomes hot, the built-in safety equipment is activated, preventing the battery from charging further, and heating the battery can destroy the safety equipment and can cause additional heating, breaking, or ignition of the battery.
- Do not continue charging the battery if it does not recharge within the specified charging time. Doing so may cause the battery to become hot, explode, or ignite.
- The temperature range over which the battery can be charged is 0–+45 °C (+32–+113 °F). Charging the battery at temperatures outside of this range may cause the battery to become hot or to break. Charging the battery outside of this temperature range may also harm the performance of the battery or reduce the battery's life expectancy.
- Do not discharge the battery using any device except for the specified device. When the battery is used in devices aside from the specified device it may damage the performance of the battery or reduce its life expectancy, and if the device causes an abnormal current to flow, it may cause the battery to become hot, explode, or ignite and cause serious injury.

- The temperature range over which the battery can be discharged is  $-15$ – $+45$  °C ( $+18.8$ – $+113$  °F). Use of the battery outside of this temperature range may damage the performance of the battery or may reduce its life expectancy.

---

# 12 Maintenance & cleaning

## 12.1 Camera body, cables & accessories

The camera body, cables and accessories may be cleaned by wiping with a soft cloth. To remove stains, wipe with a soft cloth moistened with a mild detergent solution and wrung dry, then wipe with a dry soft cloth.

⚠ Do not use benzene, thinner, or any other chemical product on the camera, the cables or the accessories, as this may cause deterioration.

## 12.2 Lenses

All lenses are coated with an anti-reflective coating and care must be taken when cleaning them. Cotton wool soaked in 96 % ethyl alcohol ( $\text{C}_2\text{H}_5\text{OH}$ ) may be used to clean the lenses. The lenses should be wiped once with the solution, then the cotton wool should be discarded.

If ethyl alcohol is unavailable, DEE (*i.e.* 'ether' = diethylether,  $\text{C}_4\text{H}_{10}\text{O}$ ) may be used for cleaning.

Sometimes drying marks may appear on the lenses. To prevent this, a cleaning solution of 50 % acetone (*i.e.* dimethylketone,  $(\text{CH}_3)_2\text{CO}$ ) and 50 % ethyl alcohol ( $\text{C}_2\text{H}_5\text{OH}$ ) may be used.

⚠ Please note the following:

- Excessive cleaning of the lenses may wear down the coating.
- The chemical substances described in this section may be dangerous. Carefully read all warning labels on containers before using the substances, as well as applicable MSDS (Material Safety Data Sheets).

INTENTIONALLY LEFT BLANK

# 13 Troubleshooting

| Problem                                               | Possible reason                                                                                                       | Solution                                                       |
|-------------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------|
| The LCD displays no image at all.                     | The camera may have been switched off automatically due the settings in the <b>Settings</b> dialog box.               | Press PWR/NO to switch on the camera.                          |
|                                                       | The LCD may have been switched off automatically due to the settings in the <b>Settings</b> dialog box.               | Press PWR/NO to switch on the camera.                          |
|                                                       | There is no battery in the battery compartment.                                                                       | Insert a fully charged battery.                                |
|                                                       | There is a battery in the battery compartment, but the battery is depleted.                                           | Charge the battery.                                            |
|                                                       | If you are using the power supply, the connector may not be properly inserted into the power connector on the camera. | Verify that the power supply connector is properly inserted.   |
|                                                       | If you are using the power supply, the mains plug may not be properly plugged in into a mains supply.                 | Verify that the mains plug is properly plugged in.             |
|                                                       | If you are using the power supply, the mains cable may not be properly plugged in into the power supply.              | Verify that the mains cable is properly plugged in.            |
| The LCD displays an image, but it is of poor quality. | The level needs to be changed.                                                                                        | Change the level.                                              |
|                                                       | The span needs to be changed                                                                                          | Change the span.                                               |
|                                                       | The camera needs to be autoadjusted.                                                                                  | Carry out an autoadjust maneuver.                              |
|                                                       | The target may be hotter or colder than the temperature range you are currently using.                                | If your camera features an additional range, change the range. |
|                                                       | A different palette may be more suitable for imaging the target than the one you are currently using.                 | Change the palette.                                            |
| The LCD displays an image, but it is blurry.          | The target may be out of focus.                                                                                       | Focus the camera by rotating the focus ring on the lens.       |
| The LCD displays an image, but it is of low contrast. | The contrast of the LCD may have accidentally been set to too low a value.                                            | Change the contrast of the LCD.                                |

| Problem                                                                             | Possible reason                                                                                                                              | Solution                                                                                          |
|-------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------|
| The trigger button does not work as expected.                                       | The function of the trigger button may have accidentally been changed.                                                                       | Change the function of the trigger button.                                                        |
| The trigger button does not work at all.                                            | The trigger button may have accidentally been disabled.                                                                                      | Enable the trigger button.                                                                        |
| When connecting the infrared camera to an external video monitor, no image appears. | The video cable connector may not be properly inserted into the video connector on the camera.                                               | Verify that the video connector is properly inserted.                                             |
|                                                                                     | The video cable connector may not be properly inserted into the video connector on the external monitor.                                     | Verify that the video connector is properly inserted.                                             |
|                                                                                     | The camera may have accidentally been set to PAL video format, while the external video monitor is set to NTSC video format, and vice versa. | Change the video format.                                                                          |
| The LCD does not display the correct date & time.                                   | The camera may have accidentally been set to the wrong date & time.                                                                          | Change the date & time.                                                                           |
| It is not possible to store any more images in the camera.                          | The internal flash memory may be full.                                                                                                       | To be able to save more images, download the images to your computer using ThermoCAM™ Quick-View. |

# 14 Technical specifications & dimensional drawings

FLIR Systems reserves the right to discontinue models, parts and accessories, and other items, or change specifications at any time without prior notice.

## 14.1 Imaging performance

|                             |                                                                      |
|-----------------------------|----------------------------------------------------------------------|
| Focus                       | Manual                                                               |
| Start-up time               | Approx. 15 seconds                                                   |
| Start-up time from stand-by | < 1 second @ +25 °C (+77 °F)                                         |
| Detector type               | Focal Plane Array (FPA), uncooled microbolometer<br>160 × 120 pixels |
| Spectral range              | 7.5–13 µm                                                            |

## 14.2 Image presentation

|              |                                                         |
|--------------|---------------------------------------------------------|
| Display      | 2.5" color LCD, 16-bit colors                           |
| Video output | Composite video CVBS (ITU-R BT.470 PAL/SMPTE 170M NTSC) |

## 14.3 Laser LocatIR

|                |                                                         |
|----------------|---------------------------------------------------------|
| Classification | Class 2                                                 |
| Type           | Semiconductor AlGaInP diode laser,<br>1 mW/635 nm (red) |

## 14.4 Electrical power system

|                        |                                                                        |
|------------------------|------------------------------------------------------------------------|
| Battery type           | Rechargeable Li/Ion battery                                            |
| Battery operating time | 1.5 hours. Display shows battery status                                |
| Battery charging       | Internal, AC adapter, or 12 VDC car adapter.<br>2-bay desktop charger. |
| AC operation           | AC adapter, 90–260 VAC, 50/60 Hz, 12 VDC out                           |
| Voltage                | 11–16 VDC                                                              |

|                  |                                                      |
|------------------|------------------------------------------------------|
| Power management | Automatic shut-down and sleep mode (user-selectable) |
|------------------|------------------------------------------------------|

## 14.5 Environmental specifications

|                             |                                                                                                                                                                                                                                                                                                                                                    |
|-----------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Operating temperature range | <p>For camera type 215 &amp; 247:<br/>-15–+45 °C (+5–+113 °F)</p> <p>For camera type 243:<br/>-15–+50 °C (+5–+122 °F)</p> <p>The three-digit camera type number is the three first digits in the camera S/N.</p>                                                                                                                                   |
| Storage temperature range   | -40–+70 °C (-40–+158 °F)                                                                                                                                                                                                                                                                                                                           |
| Humidity                    | Operating & storage, 10–95 %, non-condensing, IEC 359.                                                                                                                                                                                                                                                                                             |
| Encapsulation               | IP 54                                                                                                                                                                                                                                                                                                                                              |
| Shock                       | 25 g, IEC 68-2-29                                                                                                                                                                                                                                                                                                                                  |
| Vibration                   | 2 g, IEC 68-2-6                                                                                                                                                                                                                                                                                                                                    |
| EMC                         | <p>The applicable EMC standards depend on the three-digit camera type number. One or more of the following standards apply:</p> <p>EN 61000-6-3:2001<br/>EN 61000-6-2:2001<br/>EN 50081-2 (emission)<br/>EN 50082-2 (immunity)<br/>FCC 47 CFR Part 15 B</p> <p>The three-digit camera type number is the three first digits in the camera S/N.</p> |

## 14.6 Physical specifications

|                  |                                                      |
|------------------|------------------------------------------------------|
| Weight           | 0.7 kg (1.54 lb), including battery and 17 mm lens   |
| Size (L × W × H) | 246 × 80 × 135 mm (9.7 × 3.2 × 5.3") with 17 mm lens |
| Tripod mount     | Standard, 1/4"-20                                    |
| Housing          | Plastics & rubber                                    |

## 14.7 Communications interfaces

|     |                                                                     |
|-----|---------------------------------------------------------------------|
| USB | <p>Image transfer to PC</p> <p>USB Rev 2.0 (full speed 12 Mbit)</p> |
|-----|---------------------------------------------------------------------|


RS-232 (optional)

Image transfer to PC

## 14.8 Pin configurations

### 14.8.1 RS-232/USB connector

10384403.a4




**Figure 14.1** Pin configuration – RS-232/USB (on camera – operator's side)

**Figure 14.2** Pin configuration

| Pin | Signal name |
|-----|-------------|
| 1   | USB -       |
| 2   | RS-232_TX   |
| 3   | GND         |
| 4   | N/C         |
| 5   | USB POWER   |
| 6   | USB +       |
| 7   | N/C         |
| 8   | RS-232_RX   |

### 14.8.2 Power connector


10402503.a1

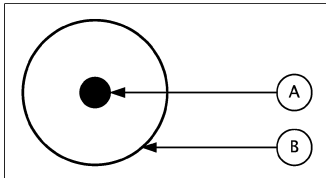

**Figure 14.3** Pin configuration for power connector (on camera – operator's side). **A:** Center pin; **B:** Chassis

|                 |           |            |
|-----------------|-----------|------------|
| Connector type: | 2.5 mm DC |            |
| Signal name     | Type      | Pin number |
| +12V            | POWER     | CENTER PIN |
| GND             | POWER     | CHASSIS    |

14.8.3 CVBS connector

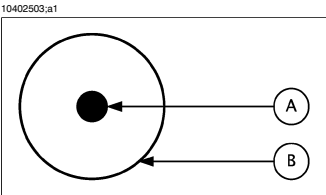

**Figure 14.4** Pin configuration for CVBS connector (on camera – operator’s side). **A:** Center pin; **B:** Chassis

|                 |           |            |
|-----------------|-----------|------------|
| Connector type: | RCA/PHONO |            |
| Signal name     | Type      | Pin number |
| CVBS            | VIDEO     | CENTER PIN |
| GND             | POWER     | CHASSIS    |

## 14.9 Relationship between fields of view and distance

10563503.a3

| <b>This table only applies to camera type number 215</b>                                  |      |      |      |       |       |       |        |        |     |
|-------------------------------------------------------------------------------------------|------|------|------|-------|-------|-------|--------|--------|-----|
| The three-digit camera type number is the three first digits in the camera S/N.           |      |      |      |       |       |       |        |        |     |
| Focal length: 87 mm                                                                       |      |      |      |       |       |       |        |        |     |
| Resolution: 160 x 120 pixels                                                              |      |      |      |       |       |       |        |        |     |
| Field of view in degrees: 4.87                                                            |      |      |      |       |       |       |        |        |     |
| D --->                                                                                    | 0.50 | 1.00 | 2.00 | 5.00  | 10.00 | 25.00 | 50.00  | 100.00 | m   |
| HFOV                                                                                      | 0.04 | 0.09 | 0.17 | 0.43  | 0.85  | 2.13  | 4.25   | 8.51   | m   |
| VFOV                                                                                      | 0.03 | 0.06 | 0.13 | 0.32  | 0.64  | 1.59  | 3.19   | 6.38   | m   |
| IFOV                                                                                      | 0.27 | 0.53 | 1.06 | 2.66  | 5.32  | 13.29 | 26.58  | 53.16  | mm  |
| D --->                                                                                    | 1.64 | 3.28 | 6.56 | 16.39 | 32.79 | 81.97 | 163.93 | 327.87 | ft. |
| HFOV                                                                                      | 0.14 | 0.28 | 0.56 | 1.39  | 2.79  | 6.97  | 13.94  | 27.89  | ft. |
| VFOV                                                                                      | 0.10 | 0.21 | 0.42 | 1.05  | 2.09  | 5.23  | 10.46  | 20.92  | ft. |
| IFOV                                                                                      | 0.01 | 0.02 | 0.04 | 0.10  | 0.21  | 0.52  | 1.05   | 2.09   | in. |
| <b>Legend:</b>                                                                            |      |      |      |       |       |       |        |        |     |
| D = Distance to target in meters & feet                                                   |      |      |      |       |       |       |        |        |     |
| HFOV = Horizontal field of view in meters & feet                                          |      |      |      |       |       |       |        |        |     |
| VFOV = Vertical field of view in meters & feet                                            |      |      |      |       |       |       |        |        |     |
| IFOV = Instantaneous field of view (size of one detector element) in millimeters & inches |      |      |      |       |       |       |        |        |     |

**Figure 14.5** Horizontal, vertical and instantaneous fields of view for certain distances to targets. **D** = distance to target. 87 mm IR lens. Applies to camera type 215 only.

10564203.a3

| <b>This table only applies to camera type number 215</b>                                             |             |             |             |              |              |              |               |               |            |
|------------------------------------------------------------------------------------------------------|-------------|-------------|-------------|--------------|--------------|--------------|---------------|---------------|------------|
| <i>The three-digit camera type number is the three first digits in the camera S/N.</i>               |             |             |             |              |              |              |               |               |            |
| <i>Focal length: 54 mm</i>                                                                           |             |             |             |              |              |              |               |               |            |
| <i>Resolution: 160 x 120 pixels</i>                                                                  |             |             |             |              |              |              |               |               |            |
| <i>Field of view in degrees: 7.83</i>                                                                |             |             |             |              |              |              |               |               |            |
| <b>D ---&gt;</b>                                                                                     | <b>0.50</b> | <b>1.00</b> | <b>2.00</b> | <b>5.00</b>  | <b>10.00</b> | <b>25.00</b> | <b>50.00</b>  | <b>100.00</b> | <b>m</b>   |
| HFOV                                                                                                 | 0.07        | 0.14        | 0.27        | 0.69         | 1.37         | 3.43         | 6.85          | 13.70         | m          |
| VFOV                                                                                                 | 0.05        | 0.10        | 0.21        | 0.51         | 1.03         | 2.57         | 5.14          | 10.28         | m          |
| IFOV                                                                                                 | 0.43        | 0.86        | 1.71        | 4.28         | 8.56         | 21.41        | 42.82         | 85.65         | mm         |
| <b>D ---&gt;</b>                                                                                     | <b>1.64</b> | <b>3.28</b> | <b>6.56</b> | <b>16.39</b> | <b>32.79</b> | <b>81.97</b> | <b>163.93</b> | <b>327.87</b> | <b>ft.</b> |
| HFOV                                                                                                 | 0.22        | 0.45        | 0.90        | 2.25         | 4.49         | 11.23        | 22.47         | 44.93         | ft.        |
| VFOV                                                                                                 | 0.17        | 0.34        | 0.67        | 1.68         | 3.37         | 8.42         | 16.85         | 33.70         | ft.        |
| IFOV                                                                                                 | 0.02        | 0.03        | 0.07        | 0.17         | 0.34         | 0.84         | 1.69          | 3.37          | in.        |
| <b>Legend:</b>                                                                                       |             |             |             |              |              |              |               |               |            |
| <i>D = Distance to target in meters &amp; feet</i>                                                   |             |             |             |              |              |              |               |               |            |
| <i>HFOV = Horizontal field of view in meters &amp; feet</i>                                          |             |             |             |              |              |              |               |               |            |
| <i>VFOV = Vertical field of view in meters &amp; feet</i>                                            |             |             |             |              |              |              |               |               |            |
| <i>IFOV = Instantaneous field of view (size of one detector element) in millimeters &amp; inches</i> |             |             |             |              |              |              |               |               |            |

**Figure 14.6** Horizontal, vertical and instantaneous fields of view for certain distances to targets. **D** = distance to target. 54 mm IR lens. Applies to camera type 215 only.

10564503.a3

|                                                                                           |      |      |      |       |       |       |        |        |     |
|-------------------------------------------------------------------------------------------|------|------|------|-------|-------|-------|--------|--------|-----|
| <b>This table only applies to camera type number 215</b>                                  |      |      |      |       |       |       |        |        |     |
| The three-digit camera type number is the three first digits in the camera S/N.           |      |      |      |       |       |       |        |        |     |
| Focal length: 36 mm                                                                       |      |      |      |       |       |       |        |        |     |
| Resolution: 160 x 120 pixels                                                              |      |      |      |       |       |       |        |        |     |
| Field of view in degrees: 11.7                                                            |      |      |      |       |       |       |        |        |     |
| D --->                                                                                    | 0.50 | 1.00 | 2.00 | 5.00  | 10.00 | 25.00 | 50.00  | 100.00 | m   |
| HFOV                                                                                      | 0.10 | 0.21 | 0.41 | 1.03  | 2.06  | 5.14  | 10.28  | 20.56  | m   |
| VFOV                                                                                      | 0.08 | 0.15 | 0.31 | 0.77  | 1.54  | 3.85  | 7.71   | 15.42  | m   |
| IFOV                                                                                      | 0.64 | 1.28 | 2.57 | 6.42  | 12.85 | 32.12 | 64.24  | 128.47 | mm  |
| D --->                                                                                    | 1.64 | 3.28 | 6.56 | 16.39 | 32.79 | 81.97 | 163.93 | 327.87 | ft. |
| HFOV                                                                                      | 0.34 | 0.67 | 1.35 | 3.37  | 6.74  | 16.85 | 33.70  | 67.40  | ft. |
| VFOV                                                                                      | 0.25 | 0.51 | 1.01 | 2.53  | 5.05  | 12.64 | 25.27  | 50.55  | ft. |
| IFOV                                                                                      | 0.03 | 0.05 | 0.10 | 0.25  | 0.51  | 1.26  | 2.53   | 5.06   | in. |
| <b>Legend:</b>                                                                            |      |      |      |       |       |       |        |        |     |
| D = Distance to target in meters & feet                                                   |      |      |      |       |       |       |        |        |     |
| HFOV = Horizontal field of view in meters & feet                                          |      |      |      |       |       |       |        |        |     |
| VFOV = Vertical field of view in meters & feet                                            |      |      |      |       |       |       |        |        |     |
| IFOV = Instantaneous field of view (size of one detector element) in millimeters & inches |      |      |      |       |       |       |        |        |     |

**Figure 14.7** Horizontal, vertical and instantaneous fields of view for certain distances to targets. **D** = distance to target. 36 mm IR lens. Applies to camera type 215 only.

10564803.a3

| <b>This table only applies to camera type number 215</b>                                             |             |             |             |              |              |              |               |               |            |
|------------------------------------------------------------------------------------------------------|-------------|-------------|-------------|--------------|--------------|--------------|---------------|---------------|------------|
| <i>The three-digit camera type number is the three first digits in the camera S/N.</i>               |             |             |             |              |              |              |               |               |            |
| <i>Focal length: 17 mm</i>                                                                           |             |             |             |              |              |              |               |               |            |
| <i>Resolution: 160 x 120 pixels</i>                                                                  |             |             |             |              |              |              |               |               |            |
| <i>Field of view in degrees: 24.5</i>                                                                |             |             |             |              |              |              |               |               |            |
| <b>D ---&gt;</b>                                                                                     | <b>0.50</b> | <b>1.00</b> | <b>2.00</b> | <b>5.00</b>  | <b>10.00</b> | <b>25.00</b> | <b>50.00</b>  | <b>100.00</b> | <b>m</b>   |
| HFOV                                                                                                 | 0.22        | 0.44        | 0.87        | 2.18         | 4.35         | 10.88        | 21.76         | 43.53         | m          |
| VFOV                                                                                                 | 0.16        | 0.33        | 0.65        | 1.63         | 3.26         | 8.16         | 16.32         | 32.65         | m          |
| IFOV                                                                                                 | 1.36        | 2.72        | 5.44        | 13.60        | 27.21        | 68.01        | 136.03        | 272.06        | mm         |
| <b>D ---&gt;</b>                                                                                     | <b>1.64</b> | <b>3.28</b> | <b>6.56</b> | <b>16.39</b> | <b>32.79</b> | <b>81.97</b> | <b>163.93</b> | <b>327.87</b> | <b>ft.</b> |
| HFOV                                                                                                 | 0.71        | 1.43        | 2.85        | 7.14         | 14.27        | 35.68        | 71.36         | 142.72        | ft.        |
| VFOV                                                                                                 | 0.54        | 1.07        | 2.14        | 5.35         | 10.70        | 26.76        | 53.52         | 107.04        | ft.        |
| IFOV                                                                                                 | 0.05        | 0.11        | 0.21        | 0.54         | 1.07         | 2.68         | 5.36          | 10.71         | in.        |
| <b>Legend:</b>                                                                                       |             |             |             |              |              |              |               |               |            |
| <i>D = Distance to target in meters &amp; feet</i>                                                   |             |             |             |              |              |              |               |               |            |
| <i>HFOV = Horizontal field of view in meters &amp; feet</i>                                          |             |             |             |              |              |              |               |               |            |
| <i>VFOV = Vertical field of view in meters &amp; feet</i>                                            |             |             |             |              |              |              |               |               |            |
| <i>IFOV = Instantaneous field of view (size of one detector element) in millimeters &amp; inches</i> |             |             |             |              |              |              |               |               |            |

**Figure 14.8** Horizontal, vertical and instantaneous fields of view for certain distances to targets. **D** = distance to target. 17 mm IR lens. Applies to camera type 215 only.

10565103.a3

|                                                                                                      |             |             |             |              |              |              |               |               |            |
|------------------------------------------------------------------------------------------------------|-------------|-------------|-------------|--------------|--------------|--------------|---------------|---------------|------------|
| <b>This table only applies to camera type number 215</b>                                             |             |             |             |              |              |              |               |               |            |
| <i>The three-digit camera type number is the three first digits in the camera S/N.</i>               |             |             |             |              |              |              |               |               |            |
| <i>Focal length: 9.2 mm</i>                                                                          |             |             |             |              |              |              |               |               |            |
| <i>Resolution: 160 x 120 pixels</i>                                                                  |             |             |             |              |              |              |               |               |            |
| <i>Field of view in degrees: 43.8</i>                                                                |             |             |             |              |              |              |               |               |            |
| <b>D ---&gt;</b>                                                                                     | <b>0.50</b> | <b>1.00</b> | <b>2.00</b> | <b>5.00</b>  | <b>10.00</b> | <b>25.00</b> | <b>50.00</b>  | <b>100.00</b> | <b>m</b>   |
| HFOV                                                                                                 | 0.40        | 0.80        | 1.61        | 4.02         | 8.04         | 20.11        | 40.22         | 80.43         | m          |
| VFOV                                                                                                 | 0.30        | 0.60        | 1.21        | 3.02         | 6.03         | 15.08        | 30.16         | 60.33         | m          |
| IFOV                                                                                                 | 2.51        | 5.03        | 10.05       | 25.14        | 50.27        | 125.68       | 251.36        | 502.72        | mm         |
| <b>D ---&gt;</b>                                                                                     | <b>1.64</b> | <b>3.28</b> | <b>6.56</b> | <b>16.39</b> | <b>32.79</b> | <b>81.97</b> | <b>163.93</b> | <b>327.87</b> | <b>ft.</b> |
| HFOV                                                                                                 | 1.32        | 2.64        | 5.27        | 13.19        | 26.37        | 65.93        | 131.86        | 263.72        | ft.        |
| VFOV                                                                                                 | 0.99        | 1.98        | 3.96        | 9.89         | 19.78        | 49.45        | 98.90         | 197.79        | ft.        |
| IFOV                                                                                                 | 0.10        | 0.20        | 0.40        | 0.99         | 1.98         | 4.95         | 9.90          | 19.79         | in.        |
| <b>Legend:</b>                                                                                       |             |             |             |              |              |              |               |               |            |
| <i>D = Distance to target in meters &amp; feet</i>                                                   |             |             |             |              |              |              |               |               |            |
| <i>HFOV = Horizontal field of view in meters &amp; feet</i>                                          |             |             |             |              |              |              |               |               |            |
| <i>VFOV = Vertical field of view in meters &amp; feet</i>                                            |             |             |             |              |              |              |               |               |            |
| <i>IFOV = Instantaneous field of view (size of one detector element) in millimeters &amp; inches</i> |             |             |             |              |              |              |               |               |            |

**Figure 14.9** Horizontal, vertical and instantaneous fields of view for certain distances to targets. **D** = distance to target. 9.2 mm IR lens. Applies to camera type 215 only.

10563703.a3

| <b>This table only applies to camera type number 215</b>                                             |             |             |             |              |              |              |               |               |            |
|------------------------------------------------------------------------------------------------------|-------------|-------------|-------------|--------------|--------------|--------------|---------------|---------------|------------|
| <i>The three-digit camera type number is the three first digits in the camera S/N.</i>               |             |             |             |              |              |              |               |               |            |
| <i>Focal length: 4.5 mm</i>                                                                          |             |             |             |              |              |              |               |               |            |
| <i>Resolution: 160 x 120 pixels</i>                                                                  |             |             |             |              |              |              |               |               |            |
| <i>Field of view in degrees: 78.8</i>                                                                |             |             |             |              |              |              |               |               |            |
| <b>D ---&gt;</b>                                                                                     | <b>0.50</b> | <b>1.00</b> | <b>2.00</b> | <b>5.00</b>  | <b>10.00</b> | <b>25.00</b> | <b>50.00</b>  | <b>100.00</b> | <b>m</b>   |
| HFOV                                                                                                 | 0.82        | 1.64        | 3.29        | 8.22         | 16.44        | 41.11        | 82.22         | 164.44        | m          |
| VFOV                                                                                                 | 0.62        | 1.23        | 2.47        | 6.17         | 12.33        | 30.83        | 61.67         | 123.33        | m          |
| IFOV                                                                                                 | 5.14        | 10.28       | 20.56       | 51.39        | 102.78       | 256.94       | 513.89        | 1 027.78      | mm         |
| <b>D ---&gt;</b>                                                                                     | <b>1.64</b> | <b>3.28</b> | <b>6.56</b> | <b>16.39</b> | <b>32.79</b> | <b>81.97</b> | <b>163.93</b> | <b>327.87</b> | <b>ft.</b> |
| HFOV                                                                                                 | 2.70        | 5.39        | 10.78       | 26.96        | 53.92        | 134.79       | 269.58        | 539.16        | ft.        |
| VFOV                                                                                                 | 2.02        | 4.04        | 8.09        | 20.22        | 40.44        | 101.09       | 202.19        | 404.37        | ft.        |
| IFOV                                                                                                 | 0.20        | 0.40        | 0.81        | 2.02         | 4.05         | 10.12        | 20.23         | 40.46         | in.        |
| <b>Legend:</b>                                                                                       |             |             |             |              |              |              |               |               |            |
| <i>D = Distance to target in meters &amp; feet</i>                                                   |             |             |             |              |              |              |               |               |            |
| <i>HFOV = Horizontal field of view in meters &amp; feet</i>                                          |             |             |             |              |              |              |               |               |            |
| <i>VFOV = Vertical field of view in meters &amp; feet</i>                                            |             |             |             |              |              |              |               |               |            |
| <i>IFOV = Instantaneous field of view (size of one detector element) in millimeters &amp; inches</i> |             |             |             |              |              |              |               |               |            |

**Figure 14.10** Horizontal, vertical and instantaneous fields of view for certain distances to targets. **D** = distance to target. 4.5 mm IR lens. Applies to camera type 215 only.

10564003.a3

**This table only applies to camera type number 243***The three-digit camera type number is the three first digits in the camera S/N.**Focal length: 87 mm**Resolution: 160 x 120 pixels**Field of view in degrees: 3.68*

| D ---> | 0.50 | 1.00 | 2.00 | 5.00  | 10.00 | 25.00 | 50.00  | 100.00 | m   |
|--------|------|------|------|-------|-------|-------|--------|--------|-----|
| HFOV   | 0.03 | 0.06 | 0.13 | 0.32  | 0.64  | 1.61  | 3.22   | 6.44   | m   |
| VFOV   | 0.02 | 0.05 | 0.10 | 0.24  | 0.48  | 1.21  | 2.41   | 4.83   | m   |
| IFOV   | 0.20 | 0.40 | 0.80 | 2.01  | 4.02  | 10.06 | 20.11  | 40.23  | mm  |
| D ---> | 1.64 | 3.28 | 6.56 | 16.39 | 32.79 | 81.97 | 163.93 | 327.87 | ft. |
| HFOV   | 0.11 | 0.21 | 0.42 | 1.06  | 2.11  | 5.28  | 10.55  | 21.10  | ft. |
| VFOV   | 0.08 | 0.16 | 0.32 | 0.79  | 1.58  | 3.96  | 7.91   | 15.83  | ft. |
| IFOV   | 0.01 | 0.02 | 0.03 | 0.08  | 0.16  | 0.40  | 0.79   | 1.58   | in. |

**Legend:***D = Distance to target in meters & feet**HFOV = Horizontal field of view in meters & feet**VFOV = Vertical field of view in meters & feet**IFOV = Instantaneous field of view (size of one detector element) in millimeters & inches***Figure 14.11** Horizontal, vertical and instantaneous fields of view for certain distances to targets. **D** = distance to target. 87 mm IR lens. Applies to camera type 243 only.

10564303.a3

| <b>This table only applies to camera type number 243</b>                                             |             |             |             |              |              |              |               |               |            |
|------------------------------------------------------------------------------------------------------|-------------|-------------|-------------|--------------|--------------|--------------|---------------|---------------|------------|
| <i>The three-digit camera type number is the three first digits in the camera S/N.</i>               |             |             |             |              |              |              |               |               |            |
| <i>Focal length: 54 mm</i>                                                                           |             |             |             |              |              |              |               |               |            |
| <i>Resolution: 160 x 120 pixels</i>                                                                  |             |             |             |              |              |              |               |               |            |
| <i>Field of view in degrees: 5.93</i>                                                                |             |             |             |              |              |              |               |               |            |
| <b>D ---&gt;</b>                                                                                     | <b>0.50</b> | <b>1.00</b> | <b>2.00</b> | <b>5.00</b>  | <b>10.00</b> | <b>25.00</b> | <b>50.00</b>  | <b>100.00</b> | <b>m</b>   |
| HFOV                                                                                                 | 0.05        | 0.10        | 0.21        | 0.52         | 1.04         | 2.59         | 5.19          | 10.37         | m          |
| VFOV                                                                                                 | 0.04        | 0.08        | 0.16        | 0.39         | 0.78         | 1.94         | 3.89          | 7.78          | m          |
| IFOV                                                                                                 | 0.32        | 0.65        | 1.30        | 3.24         | 6.48         | 16.20        | 32.41         | 64.81         | mm         |
| <b>D ---&gt;</b>                                                                                     | <b>1.64</b> | <b>3.28</b> | <b>6.56</b> | <b>16.39</b> | <b>32.79</b> | <b>81.97</b> | <b>163.93</b> | <b>327.87</b> | <b>ft.</b> |
| HFOV                                                                                                 | 0.17        | 0.34        | 0.68        | 1.70         | 3.40         | 8.50         | 17.00         | 34.00         | ft.        |
| VFOV                                                                                                 | 0.13        | 0.26        | 0.51        | 1.28         | 2.55         | 6.38         | 12.75         | 25.50         | ft.        |
| IFOV                                                                                                 | 0.01        | 0.03        | 0.05        | 0.13         | 0.26         | 0.64         | 1.28          | 2.55          | in.        |
| <b>Legend:</b>                                                                                       |             |             |             |              |              |              |               |               |            |
| <i>D = Distance to target in meters &amp; feet</i>                                                   |             |             |             |              |              |              |               |               |            |
| <i>HFOV = Horizontal field of view in meters &amp; feet</i>                                          |             |             |             |              |              |              |               |               |            |
| <i>VFOV = Vertical field of view in meters &amp; feet</i>                                            |             |             |             |              |              |              |               |               |            |
| <i>IFOV = Instantaneous field of view (size of one detector element) in millimeters &amp; inches</i> |             |             |             |              |              |              |               |               |            |

**Figure 14.12** Horizontal, vertical and instantaneous fields of view for certain distances to targets. **D** = distance to target. 54 mm IR lens. Applies to camera type 243 only.

10564603.a3

|                                                                                                      |      |      |      |       |       |       |        |        |     |
|------------------------------------------------------------------------------------------------------|------|------|------|-------|-------|-------|--------|--------|-----|
| <b>This table only applies to camera type number 243</b>                                             |      |      |      |       |       |       |        |        |     |
| <i>The three-digit camera type number is the three first digits in the camera S/N.</i>               |      |      |      |       |       |       |        |        |     |
| <i>Focal length: 36 mm</i>                                                                           |      |      |      |       |       |       |        |        |     |
| <i>Resolution: 160 x 120 pixels</i>                                                                  |      |      |      |       |       |       |        |        |     |
| <i>Field of view in degrees: 8.89</i>                                                                |      |      |      |       |       |       |        |        |     |
| D --->                                                                                               | 0.50 | 1.00 | 2.00 | 5.00  | 10.00 | 25.00 | 50.00  | 100.00 | m   |
| HFOV                                                                                                 | 0.08 | 0.16 | 0.31 | 0.78  | 1.56  | 3.89  | 7.78   | 15.56  | m   |
| VFOV                                                                                                 | 0.06 | 0.12 | 0.23 | 0.58  | 1.17  | 2.92  | 5.83   | 11.67  | m   |
| IFOV                                                                                                 | 0.49 | 0.97 | 1.94 | 4.86  | 9.72  | 24.31 | 48.61  | 97.22  | mm  |
| D --->                                                                                               | 1.64 | 3.28 | 6.56 | 16.39 | 32.79 | 81.97 | 163.93 | 327.87 | ft. |
| HFOV                                                                                                 | 0.26 | 0.51 | 1.02 | 2.55  | 5.10  | 12.75 | 25.50  | 51.00  | ft. |
| VFOV                                                                                                 | 0.19 | 0.38 | 0.77 | 1.91  | 3.83  | 9.56  | 19.13  | 38.25  | ft. |
| IFOV                                                                                                 | 0.02 | 0.04 | 0.08 | 0.19  | 0.38  | 0.96  | 1.91   | 3.83   | in. |
| <b>Legend:</b>                                                                                       |      |      |      |       |       |       |        |        |     |
| <i>D = Distance to target in meters &amp; feet</i>                                                   |      |      |      |       |       |       |        |        |     |
| <i>HFOV = Horizontal field of view in meters &amp; feet</i>                                          |      |      |      |       |       |       |        |        |     |
| <i>VFOV = Vertical field of view in meters &amp; feet</i>                                            |      |      |      |       |       |       |        |        |     |
| <i>IFOV = Instantaneous field of view (size of one detector element) in millimeters &amp; inches</i> |      |      |      |       |       |       |        |        |     |

**Figure 14.13** Horizontal, vertical and instantaneous fields of view for certain distances to targets. **D** = distance to target. 36 mm IR lens. Applies to camera type 243 only.

10564903.a3

|                                                                                                      |             |             |             |              |              |              |               |               |            |
|------------------------------------------------------------------------------------------------------|-------------|-------------|-------------|--------------|--------------|--------------|---------------|---------------|------------|
| <b>This table only applies to camera type number 243</b>                                             |             |             |             |              |              |              |               |               |            |
| <i>The three-digit camera type number is the three first digits in the camera S/N.</i>               |             |             |             |              |              |              |               |               |            |
| <i>Focal length: 17 mm</i>                                                                           |             |             |             |              |              |              |               |               |            |
| <i>Resolution: 160 x 120 pixels</i>                                                                  |             |             |             |              |              |              |               |               |            |
| <i>Field of view in degrees: 18.7</i>                                                                |             |             |             |              |              |              |               |               |            |
| <b>D ---&gt;</b>                                                                                     | <b>0.50</b> | <b>1.00</b> | <b>2.00</b> | <b>5.00</b>  | <b>10.00</b> | <b>25.00</b> | <b>50.00</b>  | <b>100.00</b> | <b>m</b>   |
| HFOV                                                                                                 | 0.16        | 0.33        | 0.66        | 1.65         | 3.29         | 8.24         | 16.47         | 32.94         | m          |
| VFOV                                                                                                 | 0.12        | 0.25        | 0.49        | 1.24         | 2.47         | 6.18         | 12.35         | 24.71         | m          |
| IFOV                                                                                                 | 1.03        | 2.06        | 4.12        | 10.29        | 20.59        | 51.47        | 102.94        | 205.88        | mm         |
| <b>D ---&gt;</b>                                                                                     | <b>1.64</b> | <b>3.28</b> | <b>6.56</b> | <b>16.39</b> | <b>32.79</b> | <b>81.97</b> | <b>163.93</b> | <b>327.87</b> | <b>ft.</b> |
| HFOV                                                                                                 | 0.54        | 1.08        | 2.16        | 5.40         | 10.80        | 27.00        | 54.00         | 108.00        | ft.        |
| VFOV                                                                                                 | 0.41        | 0.81        | 1.62        | 4.05         | 8.10         | 20.25        | 40.50         | 81.00         | ft.        |
| IFOV                                                                                                 | 0.04        | 0.08        | 0.16        | 0.41         | 0.81         | 2.03         | 4.05          | 8.11          | in.        |
| <b>Legend:</b>                                                                                       |             |             |             |              |              |              |               |               |            |
| <i>D = Distance to target in meters &amp; feet</i>                                                   |             |             |             |              |              |              |               |               |            |
| <i>HFOV = Horizontal field of view in meters &amp; feet</i>                                          |             |             |             |              |              |              |               |               |            |
| <i>VFOV = Vertical field of view in meters &amp; feet</i>                                            |             |             |             |              |              |              |               |               |            |
| <i>IFOV = Instantaneous field of view (size of one detector element) in millimeters &amp; inches</i> |             |             |             |              |              |              |               |               |            |

**Figure 14.14** Horizontal, vertical and instantaneous fields of view for certain distances to targets. **D** = distance to target. 17 mm IR lens. Applies to camera type 243 only.

10565203.a3

**This table only applies to camera type number 243**

The three-digit camera type number is the three first digits in the camera S/N.

Focal length: 9.2 mm

Resolution: 160 x 120 pixels

Field of view in degrees: 33.8

| D ---> | 0.50 | 1.00 | 2.00 | 5.00  | 10.00 | 25.00 | 50.00  | 100.00 | m   |
|--------|------|------|------|-------|-------|-------|--------|--------|-----|
| HFOV   | 0.30 | 0.61 | 1.22 | 3.04  | 6.09  | 15.22 | 30.43  | 60.87  | m   |
| VFOV   | 0.23 | 0.46 | 0.91 | 2.28  | 4.57  | 11.41 | 22.83  | 45.65  | m   |
| IFOV   | 1.90 | 3.80 | 7.61 | 19.02 | 38.04 | 95.11 | 190.22 | 380.43 | mm  |
| D ---> | 1.64 | 3.28 | 6.56 | 16.39 | 32.79 | 81.97 | 163.93 | 327.87 | ft. |
| HFOV   | 1.00 | 2.00 | 3.99 | 9.98  | 19.96 | 49.89 | 99.79  | 199.57 | ft. |
| VFOV   | 0.75 | 1.50 | 2.99 | 7.48  | 14.97 | 37.42 | 74.84  | 149.68 | ft. |
| IFOV   | 0.07 | 0.15 | 0.30 | 0.75  | 1.50  | 3.74  | 7.49   | 14.98  | in. |

**Legend:***D = Distance to target in meters & feet**HFOV = Horizontal field of view in meters & feet**VFOV = Vertical field of view in meters & feet**IFOV = Instantaneous field of view (size of one detector element) in millimeters & inches***Figure 14.15** Horizontal, vertical and instantaneous fields of view for certain distances to targets. **D** = distance to target. 9.2 mm IR lens. Applies to camera type 243 only.

10563803.a3

|                                                                                           |      |      |       |       |       |        |        |        |     |
|-------------------------------------------------------------------------------------------|------|------|-------|-------|-------|--------|--------|--------|-----|
| <b>This table only applies to camera type number 243</b>                                  |      |      |       |       |       |        |        |        |     |
| The three-digit camera type number is the three first digits in the camera S/N.           |      |      |       |       |       |        |        |        |     |
| Focal length: 4.5 mm                                                                      |      |      |       |       |       |        |        |        |     |
| Resolution: 160 x 120 pixels                                                              |      |      |       |       |       |        |        |        |     |
| Field of view in degrees: 63.7                                                            |      |      |       |       |       |        |        |        |     |
| D --->                                                                                    | 0.50 | 1.00 | 2.00  | 5.00  | 10.00 | 25.00  | 50.00  | 100.00 | m   |
| HFOV                                                                                      | 0.62 | 1.24 | 2.49  | 6.22  | 12.44 | 31.11  | 62.22  | 124.44 | m   |
| VFOV                                                                                      | 0.47 | 0.93 | 1.87  | 4.67  | 9.33  | 23.33  | 46.67  | 93.33  | m   |
| IFOV                                                                                      | 3.89 | 7.78 | 15.56 | 38.89 | 77.78 | 194.44 | 388.89 | 777.78 | mm  |
| D --->                                                                                    | 1.64 | 3.28 | 6.56  | 16.39 | 32.79 | 81.97  | 163.93 | 327.87 | ft. |
| HFOV                                                                                      | 2.04 | 4.08 | 8.16  | 20.40 | 40.80 | 102.00 | 204.01 | 408.01 | ft. |
| VFOV                                                                                      | 1.53 | 3.06 | 6.12  | 15.30 | 30.60 | 76.50  | 153.01 | 306.01 | ft. |
| IFOV                                                                                      | 0.15 | 0.31 | 0.61  | 1.53  | 3.06  | 7.66   | 15.31  | 30.62  | in. |
| <b>Legend:</b>                                                                            |      |      |       |       |       |        |        |        |     |
| D = Distance to target in meters & feet                                                   |      |      |       |       |       |        |        |        |     |
| HFOV = Horizontal field of view in meters & feet                                          |      |      |       |       |       |        |        |        |     |
| VFOV = Vertical field of view in meters & feet                                            |      |      |       |       |       |        |        |        |     |
| IFOV = Instantaneous field of view (size of one detector element) in millimeters & inches |      |      |       |       |       |        |        |        |     |

**Figure 14.16** Horizontal, vertical and instantaneous fields of view for certain distances to targets. **D** = distance to target. 4.5 mm IR lens. Applies to camera type 243 only.

10564103.a3

|                                                                                           |      |      |      |       |       |       |        |        |     |
|-------------------------------------------------------------------------------------------|------|------|------|-------|-------|-------|--------|--------|-----|
| <b>This table only applies to camera type number 247</b>                                  |      |      |      |       |       |       |        |        |     |
| The three-digit camera type number is the three first digits in the camera S/N.           |      |      |      |       |       |       |        |        |     |
| Focal length: 87 mm                                                                       |      |      |      |       |       |       |        |        |     |
| Resolution: 160 x 120 pixels                                                              |      |      |      |       |       |       |        |        |     |
| Field of view in degrees: 4.00                                                            |      |      |      |       |       |       |        |        |     |
| D --->                                                                                    | 0.50 | 1.00 | 2.00 | 5.00  | 10.00 | 25.00 | 50.00  | 100.00 | m   |
| HFOV                                                                                      | 0.03 | 0.07 | 0.14 | 0.35  | 0.70  | 1.75  | 3.49   | 6.99   | m   |
| VFOV                                                                                      | 0.03 | 0.05 | 0.10 | 0.26  | 0.52  | 1.31  | 2.62   | 5.24   | m   |
| IFOV                                                                                      | 0.22 | 0.44 | 0.87 | 2.18  | 4.37  | 10.92 | 21.84  | 43.68  | mm  |
| D --->                                                                                    | 1.64 | 3.28 | 6.56 | 16.39 | 32.79 | 81.97 | 163.93 | 327.87 | ft. |
| HFOV                                                                                      | 0.11 | 0.23 | 0.46 | 1.15  | 2.29  | 5.73  | 11.46  | 22.91  | ft. |
| VFOV                                                                                      | 0.09 | 0.17 | 0.34 | 0.86  | 1.72  | 4.30  | 8.59   | 17.18  | ft. |
| IFOV                                                                                      | 0.01 | 0.02 | 0.03 | 0.09  | 0.17  | 0.43  | 0.86   | 1.72   | in. |
| <b>Legend:</b>                                                                            |      |      |      |       |       |       |        |        |     |
| D = Distance to target in meters & feet                                                   |      |      |      |       |       |       |        |        |     |
| HFOV = Horizontal field of view in meters & feet                                          |      |      |      |       |       |       |        |        |     |
| VFOV = Vertical field of view in meters & feet                                            |      |      |      |       |       |       |        |        |     |
| IFOV = Instantaneous field of view (size of one detector element) in millimeters & inches |      |      |      |       |       |       |        |        |     |

**Figure 14.17** Horizontal, vertical and instantaneous fields of view for certain distances to targets. **D** = distance to target. 87 mm IR lens. Applies to camera type 247 only.

10564403.a3

|                                                                                           |      |      |      |       |       |       |        |        |     |
|-------------------------------------------------------------------------------------------|------|------|------|-------|-------|-------|--------|--------|-----|
| <b>This table only applies to camera type number 247</b>                                  |      |      |      |       |       |       |        |        |     |
| The three-digit camera type number is the three first digits in the camera S/N.           |      |      |      |       |       |       |        |        |     |
| Focal length: 54 mm                                                                       |      |      |      |       |       |       |        |        |     |
| Resolution: 160 x 120 pixels                                                              |      |      |      |       |       |       |        |        |     |
| Field of view in degrees: 6.44                                                            |      |      |      |       |       |       |        |        |     |
| D --->                                                                                    | 0.50 | 1.00 | 2.00 | 5.00  | 10.00 | 25.00 | 50.00  | 100.00 | m   |
| HFOV                                                                                      | 0.06 | 0.11 | 0.23 | 0.56  | 1.13  | 2.81  | 5.63   | 11.26  | m   |
| VFOV                                                                                      | 0.04 | 0.08 | 0.17 | 0.42  | 0.84  | 2.11  | 4.22   | 8.44   | m   |
| IFOV                                                                                      | 0.35 | 0.70 | 1.41 | 3.52  | 7.04  | 17.59 | 35.19  | 70.37  | mm  |
| D --->                                                                                    | 1.64 | 3.28 | 6.56 | 16.39 | 32.79 | 81.97 | 163.93 | 327.87 | ft. |
| HFOV                                                                                      | 0.18 | 0.37 | 0.74 | 1.85  | 3.69  | 9.23  | 18.46  | 36.92  | ft. |
| VFOV                                                                                      | 0.14 | 0.28 | 0.55 | 1.38  | 2.77  | 6.92  | 13.84  | 27.69  | ft. |
| IFOV                                                                                      | 0.01 | 0.03 | 0.06 | 0.14  | 0.28  | 0.69  | 1.39   | 2.77   | in. |
| <b>Legend:</b>                                                                            |      |      |      |       |       |       |        |        |     |
| D = Distance to target in meters & feet                                                   |      |      |      |       |       |       |        |        |     |
| HFOV = Horizontal field of view in meters & feet                                          |      |      |      |       |       |       |        |        |     |
| VFOV = Vertical field of view in meters & feet                                            |      |      |      |       |       |       |        |        |     |
| IFOV = Instantaneous field of view (size of one detector element) in millimeters & inches |      |      |      |       |       |       |        |        |     |

**Figure 14.18** Horizontal, vertical and instantaneous fields of view for certain distances to targets. **D** = distance to target. 54 mm IR lens. Applies to camera type 247 only.

10564703.a3

|                                                                                                      |             |             |             |              |              |              |               |               |            |
|------------------------------------------------------------------------------------------------------|-------------|-------------|-------------|--------------|--------------|--------------|---------------|---------------|------------|
| <b>This table only applies to camera type number 247</b>                                             |             |             |             |              |              |              |               |               |            |
| <i>The three-digit camera type number is the three first digits in the camera S/N.</i>               |             |             |             |              |              |              |               |               |            |
| <i>Focal length: 36 mm</i>                                                                           |             |             |             |              |              |              |               |               |            |
| <i>Resolution: 160 x 120 pixels</i>                                                                  |             |             |             |              |              |              |               |               |            |
| <i>Field of view in degrees: 9.65</i>                                                                |             |             |             |              |              |              |               |               |            |
| <b>D ---&gt;</b>                                                                                     | <b>0.50</b> | <b>1.00</b> | <b>2.00</b> | <b>5.00</b>  | <b>10.00</b> | <b>25.00</b> | <b>50.00</b>  | <b>100.00</b> | <b>m</b>   |
| HFOV                                                                                                 | 0.08        | 0.17        | 0.34        | 0.84         | 1.69         | 4.22         | 8.44          | 16.89         | m          |
| VFOV                                                                                                 | 0.06        | 0.13        | 0.25        | 0.63         | 1.27         | 3.17         | 6.33          | 12.67         | m          |
| IFOV                                                                                                 | 0.53        | 1.06        | 2.11        | 5.28         | 10.56        | 26.39        | 52.78         | 105.56        | mm         |
| <b>D ---&gt;</b>                                                                                     | <b>1.64</b> | <b>3.28</b> | <b>6.56</b> | <b>16.39</b> | <b>32.79</b> | <b>81.97</b> | <b>163.93</b> | <b>327.87</b> | <b>ft.</b> |
| HFOV                                                                                                 | 0.28        | 0.55        | 1.11        | 2.77         | 5.54         | 13.84        | 27.69         | 55.37         | ft.        |
| VFOV                                                                                                 | 0.21        | 0.42        | 0.83        | 2.08         | 4.15         | 10.38        | 20.77         | 41.53         | ft.        |
| IFOV                                                                                                 | 0.02        | 0.04        | 0.08        | 0.21         | 0.42         | 1.04         | 2.08          | 4.16          | in.        |
| <b>Legend:</b>                                                                                       |             |             |             |              |              |              |               |               |            |
| <i>D = Distance to target in meters &amp; feet</i>                                                   |             |             |             |              |              |              |               |               |            |
| <i>HFOV = Horizontal field of view in meters &amp; feet</i>                                          |             |             |             |              |              |              |               |               |            |
| <i>VFOV = Vertical field of view in meters &amp; feet</i>                                            |             |             |             |              |              |              |               |               |            |
| <i>IFOV = Instantaneous field of view (size of one detector element) in millimeters &amp; inches</i> |             |             |             |              |              |              |               |               |            |

**Figure 14.19** Horizontal, vertical and instantaneous fields of view for certain distances to targets. **D** = distance to target. 36 mm IR lens. Applies to camera type 247 only.

10565003.a3

|                                                                                           |      |      |      |       |       |       |        |        |     |
|-------------------------------------------------------------------------------------------|------|------|------|-------|-------|-------|--------|--------|-----|
| <b>This table only applies to camera type number 247</b>                                  |      |      |      |       |       |       |        |        |     |
| The three-digit camera type number is the three first digits in the camera S/N.           |      |      |      |       |       |       |        |        |     |
| Focal length: 17 mm                                                                       |      |      |      |       |       |       |        |        |     |
| Resolution: 160 x 120 pixels                                                              |      |      |      |       |       |       |        |        |     |
| Field of view in degrees: 20.2                                                            |      |      |      |       |       |       |        |        |     |
| D --->                                                                                    | 0.50 | 1.00 | 2.00 | 5.00  | 10.00 | 25.00 | 50.00  | 100.00 | m   |
| HFOV                                                                                      | 0.18 | 0.36 | 0.72 | 1.79  | 3.58  | 8.94  | 17.88  | 35.76  | m   |
| VFOV                                                                                      | 0.13 | 0.27 | 0.54 | 1.34  | 2.68  | 6.71  | 13.41  | 26.82  | m   |
| IFOV                                                                                      | 1.12 | 2.24 | 4.47 | 11.18 | 22.35 | 55.88 | 111.76 | 223.53 | mm  |
| D --->                                                                                    | 1.64 | 3.28 | 6.56 | 16.39 | 32.79 | 81.97 | 163.93 | 327.87 | ft. |
| HFOV                                                                                      | 0.59 | 1.17 | 2.35 | 5.86  | 11.73 | 29.32 | 58.63  | 117.26 | ft. |
| VFOV                                                                                      | 0.44 | 0.88 | 1.76 | 4.40  | 8.79  | 21.99 | 43.97  | 87.95  | ft. |
| IFOV                                                                                      | 0.04 | 0.09 | 0.18 | 0.44  | 0.88  | 2.20  | 4.40   | 8.80   | in. |
| <b>Legend:</b>                                                                            |      |      |      |       |       |       |        |        |     |
| D = Distance to target in meters & feet                                                   |      |      |      |       |       |       |        |        |     |
| HFOV = Horizontal field of view in meters & feet                                          |      |      |      |       |       |       |        |        |     |
| VFOV = Vertical field of view in meters & feet                                            |      |      |      |       |       |       |        |        |     |
| IFOV = Instantaneous field of view (size of one detector element) in millimeters & inches |      |      |      |       |       |       |        |        |     |

**Figure 14.20** Horizontal, vertical and instantaneous fields of view for certain distances to targets. **D** = distance to target. 17 mm IR lens. Applies to camera type 247 only.

10563603.a3

|                                                                                           |      |      |      |       |       |        |        |        |     |
|-------------------------------------------------------------------------------------------|------|------|------|-------|-------|--------|--------|--------|-----|
| <b>This table only applies to camera type number 247</b>                                  |      |      |      |       |       |        |        |        |     |
| The three-digit camera type number is the three first digits in the camera S/N.           |      |      |      |       |       |        |        |        |     |
| Focal length: 9.2 mm                                                                      |      |      |      |       |       |        |        |        |     |
| Resolution: 160 x 120 pixels                                                              |      |      |      |       |       |        |        |        |     |
| Field of view in degrees: 36.5                                                            |      |      |      |       |       |        |        |        |     |
| D --->                                                                                    | 0.50 | 1.00 | 2.00 | 5.00  | 10.00 | 25.00  | 50.00  | 100.00 | m   |
| HFOV                                                                                      | 0.33 | 0.66 | 1.32 | 3.30  | 6.61  | 16.52  | 33.04  | 66.09  | m   |
| VFOV                                                                                      | 0.25 | 0.50 | 0.99 | 2.48  | 4.96  | 12.39  | 24.78  | 49.57  | m   |
| IFOV                                                                                      | 2.07 | 4.13 | 8.26 | 20.65 | 41.30 | 103.26 | 206.52 | 413.04 | mm  |
| D --->                                                                                    | 1.64 | 3.28 | 6.56 | 16.39 | 32.79 | 81.97  | 163.93 | 327.87 | ft. |
| HFOV                                                                                      | 1.08 | 2.17 | 4.33 | 10.83 | 21.67 | 54.17  | 108.34 | 216.68 | ft. |
| VFOV                                                                                      | 0.81 | 1.63 | 3.25 | 8.13  | 16.25 | 40.63  | 81.25  | 162.51 | ft. |
| IFOV                                                                                      | 0.08 | 0.16 | 0.33 | 0.81  | 1.63  | 4.07   | 8.13   | 16.26  | in. |
| <b>Legend:</b>                                                                            |      |      |      |       |       |        |        |        |     |
| D = Distance to target in meters & feet                                                   |      |      |      |       |       |        |        |        |     |
| HFOV = Horizontal field of view in meters & feet                                          |      |      |      |       |       |        |        |        |     |
| VFOV = Vertical field of view in meters & feet                                            |      |      |      |       |       |        |        |        |     |
| IFOV = Instantaneous field of view (size of one detector element) in millimeters & inches |      |      |      |       |       |        |        |        |     |

**Figure 14.21** Horizontal, vertical and instantaneous fields of view for certain distances to targets. **D** = distance to target. 9.2 mm IR lens. Applies to camera type 247 only.

10563903.a3

|                                                                                                      |             |             |             |              |              |              |               |               |            |
|------------------------------------------------------------------------------------------------------|-------------|-------------|-------------|--------------|--------------|--------------|---------------|---------------|------------|
| <b>This table only applies to camera type number 247</b>                                             |             |             |             |              |              |              |               |               |            |
| <i>The three-digit camera type number is the three first digits in the camera S/N.</i>               |             |             |             |              |              |              |               |               |            |
| <i>Focal length: 4.5 mm</i>                                                                          |             |             |             |              |              |              |               |               |            |
| <i>Resolution: 160 x 120 pixels</i>                                                                  |             |             |             |              |              |              |               |               |            |
| <i>Field of view in degrees: 68.0</i>                                                                |             |             |             |              |              |              |               |               |            |
| <b>D ---&gt;</b>                                                                                     | <b>0.50</b> | <b>1.00</b> | <b>2.00</b> | <b>5.00</b>  | <b>10.00</b> | <b>25.00</b> | <b>50.00</b>  | <b>100.00</b> | <b>m</b>   |
| HFOV                                                                                                 | 0.68        | 1.35        | 2.70        | 6.76         | 13.51        | 33.78        | 67.56         | 135.11        | m          |
| VFOV                                                                                                 | 0.51        | 1.01        | 2.03        | 5.07         | 10.13        | 25.33        | 50.67         | 101.33        | m          |
| IFOV                                                                                                 | 4.22        | 8.44        | 16.89       | 42.22        | 84.44        | 211.11       | 422.22        | 844.44        | mm         |
| <b>D ---&gt;</b>                                                                                     | <b>1.64</b> | <b>3.28</b> | <b>6.56</b> | <b>16.39</b> | <b>32.79</b> | <b>81.97</b> | <b>163.93</b> | <b>327.87</b> | <b>ft.</b> |
| HFOV                                                                                                 | 2.21        | 4.43        | 8.86        | 22.15        | 44.30        | 110.75       | 221.49        | 442.99        | ft.        |
| VFOV                                                                                                 | 1.66        | 3.32        | 6.64        | 16.61        | 33.22        | 83.06        | 166.12        | 332.24        | ft.        |
| IFOV                                                                                                 | 0.17        | 0.33        | 0.66        | 1.66         | 3.32         | 8.31         | 16.62         | 33.25         | in.        |
| <b>Legend:</b>                                                                                       |             |             |             |              |              |              |               |               |            |
| <i>D = Distance to target in meters &amp; feet</i>                                                   |             |             |             |              |              |              |               |               |            |
| <i>HFOV = Horizontal field of view in meters &amp; feet</i>                                          |             |             |             |              |              |              |               |               |            |
| <i>VFOV = Vertical field of view in meters &amp; feet</i>                                            |             |             |             |              |              |              |               |               |            |
| <i>IFOV = Instantaneous field of view (size of one detector element) in millimeters &amp; inches</i> |             |             |             |              |              |              |               |               |            |


**Figure 14.22** Horizontal, vertical and instantaneous fields of view for certain distances to targets. **D** = distance to target. 4.5 mm IR lens. Applies to camera type 247 only.

**Figure 14.23** F-number and close focus limits for various lenses

| <b>IR lens →</b>        | <b>36 mm</b> | <b>17 mm</b> | <b>9.2 mm</b> |
|-------------------------|--------------|--------------|---------------|
| Close focus limit (m)   | 0.70         | 0.30         | 0.01          |
| Close focus limit (ft.) | 2.30         | 0.98         | 0.03          |
| f-number                | 1.2          | 1.2          | 1.2           |


## 14.10 Camera – dimensional drawings

10384503.a4

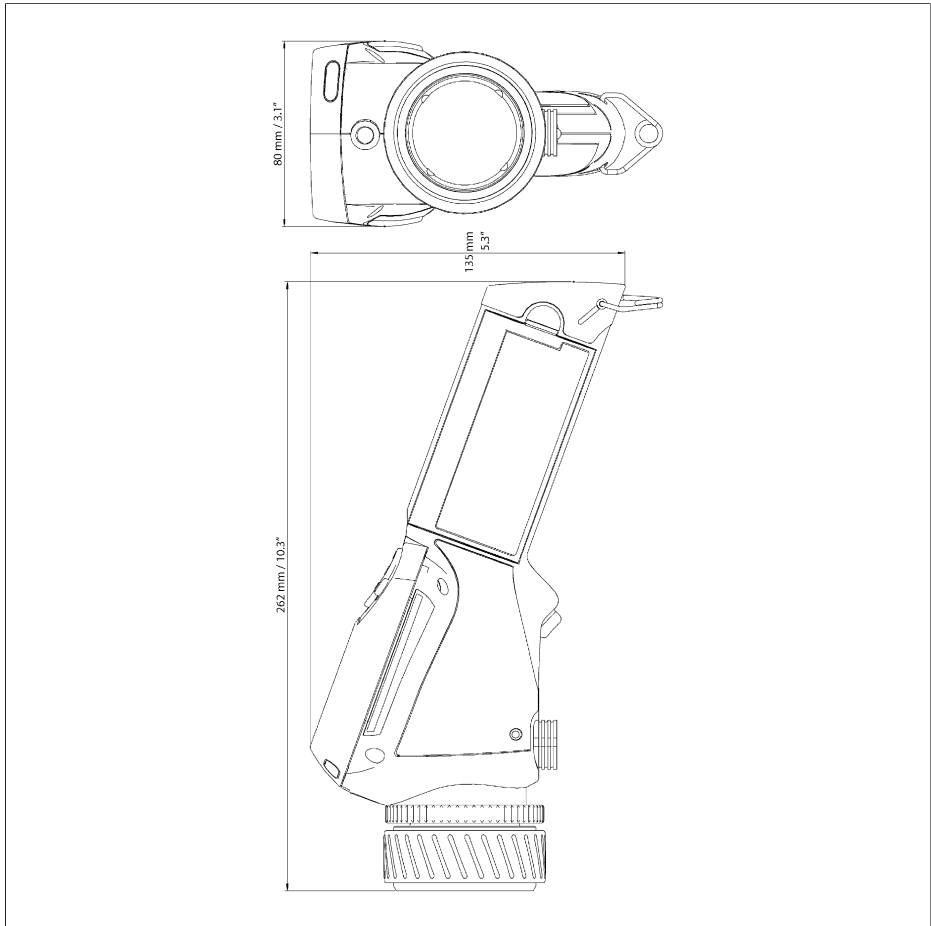


**Figure 14.24** Overall dimensions of the camera with a 36 mm IR lens.

10384603.a4

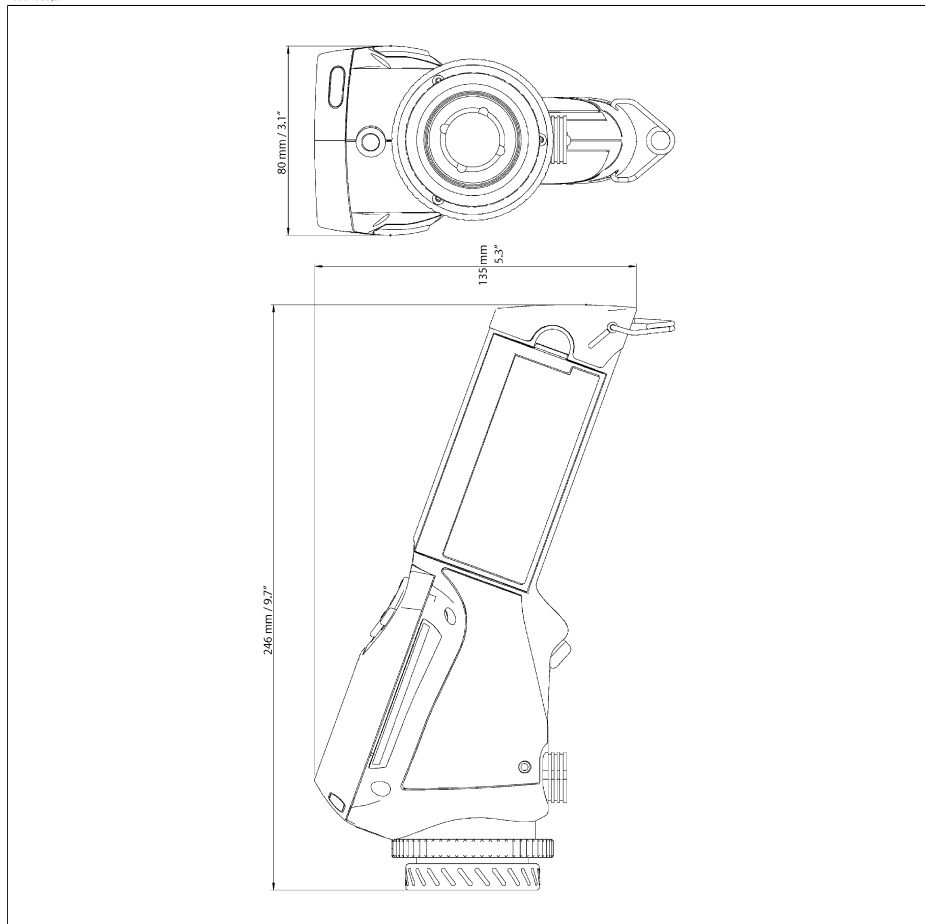


**Figure 14.25** Overall dimensions of the camera with a 17 mm IR lens.

10384703.a4

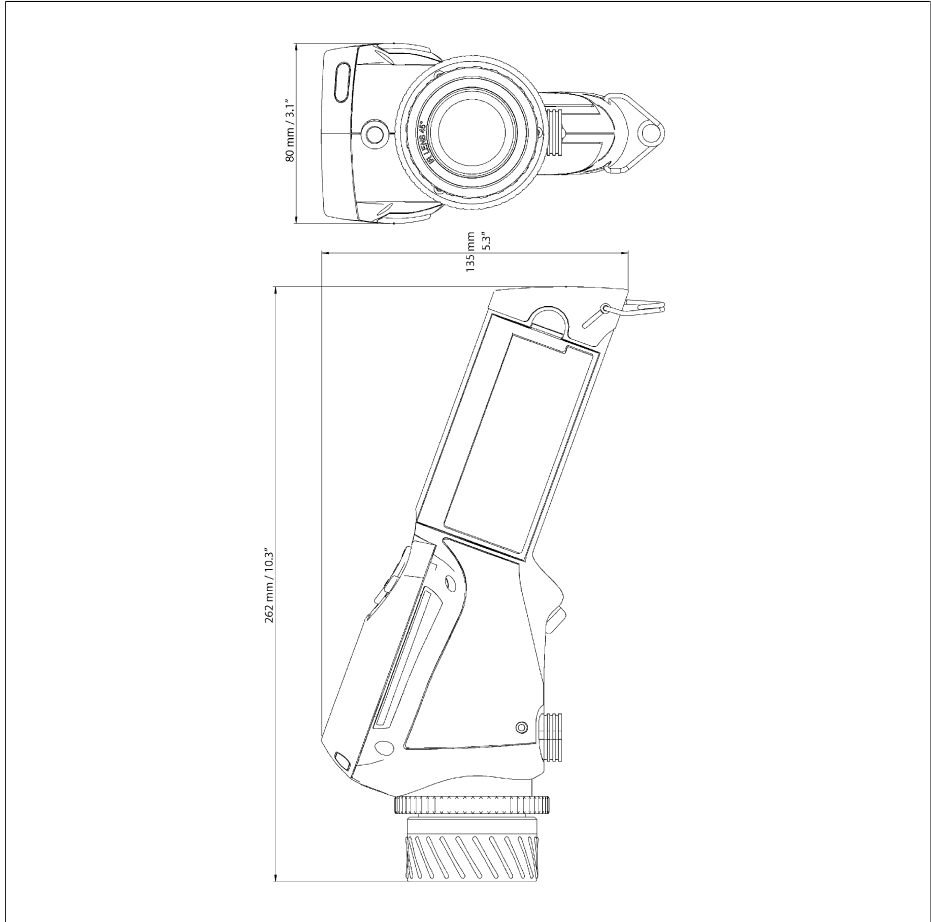

**Figure 14.26** Overall dimensions of the camera with a 9.2 mm IR lens.


14.11      *Battery charger – dimensional drawing*

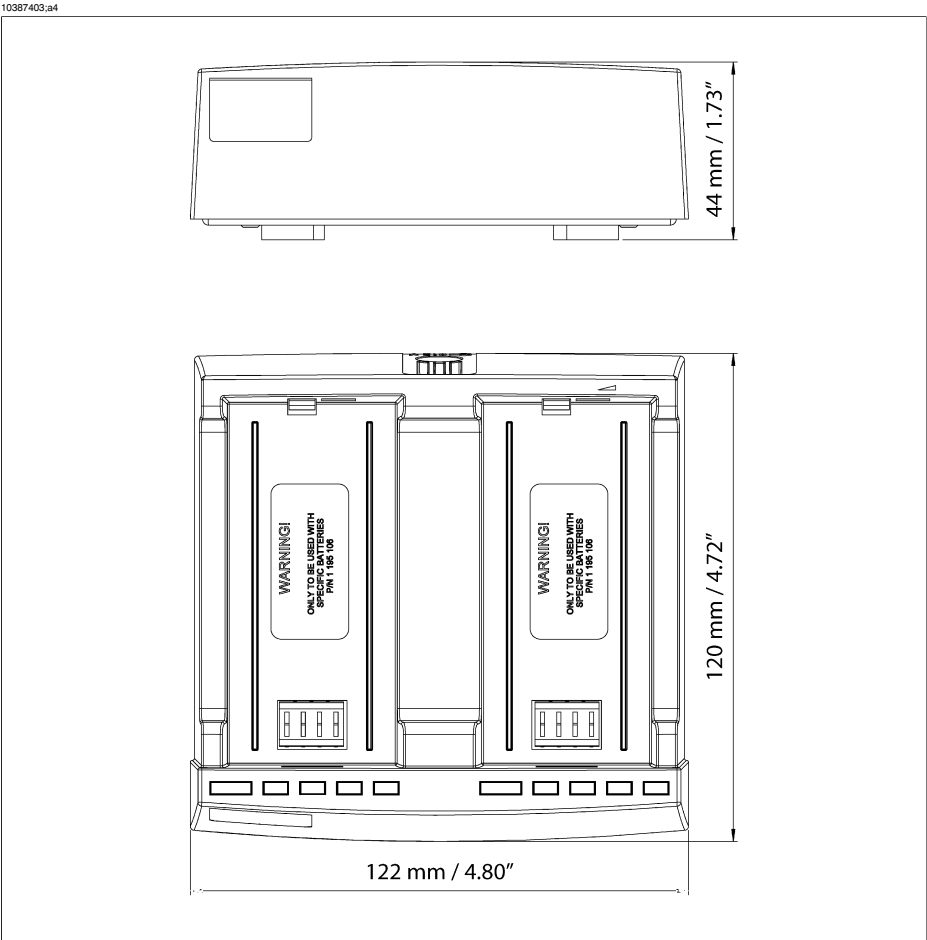

**Figure 14.27** Overall dimensions of the battery charger

## 14.12 Battery – dimensional drawing

10387503.a4

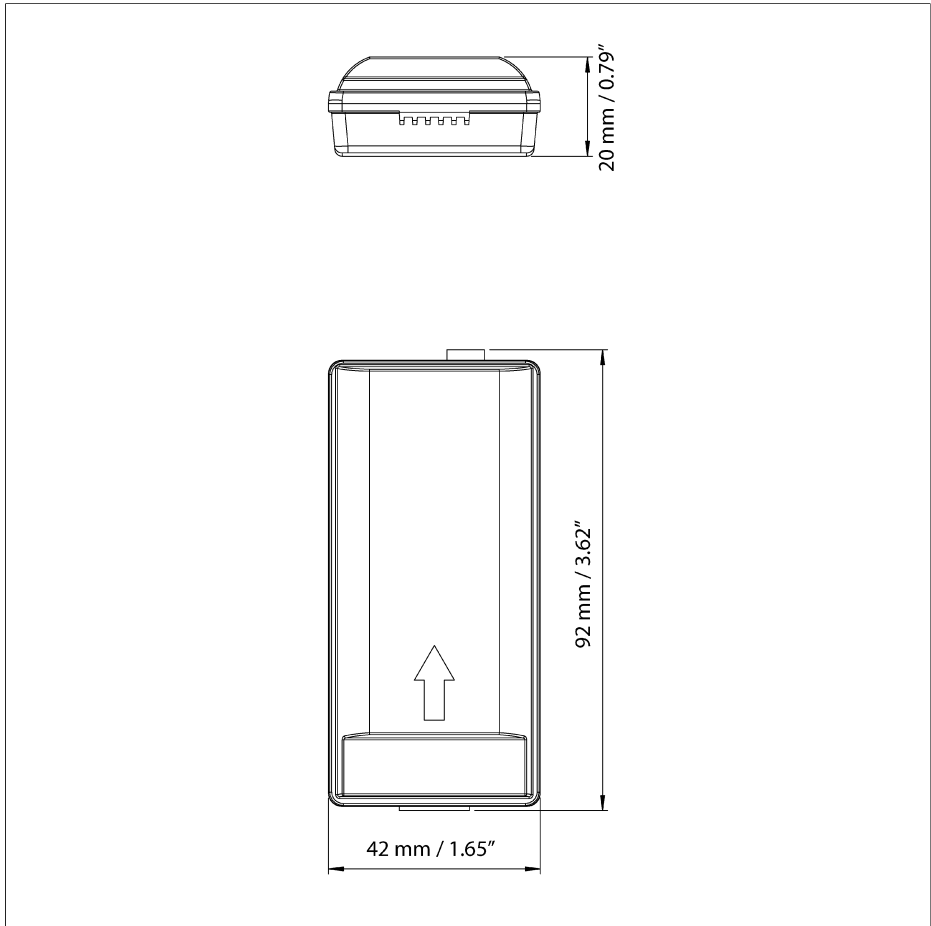

**Figure 14.28** Overall dimensions of the battery

INTENTIONALLY LEFT BLANK

# 15 Glossary

| Term or expression                  | Explanation                                                                                                                                        |
|-------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------|
| absorption (absorption factor)      | The amount of radiation absorbed by an object relative to the received radiation. A number between 0 and 1.                                        |
| ambient                             | Objects and gases that emit radiation towards the object being measured.                                                                           |
| atmosphere                          | The gases between the object being measured and the camera, normally air.                                                                          |
| autoadjust                          | A function making a camera perform an internal image correction.                                                                                   |
| autopalette                         | The IR image is shown with an uneven spread of colors, displaying cold objects as well as hot ones at the same time.                               |
| blackbody                           | Totally non-reflective object. All its radiation is due to its own temperature.                                                                    |
| blackbody radiator                  | An IR radiating equipment with blackbody properties used to calibrate IR cameras.                                                                  |
| calculated atmospheric transmission | A transmission value computed from the temperature, the relative humidity of air and the distance to the object.                                   |
| cavity radiator                     | A bottle shaped radiator with an absorbing inside, viewed through the bottleneck.                                                                  |
| color temperature                   | The temperature for which the color of a blackbody matches a specific color.                                                                       |
| conduction                          | The process that makes heat spread into a material.                                                                                                |
| continuous adjust                   | A function that adjusts the image. The function works all the time, continuously adjusting brightness and contrast according to the image content. |
| convection                          | The process that makes hot air or liquid rise.                                                                                                     |
| difference temperature              | A value which is the result of a subtraction between two temperature values.                                                                       |
| dual isotherm                       | An isotherm with two color bands, instead of one.                                                                                                  |

| Term or expression                      | Explanation                                                                                                                                                                |
|-----------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| emissivity (emissivity factor)          | The amount of radiation coming from an object, compared to that of a blackbody. A number between 0 and 1.                                                                  |
| emittance                               | Amount of energy emitted from an object per unit of time and area (W/m <sup>2</sup> )                                                                                      |
| estimated atmospheric transmission      | A transmission value, supplied by a user, replacing a calculated one                                                                                                       |
| external optics                         | Extra lenses, filters, heat shields etc. that can be put between the camera and the object being measured.                                                                 |
| filter                                  | A material transparent only to some of the infrared wavelengths.                                                                                                           |
| FOV                                     | Field of view: The horizontal angle that can be viewed through an IR lens.                                                                                                 |
| FPA                                     | Focal plane array: A type of IR detector.                                                                                                                                  |
| graybody                                | An object that emits a fixed fraction of the amount of energy of a blackbody for each wavelength.                                                                          |
| IFOV                                    | Instantaneous field of view: A measure of the geometrical resolution of an IR camera.                                                                                      |
| image correction (internal or external) | A way of compensating for sensitivity differences in various parts of live images and also of stabilizing the camera.                                                      |
| infrared                                | Non-visible radiation, having a wavelength from about 2–13 µm.                                                                                                             |
| IR                                      | infrared                                                                                                                                                                   |
| isotherm                                | A function highlighting those parts of an image that fall above, below or between one or more temperature intervals.                                                       |
| isothermal cavity                       | A bottle-shaped radiator with a uniform temperature viewed through the bottleneck.                                                                                         |
| Laser LocatIR                           | An electrically powered light source on the camera that emits laser radiation in a thin, concentrated beam to point at certain parts of the object in front of the camera. |
| laser pointer                           | An electrically powered light source on the camera that emits laser radiation in a thin, concentrated beam to point at certain parts of the object in front of the camera. |

| Term or expression    | Explanation                                                                                                                                                                          |
|-----------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| level                 | The center value of the temperature scale, usually expressed as a signal value.                                                                                                      |
| manual adjust         | A way to adjust the image by manually changing certain parameters.                                                                                                                   |
| NETD                  | Noise equivalent temperature difference. A measure of the image noise level of an IR camera.                                                                                         |
| noise                 | Undesired small disturbance in the infrared image                                                                                                                                    |
| object parameters     | A set of values describing the circumstances under which the measurement of an object was made, and the object itself. (such as emissivity, ambient temperature, distance etc.)      |
| object signal         | A non-calibrated value related to the amount of radiation received by the camera from the object.                                                                                    |
| palette               | The set of colors used to display an IR image.                                                                                                                                       |
| pixel                 | Stands for <i>picture element</i> . One single spot in an image.                                                                                                                     |
| radiance              | Amount of energy emitted from an object per unit of time, area and angle ( $W/m^2/sr$ )                                                                                              |
| radiant power         | Amount of energy emitted from an object per unit of time (W)                                                                                                                         |
| radiation             | The process by which electromagnetic energy is emitted by an object or a gas.                                                                                                        |
| radiator              | A piece of IR radiating equipment.                                                                                                                                                   |
| range                 | The current overall temperature measurement limitation of an IR camera. Cameras can have several ranges. Expressed as two blackbody temperatures that limit the current calibration. |
| reference temperature | A temperature which the ordinary measured values can be compared with.                                                                                                               |
| reflection            | The amount of radiation reflected by an object relative to the received radiation. A number between 0 and 1.                                                                         |
| relative humidity     | Percentage of water in the air, relative to what is physically possible. Air temperature dependent.                                                                                  |

| Term or expression                       | Explanation                                                                                                                                                                                                                                                                                                                                                    |
|------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| saturation color                         | <p>The areas that contain temperatures outside the present level/span settings are colored with the saturation colors. The saturation colors contain an 'overflow' color and an 'underflow' color.</p> <p>There is also a third red saturation color that marks everything saturated by the detector indicating that the range should probably be changed.</p> |
| span                                     | The interval of the temperature scale, usually expressed as a signal value.                                                                                                                                                                                                                                                                                    |
| spectral (radiant) emittance             | Amount of energy emitted from an object per unit of time, area and wavelength ( $W/m^2/\mu m$ )                                                                                                                                                                                                                                                                |
| temperature range                        | The current overall temperature measurement limitation of an IR camera. Cameras can have several ranges. Expressed as two blackbody temperatures that limit the current calibration.                                                                                                                                                                           |
| temperature scale                        | The way in which an IR image currently is displayed. Expressed as two temperature values limiting the colors.                                                                                                                                                                                                                                                  |
| thermogram                               | infrared image                                                                                                                                                                                                                                                                                                                                                 |
| transmission (or transmittance) (factor) | Gases and materials can be more or less transparent. Transmission is the amount of IR radiation passing through them. A number between 0 and 1.                                                                                                                                                                                                                |
| transparent isotherm                     | An isotherm showing a linear spread of colors, instead of covering the highlighted parts of the image.                                                                                                                                                                                                                                                         |

# 16 Thermographic measurement techniques

## 16.1 *Introduction*

An infrared camera measures and images the emitted infrared radiation from an object. The fact that radiation is a function of object surface temperature makes it possible for the camera to calculate and display this temperature.

However, the radiation measured by the camera does not only depend on the temperature of the object but is also a function of the emissivity. Radiation also originates from the surroundings and is reflected in the object. The radiation from the object and the reflected radiation will also be influenced by the absorption of the atmosphere.

To measure temperature accurately, it is therefore necessary to compensate for the effects of a number of different radiation sources. This is done on-line automatically by the camera. The following object parameters must, however, be supplied for the camera:

- The emissivity of the object
- The reflected apparent temperature
- The distance between the object and the camera
- The relative humidity
- Temperature of the atmosphere

## 16.2 *Emissivity*

The most important object parameter to set correctly is the emissivity which, in short, is a measure of how much radiation is emitted from the object, compared to that from a perfect blackbody of the same temperature.



Normally, object materials and surface treatments exhibit emissivity ranging from approximately 0.1 to 0.95. A highly polished (mirror) surface falls below 0.1, while an oxidized or painted surface has a higher emissivity. Oil-based paint, regardless of color in the visible spectrum, has an emissivity over 0.9 in the infrared. Human skin exhibits an emissivity 0.97 to 0.98.


Non-oxidized metals represent an extreme case of perfect opacity and high reflexivity, which does not vary greatly with wavelength. Consequently, the emissivity of metals is low – only increasing with temperature. For non-metals, emissivity tends to be high, and decreases with temperature.

**16.2.1 Finding the emissivity of a sample****16.2.1.1 Step 1: Determining reflected apparent temperature**

Use one of the following two methods to determine reflected apparent temperature:

**16.2.1.1.1 Method 1: Direct method**
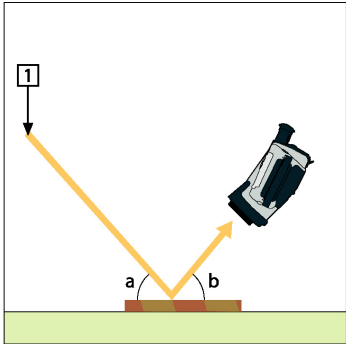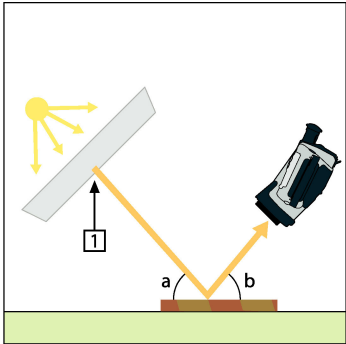
| Step | Action                                                                                                                                                                                                                                                                         |
|------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 1    | <p>Look for possible reflection sources, considering that the incident angle = reflection angle (<math>a = b</math>).</p> <p>10588903.a1</p>  <p><b>Figure 16.1</b> 1 = Reflection source</p> |
| 2    | <p>If the reflection source is a spot source, modify the source by obstructing it using a piece of cardboard.</p> <p>10589103.a2</p>  <p><b>Figure 16.2</b> 1 = Reflection source</p>        |
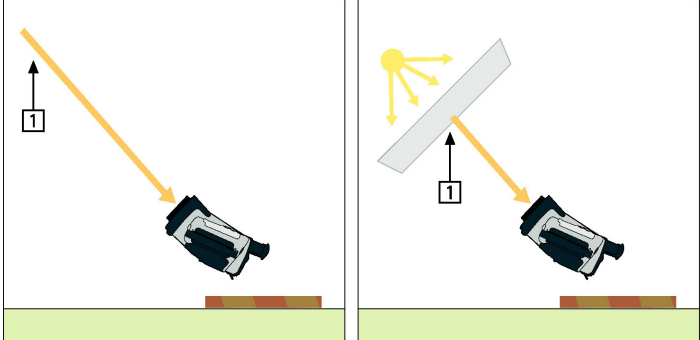
| Step | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                                       |
|------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 3    | <p>Measure the radiation intensity (= apparent temperature) from the reflecting source using the following settings:</p> <ul style="list-style-type: none"> <li>■ Emissivity: 1.0</li> <li>■ <math>D_{obj}</math>: 0</li> </ul> <p>You can measure the radiation intensity using one of the following two methods:</p> <p>10589003.a2</p>  <p><b>Figure 16.3</b> 1 = Reflection source</p> |


☞ Please note the following:

Using a thermocouple to measure reflecting temperature is not recommended for two important reasons:

- A thermocouple does not measure radiation intensity
- A thermocouple requires a very good thermal contact to the surface, usually by gluing and covering the sensor by a thermal isolator.

#### 16.2.1.1.2 Method 2: Reflector method

| Step | Action                                                                                                                                  |
|------|-----------------------------------------------------------------------------------------------------------------------------------------|
| 1    | Crumble up a large piece of aluminum foil.                                                                                              |
| 2    | Uncrumble the aluminum foil and attach it to a piece of cardboard of the same size.                                                     |
| 3    | Put the piece of cardboard in front of the object you want to measure. Make sure that the side with aluminum foil points to the camera. |
| 4    | Set the emissivity to 1.0.                                                                                                              |
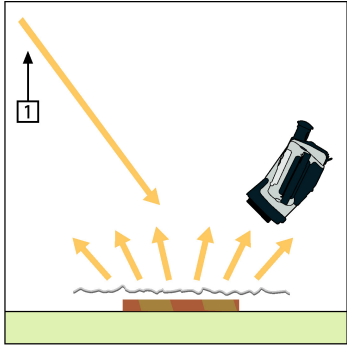
| Step | Action                                                                                                                                                                                                                                              |
|------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 5    | <p>Measure the apparent temperature of the aluminum foil and write it down.</p>  <p><b>Figure 16.4</b> Measuring the apparent temperature of the aluminum foil</p> |

#### 16.2.1.2 Step 2: Determining the emissivity

| Step | Action                                                                                                                                                                                                                                                                                                                                                           |
|------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 1    | Select a place to put the sample.                                                                                                                                                                                                                                                                                                                                |
| 2    | Determine and set reflected apparent temperature according to the previous procedure.                                                                                                                                                                                                                                                                            |
| 3    | Put a piece of electrical tape with known high emissivity on the sample.                                                                                                                                                                                                                                                                                         |
| 4    | Heat the sample at least 20 K above room temperature. Heating must be reasonably even.                                                                                                                                                                                                                                                                           |
| 5    | Focus and auto-adjust the camera, and freeze the image.                                                                                                                                                                                                                                                                                                          |
| 6    | Adjust <b>Level</b> and <b>Span</b> for best image brightness and contrast.                                                                                                                                                                                                                                                                                      |
| 7    | Set emissivity to that of the tape (usually 0.97).                                                                                                                                                                                                                                                                                                               |
| 8    | <p>Measure the temperature of the tape using one of the following measurement functions:</p> <ul style="list-style-type: none"> <li>▪ <b>Isotherm</b> (helps you to determine both the temperature and how evenly you have heated the sample)</li> <li>▪ <b>Spot</b> (simpler)</li> <li>▪ <b>Box Avg</b> (good for surfaces with varying emissivity).</li> </ul> |
| 9    | Write down the temperature.                                                                                                                                                                                                                                                                                                                                      |
| 10   | Move your measurement function to the sample surface.                                                                                                                                                                                                                                                                                                            |
| 11   | Change the emissivity setting until you read the same temperature as your previous measurement.                                                                                                                                                                                                                                                                  |

| Step | Action                     |
|------|----------------------------|
| 12   | Write down the emissivity. |

➡ Please note the following:

- Avoid forced convection
- Look for a thermally stable surrounding that will not generate spot reflections
- Use high quality tape that you know is not transparent, and has a high emissivity you are certain of
- This method assumes that the temperature of your tape and the sample surface are the same. If they are not, your emissivity measurement will be wrong.

### 16.3 *Reflected apparent temperature*

This parameter is used to compensate for the radiation reflected in the object. If the emissivity is low and the object temperature relatively far from that of the reflected it will be important to set and compensate for the reflected apparent temperature correctly.


INTENTIONALLY LEFT BLANK

# 17 History of infrared technology

17

Less than 200 years ago the existence of the infrared portion of the electromagnetic spectrum wasn't even suspected. The original significance of the infrared spectrum, or simply 'the infrared' as it is often called, as a form of heat radiation is perhaps less obvious today than it was at the time of its discovery by Herschel in 1800.

10386703.a1



**Figure 17.1** Sir William Herschel (1738–1822)

The discovery was made accidentally during the search for a new optical material. Sir William Herschel—Royal Astronomer to King George III of England, and already famous for his discovery of the planet Uranus—was searching for an optical filter material to reduce the brightness of the sun's image in telescopes during solar observations. While testing different samples of colored glass which gave similar reductions in brightness he was intrigued to find that some of the samples passed very little of the sun's heat, while others passed so much heat that he risked eye damage after only a few seconds' observation.

Herschel was soon convinced of the necessity of setting up a systematic experiment, with the objective of finding a single material that would give the desired reduction in brightness as well as the maximum reduction in heat. He began the experiment by actually repeating Newton's prism experiment, but looking for the heating effect rather than the visual distribution of intensity in the spectrum. He first blackened the bulb of a sensitive mercury-in-glass thermometer with ink, and with this as his radiation detector he proceeded to test the heating effect of the various colors of the spectrum formed on the top of a table by passing sunlight through a glass prism. Other thermometers, placed outside the sun's rays, served as controls.

As the blackened thermometer was moved slowly along the colors of the spectrum, the temperature readings showed a steady increase from the violet end to the red end. This was not entirely unexpected, since the Italian researcher, Landriani, in a similar experiment in 1777 had observed much the same effect. It was Herschel,

however, who was the first to recognize that there must be a point where the heating effect reaches a maximum, and that measurements confined to the visible portion of the spectrum failed to locate this point.

17

10388903.a1



**Figure 17.2** Marsilio Landriani (1746–1815)

Moving the thermometer into the dark region beyond the red end of the spectrum, Herschel confirmed that the heating continued to increase. The maximum point, when he found it, lay well beyond the red end—in what is known today as the ‘infrared wavelengths.’

When Herschel revealed his discovery, he referred to this new portion of the electromagnetic spectrum as the ‘thermometrical spectrum.’ The radiation itself he sometimes referred to as ‘dark heat,’ or simply ‘the invisible rays.’ Ironically, and contrary to popular opinion, it wasn’t Herschel who originated the term ‘infrared.’ The word only began to appear in print around 75 years later, and it is still unclear who should receive credit as the originator.

Herschel’s use of glass in the prism of his original experiment led to some early controversies with his contemporaries about the actual existence of the infrared wavelengths. Different investigators, in attempting to confirm his work, used various types of glass indiscriminately, having different transparencies in the infrared. Through his later experiments, Herschel was aware of the limited transparency of glass to the newly-discovered thermal radiation, and he was forced to conclude that optics for the infrared would probably be doomed to the use of reflective elements exclusively (i.e. plane and curved mirrors). Fortunately, this proved to be true only until 1830, when the Italian investigator, Melloni, made his great discovery that naturally occurring rock salt (NaCl)—which was available in large enough natural crystals to be made into lenses and prisms—is remarkably transparent to the infrared. The result was that rock salt became the principal infrared transparent material, and remained so for the next hundred years, until the art of synthetic crystal growing was mastered in the 1930’s.

10399103.a1



**Figure 17.3** Macedonio Melloni (1798–1854)

Thermometers, as radiation detectors, remained unchallenged until 1829, the year Nobili invented the thermocouple. (Herschel's own thermometer could be read to  $0.2^{\circ}\text{C}$  ( $0.036^{\circ}\text{F}$ ), and later models were able to be read to  $0.05^{\circ}\text{C}$  ( $0.09^{\circ}\text{F}$ ). Then a breakthrough occurred; Melloni connected a number of thermocouples in series to form the first thermopile. The new device was at least 40 times as sensitive as the best thermometer of the day for detecting heat radiation—capable of detecting the heat from a person standing 3 meters away (10 ft.).

The first so-called 'heat-picture' became possible in 1840, the result of work by Sir John Herschel, son of the discoverer of the infrared and a famous astronomer in his own right. Based upon the differential evaporation of a thin film of oil when exposed to a heat pattern focused upon it, the thermal image could be seen by reflected light where the interference effects of the oil film made the image visible to the eye. Sir John also managed to obtain a primitive record of the thermal image on paper, which he called a 'thermograph.'

10399003.a2



**Figure 17.4** Samuel P. Langley (1834–1906)

The improvement of infrared-detector sensitivity progressed slowly. Another major breakthrough, made by Langley in 1880, was the invention of the bolometer. This consisted of a thin blackened strip of platinum connected in one arm of a Wheatstone bridge circuit upon which the infrared radiation was focused and to which a sensitive galvanometer responded. This instrument is said to have been able to detect the heat from a cow at a distance of 400 meters (1311 ft.).

An English scientist, Sir James Dewar, first introduced the use of liquefied gases as cooling agents (such as liquid nitrogen with a temperature of  $-196^{\circ}\text{C}$  ( $-320.8^{\circ}\text{F}$ )) in low temperature research. In 1892 he invented a unique vacuum insulating container in which it is possible to store liquefied gases for entire days. The common 'thermos bottle', used for storing hot and cold drinks, is based upon his invention.

Between the years 1900 and 1920, the inventors of the world 'discovered' the infrared. Many patents were issued for devices to detect personnel, artillery, aircraft, ships—and even icebergs. The first operating systems, in the modern sense, began to be developed during the 1914–18 war, when both sides had research programs devoted to the military exploitation of the infrared. These programs included experimental systems for enemy intrusion/detection, remote temperature sensing, secure communications, and 'flying torpedo' guidance. An infrared search system tested during this period was able to detect an approaching airplane at a distance of 1.5 km (0.94 miles), or a person more than 300 meters (984 ft.) away.

The most sensitive systems up to this time were all based upon variations of the bolometer idea, but the period between the two wars saw the development of two revolutionary new infrared detectors: the image converter and the photon detector. At first, the image converter received the greatest attention by the military, because it enabled an observer for the first time in history to literally 'see in the dark.' However, the sensitivity of the image converter was limited to the near infrared wavelengths, and the most interesting military targets (i.e. enemy soldiers) had to be illuminated by infrared search beams. Since this involved the risk of giving away the observer's position to a similarly-equipped enemy observer, it is understandable that military interest in the image converter eventually faded.

The tactical military disadvantages of so-called 'active' (i.e. search beam-equipped) thermal imaging systems provided impetus following the 1939–45 war for extensive secret military infrared-research programs into the possibilities of developing 'passive' (no search beam) systems around the extremely sensitive photon detector. During this period, military secrecy regulations completely prevented disclosure of the status of infrared-imaging technology. This secrecy only began to be lifted in the middle of the 1950's, and from that time adequate thermal-imaging devices finally began to be available to civilian science and industry.

# 18 Theory of thermography


## 18.1 Introduction

The subjects of infrared radiation and the related technique of thermography are still new to many who will use an infrared camera. In this section the theory behind thermography will be given.

## 18.2 The electromagnetic spectrum

The electromagnetic spectrum is divided arbitrarily into a number of wavelength regions, called *bands*, distinguished by the methods used to produce and detect the radiation. There is no fundamental difference between radiation in the different bands of the electromagnetic spectrum. They are all governed by the same laws and the only differences are those due to differences in wavelength.

10067803.a1

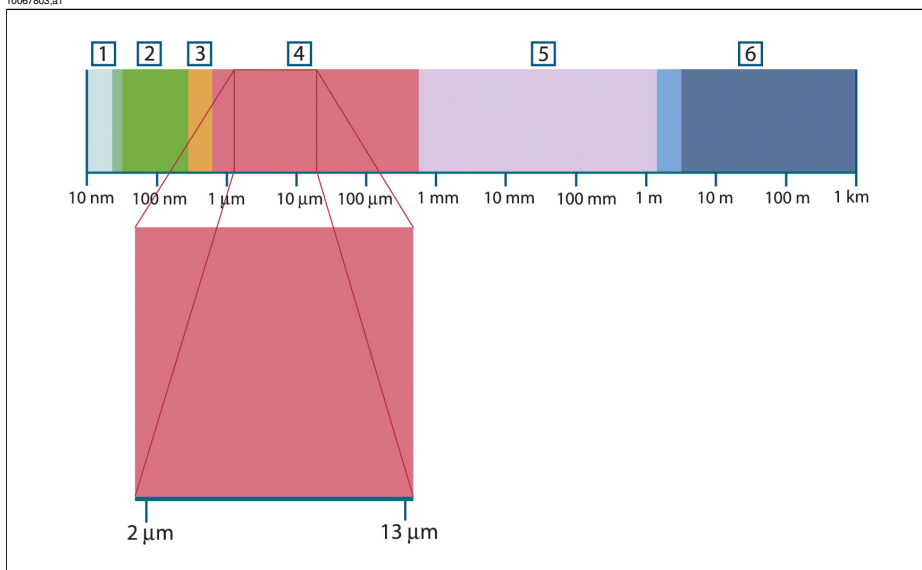

**Figure 18.1** The electromagnetic spectrum. 1: X-ray; 2: UV; 3: Visible; 4: IR; 5: Microwaves; 6: Radiowaves.

Thermography makes use of the infrared spectral band. At the short-wavelength end the boundary lies at the limit of visual perception, in the deep red. At the long-wavelength end it merges with the microwave radio wavelengths, in the millimeter range.

The infrared band is often further subdivided into four smaller bands, the boundaries of which are also arbitrarily chosen. They include: the *near infrared* (0.75–3 μm), the *middle infrared* (3–6 μm), the *far infrared* (6–15 μm) and the *extreme infrared* (15–100

$\mu\text{m}$ ). Although the wavelengths are given in  $\mu\text{m}$  (micrometers), other units are often still used to measure wavelength in this spectral region, e.g. nanometer (nm) and Ångström (Å).

The relationships between the different wavelength measurements is:


$$10\,000\text{ Å} = 1\,000\text{ nm} = 1\text{ }\mu = 1\text{ }\mu\text{m}$$

18

### 18.3 Blackbody radiation

A blackbody is defined as an object which absorbs all radiation that impinges on it at any wavelength. The apparent misnomer *black* relating to an object emitting radiation is explained by Kirchhoff's Law (after *Gustav Robert Kirchhoff*, 1824–1887), which states that a body capable of absorbing all radiation at any wavelength is equally capable in the emission of radiation.

10388803.a1

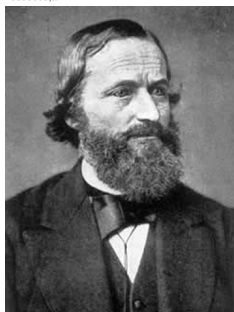

**Figure 18.2** Gustav Robert Kirchhoff (1824–1887)

The construction of a blackbody source is, in principle, very simple. The radiation characteristics of an aperture in an isotherm cavity made of an opaque absorbing material represents almost exactly the properties of a blackbody. A practical application of the principle to the construction of a perfect absorber of radiation consists of a box that is light tight except for an aperture in one of the sides. Any radiation which then enters the hole is scattered and absorbed by repeated reflections so only an infinitesimal fraction can possibly escape. The blackness which is obtained at the aperture is nearly equal to a blackbody and almost perfect for all wavelengths.

By providing such an isothermal cavity with a suitable heater it becomes what is termed a *cavity radiator*. An isothermal cavity heated to a uniform temperature generates blackbody radiation, the characteristics of which are determined solely by the temperature of the cavity. Such cavity radiators are commonly used as sources of radiation in temperature reference standards in the laboratory for calibrating thermographic instruments, such as a FLIR Systems camera for example.

If the temperature of blackbody radiation increases to more than 525 °C (977 °F), the source begins to be visible so that it appears to the eye no longer black. This is the incipient red heat temperature of the radiator, which then becomes orange or yellow as the temperature increases further. In fact, the definition of the so-called *color temperature* of an object is the temperature to which a blackbody would have to be heated to have the same appearance.

Now consider three expressions that describe the radiation emitted from a blackbody.

### 18.3.1 Planck's law

10389203,a1



**Figure 18.3** Max Planck (1858–1947)

*Max Planck* (1858–1947) was able to describe the spectral distribution of the radiation from a blackbody by means of the following formula:

$$W_{\lambda b} = \frac{2\pi hc^3}{\lambda^5 \left( e^{\frac{hc}{\lambda kT}} - 1 \right)} \times 10^{-6} \left[ \text{Watt/m}^2 \mu\text{m} \right]$$


where:

|                 |                                                                |
|-----------------|----------------------------------------------------------------|
| $W_{\lambda b}$ | Blackbody spectral radiant emittance at wavelength $\lambda$ . |
| $c$             | Velocity of light = $3 \times 10^8$ m/s                        |
| $h$             | Planck's constant = $6.6 \times 10^{-34}$ Joule sec.           |
| $k$             | Boltzmann's constant = $1.4 \times 10^{-23}$ Joule/K.          |
| $T$             | Absolute temperature (K) of a blackbody.                       |
| $\lambda$       | Wavelength ( $\mu\text{m}$ ).                                  |

☞ The factor  $10^{-6}$  is used since spectral emittance in the curves is expressed in Watt/m<sup>2</sup>m. If the factor is excluded, the dimension will be Watt/m<sup>2</sup>μm.

Planck's formula, when plotted graphically for various temperatures, produces a family of curves. Following any particular Planck curve, the spectral emittance is zero at  $\lambda = 0$ , then increases rapidly to a maximum at a wavelength  $\lambda_{\max}$  and after passing it approaches zero again at very long wavelengths. The higher the temperature, the shorter the wavelength at which maximum occurs.

18

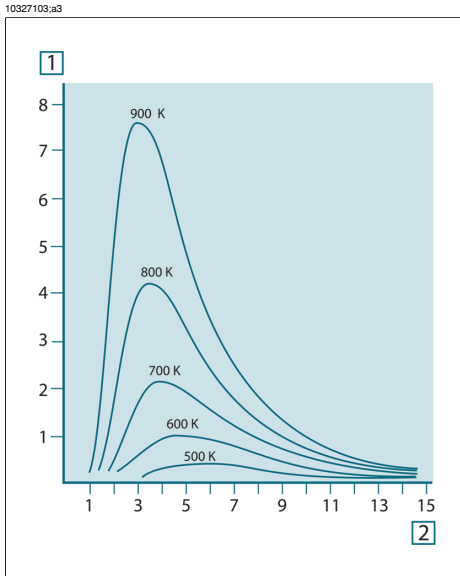

**Figure 18.4** Blackbody spectral radiant emittance according to Planck's law, plotted for various absolute temperatures. **1:** Spectral radiant emittance ( $\text{W}/\text{cm}^2 \times 10^3(\mu\text{m})$ ); **2:** Wavelength ( $\mu\text{m}$ )


### 18.3.2 Wien's displacement law

By differentiating Planck's formula with respect to  $\lambda$ , and finding the maximum, we have:

$$\lambda_{\max} = \frac{2898}{T} [\mu\text{m}]$$

This is Wien's formula (after *Wilhelm Wien*, 1864–1928), which expresses mathematically the common observation that colors vary from red to orange or yellow as the temperature of a thermal radiator increases. The wavelength of the color is the same as the wavelength calculated for  $\lambda_{\max}$ . A good approximation of the value of  $\lambda_{\max}$  for a given blackbody temperature is obtained by applying the rule-of-thumb  $3\,000/T$   $\mu\text{m}$ . Thus, a very hot star such as Sirius (11 000 K), emitting bluish-white light, radiates with the peak of spectral radiant emittance occurring within the invisible ultraviolet spectrum, at wavelength 0.27  $\mu\text{m}$ .

10389403.a1

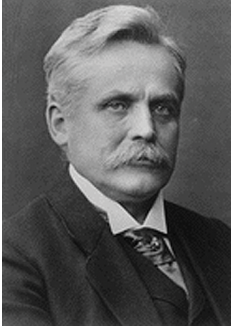


**Figure 18.5** Wilhelm Wien (1864–1928)

The sun (approx. 6 000 K) emits yellow light, peaking at about  $0.5\ \mu\text{m}$  in the middle of the visible light spectrum.

At room temperature (300 K) the peak of radiant emittance lies at  $9.7\ \mu\text{m}$ , in the far infrared, while at the temperature of liquid nitrogen (77 K) the maximum of the almost insignificant amount of radiant emittance occurs at  $38\ \mu\text{m}$ , in the extreme infrared wavelengths.

10327203.a3

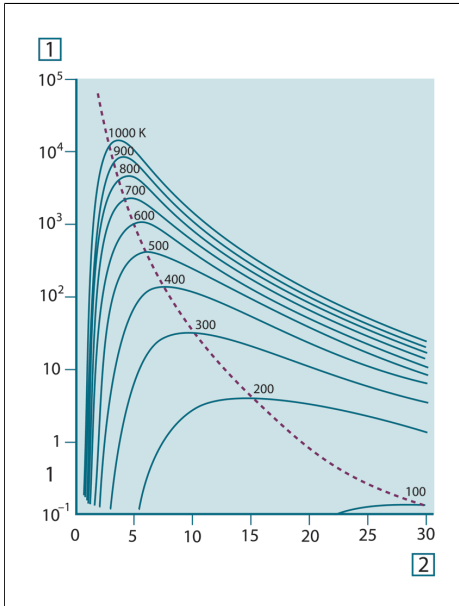

**Figure 18.6** Planckian curves plotted on semi-log scales from 100 K to 1000 K. The dotted line represents the locus of maximum radiant emittance at each temperature as described by Wien's displacement law. 1: Spectral radiant emittance ( $\text{W}/\text{cm}^2\ (\mu\text{m})$ ); 2: Wavelength ( $\mu\text{m}$ ).

### 18.3.3 Stefan-Boltzmann's law

By integrating Planck's formula from  $\lambda = 0$  to  $\lambda = \infty$ , we obtain the total radiant emittance ( $W_b$ ) of a blackbody:

$$W_b = \sigma T^4 \text{ [Watt/m}^2\text{]}$$

18

This is the Stefan-Boltzmann formula (after *Josef Stefan*, 1835–1893, and *Ludwig Boltzmann*, 1844–1906), which states that the total emissive power of a blackbody is proportional to the fourth power of its absolute temperature. Graphically,  $W_b$  represents the area below the Planck curve for a particular temperature. It can be shown that the radiant emittance in the interval  $\lambda = 0$  to  $\lambda_{\text{max}}$  is only 25 % of the total, which represents about the amount of the sun's radiation which lies inside the visible light spectrum.

10399303.a1



**Figure 18.7** Josef Stefan (1835–1893), and Ludwig Boltzmann (1844–1906)

Using the Stefan-Boltzmann formula to calculate the power radiated by the human body, at a temperature of 300 K and an external surface area of approx. 2 m<sup>2</sup>, we obtain 1 kW. This power loss could not be sustained if it were not for the compensating absorption of radiation from surrounding surfaces, at room temperatures which do not vary too drastically from the temperature of the body – or, of course, the addition of clothing.

### 18.3.4 Non-blackbody emitters

So far, only blackbody radiators and blackbody radiation have been discussed. However, real objects almost never comply with these laws over an extended wavelength region – although they may approach the blackbody behavior in certain spectral intervals. For example, a certain type of white paint may appear perfectly *white* in the visible light spectrum, but becomes distinctly *gray* at about 2 μm, and beyond 3 μm it is almost *black*.

There are three processes which can occur that prevent a real object from acting like a blackbody: a fraction of the incident radiation  $\alpha$  may be absorbed, a fraction  $\rho$  may be reflected, and a fraction  $\tau$  may be transmitted. Since all of these factors are more or less wavelength dependent, the subscript  $\lambda$  is used to imply the spectral dependence of their definitions. Thus:

- The spectral absorptance  $\alpha_\lambda$  = the ratio of the spectral radiant power absorbed by an object to that incident upon it.
- The spectral reflectance  $\rho_\lambda$  = the ratio of the spectral radiant power reflected by an object to that incident upon it.
- The spectral transmittance  $\tau_\lambda$  = the ratio of the spectral radiant power transmitted through an object to that incident upon it.

The sum of these three factors must always add up to the whole at any wavelength, so we have the relation:

$$\alpha_\lambda + \rho_\lambda + \tau_\lambda = 1$$

For opaque materials  $\tau_\lambda = 0$  and the relation simplifies to:

$$\alpha_\lambda + \rho_\lambda = 1$$

Another factor, called the emissivity, is required to describe the fraction  $\varepsilon$  of the radiant emittance of a blackbody produced by an object at a specific temperature. Thus, we have the definition:

The spectral emissivity  $\varepsilon_\lambda$  = the ratio of the spectral radiant power from an object to that from a blackbody at the same temperature and wavelength.

Expressed mathematically, this can be written as the ratio of the spectral emittance of the object to that of a blackbody as follows:

$$\varepsilon_\lambda = \frac{W_{\lambda o}}{W_{\lambda b}}$$

Generally speaking, there are three types of radiation source, distinguished by the ways in which the spectral emittance of each varies with wavelength.

- A blackbody, for which  $\varepsilon_\lambda = \varepsilon = 1$
- A graybody, for which  $\varepsilon_\lambda = \varepsilon = \text{constant less than } 1$
- A selective radiator, for which  $\varepsilon$  varies with wavelength

According to Kirchhoff's law, for any material the spectral emissivity and spectral absorptance of a body are equal at any specified temperature and wavelength. That is:

$$\varepsilon_\lambda = \alpha_\lambda$$

From this we obtain, for an opaque material (since  $\alpha_\lambda + \rho_\lambda = 1$ ):

$$\varepsilon_{\lambda} + \rho_{\lambda} = 1$$

For highly polished materials  $\varepsilon_{\lambda}$  approaches zero, so that for a perfectly reflecting material (i.e. a perfect mirror) we have:

$$\rho_{\lambda} = 1$$


18

For a graybody radiator, the Stefan-Boltzmann formula becomes:

$$W = \varepsilon \sigma T^4 \text{ [Watt/m}^2\text{]}$$


This states that the total emissive power of a graybody is the same as a blackbody at the same temperature reduced in proportion to the value of  $\varepsilon$  from the graybody.

10401203.a1

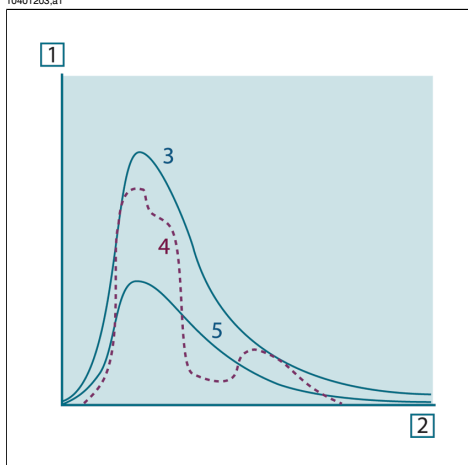

**Figure 18.8** Spectral radiant emittance of three types of radiators. 1: Spectral radiant emittance; 2: Wavelength; 3: Blackbody; 4: Selective radiator; 5: Graybody.

10327303.a3

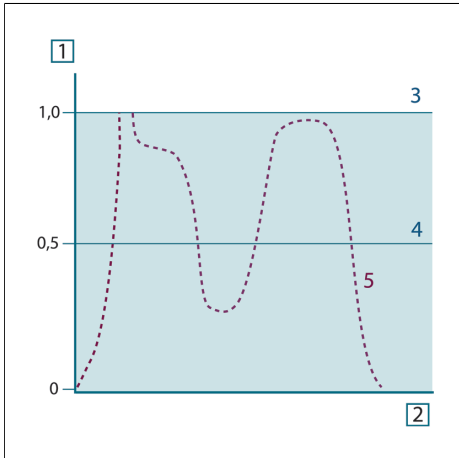

**Figure 18.9** Spectral emissivity of three types of radiators. 1: Spectral emissivity; 2: Wavelength; 3: Blackbody; 4: Graybody; 5: Selective radiator.

### 18.4 Infrared semi-transparent materials

Consider now a non-metallic, semi-transparent body – let us say, in the form of a thick flat plate of plastic material. When the plate is heated, radiation generated within its volume must work its way toward the surfaces through the material in which it is partially absorbed. Moreover, when it arrives at the surface, some of it is reflected back into the interior. The back-reflected radiation is again partially absorbed, but some of it arrives at the other surface, through which most of it escapes; part of it is reflected back again. Although the progressive reflections become weaker and weaker they must all be added up when the total emittance of the plate is sought. When the resulting geometrical series is summed, the effective emissivity of a semi-transparent plate is obtained as:

$$\varepsilon_{\lambda} = \frac{(1 - \rho_{\lambda})(1 - \tau_{\lambda})}{1 - \rho_{\lambda}\tau_{\lambda}}$$

When the plate becomes opaque this formula is reduced to the single formula:

$$\varepsilon_{\lambda} = 1 - \rho_{\lambda}$$

This last relation is a particularly convenient one, because it is often easier to measure reflectance than to measure emissivity directly.

INTENTIONALLY LEFT BLANK

# 19 Emissivity tables

This section presents a compilation of emissivity data from the infrared literature and measurements made by FLIR Systems.

## 19.1 References

|   |                                                                                                                                                                                                                             |
|---|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 1 | Mikaél A. Bramson: <i>Infrared Radiation, A Handbook for Applications</i> , Plenum press, N.Y.                                                                                                                              |
| 2 | William L. Wolfe, George J. Zissis: <i>The Infrared Handbook</i> , Office of Naval Research, Department of Navy, Washington, D.C.                                                                                           |
| 3 | Madding, R. P.: <i>Thermographic Instruments and systems</i> . Madison, Wisconsin: University of Wisconsin – Extension, Department of Engineering and Applied Science.                                                      |
| 4 | William L. Wolfe: <i>Handbook of Military Infrared Technology</i> , Office of Naval Research, Department of Navy, Washington, D.C.                                                                                          |
| 5 | Jones, Smith, Probert: <i>External thermography of buildings...</i> , Proc. of the Society of Photo-Optical Instrumentation Engineers, vol.110, Industrial and Civil Applications of Infrared Technology, June 1977 London. |
| 6 | Paljak, Pettersson: <i>Thermography of Buildings</i> , Swedish Building Research Institute, Stockholm 1972.                                                                                                                 |
| 7 | Vlcek, J.: <i>Determination of emissivity with imaging radiometers and some emissivities at <math>\lambda = 5 \mu\text{m}</math></i> . Photogrammetric Engineering and Remote Sensing.                                      |
| 8 | Kern: <i>Evaluation of infrared emission of clouds and ground as measured by weather satellites</i> , Defence Documentation Center, AD 617 417.                                                                             |
| 9 | Öhman, Claes: <i>Emittansmätningar med AGEMA E-Box</i> . Teknisk rapport, AGEMA 1999. (Emittance measurements using AGEMA E-Box. Technical report, AGEMA 1999.)                                                             |

## 19.2 Important note about the emissivity tables

The emissivity values in the table below are recorded using a shortwave (SW) camera. The values should be regarded as recommendations only and used by caution.

## 19.3 Tables

**Figure 19.1 T:** Total spectrum; **SW:** 2–5  $\mu\text{m}$ ; **LW:** 8–14  $\mu\text{m}$ , **LLW:** 6.5–20  $\mu\text{m}$ ; **1:** Material; **2:** Specification; **3:** Temperature in  $^{\circ}\text{C}$ ; **4:** Spectrum; **5:** Emissivity; **6:** Reference

| 1        | 2                     | 3  | 4  | 5    | 6 |
|----------|-----------------------|----|----|------|---|
| Aluminum | anodized, black, dull | 70 | LW | 0.95 | 9 |
| Aluminum | anodized, black, dull | 70 | SW | 0.67 | 9 |

| 1                  | 2                                      | 3      | 4          | 5         | 6 |
|--------------------|----------------------------------------|--------|------------|-----------|---|
| Aluminum           | anodized, light gray, dull             | 70     | LW         | 0.97      | 9 |
| Aluminum           | anodized, light gray, dull             | 70     | SW         | 0.61      | 9 |
| Aluminum           | anodized sheet                         | 100    | T          | 0.55      | 2 |
| Aluminum           | as received, plate                     | 100    | T          | 0.09      | 4 |
| Aluminum           | as received, sheet                     | 100    | T          | 0.09      | 2 |
| Aluminum           | cast, blast cleaned                    | 70     | LW         | 0.46      | 9 |
| Aluminum           | cast, blast cleaned                    | 70     | SW         | 0.47      | 9 |
| Aluminum           | dipped in HNO <sub>3</sub> , plate     | 100    | T          | 0.05      | 4 |
| Aluminum           | foil                                   | 27     | 3 $\mu$ m  | 0.09      | 3 |
| Aluminum           | foil                                   | 27     | 10 $\mu$ m | 0.04      | 3 |
| Aluminum           | oxidized, strongly                     | 50–500 | T          | 0.2–0.3   | 1 |
| Aluminum           | polished                               | 50–100 | T          | 0.04–0.06 | 1 |
| Aluminum           | polished, sheet                        | 100    | T          | 0.05      | 2 |
| Aluminum           | polished plate                         | 100    | T          | 0.05      | 4 |
| Aluminum           | roughened                              | 27     | 3 $\mu$ m  | 0.28      | 3 |
| Aluminum           | roughened                              | 27     | 10 $\mu$ m | 0.18      | 3 |
| Aluminum           | rough surface                          | 20–50  | T          | 0.06–0.07 | 1 |
| Aluminum           | sheet, 4 samples differently scratched | 70     | LW         | 0.03–0.06 | 9 |
| Aluminum           | sheet, 4 samples differently scratched | 70     | SW         | 0.05–0.08 | 9 |
| Aluminum           | vacuum deposited                       | 20     | T          | 0.04      | 2 |
| Aluminum           | weathered, heavily                     | 17     | SW         | 0.83–0.94 | 5 |
| Aluminum bronze    |                                        | 20     | T          | 0.60      | 1 |
| Aluminum hydroxide | powder                                 |        | T          | 0.28      | 1 |
| Aluminum oxide     | activated, powder                      |        | T          | 0.46      | 1 |

| 1              | 2                             | 3       | 4   | 5         | 6 |
|----------------|-------------------------------|---------|-----|-----------|---|
| Aluminum oxide | pure, powder (alumina)        |         | T   | 0.16      | 1 |
| Asbestos       | board                         | 20      | T   | 0.96      | 1 |
| Asbestos       | fabric                        |         | T   | 0.78      | 1 |
| Asbestos       | floor tile                    | 35      | SW  | 0.94      | 7 |
| Asbestos       | paper                         | 40–400  | T   | 0.93–0.95 | 1 |
| Asbestos       | powder                        |         | T   | 0.40–0.60 | 1 |
| Asbestos       | slate                         | 20      | T   | 0.96      | 1 |
| Asphalt paving |                               | 4       | LLW | 0.967     | 8 |
| Brass          | dull, tarnished               | 20–350  | T   | 0.22      | 1 |
| Brass          | oxidized                      | 70      | SW  | 0.04–0.09 | 9 |
| Brass          | oxidized                      | 70      | LW  | 0.03–0.07 | 9 |
| Brass          | oxidized                      | 100     | T   | 0.61      | 2 |
| Brass          | oxidized at 600 °C            | 200–600 | T   | 0.59–0.61 | 1 |
| Brass          | polished                      | 200     | T   | 0.03      | 1 |
| Brass          | polished, highly              | 100     | T   | 0.03      | 2 |
| Brass          | rubbed with 80-grit emery     | 20      | T   | 0.20      | 2 |
| Brass          | sheet, rolled                 | 20      | T   | 0.06      | 1 |
| Brass          | sheet, worked with emery      | 20      | T   | 0.2       | 1 |
| Brick          | alumina                       | 17      | SW  | 0.68      | 5 |
| Brick          | common                        | 17      | SW  | 0.86–0.81 | 5 |
| Brick          | Dinas silica, glazed, rough   | 1100    | T   | 0.85      | 1 |
| Brick          | Dinas silica, refractory      | 1000    | T   | 0.66      | 1 |
| Brick          | Dinas silica, unglazed, rough | 1000    | T   | 0.80      | 1 |
| Brick          | firebrick                     | 17      | SW  | 0.68      | 5 |
| Brick          | fireclay                      | 20      | T   | 0.85      | 1 |

| 1         | 2                                                                        | 3         | 4  | 5         | 6 |
|-----------|--------------------------------------------------------------------------|-----------|----|-----------|---|
| Brick     | fireclay                                                                 | 1000      | T  | 0.75      | 1 |
| Brick     | fireclay                                                                 | 1200      | T  | 0.59      | 1 |
| Brick     | masonry                                                                  | 35        | SW | 0.94      | 7 |
| Brick     | masonry, plastered                                                       | 20        | T  | 0.94      | 1 |
| Brick     | red, common                                                              | 20        | T  | 0.93      | 2 |
| Brick     | red, rough                                                               | 20        | T  | 0.88–0.93 | 1 |
| Brick     | refractory, corundum                                                     | 1000      | T  | 0.46      | 1 |
| Brick     | refractory, magnesite                                                    | 1000–1300 | T  | 0.38      | 1 |
| Brick     | refractory, strongly radiating                                           | 500–1000  | T  | 0.8–0.9   | 1 |
| Brick     | refractory, weakly radiating                                             | 500–1000  | T  | 0.65–0.75 | 1 |
| Brick     | silica, 95 % SiO <sub>2</sub>                                            | 1230      | T  | 0.66      | 1 |
| Brick     | sillimanite, 33 % SiO <sub>2</sub> , 64 % Al <sub>2</sub> O <sub>3</sub> | 1500      | T  | 0.29      | 1 |
| Brick     | waterproof                                                               | 17        | SW | 0.87      | 5 |
| Bronze    | phosphor bronze                                                          | 70        | LW | 0.06      | 9 |
| Bronze    | phosphor bronze                                                          | 70        | SW | 0.08      | 9 |
| Bronze    | polished                                                                 | 50        | T  | 0.1       | 1 |
| Bronze    | porous, rough                                                            | 50–150    | T  | 0.55      | 1 |
| Bronze    | powder                                                                   |           | T  | 0.76–0.80 | 1 |
| Carbon    | candle soot                                                              | 20        | T  | 0.95      | 2 |
| Carbon    | charcoal powder                                                          |           | T  | 0.96      | 1 |
| Carbon    | graphite, filed surface                                                  | 20        | T  | 0.98      | 2 |
| Carbon    | graphite powder                                                          |           | T  | 0.97      | 1 |
| Carbon    | lampblack                                                                | 20–400    | T  | 0.95–0.97 | 1 |
| Chipboard | untreated                                                                | 20        | SW | 0.90      | 6 |

| 1              | 2                                 | 3         | 4   | 5         | 6 |
|----------------|-----------------------------------|-----------|-----|-----------|---|
| Chromium       | polished                          | 50        | T   | 0.10      | 1 |
| Chromium       | polished                          | 500–1000  | T   | 0.28–0.38 | 1 |
| Clay           | fired                             | 70        | T   | 0.91      | 1 |
| Cloth          | black                             | 20        | T   | 0.98      | 1 |
| Concrete       |                                   | 20        | T   | 0.92      | 2 |
| Concrete       | dry                               | 36        | SW  | 0.95      | 7 |
| Concrete       | rough                             | 17        | SW  | 0.97      | 5 |
| Concrete       | walkway                           | 5         | LLW | 0.974     | 8 |
| Copper         | commercial, bur-nished            | 20        | T   | 0.07      | 1 |
| Copper         | electrolytic, careful-ly polished | 80        | T   | 0.018     | 1 |
| Copper         | electrolytic, pol-ished           | –34       | T   | 0.006     | 4 |
| Copper         | molten                            | 1100–1300 | T   | 0.13–0.15 | 1 |
| Copper         | oxidized                          | 50        | T   | 0.6–0.7   | 1 |
| Copper         | oxidized, black                   | 27        | T   | 0.78      | 4 |
| Copper         | oxidized, heavily                 | 20        | T   | 0.78      | 2 |
| Copper         | oxidized to black-ness            |           | T   | 0.88      | 1 |
| Copper         | polished                          | 50–100    | T   | 0.02      | 1 |
| Copper         | polished                          | 100       | T   | 0.03      | 2 |
| Copper         | polished, commer-cial             | 27        | T   | 0.03      | 4 |
| Copper         | polished, mechan-ical             | 22        | T   | 0.015     | 4 |
| Copper         | pure, carefully prepared surface  | 22        | T   | 0.008     | 4 |
| Copper         | scraped                           | 27        | T   | 0.07      | 4 |
| Copper dioxide | powder                            |           | T   | 0.84      | 1 |
| Copper oxide   | red, powder                       |           | T   | 0.70      | 1 |

| 1              | 2                          | 3        | 4   | 5         | 6 |
|----------------|----------------------------|----------|-----|-----------|---|
| Ebonite        |                            |          | T   | 0.89      | 1 |
| Emery          | coarse                     | 80       | T   | 0.85      | 1 |
| Enamel         |                            | 20       | T   | 0.9       | 1 |
| Enamel         | lacquer                    | 20       | T   | 0.85–0.95 | 1 |
| Fiber board    | hard, untreated            | 20       | SW  | 0.85      | 6 |
| Fiber board    | masonite                   | 70       | LW  | 0.88      | 9 |
| Fiber board    | masonite                   | 70       | SW  | 0.75      | 9 |
| Fiber board    | particle board             | 70       | LW  | 0.89      | 9 |
| Fiber board    | particle board             | 70       | SW  | 0.77      | 9 |
| Fiber board    | porous, untreated          | 20       | SW  | 0.85      | 6 |
| Gold           | polished                   | 130      | T   | 0.018     | 1 |
| Gold           | polished, carefully        | 200–600  | T   | 0.02–0.03 | 1 |
| Gold           | polished, highly           | 100      | T   | 0.02      | 2 |
| Granite        | polished                   | 20       | LLW | 0.849     | 8 |
| Granite        | rough                      | 21       | LLW | 0.879     | 8 |
| Granite        | rough, 4 different samples | 70       | LW  | 0.77–0.87 | 9 |
| Granite        | rough, 4 different samples | 70       | SW  | 0.95–0.97 | 9 |
| Gypsum         |                            | 20       | T   | 0.8–0.9   | 1 |
| Ice: See Water |                            |          |     |           |   |
| Iron, cast     | casting                    | 50       | T   | 0.81      | 1 |
| Iron, cast     | ingots                     | 1000     | T   | 0.95      | 1 |
| Iron, cast     | liquid                     | 1300     | T   | 0.28      | 1 |
| Iron, cast     | machined                   | 800–1000 | T   | 0.60–0.70 | 1 |
| Iron, cast     | oxidized                   | 38       | T   | 0.63      | 4 |
| Iron, cast     | oxidized                   | 100      | T   | 0.64      | 2 |
| Iron, cast     | oxidized                   | 260      | T   | 0.66      | 4 |
| Iron, cast     | oxidized                   | 538      | T   | 0.76      | 4 |

| 1              | 2                                | 3        | 4  | 5         | 6 |
|----------------|----------------------------------|----------|----|-----------|---|
| Iron, cast     | oxidized at 600 °C               | 200–600  | T  | 0.64–0.78 | 1 |
| Iron, cast     | polished                         | 38       | T  | 0.21      | 4 |
| Iron, cast     | polished                         | 40       | T  | 0.21      | 2 |
| Iron, cast     | polished                         | 200      | T  | 0.21      | 1 |
| Iron, cast     | unworked                         | 900–1100 | T  | 0.87–0.95 | 1 |
| Iron and steel | cold rolled                      | 70       | LW | 0.09      | 9 |
| Iron and steel | cold rolled                      | 70       | SW | 0.20      | 9 |
| Iron and steel | covered with red rust            | 20       | T  | 0.61–0.85 | 1 |
| Iron and steel | electrolytic                     | 22       | T  | 0.05      | 4 |
| Iron and steel | electrolytic                     | 100      | T  | 0.05      | 4 |
| Iron and steel | electrolytic                     | 260      | T  | 0.07      | 4 |
| Iron and steel | electrolytic, carefully polished | 175–225  | T  | 0.05–0.06 | 1 |
| Iron and steel | freshly worked with emery        | 20       | T  | 0.24      | 1 |
| Iron and steel | ground sheet                     | 950–1100 | T  | 0.55–0.61 | 1 |
| Iron and steel | heavily rusted sheet             | 20       | T  | 0.69      | 2 |
| Iron and steel | hot rolled                       | 20       | T  | 0.77      | 1 |
| Iron and steel | hot rolled                       | 130      | T  | 0.60      | 1 |
| Iron and steel | oxidized                         | 100      | T  | 0.74      | 1 |
| Iron and steel | oxidized                         | 100      | T  | 0.74      | 4 |
| Iron and steel | oxidized                         | 125–525  | T  | 0.78–0.82 | 1 |
| Iron and steel | oxidized                         | 200      | T  | 0.79      | 2 |
| Iron and steel | oxidized                         | 1227     | T  | 0.89      | 4 |
| Iron and steel | oxidized                         | 200–600  | T  | 0.80      | 1 |
| Iron and steel | oxidized strongly                | 50       | T  | 0.88      | 1 |
| Iron and steel | oxidized strongly                | 500      | T  | 0.98      | 1 |
| Iron and steel | polished                         | 100      | T  | 0.07      | 2 |

| 1               | 2                             | 3        | 4  | 5         | 6 |
|-----------------|-------------------------------|----------|----|-----------|---|
| Iron and steel  | polished                      | 400–1000 | T  | 0.14–0.38 | 1 |
| Iron and steel  | polished sheet                | 750–1050 | T  | 0.52–0.56 | 1 |
| Iron and steel  | rolled, freshly               | 20       | T  | 0.24      | 1 |
| Iron and steel  | rolled sheet                  | 50       | T  | 0.56      | 1 |
| Iron and steel  | rough, plane surface          | 50       | T  | 0.95–0.98 | 1 |
| Iron and steel  | rusted, heavily               | 17       | SW | 0.96      | 5 |
| Iron and steel  | rusted red, sheet             | 22       | T  | 0.69      | 4 |
| Iron and steel  | rusty, red                    | 20       | T  | 0.69      | 1 |
| Iron and steel  | shiny, etched                 | 150      | T  | 0.16      | 1 |
| Iron and steel  | shiny oxide layer, sheet,     | 20       | T  | 0.82      | 1 |
| Iron and steel  | wrought, carefully polished   | 40–250   | T  | 0.28      | 1 |
| Iron galvanized | heavily oxidized              | 70       | LW | 0.85      | 9 |
| Iron galvanized | heavily oxidized              | 70       | SW | 0.64      | 9 |
| Iron galvanized | sheet                         | 92       | T  | 0.07      | 4 |
| Iron galvanized | sheet, burnished              | 30       | T  | 0.23      | 1 |
| Iron galvanized | sheet, oxidized               | 20       | T  | 0.28      | 1 |
| Iron tinned     | sheet                         | 24       | T  | 0.064     | 4 |
| Lacquer         | 3 colors sprayed on Aluminum  | 70       | LW | 0.92–0.94 | 9 |
| Lacquer         | 3 colors sprayed on Aluminum  | 70       | SW | 0.50–0.53 | 9 |
| Lacquer         | Aluminum on rough surface     | 20       | T  | 0.4       | 1 |
| Lacquer         | bakelite                      | 80       | T  | 0.83      | 1 |
| Lacquer         | black, dull                   | 40–100   | T  | 0.96–0.98 | 1 |
| Lacquer         | black, matte                  | 100      | T  | 0.97      | 2 |
| Lacquer         | black, shiny, sprayed on iron | 20       | T  | 0.87      | 1 |

| 1                | 2                    | 3         | 4  | 5         | 6 |
|------------------|----------------------|-----------|----|-----------|---|
| Lacquer          | heat-resistant       | 100       | T  | 0.92      | 1 |
| Lacquer          | white                | 40–100    | T  | 0.8–0.95  | 1 |
| Lacquer          | white                | 100       | T  | 0.92      | 2 |
| Lead             | oxidized, gray       | 20        | T  | 0.28      | 1 |
| Lead             | oxidized, gray       | 22        | T  | 0.28      | 4 |
| Lead             | oxidized at 200 °C   | 200       | T  | 0.63      | 1 |
| Lead             | shiny                | 250       | T  | 0.08      | 1 |
| Lead             | unoxidized, polished | 100       | T  | 0.05      | 4 |
| Lead red         |                      | 100       | T  | 0.93      | 4 |
| Lead red, powder |                      | 100       | T  | 0.93      | 1 |
| Leather          | tanned               |           | T  | 0.75–0.80 | 1 |
| Lime             |                      |           | T  | 0.3–0.4   | 1 |
| Magnesium        |                      | 22        | T  | 0.07      | 4 |
| Magnesium        |                      | 260       | T  | 0.13      | 4 |
| Magnesium        |                      | 538       | T  | 0.18      | 4 |
| Magnesium        | polished             | 20        | T  | 0.07      | 2 |
| Magnesium powder |                      |           | T  | 0.86      | 1 |
| Molybdenum       |                      | 600–1000  | T  | 0.08–0.13 | 1 |
| Molybdenum       |                      | 1500–2200 | T  | 0.19–0.26 | 1 |
| Molybdenum       | filament             | 700–2500  | T  | 0.1–0.3   | 1 |
| Mortar           |                      | 17        | SW | 0.87      | 5 |
| Mortar           | dry                  | 36        | SW | 0.94      | 7 |
| Nichrome         | rolled               | 700       | T  | 0.25      | 1 |
| Nichrome         | sandblasted          | 700       | T  | 0.70      | 1 |
| Nichrome         | wire, clean          | 50        | T  | 0.65      | 1 |
| Nichrome         | wire, clean          | 500–1000  | T  | 0.71–0.79 | 1 |
| Nichrome         | wire, oxidized       | 50–500    | T  | 0.95–0.98 | 1 |

| 1                | 2                                 | 3         | 4 | 5         | 6 |
|------------------|-----------------------------------|-----------|---|-----------|---|
| Nickel           | bright matte                      | 122       | T | 0.041     | 4 |
| Nickel           | commercially pure, polished       | 100       | T | 0.045     | 1 |
| Nickel           | commercially pure, polished       | 200–400   | T | 0.07–0.09 | 1 |
| Nickel           | electrolytic                      | 22        | T | 0.04      | 4 |
| Nickel           | electrolytic                      | 38        | T | 0.06      | 4 |
| Nickel           | electrolytic                      | 260       | T | 0.07      | 4 |
| Nickel           | electrolytic                      | 538       | T | 0.10      | 4 |
| Nickel           | electroplated, polished           | 20        | T | 0.05      | 2 |
| Nickel           | electroplated on iron, polished   | 22        | T | 0.045     | 4 |
| Nickel           | electroplated on iron, unpolished | 20        | T | 0.11–0.40 | 1 |
| Nickel           | electroplated on iron, unpolished | 22        | T | 0.11      | 4 |
| Nickel           | oxidized                          | 200       | T | 0.37      | 2 |
| Nickel           | oxidized                          | 227       | T | 0.37      | 4 |
| Nickel           | oxidized                          | 1227      | T | 0.85      | 4 |
| Nickel           | oxidized at 600 °C                | 200–600   | T | 0.37–0.48 | 1 |
| Nickel           | polished                          | 122       | T | 0.045     | 4 |
| Nickel           | wire                              | 200–1000  | T | 0.1–0.2   | 1 |
| Nickel oxide     |                                   | 500–650   | T | 0.52–0.59 | 1 |
| Nickel oxide     |                                   | 1000–1250 | T | 0.75–0.86 | 1 |
| Oil, lubricating | 0.025 mm film                     | 20        | T | 0.27      | 2 |
| Oil, lubricating | 0.050 mm film                     | 20        | T | 0.46      | 2 |
| Oil, lubricating | 0.125 mm film                     | 20        | T | 0.72      | 2 |
| Oil, lubricating | film on Ni base: Ni base only     | 20        | T | 0.05      | 2 |
| Oil, lubricating | thick coating                     | 20        | T | 0.82      | 2 |

| 1     | 2                                | 3      | 4  | 5         | 6 |
|-------|----------------------------------|--------|----|-----------|---|
| Paint | 8 different colors and qualities | 70     | LW | 0.92–0.94 | 9 |
| Paint | 8 different colors and qualities | 70     | SW | 0.88–0.96 | 9 |
| Paint | Aluminum, various ages           | 50–100 | T  | 0.27–0.67 | 1 |
| Paint | cadmium yellow                   |        | T  | 0.28–0.33 | 1 |
| Paint | chrome green                     |        | T  | 0.65–0.70 | 1 |
| Paint | cobalt blue                      |        | T  | 0.7–0.8   | 1 |
| Paint | oil                              | 17     | SW | 0.87      | 5 |
| Paint | oil, black flat                  | 20     | SW | 0.94      | 6 |
| Paint | oil, black gloss                 | 20     | SW | 0.92      | 6 |
| Paint | oil, gray flat                   | 20     | SW | 0.97      | 6 |
| Paint | oil, gray gloss                  | 20     | SW | 0.96      | 6 |
| Paint | oil, various colors              | 100    | T  | 0.92–0.96 | 1 |
| Paint | oil based, average of 16 colors  | 100    | T  | 0.94      | 2 |
| Paint | plastic, black                   | 20     | SW | 0.95      | 6 |
| Paint | plastic, white                   | 20     | SW | 0.84      | 6 |
| Paper | 4 different colors               | 70     | LW | 0.92–0.94 | 9 |
| Paper | 4 different colors               | 70     | SW | 0.68–0.74 | 9 |
| Paper | black                            |        | T  | 0.90      | 1 |
| Paper | black, dull                      |        | T  | 0.94      | 1 |
| Paper | black, dull                      | 70     | LW | 0.89      | 9 |
| Paper | black, dull                      | 70     | SW | 0.86      | 9 |
| Paper | blue, dark                       |        | T  | 0.84      | 1 |
| Paper | coated with black lacquer        |        | T  | 0.93      | 1 |
| Paper | green                            |        | T  | 0.85      | 1 |
| Paper | red                              |        | T  | 0.76      | 1 |
| Paper | white                            | 20     | T  | 0.7–0.9   | 1 |

| 1        | 2                                          | 3         | 4  | 5         | 6 |
|----------|--------------------------------------------|-----------|----|-----------|---|
| Paper    | white, 3 different glosses                 | 70        | LW | 0.88–0.90 | 9 |
| Paper    | white, 3 different glosses                 | 70        | SW | 0.76–0.78 | 9 |
| Paper    | white bond                                 | 20        | T  | 0.93      | 2 |
| Paper    | yellow                                     |           | T  | 0.72      | 1 |
| Plaster  |                                            | 17        | SW | 0.86      | 5 |
| Plaster  | plasterboard, untreated                    | 20        | SW | 0.90      | 6 |
| Plaster  | rough coat                                 | 20        | T  | 0.91      | 2 |
| Plastic  | glass fibre laminate (printed circ. board) | 70        | LW | 0.91      | 9 |
| Plastic  | glass fibre laminate (printed circ. board) | 70        | SW | 0.94      | 9 |
| Plastic  | polyurethane isolation board               | 70        | LW | 0.55      | 9 |
| Plastic  | polyurethane isolation board               | 70        | SW | 0.29      | 9 |
| Plastic  | PVC, plastic floor, dull, structured       | 70        | LW | 0.93      | 9 |
| Plastic  | PVC, plastic floor, dull, structured       | 70        | SW | 0.94      | 9 |
| Platinum |                                            | 17        | T  | 0.016     | 4 |
| Platinum |                                            | 22        | T  | 0.03      | 4 |
| Platinum |                                            | 100       | T  | 0.05      | 4 |
| Platinum |                                            | 260       | T  | 0.06      | 4 |
| Platinum |                                            | 538       | T  | 0.10      | 4 |
| Platinum |                                            | 1000–1500 | T  | 0.14–0.18 | 1 |
| Platinum |                                            | 1094      | T  | 0.18      | 4 |
| Platinum | pure, polished                             | 200–600   | T  | 0.05–0.10 | 1 |
| Platinum | ribbon                                     | 900–1100  | T  | 0.12–0.17 | 1 |

| 1               | 2                         | 3         | 4   | 5         | 6 |
|-----------------|---------------------------|-----------|-----|-----------|---|
| Platinum        | wire                      | 50–200    | T   | 0.06–0.07 | 1 |
| Platinum        | wire                      | 500–1000  | T   | 0.10–0.16 | 1 |
| Platinum        | wire                      | 1400      | T   | 0.18      | 1 |
| Porcelain       | glazed                    | 20        | T   | 0.92      | 1 |
| Porcelain       | white, shiny              |           | T   | 0.70–0.75 | 1 |
| Rubber          | hard                      | 20        | T   | 0.95      | 1 |
| Rubber          | soft, gray, rough         | 20        | T   | 0.95      | 1 |
| Sand            |                           |           | T   | 0.60      | 1 |
| Sand            |                           | 20        | T   | 0.90      | 2 |
| Sandstone       | polished                  | 19        | LLW | 0.909     | 8 |
| Sandstone       | rough                     | 19        | LLW | 0.935     | 8 |
| Silver          | polished                  | 100       | T   | 0.03      | 2 |
| Silver          | pure, polished            | 200–600   | T   | 0.02–0.03 | 1 |
| Skin            | human                     | 32        | T   | 0.98      | 2 |
| Slag            | boiler                    | 0–100     | T   | 0.97–0.93 | 1 |
| Slag            | boiler                    | 200–500   | T   | 0.89–0.78 | 1 |
| Slag            | boiler                    | 600–1200  | T   | 0.76–0.70 | 1 |
| Slag            | boiler                    | 1400–1800 | T   | 0.69–0.67 | 1 |
| Snow: See Water |                           |           |     |           |   |
| Soil            | dry                       | 20        | T   | 0.92      | 2 |
| Soil            | saturated with water      | 20        | T   | 0.95      | 2 |
| Stainless steel | alloy, 8 % Ni,<br>18 % Cr | 500       | T   | 0.35      | 1 |
| Stainless steel | rolled                    | 700       | T   | 0.45      | 1 |
| Stainless steel | sandblasted               | 700       | T   | 0.70      | 1 |
| Stainless steel | sheet, polished           | 70        | LW  | 0.14      | 9 |
| Stainless steel | sheet, polished           | 70        | SW  | 0.18      | 9 |

| 1               | 2                                    | 3         | 4  | 5         | 6 |
|-----------------|--------------------------------------|-----------|----|-----------|---|
| Stainless steel | sheet, untreated, somewhat scratched | 70        | LW | 0.28      | 9 |
| Stainless steel | sheet, untreated, somewhat scratched | 70        | SW | 0.30      | 9 |
| Stainless steel | type 18-8, buffed                    | 20        | T  | 0.16      | 2 |
| Stainless steel | type 18-8, oxidized at 800 °C        | 60        | T  | 0.85      | 2 |
| Stucco          | rough, lime                          | 10–90     | T  | 0.91      | 1 |
| Styrofoam       | insulation                           | 37        | SW | 0.60      | 7 |
| Tar             |                                      |           | T  | 0.79–0.84 | 1 |
| Tar             | paper                                | 20        | T  | 0.91–0.93 | 1 |
| Tile            | glazed                               | 17        | SW | 0.94      | 5 |
| Tin             | burnished                            | 20–50     | T  | 0.04–0.06 | 1 |
| Tin             | tin-plated sheet iron                | 100       | T  | 0.07      | 2 |
| Titanium        | oxidized at 540 °C                   | 200       | T  | 0.40      | 1 |
| Titanium        | oxidized at 540 °C                   | 500       | T  | 0.50      | 1 |
| Titanium        | oxidized at 540 °C                   | 1000      | T  | 0.60      | 1 |
| Titanium        | polished                             | 200       | T  | 0.15      | 1 |
| Titanium        | polished                             | 500       | T  | 0.20      | 1 |
| Titanium        | polished                             | 1000      | T  | 0.36      | 1 |
| Tungsten        |                                      | 200       | T  | 0.05      | 1 |
| Tungsten        |                                      | 600–1000  | T  | 0.1–0.16  | 1 |
| Tungsten        |                                      | 1500–2200 | T  | 0.24–0.31 | 1 |
| Tungsten        | filament                             | 3300      | T  | 0.39      | 1 |
| Varnish         | flat                                 | 20        | SW | 0.93      | 6 |
| Varnish         | on oak parquet floor                 | 70        | LW | 0.90–0.93 | 9 |
| Varnish         | on oak parquet floor                 | 70        | SW | 0.90      | 9 |

| 1         | 2                             | 3         | 4   | 5         | 6 |
|-----------|-------------------------------|-----------|-----|-----------|---|
| Wallpaper | slight pattern, light gray    | 20        | SW  | 0.85      | 6 |
| Wallpaper | slight pattern, red           | 20        | SW  | 0.90      | 6 |
| Water     | distilled                     | 20        | T   | 0.96      | 2 |
| Water     | frost crystals                | –10       | T   | 0.98      | 2 |
| Water     | ice, covered with heavy frost | 0         | T   | 0.98      | 1 |
| Water     | ice, smooth                   | –10       | T   | 0.96      | 2 |
| Water     | ice, smooth                   | 0         | T   | 0.97      | 1 |
| Water     | layer >0.1 mm thick           | 0–100     | T   | 0.95–0.98 | 1 |
| Water     | snow                          |           | T   | 0.8       | 1 |
| Water     | snow                          | –10       | T   | 0.85      | 2 |
| Wood      |                               | 17        | SW  | 0.98      | 5 |
| Wood      |                               | 19        | LLW | 0.962     | 8 |
| Wood      | ground                        |           | T   | 0.5–0.7   | 1 |
| Wood      | pine, 4 different samples     | 70        | LW  | 0.81–0.89 | 9 |
| Wood      | pine, 4 different samples     | 70        | SW  | 0.67–0.75 | 9 |
| Wood      | planed                        | 20        | T   | 0.8–0.9   | 1 |
| Wood      | planed oak                    | 20        | T   | 0.90      | 2 |
| Wood      | planed oak                    | 70        | LW  | 0.88      | 9 |
| Wood      | planed oak                    | 70        | SW  | 0.77      | 9 |
| Wood      | plywood, smooth, dry          | 36        | SW  | 0.82      | 7 |
| Wood      | plywood, untreated            | 20        | SW  | 0.83      | 6 |
| Wood      | white, damp                   | 20        | T   | 0.7–0.8   | 1 |
| Zinc      | oxidized at 400 °C            | 400       | T   | 0.11      | 1 |
| Zinc      | oxidized surface              | 1000–1200 | T   | 0.50–0.60 | 1 |

| 1    | 2        | 3       | 4 | 5         | 6 |
|------|----------|---------|---|-----------|---|
| Zinc | polished | 200–300 | T | 0.04–0.05 | 1 |
| Zinc | sheet    | 50      | T | 0.20      | 1 |

# Index

\*.tcf

creating: 62

## 1

1 120 987: 11

1 195 49: 11

1 195 106: 11

1 195 128: 11

1 195 221: 11

1 909 528: 11

1 909 775: 11

## A

about FLIR Systems: 6

absolute humidity: 51

accessories

cleaning: 99

acquiring

image: 56

address: viii

adjusting

audible alarm: 61

color alarm: 60

focus: 67

level: 63

span: 63

system settings

date & time: 65

date format: 64

language: 64

temperature unit: 64

time format: 64

visual alarm: 61

air infiltration: 32

air movement: 41

airtightness: 41

Alarm

label: 84

Alarm output

label: 84

Alarm temp

label: 84

area

laying out: 58

audible alarm

changing: 61

Automatic adjust

command: 84

Auto power off

label: 89

## B

balconies: 26

bands

extreme infrared: 145

far infrared: 145

middle infrared: 145

near infrared: 145

battery: 93

cover: 71, 73

in packing list: 11

inserting: 68

operating time: 103

removing: 68

type: 103

battery charger

internal: 93

battery charging

externally: 96

internally: 95

battery system: 93

blackbody

construction: 146

explanation: 146

practical application: 146

breaks, plumbing: 29

building codes

national: 53

regional: 53

building science: 39

building structures, commented: 21, 24, 27, 32, 35

buttons

functions

MENU/YES: 75

PWR/NO: 75

SAVE/FRZ: 75

SEL: 75

location

MENU/YES: 74

navigation pad: 74

PWR/NO: 74

SAVE/FRZ: 74

SEL: 74

## C

- cables
  - cleaning: 99
- calibration: 1
  - time between: 1
- camera
  - switching off: 55
  - switching on: 55
- camera body
  - cleaning: 99
- Camera info
  - command: 91
  - dialog box: 91
- camera overview: 72
- camera parts
  - location: 71
    - battery cover: 71, 73
    - focus ring: 72
    - IrDA link: 71
    - Laser LocatIR: 72
    - LED indicator: 74
    - lens cap: 72
    - MENU/YES: 74
    - navigation pad: 74
    - PWR/NO: 74
    - ring for hand strap: 71
    - SAVE/FRZ: 74
    - SEL: 74
    - trigger: 73
    - tripod mount: 73
- camera warm-up time: 58
- canceling
  - selections: 83
- cavity radiator
  - applications: 146
  - explanation: 146
- certification: 53
- changing
  - audible alarm: 21
  - color alarm: 60
  - date & time: 65
  - date format: 64
  - emissivity: 85
  - focus: 67
  - language: 64
  - level: 63, 84
  - palette: 86
  - reflected ambient temperature: 85
  - span: 63, 84
  - system settings
    - date & time: 65
    - date format: 64
    - language: 64
  - changing (*continued*)
    - system settings (*continued*)
      - temperature unit: 64
      - time format: 64
    - temperature unit: 64
    - time format: 64
    - T Refl: 85
    - visual alarm: 61
  - charging battery
    - externally: 96
    - internally: 95
  - checking, effects of: 40
  - cleaning
    - accessories: 99
    - cables: 99
    - camera body: 99
    - lenses: 99
  - color alarm
    - changing: 60
  - commands
    - Automatic adjust: 84
    - Camera info: 91
    - Date/time: 90
    - Delete all images: 87
    - Delete image: 87
    - Emissivity: 85
    - Factory default: 91
    - Hide graphics: 86
    - Image description: 88
    - Images: 87
    - Local settings: 91
    - Manual adjust: 84
    - Meas. mode: 83
    - Palette: 86
    - Settings: 88
    - Setup: 88
    - Show graphics: 86
  - commented building structures: 21, 24, 27, 32, 35
  - commented infrared images: 22, 26, 29, 30, 34, 37
  - commercial façades: 24
  - commercial roofs, low-slope: 19
  - communications interfaces
    - RS-232: 105
    - USB: 104
  - conditions
    - measuring: 49
    - pressure: 43
    - wind: 46
  - confirming
    - selections: 83
  - copyright: viii

courses: 53  
 creating  
   image description: 62  
   text files: 62

## D

Date/time  
   command: 90  
   dialog box: 90  
 date & time  
   changing: 65  
 date format  
   changing: 64  
 Date format  
   label: 91  
 Day  
   label: 90  
 decks: 26  
 deficiencies, insulation : 35, 40  
 definition of dew point: 52  
 Delete all images  
   command: 87  
 Delete image  
   command: 87  
 deleting  
   file: 57  
   image: 57  
 Delta alarm  
   label: 84  
 detection, moisture: 19  
 detector type: 103  
 deviations: 51  
 Dewar, James: 144  
 dew point, definition of: 52  
 dialog boxes  
   Camera info: 91  
   Date/time: 90  
   Emissivity: 85  
   Local Settings: 91  
   Meas. mode: 83  
   Palette: 86  
   Settings: 88  
 dimensional drawings: 103  
 displaying  
   menu system: 83  
 Display power off  
   label: 89  
 disruption, sources of: 41

## E

education: 53  
 effects of  
   checking: 40

effects of (*continued*)  
   testing: 40  
 electrical power system: 93  
   power management: 104  
   specifications: 103  
   voltage: 103  
 electromagnetic spectrum: 145  
 EMC: 104  
 emissivity  
   changing: 85  
   data: 155  
   explanation: 135  
   tables: 155  
 Emissivity  
   command: 85  
   dialog box: 85  
 encapsulation: 104  
 environmental specifications  
   EMC: 104  
   encapsulation: 104  
   humidity: 104  
   operating temperature range: 104  
   shock: 104  
   storage temperature range: 104  
   vibration: 104  
 error messages: 80  
 exiting  
   menu system: 83  
 external leaks: 19  
 extreme infrared band: 145

## F

façades, commercial & residential : 24  
 Factory default  
   command: 91  
 far infrared band: 145  
 field of view: 103  
 file  
   deleting: 57  
   opening: 57  
   saving: 56  
 FLIR Systems  
   about: 6  
   copyright: viii  
   history: 6  
     E series: 7  
       first thermo-electrically cooled: 6  
       model 525: 6  
       model 650: 6  
       model 750: 6  
       model 780: 6  
       model P60: 7  
       thermo-electrically cooled, first: 6

(continued)

- ISO 9001: viii
- legal disclaimer: viii
- patents: viii
- patents pending: viii
- postal address: viii
- product warranty: viii
- quality assurance: viii
- quality management system: viii
- requests for enhancement: 10
- RFE: 10
- trademarks: viii
- warranty: viii
- focus
  - adjusting: 67
- focusing: 67
- focus ring: 66, 67
- formulas
  - Planck's law: 147
  - Stefan Boltzmann's formula: 150
  - Wien's displacement law: 148
- FOV: 103
- freezing
  - image: 56

## G

- glossary: 134
- graybody: 151
- guidelines
  - air infiltration: 18
  - general: 17
  - insulation deficiencies: 18
  - moisture detection: 18
  - mold detection: 18
  - water damage: 18
- Gustav Robert Kirchhoff: 146

## H

- hand strap
  - in packing list: 11
- heat picture: 143
- Herschel, William: 141
- Hide graphics
  - command: 86
- history: 6
  - E series: 7
  - first thermo-electrically cooled: 6
  - infrared technology: 141
  - model 525: 6
  - model 650: 6
  - model 750: 6
  - model 780: 6
  - model P60: 7

history (continued)

- thermo-electrically cooled, first: 6
- Hour
  - label: 90
- humidity: 104
  - absolute: 51
  - relative: 51

## I

- image
  - acquiring: 56
  - deleting: 57
  - freezing: 56
  - opening: 57
  - saving: 56
- image description
  - creating: 62
- Image description
  - command: 88
- image presentation: 103
- Images
  - command: 87
- imaging performance: 103
- indicators
  - LED: 74
  - on battery charger: 96
- infiltration, air: 32
- Info field
  - label: 89
- infrared images
  - commented: 22, 26, 29, 30, 34, 37
  - interpretation of: 49
- infrared semi-transparent body: 153
- infrared technology
  - history: 141
- inserting
  - battery: 68
- insulation deficiencies: 35, 40
- interfaces
  - RS-232: 105
  - USB: 104
- internal battery charger: 93
- internal leaks: 19
- interpretation of infrared images: 49
- IrDA link
  - location: 71
- irregularities: 51
- ISO 9001: viii

## J

- James Dewar: 144
- Josef Stefan: 150

**K**

## keys

## functions

MENU/YES: 75

PWR/NO: 75

SAVE/FRZ: 75

SEL: 75

## location

MENU/YES: 74

navigation pad: 74

PWR/NO: 74

SAVE/FRZ: 74

SEL: 74

Kirchhoff, Gustav Robert: 146

**L**

## labels

Alarm: 84

Alarm output: 84

Alarm temp: 84

Auto power off: 89

Date format: 91

Day: 90

Delta alarm: 84

Display power off: 89

Hour: 90

Info field: 89

Language: 91

LCD intensity: 89

Meas. mode: 83

Minute: 90

Month: 90

Prompt img. desc.: 89

Ref temp: 84

Scale: 88

Second: 90

Temp unit: 91

Time format: 91

Trigger: 89

Video output: 91

Year: 90

Landriani, Marsilio: 141

Langley, Samuel P.: 144

## language

changing: 64

## Language

label: 91

## Laser LocatIR

classification: 103

description: 77

distance: 77

output power: 77

overriding: 86

## Laser LocatIR (continued)

type: 103

warning: 77

wavelength: 77

## laser pointer

overriding: 86

## laws

Planck's law: 147

Stefan-Boltzmann's formula: 150

Wien's displacement law: 148

## laying out

measurement area: 58

spot: 58

## LCD intensity

label: 89

## LCD protection: 1, 90

## leaks: 29

external: 19

internal: 19

## LED indicators

on battery charger: 96

## legal disclaimer: viii

## lens

cleaning: 99

focus ring: 66, 67

locking ring: 66, 67

removing: 67

## lens cap camera body

in packing list: 11

## Leopoldo Nobili: 143

## level

changing: 63, 84

## Local settings

command: 91

dialog box: 91

## locking ring: 66, 67

## low-slope commercial roofs: 19

## Ludwig Boltzmann: 150

**M**

## Macedonio Melloni: 142

## Manual adjust

command: 84

## Marsilio Landriani: 141

## Material Safety Data Sheets: 99

## Max Planck: 147

## Meas. mode

command: 83

dialog box: 83

label: 83

## measurement area

laying out: 58

## measuring conditions: 49

measuring season: 49  
measuring temperature: 58  
mechanical ventilation: 46  
Melloni, Macedonio: 142  
MENU/YES  
    function: 75  
    location: 74  
menus  
    Setup: 88  
menu system  
    canceling  
        selections: 83  
    confirming  
        selections: 83  
    displaying: 83  
    exiting: 83  
    navigating: 83  
messages: 80  
middle infrared band: 145  
minimum focus distance: 103  
Minute  
    label: 90  
moisture detection: 19  
    commercial & residential façades: 24  
    decks & balconies: 26  
    low-slope commercial roofs: 19  
    plumbing breaks & leaks: 29  
mold: 18  
Month  
    label: 90  
movement, air: 41  
MSDS: 99

## N

navigating  
    menu system: 83  
navigation pad  
    function: 75  
    location: 74  
near infrared band: 145  
Nobili, Leopoldo : 143  
non-blackbody emitters: 150  
NTSC/EIA: 103

## O

opening  
    file: 57  
    image: 57  
operating temperature range: 104  
operating time: 103

## P

packing list: 11  
    battery: 11  
    hand strap: 11  
    lens cap camera body: 11  
    power supply: 11  
    TrainIR CD: 11  
    USB cable: 11  
    video cable: 11  
PAL/CCIR: 103  
palette  
    changing: 86  
Palette  
    command: 86  
    dialog box: 86  
part numbers  
    1 120 987: 11  
    1 195 106: 11  
    1 195 128: 11  
    1 195 221: 11  
    1 195 494: 11  
    1 909 528: 11  
    1 909 775: 11  
patents: viii  
patents pending: viii  
physical specifications  
    size: 104  
    tripod mount: 104  
    weight: 104  
pin configuration  
    RS-232: 105  
    USB: 104  
Planck, Max: 147  
plumbing breaks: 29  
postal address: viii  
power supply: 93  
    in packing list: 11  
pressure  
    dynamic: 44  
    static: 44  
    total: 44  
pressure conditions: 43  
product warranty: viii  
Prompt img. desc.  
    label: 89  
PWR/NO  
    function: 75  
    location: 74

## Q

quality assurance: viii  
quality management system: viii

**R**

- radiators
  - cavity radiator: 146
  - graybody radiators: 151
  - selective radiators: 151
- reflected ambient temperature
  - changing: 85
  - explanation: 139
- Ref temp
  - label: 84
- relative humidity: 51
- removing
  - battery: 68
  - lens: 67
- requests for enhancement: 10
- residential façades: 24
- result table
  - screen object: 79
  - signs in: 79
- RFE: 10
- roofs, low-slope commercial: 19
- RS-232
  - interface: 105
  - pin configuration: 105

**S**

- safety precautions: 20
- Samuel P. Langley: 144
- SAVE/FRZ
  - function: 75
  - location: 74
- saving
  - file: 56
  - image: 56
- Scale
  - label: 88
- science, building: 39
- screen objects
  - result table: 79
  - selecting: 81
- season, measuring: 49
- Second
  - label: 90
- SEL
  - function: 75
  - location: 74
- selecting
  - screen objects: 81
- selections
  - canceling: 83
  - confirming: 83
- semi-transparent body: 153

- Settings
  - command: 88
  - dialog box: 88
- Setup
  - command: 88
  - menu: 88
- shock: 104
- Show graphics
  - command: 86
- Sir James Dewar: 144
- Sir William Herschel: 141
- size: 104
- sources of disruption: 41
- span
  - changing: 63, 84
- specifications
  - environmental
    - EMC: 104
    - encapsulation: 104
    - humidity: 104
    - operating temperature range: 104
    - shock: 104
    - storage temperature range: 104
    - vibration: 104
  - physical
    - size: 104
    - tripod mount: 104
    - weight: 104
  - technical: 103
- spectral range: 103
- spectrum
  - thermometrical: 142
- spot
  - laying out: 58
- Stefan, Josef: 150
- storage temperature range: 104
- surface temperature: 43
- switching off
  - camera: 55
- switching on
  - camera: 55
- system messages
  - status messages: 80
  - warnings: 80

**T**

- tcf
  - creating: 62
- technical specifications: 103
- technical support: 10
- temperature
  - measuring: 58
  - temperature, surface: 43

temperature range  
  operating: 104  
  storage: 104  
temperature unit  
  changing: 64  
temperature variations: 41  
Temp unit  
  label: 91  
testing, effects of: 40  
text file  
  creating: 62  
theory of thermography: 145  
thermograph: 143  
thermographic measurement techniques  
  introduction: 135  
thermographic theory: 145  
thermometrical spectrum: 142  
thermos bottle: 144  
time format  
  changing: 64  
Time format  
  label: 91  
trademarks: viii  
training: 53  
TrainIR CD  
  in packing list: 11  
transferring  
  text files: 62  
T Refl  
  changing: 85  
trigger  
  function: 76  
Trigger (label): 89  
tripod mount: 104  
turning off  
  camera: 55  
turning on  
  camera: 55  
tutorials  
  acquiring  
    image: 56  
  adjusting  
    focus: 67  
  changing  
    audible alarm: 61  
    color alarm: 60  
    date & time: 65  
    date format: 64  
    focus: 67  
    language: 64  
    level: 63  
    span: 63  
    temperature unit: 64

tutorials (*continued*)  
  changing (*continued*)  
    time format: 64  
    visual alarm: 61  
  deleting  
    file: 57  
    image: 57  
  freezing  
    image: 56  
  inserting  
    battery: 68  
  laying out  
    area: 58  
    spot: 58  
  opening  
    file: 57  
    image: 57  
  removing  
    battery: 68  
    lens: 67  
  saving  
    file: 56  
    image: 56  
  switching off  
    camera: 65  
  switching on  
    camera: 55

## U

unpacking: 11  
USB  
  interface: 104  
  pin configuration: 104  
USB cable  
  in packing list: 11

## V

ventilation, mechanical: 46  
vibration: 104  
video cable  
  in packing list: 11  
Video output  
  label: 91  
visual alarm  
  changing: 61

## W

warm-up time: 58  
warning messages: 80  
warnings  
  battery: 97  
  intensive energy sources: 1

warnings (*continued*)

interference: 1

Laser LocatIR: 77

radio frequency energy: 1

warranty: viii

weight: 104

Wien, Wilhelm: 148

Wilhelm Wien: 148

William Herschel: 141

wind conditions: 46

working with camera

adjusting

focus: 67

inserting

battery: 68

removing

battery: 68

lens: 67

**Y**

Year

label: 90

---

#### A note on the technical production of this manual

This manual was produced using XML – eXtensible Markup Language. For more information about XML, point your browser to:  
<http://www.w3.org/XML/>

Readers interested in the history & theory of markup languages may also want to visit the following sites:

- <http://www.gla.ac.uk/staff/strategy/information/socarcp/>
- <http://www.renater.fr/Video/2002ATHENS/P/DC/History/plan.htm>

#### A note on the typeface used in this manual

This manual was typeset using Swiss 721, which is Bitstream's pan-European version of Max Miedinger's Helvetica™ typeface. Max Miedinger was born December 24th, 1910 in Zürich, Switzerland and died March 8th, 1980 in Zürich, Switzerland.

10595503.a1



- 1926-30: Trains as a typesetter in Zürich, after which he attends evening classes at the Kunstgewerbeschule in Zürich.
- 1936-46: Typographer for Globus department store's advertising studio in Zürich.
- 1947-56: Customer counselor and typeface sales representative for the Haas'sche Schriftgießerei in Münchenstein near Basel. From 1956 onwards: freelance graphic artist in Zürich.
- 1956: Eduard Hoffmann, the director of the Haas'sche Schriftgießerei, commissions Miedinger to develop a new sans-serif typeface.
- 1957: The Haas-Grotesk face is introduced.
- 1958: Introduction of the roman (or normal) version of Haas-Grotesk.
- 1959: Introduction of a bold Haas-Grotesk.
- 1960: The typeface changes its name from Neue Haas Grotesk to Helvetica™.
- 1983: Linotype publishes its Neue Helvetica™, based on the earlier Helvetica™.

For more information about Max Miedinger, his typeface and its influences, please visit <http://www.rit.edu/~rlv5703/imm/project2/index.html>

**The following file identities and file versions were used in the formatting stream output for this manual:**

20234203.xml a29  
20234303.xml a25  
20234403.xml a32  
20234603.xml a20  
20234703.xml a34  
20234803.xml a21  
20234903.xml a11  
20235003.xml a34  
20235103.xml a17  
20235203.xml a18  
20235303.xml a13  
20236403.xml b9  
20236703.xml a32  
20236903.xml a10  
20237003.xml a8  
20237403.xml a11  
20237603.xml a22  
20248603.xml b12  
20254903.xml a25  
20255203.xml a4  
20273903.xml a2  
20275203.xml a3  
R0065.rcp a15  
config.xml a4



#### ■ BELGIUM

FLIR Systems  
Uitbreidingstraat 60-62  
B-2600 Berchem  
BELGIUM  
Phone: +32 (0)3 287 87 11  
Fax: +32 (0)3 287 87 29  
E-mail: [info@flir.be](mailto:info@flir.be)  
Web: [www.flirthermography.com](http://www.flirthermography.com)

#### ■ BRAZIL

FLIR Systems  
Av. Antonio Bardella, 320  
CEP: 18085-852 Sorocaba  
São Paulo  
BRAZIL  
Phone: +55 15 3238 8070  
Fax: +55 15 3238 8071  
E-mail: [paul.verminder@flir.com.br](mailto:paul.verminder@flir.com.br)  
E-mail: [flir@flir.com.br](mailto:flir@flir.com.br)  
Web: [www.flirthermography.com](http://www.flirthermography.com)

#### ■ CANADA

FLIR Systems  
5230 South Service Road, Suite #125  
Burlington, ON. L7L 5K2  
CANADA  
Phone: 1 800 613 0507 ext. 30  
Fax: 905 639 5488  
E-mail: [IRCana@flir.com](mailto:IRCana@flir.com)  
Web: [www.flirthermography.com](http://www.flirthermography.com)

#### ■ CHINA

FLIR Systems  
Beijing Representative Office  
Rm 203A, Dongwai Diplomatic Office  
Building  
23 Dongzhimenwai Dajie  
Beijing 100600  
P.R.C.  
Phone: +86 10 8532 2304  
Fax: +86 10 8532 2460  
E-mail: [beijing@flir.com.cn](mailto:beijing@flir.com.cn)  
Web: [www.flirthermography.com](http://www.flirthermography.com)

#### ■ CHINA

FLIR Systems  
Shanghai Representative Office  
Room 6311, West Building  
Jin Jiang Hotel  
59 Maoming Road (South)  
Shanghai 200020  
P.R.C.  
Phone: +86 21 5466 0286  
Fax: +86 21 5466 0289  
E-mail: [shanghai@flir.com.cn](mailto:shanghai@flir.com.cn)  
Web: [www.flirthermography.com](http://www.flirthermography.com)

#### ■ CHINA

FLIR Systems  
Guangzhou Representative Office  
1105 Main Tower, Guang Dong  
International Hotel  
339 Huanshai Dong Road  
Guangzhou 510098  
P.R.C.  
Phone: +86 20 8333 7492  
Fax: +86 20 8331 0976  
E-mail: [guangzhou@flir.com.cn](mailto:guangzhou@flir.com.cn)  
Web: [www.flirthermography.com](http://www.flirthermography.com)

#### ■ FRANCE

FLIR Systems  
10 rue Guynemer  
92130 Issy les Moulineaux  
Cedex  
FRANCE  
Phone: +33 (0)1 41 33 97 97  
Fax: +33 (0)1 47 36 18 32  
E-mail: [info@flir.fr](mailto:info@flir.fr)  
Web: [www.flirthermography.com](http://www.flirthermography.com)

#### ■ GERMANY

FLIR Systems  
Bernier Strasse 81  
D-60437 Frankfurt am Main  
GERMANY  
Phone: +49 (0)69 95 00 900  
Fax: +49 (0)69 95 00 9040  
E-mail: [info@flir.de](mailto:info@flir.de)  
Web: [www.flirthermography.com](http://www.flirthermography.com)

#### ■ GREAT BRITAIN

FLIR Systems  
2 Kings Hill Avenue - Kings Hill  
West Malling  
Kent, ME19 4AQ  
UNITED KINGDOM  
Phone: +44 (0)1732 220 011  
Fax: +44 (0)1732 843 707  
E-mail: [sales@flir.uk.com](mailto:sales@flir.uk.com)  
Web: [www.flirthermography.com](http://www.flirthermography.com)

#### ■ HONG KONG

FLIR Systems  
Room 1613-15, Tower 2  
Grand Central Plaza  
138 Shatin Rural Committee Rd  
Shatin, N.T.  
HONG KONG  
Phone: +852 27 92 89 55  
Fax: +852 27 92 89 52  
E-mail: [flir@flir.com.hk](mailto:flir@flir.com.hk)  
Web: [www.flirthermography.com](http://www.flirthermography.com)

#### ■ ITALY

FLIR Systems  
Via L. Manara, 2  
20051 Limbiate (MI)  
ITALY  
Phone: +39 02 99 45 10 01  
Fax: +39 02 99 69 24 08  
E-mail: [info@flir.it](mailto:info@flir.it)  
Web: [www.flirthermography.com](http://www.flirthermography.com)

#### ■ SWEDEN

FLIR Systems  
Worldwide Thermography Center  
P.O. Box 3  
SE-182 11 Danderyd  
SWEDEN  
Phone: +46 (0)8 753 25 00  
Fax: +46 (0)8 753 23 64  
E-mail: [sales@flir.se](mailto:sales@flir.se)  
Web: [www.flirthermography.com](http://www.flirthermography.com)

#### ■ USA

FLIR Systems  
Corporate headquarters  
27700A SW Parkway Avenue  
Wilsonville, OR 97070  
USA  
Phone: +1 503 498 3547  
Web: [www.flirthermography.com](http://www.flirthermography.com)

#### ■ USA (Primary sales & service contact in USA)

FLIR Systems  
USA Thermography Center  
16 Esquire Road  
North Billerica, MA. 01862  
USA  
Phone: +1 978 901 8000  
Fax: +1 978 901 8887  
E-mail: [marketing@flir.com](mailto:marketing@flir.com)  
Web: [www.flirthermography.com](http://www.flirthermography.com)

#### ■ USA

FLIR Systems  
Indigo Operations  
70 Castilian Dr.  
Goleta, CA 93117-3027  
USA  
Phone: +1 805 964 9797  
Fax: +1 805 685 2711  
E-mail: [sales@indigosystems.com](mailto:sales@indigosystems.com)  
Web: [www.corebyindigo.com](http://www.corebyindigo.com)

#### ■ USA

FLIR Systems  
Indigo Operations  
IAS Facility  
701 John Sims Parkway East  
Suite 2B  
Niceville, FL 32578  
USA  
Phone: +1 850 678 4503  
Fax: +1 850 678 4992  
E-mail: [sales@indigosystems.com](mailto:sales@indigosystems.com)  
Web: [www.corebyindigo.com](http://www.corebyindigo.com)