

Manual Supplement

Manual Title: 724/725/726 Calibration	Supplement Issue: 4
Part Number: 667581	Issue Date: 2/11
Print Date: September 1999	Page Count: 2
Revision/Date: 2, 2/06	

This supplement contains information necessary to ensure the accuracy of the above manual.



205 Westwood Ave
Long Branch, NJ 07740
1-877-742-TEST (8378)
Fax: (732) 222-7088
salesteam@Tequipment.NET

Change #1

On page 3, Table 1, add the following:

 N10140	Conforms to relevant Australian standards.
---	--

Change #2

On page 61, replace the Note with the following:

Note

For best accuracy at:

1st Cal Point: Use 8508A 200 Ω range, 4-wire, LOI On

2nd Cal Point: Use 8508A 2 k Ω range, 4-wire, LOI Off

On page 62, replace the Note with the following:


Note

For best accuracy at:

1st Cal Point: Use 8508A 2 k Ω range, 4-wire, LOI On

2nd Cal Point: Use 8508A 20 k Ω range, 4-wire, LOI Off

On page 65, replace Figure 34 with the following:

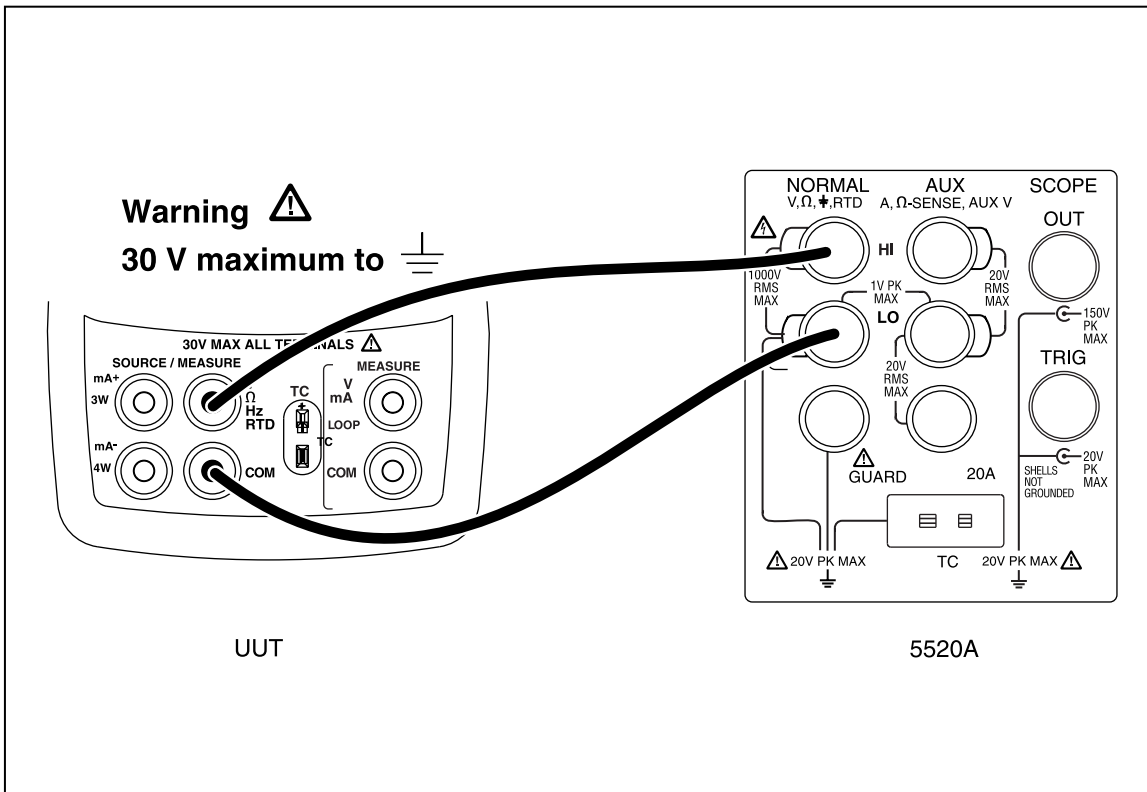

aa104.eps

On page 66, delete the second sentence in the third paragraph.

Change #3

On page 26, Table 8, under 5520A Outputs:

Change: 90.00 mV

To: 89.00 mV

Change #4

On page 67, Table 19:

Change:

18	Test lead, red	688051	1
	Test lead, black	688066	1

To:

18	Fluke-7XX Test Lead Set	3397308	1
----	-------------------------	---------	---




205 Westwood Ave
Long Branch, NJ 07740
1-877-742-TEST (8378)
Fax: (732) 222-7088
salesteam@Tequipment.NET