




## **MEMORY HICORDER 8826**

Recorders



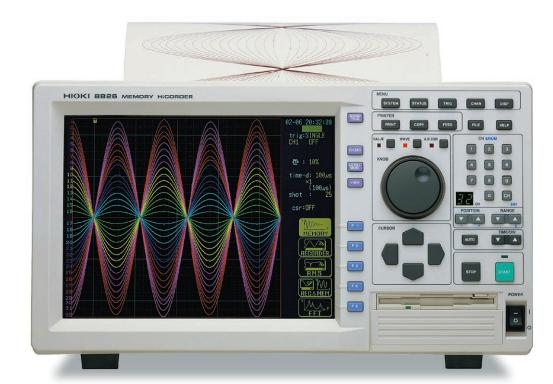




## 32-channel recorder with large display and wide printer installed

For use with the 8826, HIOKI provides a wide assortment of input units suitable for all types of signal measurement. The 8826 has a high waveform sampling rate of 1M sample/s which is carried out for all 32 channels simultaneously. In addition, the 8826 supports multichannel recording with wide 10.4-inch recording paper, a memory capacity of 64 megawords for all 32 channels (when expansion memory is installed), and a color LCD.







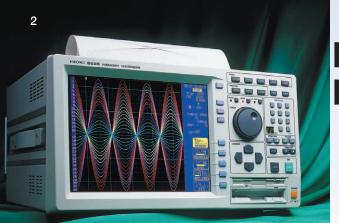

# Level Recorders Play a Vital Role in Many Areas of Modern Industry.

#### - Features -

#### • 10.4 inch color TFT display

The large, bright display shows waveforms for all channels (32 analog + 32 logic channels) in 12 colors, allowing easy visual identification. The display also greatly facilitates operation of the unit.

## Simultaneous measurement in up to 32 analog channels

Featuring the highest number of input channels in this class, the **8826** lets you simultaneously record in 32 analog + 32 logic channels. All analog inputs are isolated.

#### Built-in PC card slot

A PC card type III slot is provided as standard equipment. This makes it easy to archive measurement data. Besides its internal binary file format, the **8826** can also store data as ASCII files and display screen shots as BMP files.

#### Large-capacity memory

In the standard memory configuration, the **8826** can store a total of 16 mega-words. With expansion memory installed, capacity is a full 64 mega-words. This provides for up to 2 mega-words per channel when 32 channels are used. Even with high-speed sampling, long-term recording is possible.

#### CE Mark compliant

Complies with the EC directive determining safety standards in Europe (within the EU).

#### Internal sampling rate of 1 MS/s, 500 kS/s external sampling

The A/D converter that digitizes measurement signals operates at the high sampling rate of 1 M sample/s (1 µsec cycle). Resolution for the voltage axis is 12 bits. Sampling is carried out for all channels simultaneously.

#### Converts to text file used with a Wave viewer (supplied accessories, PC application software)

To open measurement data in PC applications such as Excel, the data must be converted to text data in the CSV format. The PC application software which comes standard in the package enables easy operation.

#### On-screen help

Explanation of button operations and many basic operations can be displayed on the screen with the provided online help function


#### Plug-in slots enhance versatility

The number of measurement channels can be matched to the application requirements by using plug-in modules. New types of converter amplifiers and other accessories to be introduced in the future will allow direct measurement of various physical quantities.

## **Digitally Process Test Data**

With a conventional pen recorder, even if all test data is written on the paper, usually only a small portion of the data is needed. However, to look for just a small important part requires very extensive search of the recording paper.


MEMORY HiCORDER 8826 stores and manages all waveform measurement data electronically. Furthermore, use of a PC for analysis.

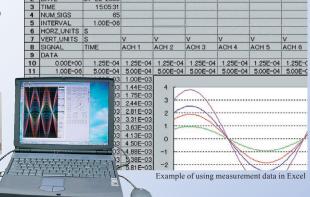


### - Application -

#### Load shutdown tests in power generation plants

For load shutdown tests in power generation plants, the pretrigger function can be used to measure and record waveforms before and after the test, enabling accurate analysis. The vernier function, which can be used to perform fine adjustment of amplitudes, is also a useful tool.




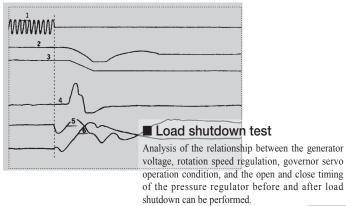


# Plant maintenance In plants, memory recorders are used to measure and record the operation of solenoid and control valves. Since the MEMORY HICORDER 8826 can simultaneously create X-Y plots, the relationship between flow and valve lift can also be observed.

#### ■ Ground fault line detection

To identify the ground fault line of transmission lines, measurement can be conducted using the trigger that combines a leak current meter and the recorder. This allows observation and recording of the waveform before and after ground faulting to identify the line.




Momentary loss of power in power-supply circuits can be recorded by using the voltage drop detection trigger, thus enabling accurate waveform recording of unexpected events.

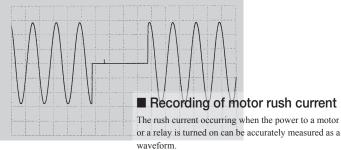

#### Vibration analysis

When installing rotating machinery, such as agitators, that create many vibrations, damping precautions are normally taken to ensure that the vibrations are not propagated directly to the floor surface. Analysis of the vibration damping measures and effects can be conducted by measuring the natural frequency and the transfer function.




#### FFT analysis function

FFT capability includes single-signal FFT for analyzing frequency components, two-signal FFT for transfer function analysis, and octave analysis for acoustic analysis. The source signal can be selected from waveform data captured by the memory recorder, and isolating required sections is also possible. (Number of data points: 1000 - 10000)

## Research and development of automobiles


In vehicle and engine running tests, the relationship among various parameters must be examined.

Multi-channel recorders are necessary to accomplish this.




#### Measurement of the damping of vibrations reaching the solid base from the rotating machinery


By striking the agitator with an impulse hammer, the vibrations propagated to the solid base can be measured by the acceleration speed pick up. Finding the transfer function can show to what extent specific frequencies are being dampened.



#### Measurement of the natural frequency of objects

Resonance phenomena can be avoided by ensuring that the natural frequency of an object is different from the vibration frequency of the surroundings. By striking the object with an impulse hammer and finding the transfer function, the natural frequency of the object can be found.





#### Analysis of engine characteristics

The pressure waveforms of injection pipes and fuelinjection pumps, etc., can be recorded and stored in the internal memory and then superimposed on a reference waveform for analysis.

## **High-Speed Response for Capturing Transient Events**

#### - Function Details -

## Large memory capacity allows long-term recording of high- speed data


In the standard configuration, the **8826** can store a total of 16 mega-words, and with memory expansion 64 mega-words, using internal solid-state memory. This provides ample capacity to store data for all 32 channels. The table at right shows possible recording times, according to the time axis setting and the number of channels in use. A reduction in the number of channels prolongs the recording time.

\* The table applies to the standard memory configuration. When the optional **MEMORY BOARD 9599** is installed, recording times are extended by a factor of 4 (from 16 mega-words/channel, 160,000 divisions for 4 channels to 2 mega-words/channel, 20,000 divisions for 32 channels).

#### ■ Memory segmentation function

When using the memory recorder function, the data memory can be divided into a maximum of 255 blocks. Data can be written sequentially to the memory blocks, and the waveform in a reference block and any other block can be superimposed and compared.

\* In the standard memory configuration (16 mega-words), the maximum number of blocks using the 32 channel setting is 127. When the memory expansion is installed, or when the channel setting is 4 to 16, the maximum number of blocks is 255.





#### ■ Zoom function \*In memory recorder function

To make the most of the large-capacity memory, it is possible to display a compressed waveform simultaneously with a magnified waveform. Since the 8826 is capable of storing a large amount of data, high-speed sampling is also possible for waveforms with a long duration. Accordingly, while observing the compressed image of the entire waveform, it is also possible to observe the magnified details of desired parts. Compressed display of a part of the entire waveform is also possible.

#### ■ Clock input for external sampling \*In memory recorder function


The sampling rate for the memory recorder can be controlled by the timing of an external clock signal. This is useful for example to collect data synchronized to the running cycle of an engine.



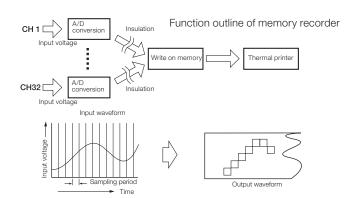


#### Recording Time on internal memory

Time axis         Sampling period         4-channel setting 4 MW/channel 40,000 DIV         32-channel setting 500 kW/channel 5,000 DIV           100μs/DIV         1μs         4 s         0.5 s           200μs/DIV         2μs         8 s         1 s           500μs/DIV         5μs         20 s         2.5 s           1ms/DIV         10μs         40 s         5 s           2ms/DIV         20μs         1 m 20 s         10 s           5ms/DIV         50μs         3 m 20 s         25 s           10ms/DIV         100μs         6 m 40 s         50 s           20ms/DIV         200μs         13 m 20 s         1 m 40 s           50ms/DIV         500μs         33 m 20 s         4 m 10 s           100ms/DIV         1ms         1 h 6 m 40 s         8 m 20 s           200ms/DIV         2ms         2 h 13 m 20 s         16 m 40 s           500ms/DIV         5ms         5 h 33 m 20 s         41 m 40 s           1s/DIV         10ms         11 h 6 m 40 s         1 h 23 m 20 s           2s/DIV         20ms         22 h 13 m 20 s         2 h 46 m 40 s           5s/DIV         50ms         2 days 7 h 33 m 20 s         6 h 56 m 40 s           10s/DIV         100ms <th colspan="6">,</th>	,					
200µs/DIV         2µs         8 s         1 s           500µs/DIV         5µs         20 s         2.5 s           1ms/DIV         10µs         40 s         5 s           2ms/DIV         20µs         1 m 20 s         10 s           5ms/DIV         50µs         3 m 20 s         25 s           10ms/DIV         100µs         6 m 40 s         50 s           20ms/DIV         200µs         13 m 20 s         1 m 40 s           50ms/DIV         500µs         33 m 20 s         4 m 10 s           100ms/DIV         1ms         1 h 6 m 40 s         8 m 20 s           200ms/DIV         2ms         2 h 13 m 20 s         16 m 40 s           500ms/DIV         5ms         5 h 33 m 20 s         41 m 40 s           1s/DIV         10ms         11 h 6 m 40 s         1 h 23 m 20 s           2s/DIV         20ms         22 h 13 m 20 s         2 h 46 m 40 s           5s/DIV         50ms         2 days 7 h 33 m 20 s         6 h 56 m 40 s           10s/DIV         100ms         4 days 15 h 6 m 40 s         13 h 53 m 20 s           30s/DIV         300ms         13 days 21 h 20 m         1 day 17 h 40 m           1min/DIV         0.6s         27 days 18 h 40 m	Time axis					
500μs/DIV         5μs         20 s         2.5 s           1ms/DIV         10μs         40 s         5 s           2ms/DIV         20μs         1 m 20 s         10 s           5ms/DIV         50μs         3 m 20 s         25 s           10ms/DIV         100μs         6 m 40 s         50 s           20ms/DIV         200μs         13 m 20 s         1 m 40 s           50ms/DIV         500μs         33 m 20 s         4 m 10 s           100ms/DIV         1ms         1 h 6 m 40 s         8 m 20 s           200ms/DIV         2ms         2 h 13 m 20 s         16 m 40 s           500ms/DIV         5ms         5 h 33 m 20 s         41 m 40 s           1s/DIV         10ms         11 h 6 m 40 s         1 h 23 m 20 s           2s/DIV         20ms         22 h 13 m 20 s         2 h 46 m 40 s           5s/DIV         50ms         2 days 7 h 33 m 20 s         6 h 56 m 40 s           10s/DIV         100ms         4 days 15 h 6 m 40 s         13 h 53 m 20 s           30s/DIV         300ms         13 days 21 h 20 m         1 day 17 h 40 m           1min/DIV         0.6s         27 days 18 h 40 m         3 days 11 h 20 m           2min/DIV         1.2s         <	100μs/DIV	1µs	4 s	0.5 s		
1ms/DIV         10μs         40 s         5 s           2ms/DIV         20μs         1 m 20 s         10 s           5ms/DIV         50μs         3 m 20 s         25 s           10ms/DIV         100μs         6 m 40 s         50 s           20ms/DIV         200μs         13 m 20 s         1 m 40 s           50ms/DIV         500μs         33 m 20 s         4 m 10 s           100ms/DIV         1ms         1 h 6 m 40 s         8 m 20 s           200ms/DIV         2ms         2 h 13 m 20 s         16 m 40 s           500ms/DIV         5ms         5 h 33 m 20 s         41 m 40 s           1s/DIV         10ms         11 h 6 m 40 s         1 h 23 m 20 s           2s/DIV         20ms         22 h 13 m 20 s         2 h 46 m 40 s           5s/DIV         50ms         2 days 7 h 33 m 20 s         6 h 56 m 40 s           10s/DIV         100ms         4 days 15 h 6 m 40 s         13 h 53 m 20 s           30s/DIV         300ms         13 days 21 h 20 m         1 day 17 h 40 m           1min/DIV         0.6s         27 days 18 h 40 m         3 days 11 h 20 m           2min/DIV         1.2s         55 days 13 h 20 m         6 days 22 h 40 m	200μs/DIV	2μs	8 s	1 s		
2ms/DIV         20µs         1 m 20 s         10 s           5ms/DIV         50µs         3 m 20 s         25 s           10ms/DIV         100µs         6 m 40 s         50 s           20ms/DIV         200µs         13 m 20 s         1 m 40 s           50ms/DIV         500µs         33 m 20 s         4 m 10 s           100ms/DIV         1ms         1 h 6 m 40 s         8 m 20 s           200ms/DIV         2ms         2 h 13 m 20 s         16 m 40 s           500ms/DIV         5ms         5 h 33 m 20 s         41 m 40 s           1s/DIV         10ms         11 h 6 m 40 s         1 h 23 m 20 s           2s/DIV         20ms         22 h 13 m 20 s         2 h 46 m 40 s           5s/DIV         50ms         2 days 7 h 33 m 20 s         6 h 56 m 40 s           10s/DIV         100ms         4 days 15 h 6 m 40 s         13 h 53 m 20 s           30s/DIV         300ms         13 days 21 h 20 m         1 day 17 h 40 m           1min/DIV         0.6s         27 days 18 h 40 m         3 days 11 h 20 m           2min/DIV         1.2s         55 days 13 h 20 m         6 days 22 h 40 m	500μs/DIV	5µs	20 s	2.5 s		
5ms/DIV         50μs         3 m 20 s         25 s           10ms/DIV         100μs         6 m 40 s         50 s           20ms/DIV         200μs         13 m 20 s         1 m 40 s           50ms/DIV         500μs         33 m 20 s         4 m 10 s           100ms/DIV         1ms         1 h 6 m 40 s         8 m 20 s           200ms/DIV         2ms         2 h 13 m 20 s         16 m 40 s           500ms/DIV         5ms         5 h 33 m 20 s         41 m 40 s           1s/DIV         10ms         11 h 6 m 40 s         1 h 23 m 20 s           2s/DIV         20ms         22 h 13 m 20 s         2 h 46 m 40 s           5s/DIV         50ms         2 days 7 h 33 m 20 s         6 h 56 m 40 s           10s/DIV         100ms         4 days 15 h 6 m 40 s         13 h 53 m 20 s           30s/DIV         300ms         13 days 21 h 20 m         1 day 17 h 40 m           1min/DIV         0.6s         27 days 18 h 40 m         3 days 11 h 20 m           2min/DIV         1.2s         55 days 13 h 20 m         6 days 22 h 40 m	1ms/DIV	10μs	40 s	5 s		
10ms/DIV         100µs         6 m 40 s         50 s           20ms/DIV         200µs         13 m 20 s         1 m 40 s           50ms/DIV         500µs         33 m 20 s         4 m 10 s           100ms/DIV         1 ms         1 h 6 m 40 s         8 m 20 s           200ms/DIV         2 ms         2 h 13 m 20 s         16 m 40 s           500ms/DIV         5 ms         5 h 33 m 20 s         41 m 40 s           1s/DIV         10ms         11 h 6 m 40 s         1 h 23 m 20 s           2s/DIV         20ms         22 h 13 m 20 s         2 h 46 m 40 s           5s/DIV         50ms         2 days 7 h 33 m 20 s         6 h 56 m 40 s           10s/DIV         100ms         4 days 15 h 6 m 40 s         13 h 53 m 20 s           30s/DIV         300ms         13 days 21 h 20 m         1 day 17 h 40 m           1min/DIV         0.6s         27 days 18 h 40 m         3 days 11 h 20 m           2min/DIV         1.2s         55 days 13 h 20 m         6 days 22 h 40 m	2ms/DIV	20μs	1 m 20 s	10 s		
20ms/DIV         200μs         13 m 20 s         1 m 40 s           50ms/DIV         500μs         33 m 20 s         4 m 10 s           100ms/DIV         1ms         1 h 6 m 40 s         8 m 20 s           200ms/DIV         2ms         2 h 13 m 20 s         16 m 40 s           500ms/DIV         5ms         5 h 33 m 20 s         41 m 40 s           1s/DIV         10ms         11 h 6 m 40 s         1 h 23 m 20 s           2s/DIV         20ms         22 h 13 m 20 s         2 h 46 m 40 s           5s/DIV         50ms         2 days 7 h 33 m 20 s         6 h 56 m 40 s           10s/DIV         100ms         4 days 15 h 6 m 40 s         13 h 53 m 20 s           30s/DIV         300ms         13 days 21 h 20 m         1 day 17 h 40 m           1min/DIV         0.6s         27 days 18 h 40 m         3 days 11 h 20 m           2min/DIV         1.2s         55 days 13 h 20 m         6 days 22 h 40 m	5ms/DIV	50μs	3 m 20 s	25 s		
50ms/DIV         500μs         33 m 20 s         4 m 10 s           100ms/DIV         1ms         1 h 6 m 40 s         8 m 20 s           200ms/DIV         2ms         2 h 13 m 20 s         16 m 40 s           500ms/DIV         5ms         5 h 33 m 20 s         41 m 40 s           1s/DIV         10ms         11 h 6 m 40 s         1 h 23 m 20 s           2s/DIV         20ms         22 h 13 m 20 s         2 h 46 m 40 s           5s/DIV         50ms         2 days 7 h 33 m 20 s         6 h 56 m 40 s           10s/DIV         100ms         4 days 15 h 6 m 40 s         13 h 53 m 20 s           30s/DIV         300ms         13 days 21 h 20 m         1 day 17 h 40 m           1min/DIV         0.6s         27 days 18 h 40 m         3 days 11 h 20 m           2min/DIV         1.2s         55 days 13 h 20 m         6 days 22 h 40 m	10ms/DIV	100μs	6 m 40 s	50 s		
100ms/DIV         1ms         1 h 6 m 40 s         8 m 20 s           200ms/DIV         2ms         2 h 13 m 20 s         16 m 40 s           500ms/DIV         5ms         5 h 33 m 20 s         41 m 40 s           1s/DIV         10ms         11 h 6 m 40 s         1 h 23 m 20 s           2s/DIV         20ms         22 h 13 m 20 s         2 h 46 m 40 s           5s/DIV         50ms         2 days 7 h 33 m 20 s         6 h 56 m 40 s           10s/DIV         100ms         4 days 15 h 6 m 40 s         13 h 53 m 20 s           30s/DIV         300ms         13 days 21 h 20 m         1 day 17 h 40 m           1min/DIV         0.6s         27 days 18 h 40 m         3 days 11 h 20 m           2min/DIV         1.2s         55 days 13 h 20 m         6 days 22 h 40 m	20ms/DIV	200μs	13 m 20 s	1 m 40 s		
200ms/DIV         2ms         2 h 13 m 20 s         16 m 40 s           500ms/DIV         5ms         5 h 33 m 20 s         41 m 40 s           1s/DIV         10ms         11 h 6 m 40 s         1 h 23 m 20 s           2s/DIV         20ms         22 h 13 m 20 s         2 h 46 m 40 s           5s/DIV         50ms         2 days 7 h 33 m 20 s         6 h 56 m 40 s           10s/DIV         100ms         4 days 15 h 6 m 40 s         13 h 53 m 20 s           30s/DIV         300ms         13 days 21 h 20 m         1 day 17 h 40 m           1min/DIV         0.6s         27 days 18 h 40 m         3 days 11 h 20 m           2min/DIV         1.2s         55 days 13 h 20 m         6 days 22 h 40 m	50ms/DIV	500μs	33 m 20 s	4 m 10 s		
500ms/DIV         5ms         5 h 33 m 20 s         41 m 40 s           1s/DIV         10ms         11 h 6 m 40 s         1 h 23 m 20 s           2s/DIV         20ms         22 h 13 m 20 s         2 h 46 m 40 s           5s/DIV         50ms         2 days 7 h 33 m 20 s         6 h 56 m 40 s           10s/DIV         100ms         4 days 15 h 6 m 40 s         13 h 53 m 20 s           30s/DIV         300ms         13 days 21 h 20 m         1 day 17 h 40 m           1min/DIV         0.6s         27 days 18 h 40 m         3 days 11 h 20 m           2min/DIV         1.2s         55 days 13 h 20 m         6 days 22 h 40 m	100ms/DIV	1ms	1 h 6 m 40 s	8 m 20 s		
1s/DIV         10ms         11 h 6 m 40 s         1 h 23 m 20 s           2s/DIV         20ms         22 h 13 m 20 s         2 h 46 m 40 s           5s/DIV         50ms         2 days 7 h 33 m 20 s         6 h 56 m 40 s           10s/DIV         100ms         4 days 15 h 6 m 40 s         13 h 53 m 20 s           30s/DIV         300ms         13 days 21 h 20 m         1 day 17 h 40 m           1min/DIV         0.6s         27 days 18 h 40 m         3 days 11 h 20 m           2min/DIV         1.2s         55 days 13 h 20 m         6 days 22 h 40 m	200ms/DIV	2ms	2 h 13 m 20 s	16 m 40 s		
2s/DIV         20ms         22 h 13 m 20 s         2 h 46 m 40 s           5s/DIV         50ms         2 days 7 h 33 m 20 s         6 h 56 m 40 s           10s/DIV         100ms         4 days 15 h 6 m 40 s         13 h 53 m 20 s           30s/DIV         300ms         13 days 21 h 20 m         1 day 17 h 40 m           1min/DIV         0.6s         27 days 18 h 40 m         3 days 11 h 20 m           2min/DIV         1.2s         55 days 13 h 20 m         6 days 22 h 40 m	500ms/DIV	5ms	5 h 33 m 20 s	41 m 40 s		
5s/DIV         50ms         2 days 7 h 33 m 20 s         6 h 56 m 40 s           10s/DIV         100ms         4 days 15 h 6 m 40 s         13 h 53 m 20 s           30s/DIV         300ms         13 days 21 h 20 m         1 day 17 h 40 m           1min/DIV         0.6s         27 days 18 h 40 m         3 days 11 h 20 m           2min/DIV         1.2s         55 days 13 h 20 m         6 days 22 h 40 m	1s/DIV	10ms	11 h 6 m 40 s	1 h 23 m 20 s		
10s/DIV         100ms         4 days 15 h 6 m 40 s         13 h 53 m 20 s           30s/DIV         300ms         13 days 21 h 20 m         1 day 17 h 40 m           1min/DIV         0.6s         27 days 18 h 40 m         3 days 11 h 20 m           2min/DIV         1.2s         55 days 13 h 20 m         6 days 22 h 40 m	2s/DIV	20ms	22 h 13 m 20 s	2 h 46 m 40 s		
30s/DIV         300ms         13 days 21 h 20 m         1 day 17 h 40 m           1min/DIV         0.6s         27 days 18 h 40 m         3 days 11 h 20 m           2min/DIV         1.2s         55 days 13 h 20 m         6 days 22 h 40 m	5s/DIV	50ms	2 days 7 h 33 m 20 s	6 h 56 m 40 s		
1min/DIV         0.6s         27 days 18 h 40 m         3 days 11 h 20 m           2min/DIV         1.2s         55 days 13 h 20 m         6 days 22 h 40 m	10s/DIV	100ms	4 days 15 h 6 m 40 s	13 h 53 m 20 s		
2min/DIV 1.2s 55 days 13 h 20 m 6 days 22 h 40 m	30s/DIV	300ms	13 days 21 h 20 m	1 day 17 h 40 m		
The state of the s	1min/DIV	0.6s	27 days 18 h 40 m	3 days 11 h 20 m		
5min/DIV 3.0s 138 days 21 h 20 m 17 days 8 h 40 m	2min/DIV	1.2s	55 days 13 h 20 m	6 days 22 h 40 m		
	5min/DIV	3.0s	138 days 21 h 20 m	17 days 8 h 40 m		



#### ■ Manipulation using the cursor

Use of the two cursors on the screen enables the user to read the time difference and potential difference.



#### - Function Details -

#### Real time save function \*supported in version 2.50 or later

The real time save function enables data to be saved to the PC card while waveform is being measured. The compressed waveform is displayed on the screen at real time. This function is valid at the recorder and memory function. Write to the PC card can be up to 1kS/s (=100ms/DIV) for 16 channels, or up to 500S/s (200ms/ DIV) for 32 channels. With the real time save function, data measured at the pre-determined sampling below the maximum sampling can be saved to the PC card at any time

In addition, since the same data is compressed along the time axis and displayed on the screen, you can check how recording is going. Compressed data is saved to the PC card for later retrieval.


#### Maximum continuous recording time using 256MB/1GB PC card

Time axis	Sampling period	256MB PC card	1GB PC card
100ms/DIV	1ms	2 h 13 m 12 s	8 h 53 m 03 s
200ms/DIV	2ms	2 h 13 m 10 s	8 h 53 m 00 s
500ms/DIV	5ms	5 h 32 m 55 s	22 h 12 m 20 s
1s/DIV	10ms	11h 5 m 30 s	1 day 20 h 23 m 50 s
2s/DIV	20ms	22 h 10 m 20 s	3 days 16 h 44 m 40 s
5s/DIV	50ms	2 days 7 h 20 m	9 days 5 h 30 m 00 s
10s/DIV	100ms	4 days 14 h 20 m	18 days 9 h 46 m 40 s
30s/DIV	300ms	13 days 15 h 10 m	54 days 14 h 50 m
1min/DIV	0.6s	26 days 19 h 10 m	107 days 11 h 20 m
2min/DIV	1.2s	51 days 19 h 40 m	208 days 5 h 40 m
5min/DIV	3.0s	117 days 21 h 10 m	208 days 8 h 00 m

Note: Saved at 16 channels for 100 ms/DIV, or at 32 channels otherwise.

Note: Maximum continuous recording time at MEM function, with time axis is 1 hour/DIV in REC function.

Note: Limit of maximum continuous recording time at MEM function is 208 days and 8 hours

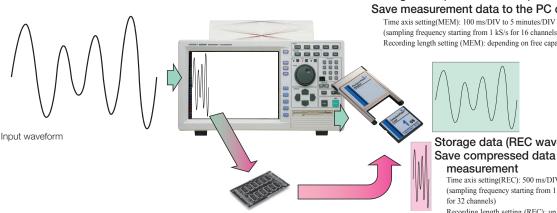

#### Storage data (MEM waveform):

#### Save measurement data to the PC card at real time

(sampling frequency starting from 1 kS/s for 16 channels or from 500S/s for 32 channels) Recording length setting (MEM): depending on free capacity of the PC card

#### Storage data (REC waveform): Save compressed data to the PC card after measurement

Time axis setting(REC): 500 ms/DIV to 1 hour/DIV

(sampling frequency starting from 1 kS/s for 16 channels or from 500S/s

Recording length setting (REC): up to 1000 DIV (or up to 5000 DIV with


#### Display data (REC waveform): compressed waveform is displayed on screen Compressed data is saved temporarily in the internal memory.

However, display time axis of REC data is 2 steps later than that of MEM data. The maximum recording time that can be set is determined by the free capacity of the PC card, and the time axis and recording length of MEM/REC. Nevertheless, since the maximum recording length of REC is fixed at 1000 DIV, or 5000 DIV if there is memory expansion, even if there is plenty of free capacity on the PC card, the recording time cannot exceed the value determined by REC time axis multiplied by 1000 DIV.

#### Trigger functions capable of monitoring all 32 channels

For all of the measurement functions, including record and memory recorder, triggers can be set on all 32 channels. In addition to a simple level trigger based on comparison with a single voltage value, the following trigger functions are also available:

- Window trigger based on 2 voltage values
- Voltage drop trigger for AC power lines
- Level trigger based on rms values
- Cycle trigger monitoring the rising edge of a voltage
- Pattern trigger monitoring the Hi/Low condition of a logic signal

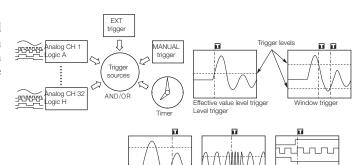

detection trigger

Period detection trigger

#### - Function Details -

#### Support for connection to PCs via Ethernet

The **8826** can be connected to Ethernet, a standard network protocol in the Internet age.


(using the optional LAN CARD and LAN COMMUNICATOR 9333. Caution: The optional LAN card has been discontinued so new LAN applications cannot be supported.)

For those who frequently analyze measurement data on PCs, this function offers a good match.


Note: Because LAN card, GP-IB card, and RS-232C card all use the same PC card slot of the 8826, when one of them is inserted into the PC card slot, other cards cannot be used at the same time.

Note: the LAN card, GP-IB card, and the RS-232C cards have been discontinued. Information provided herein only for existing customers of these applications.

■ Connect HiCORDER to departmental LAN (using TCP/IP communication protocol)

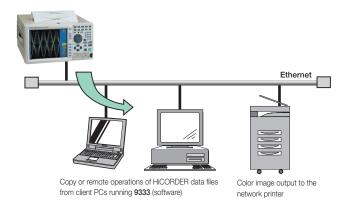

■ Save data to network server (using TCP/IP communication protocol)

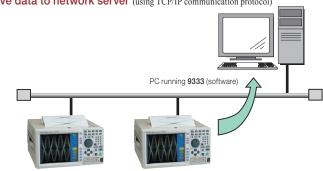


Copy measurement data files obtained from HiCORDER to PC on network

#### Offline data exchange with PCs

The supplied waveform viewer (PC application) can convert saved waveform data to text files (CSV format). For data storage, the FD/PC card (supplied as standard) can be used. This allows easy offline data exchange with PCs.

Note: The optional MO drive is discontinued.


\* In addition to HiCORDER's read/write native file (binary format), data can also be saved to text files (CSV format) which can be opened by PC spreadsheet applications, or waveform bitmap files (BMP format). However, because data saved in text files cannot be read by HiCORDER, it is recommended that text data conversion be performed on PCs.



#### **Scaling Functions**

Actual measurements usually involve parameters other than voltage. Various physical parameters such as speed, vibration and temperature commonly need to be recorded, and this signal data should be directly readable, without having to be manually converted. In such measurement conditions, the scaling function can be used to automatically convert to the desired parameter value. Additionally, waveform amplitude can be adjusted using the Variable Gain function.


In addition, if accurate input voltage amplitude measurement is not required, the amplitude can be intentionally modified with the Vernier Adjustment function.

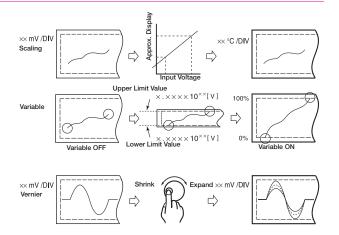

#### - Function Details -


#### **FFT** analysis functions

FFT capability includes single-signal FFT for analyzing frequency components, two-signal FFT for transfer function analysis, and octave analysis for acoustic analysis. The source signal can be selected from waveform data captured by the memory recorder, and isolating required sections is also possible. (Number of data points: 1,000 to 10,000)

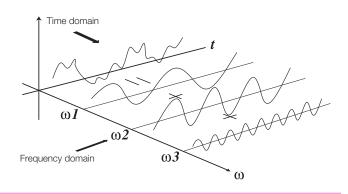

#### **Function outline of recorder (REC)**


The input signal is converted to digital form and displayed and printed in real time. The maximum chart speed is 20 mm/s (in the 500 ms/DIV range). After the end of measurement, measurement data for the last 2,000 DIV \*1 are still in memory and can be viewed with the back-scroll function or printed out again.

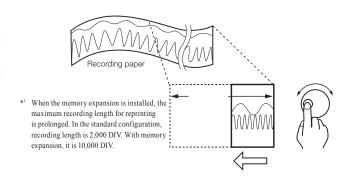

#### Effective value (RMS) recorder function

This function is designed exclusively for use on 50/60 Hz power supply lines and DC. High-speed sampling is applied to calculate the rms value from the waveform data \*2, and the result is recorded as a graph.

\*2 Using fixed 200 μs sampling, data for two waveforms are captured for calculating the rms value. This process is repeated 20 times per second, resulting in high-speed response that is 10 times faster than that of a digital tester or similar (using a 2-second update rate).




## Simultaneous execution of up to 16 mathematical functions \* In MEM function

Available waveform processing functions include all arithmetic operations as well as differentiation, integration, and other functions whose results can be displayed as waveforms. Up to 16 functions can be set.

#### Waveform parameter processing \* In MEM function


13 types of parameters such as maximum value and minimum value can be selected for processing. For simultaneous operation in all 32 analog channels, up to 4 parameters are possible.

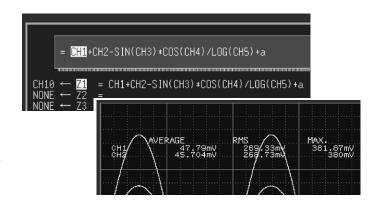

#### Waveform evaluation \* For MEM function and FFT analysis functions

After defining a reference waveform bounding area, it is possible to check whether waveforms go outside this reference area. As opposed to simple level-based triggering, even complex waveforms can be evaluated quickly and reliably, because both the level direction and the time axis direction are taken into consideration.


\* Registered patent No. 2028013 in Japan

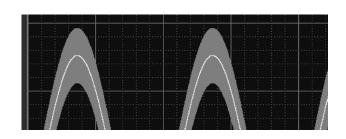


## **Example Printouts & Screen**

(WIDE mode, actual size)


B4 size paper (264 mm width) allows full-size mixed printing or division into up to 16 sections

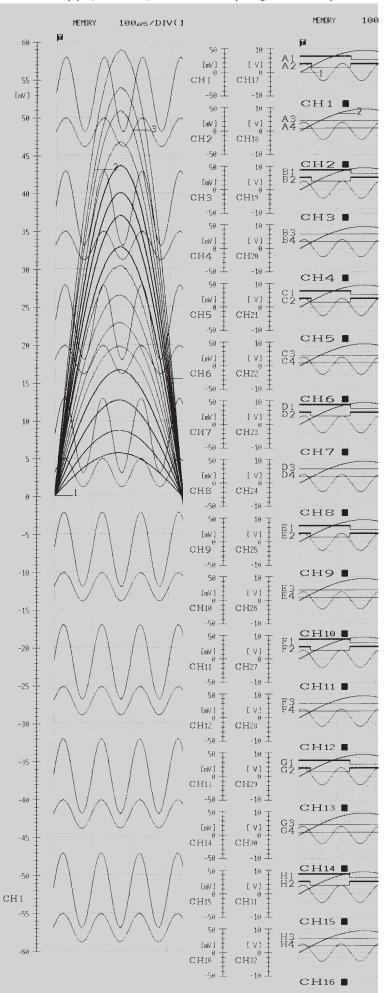

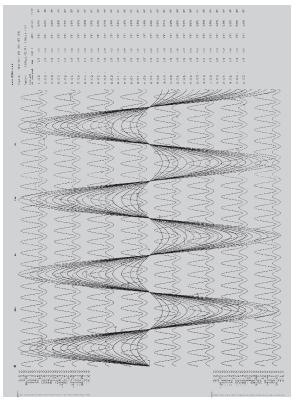

#### Example of B4 report output

Screen image output at high resolution, B4 size.

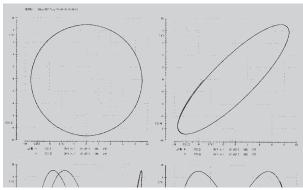


#### Example of X-Y plotting

Time-axis waveforms of each input channel can be defined on vertical and horizontal axes to create X-Y plots.

(time)	CH1 CH17	CH2 CH18	CH3 CH19	CH4 CH20	CH5 CH21	CH
0 s	125.√ 2.9625 V	البر125 2.95 V	البر187.5 V 2.95 V	62.5⊅V 2.9625 \	125,µV 2.9625	V
1 <i>µ</i> s	500.W 3.1 V	500,W 3.0875 V	562.5V 3.0875 V	437.5س 3.1 \	500 JV 7 3.1	V
2 <i>u</i> s	1mV 3.225 V	1mV 3.2125 V	1.0625mV 3.2125 V	937.5 <sub>4</sub> V 3.225 \	1mV / 3.225	V
3µs	1.4375mV	1.4375mV	1.5mV	1.375mV	1.4375mV	1.


#### **Example of Logging output**


This prints the instantaneous numerical value for each sample.




#### ■ Online help and error indication

Simply pressing the help key will bring up relevant information on functions and operation steps. If an error has occurred, the reason for it is also displayed to ease operation.







#### ■ Main unit

Logic


probe connection (for 8 units) PC card	Į
--	---

Rasic specifications	8826 (max. 16 input modules)	Memory functi	one	
Dasic specifications		Memory functi		
Input type/number of channels	Plug-in input modules  Max. 32 analog ch's+32 logic ch's (Isolated analog channels, isolated input and frame, logic has common GND)	Time axis	100µs to 5min/DIV, 20 ranges or external sampling, time axis resolution 100 points/DIV, time axis zoom: ×2 to ×10 in 3 stages, compression: 1/2 to 1/10,000 in 12 stages	
Measurement	MEM (high-speed recording), REC (real-time recording), RMS (50/60Hz, or DC only),	Sampling rate	1/100 of time axis ranges (minimum sampling period 1µs)	
functions	REC & MEM (include the Real-time save function), FFT		Max. 500kS/s (minimum sampling period 2µs)	
Maximum sampling rate	1 MS/second (1µs, all channels simultaneously) External sampling (500kS/second, 2µs)	Recording length	Settable in 1 DIV steps, 20 to 40,000 DIV*1  *1 Depending on the number of channels in use. With memory expansion max. 160,000 DIV.	
Memory capacity	16 Mwords total: (12 analog bits + 4 logic bits) × 4 Mwords/channel (4 channels used) to (12 analog bits + 4 logic bits) × 500 kwords/channel (32 channels used)	Pre-trigger	Can record data from before the trigger point, 0 to 100% or -95% of recording length; 15 settings	
Data storage media	* Memory capacity can be expanded 4 times.  PC Card Type III slot × 1: up to 2 GB (Flash ATA)  FD drive × 1: 1.44 MB, 1.2 MB, 720 KB, MS-DOS format  File format: Binary, text, BMP  Note: The optional MO UNIT 9598 is discontinued	Other functions	waveform processing, waveform parameter processing, waveform averaging, memory segmentation (up to 255 segments), logging (numerical printout), X-Y waveform plot, voltage axis zoom ×2 to ×10, 3 settings, compression 1/2, zoom, variable display, graph superimposition, waveform judgment function	
Backup functions	Clock and setting conditions: battery life of at least 10 years	Recorder func	tions (time axis waveform and X-Y format)  20ms to 1 hr/DIV with 16 ranges, time axis resolution 100 points/	
(at 25°C/77°F)  External control	Waveform data: none  Terminal board: external trigger input, trigger output, waveform		DIV, time axis compression: 1/2 to 1/500 in 8 stages	
connectors	judgment output, external start/stop, print input, external sampling input. <b>GP-IB:</b> using the 9558 GP-IB card. <i>Note: Model 9558 has been</i>	Time axis	At 20ms to 200ms/DIV, printing in real time is not possible, but waveform data are stored in memory and can be monitored on screen. Data are stored for 2,000 divisions before the end of measurement. At recording length settings other than "Continuous", the printer can be used simultaneously, for follow-up printing of waveforms.	
	discontinued; new GP-IB applications are not supported.  DS 232Cy using the 0557 DS 232C and Natural Model 0557 has been	Sampling rate	1µs to 100ms; 6 settings (selectable from 1/100 or less of time axis)	
Interfaces (option)	RS-232C: using the 9557 RS-232C card. Note: Model 9557 has been discontinued; new RS-232C applications are not supported.  LAN: using a HIOK1-tested LAN card. Note: The LAN card from HIOKI has been discontinued; new LAN applications are not supported.	Recording length	Settable in 1 DIV steps, 25 to 2,000 DIV*2, or "Continuous"*3  At X-Y format: only continuous for X-Y plotting  *2 Measure all channels. 10,000 DIV at expanded memory.  *3 When time 20 ms - 200 ms/DIV and printer is ON, continuous is not available.	
	supported.  Operation: +5°C (41°F) to +40°C (104°F), 35% to 80% rh	X-Y sampling period	500µs; fixed (dot), 500µs to 18ms (line)	
Environmental conditions (no condensation)	Storage: -10°C (14°F) to +50°C (122°F), 20% to 90% rh	X-Y axis resolution	20dots/DIV (display), 100dots (horizontal) × 80 dots (vertical)/DIV (printer)	
Compliance standard	<b>Safety:</b> EN61010 <b>EMC:</b> EN61326, EN61000-3-2, EN61000-3-3	Waveform memory	Store data for most recent 2,000 DIV (10,000 DIV at expanded memory) in memory. Backward scrolling and re-printing available.	
Power requirements	100 to 240V AC (50/60 Hz)	Other functions	logging (numerical printout), additional recording (recording is resumed without overwriting previous data), voltage axis magnification ×2 to ×10; 3 settings, compression 1/2; 1 setting, variable display.	
Power consumption (with 8936 full loaded)	300VA, max. for 100V AC (100VA with the printer off)	RMS Recorder	Function (for 50/60 Hz and DC)	
Dimensions and	401mm (15.79in) W × 235mm (9.25in) H × 382mm (15.04in) D, 11kg	Time axis	5s to 1 hr/DIV; 9 settings, time axis compression 1/2 to 500; 8 settings	
mass	(388.0oz.) (main unit only)	Sampling rate	200µs fixed (20 rms datas/s)	
Supplied	Instruction Manual × 1, Power cord × 1, Printer paper ×1, Protective	RMS calculation accuracy	±3% f.s.	
accessories	cover x1, Roll paper attachment x2, PC card protector x1, Application Disk (Wave Viewer Wv, Communication Commands table) x1	Recording length	Settable in 1 DIV steps, 25 to 2,000 DIV*4 (10,000 DIV at expanded memory) or "Continuous"  *4 Measure all channels.	
Print/display s		Waveform memory	Store data for most recent 2,000 DIV (10,000 DIV at expanded memory)	
Display	10.4 inch TFT color LCD, with English/Japanese selector (640 × 480 dots)	wavelorm memory	in memory. Backward scrolling and re-printing available.  logging (numerical printout), additional recording (recording is resumed	
Recording paper	264 mm (10.39 in) × 30 m (98.4 ft), thermal paper roll	Other functions	without overwriting previous data), voltage axis magnification ×2 to ×10; 3 settings, compression 1/2; 1 setting, variable display.	
Recording width	20/24 divisions for full scale, 1 DIV = 10 mm (0.39 in) (80 dots)  10 rows/mm (250 rows/in) * 20 rows/mm (500 rows/in with the memory	Auxiliary Funct		
Paper feed density	recorder's smooth print function	Adamai y i dilo	Printing of settings including input range, trigger time, etc, cursor	
Recording speed	Max. 25 mm/s (0.98 in/s)		measurement, scaling, free comment input, screen hard copy, start	
Trigger function	ons	General	condition retention, auto setup, auto saving, remote control, auto ranging, view function, online help, key lock, list printing, level	
Trigger sources	CH1 to CH32 (analog), CHA to CHH (logic), external, timer, manual (either ON or OFF for each source), logical AND/OR of sources		monitor, etc.  Scaling: Translation of amplitude gradation only	
	Level: Digital setting of voltage. Triggered when set value is exceeded in UP or DOWN direction.	Scaling	Variable: Arbitrary setting of the upper and lower limit of the waveform display range	
	Window: When entering or exiting a level range defined by upper or lower limit	Vernier function	Allows precision adjustment of input voltage.	
Trigger types (analog)	Voltage drop: Only for AC power lines. Triggered when the peak voltage falls below setting value  Period: When rising or falling edge of set voltage does not fall within cycle range  RMS level: Only for DC and AC power lines. Triggered when rms	Waveform judgment function (MEM function) (FFT function)	Type: Area judgment using reference waveform for time axis waveform, X-Y plot, or FFT display. Parameter judgment for waveform parameter processing. Judgment output: pass/fail output, open-collector 5V voltage output	
value crosses set value in UP or DOWN direction  Level setting resolution		Waveform parameter	Average value, effective (rms) value, peak to peak value, maximum value, time to maximum value, minimum value, time to minimum	
		calculation (MEM function)	value, time to maximum value, imminum value, time to minimum value, period, frequency, rise time, fall time, standard deviation, area value, and X-Y area value.	
(logic) Trigger filter	logical sum (OR) set for 4 channels  OFF, setting range 0.1 to 10.0 DIV; 9 ranges (MEM, MEM waveform in		(Maximum possible calculation up to 1,000 DIV, or 5,000 DIV at expanded memory; accuracy is within the tolerance of the input module.)	
(analog/logic) REC & MEM function, FFT function), ON (10 ms)/OFF (REC function)		Waveform processing calculations	Four arithmetic operations, absolute value, exponentiation, common logarithm, square root, moving average, differentiation	
Other functions	Pre-trigger function to capture pre- and post-trigger waveform, trigger output (active Low and open collector 5 voltage output), Start & stop trigger in REC function	(MEM function)	once and twice, integration once and twice, parallel displacement along the time axis, trigonometric functions, reverse trigonometric functions. 16 arbitrary operational equation.	

#### ■ Main unit specifications

REC & MEM fu	nctions (version 2.00 or later. Real-time save function: version 2.20 or later)			
Time axis (REC)	20ms to 1hour/DIV; 16 settings, 1 DIV = 100 samples, time axis compression 1/2 to 1/500, 8 settings  Note: Sampling period 1/100 of time axis range at memory recorder function			
Time axis (MEM)	100 $\mu$ s to 5 minutes/DIV; 20 settings, 1 DIV = 100 samples, time axis zoom ×2 to ×10; 3 settings, compression 1/2 to 1/10,000, 12 settings Note: Sampling period 1/100 of time axis range (min. 1 $\mu$ s)			
Recording length	REC: Settable in 1-division steps, 25 to 1,000 DIV (5,000 DIV at expanded memory), or continuous  MEM: Settable in 1-division steps, 25 to 2,000 DIV (10,000 DIV at expanded memory)			
Trigger source	REC: timer trigger, or OFF MEM: CH1 to CH32 (analog), logic A to H, or external trigger			
Real-time save functions Note: Used with the PC card, firmware version 2.50 or later	Time axis: 100ms/DIV to 5 minutes/DIV (less than 16 channels), 200ms/DIV to 5 minutes/DIV (more than 17 channels) (1 DIV=100 samples, sampling period 1/100 of time axis range)  Save destination: PC card, or MO disk in the optional MO UNIT 9598  Save time: Depending on free capacity of the PC card, or MO disk  Trigger: trigger settings are not applicable to the MEM waveform, and the start of MEM waveform recording coincides with the start of the REC waveform.  Time axis at REC: 500ms/DIV to 1 hour/DIV (less than 16 channels), 1s/DIV to 1 hour/DIV (more than 17 channels) (1 DIV=100 samples, sampling period 1/100 of time axis range)			
Other functions	Only REC waveform is output when printer output is started, reprinting of stored REC waveform data (last 1,000 DIV; or 5,000 DIV at expanded memory), Additional recording function (recording is resumed without overwriting previous data), variable display			
FFT functions	version 2.00 or later.)			
Analysis mode	Storage waveform, Linear spectrum, RMS spectrum, Power spectrum, Cross-power spectrum, Auto-correlation function, Histogram, Transfer function, Cross-correlation function, Unit-impulse response, Coherence function, Octave analysis			
Analysis channels	1 or 2 selected channels out of all analog channels			
Frequency range	133mHz to 400kHz, External, (resolution 1/400, 1/800, 1/2000, 1/4000)			
Number of sampling points	1000, 2000, 5000, 10000 points			
Windows	Rectangular, Hanning, Exponential			
Averaging function	Time axis / frequency axis simple averaging, exponential averaging, peak hold			

#### ■ Input unit specifications (sold separately)



ANALOG UNIT	(Accuracy at 23 ±5°C/73 ±9°F, 35 to 80 % rh after 30 minutes of warm-up time and zero-adjust; accuracy guaranteed for 1 year)			
Measurement functions	Number of channels: 2, for voltage measurement			
Input connectors	Isolated BNC connector (input impedance IMQ, input capacitance 30pF), Max. rated voltage to earth: 370V AC, DC (with input isolated from the unit, the maximum voltage that can be applied between input channel and chassis and between input channels without damage)			
Measurement range	5mV to 20V/DIV, 12 ranges, full scale: 20DIV, AC voltage for possible measurement/display using the memory function: 280V rms, low-pass filter: 5Hz/500Hz/5kHz/100kHz			
Measurement resolution	1/80 of measurement range (using 12-bit A/D conversion; installed in the 8826)			
Highest sampling rate	1MS/s (simultaneous sampling in 2 channels)			
Accuracy	DC amplitude: ±0.4% of full scale, zero position: ±0.1% of full scale (after zero adjustment)			
Frequency characteristics	DC to 400kHz ±3dB, with AC coupling: 7Hz to 400kHz ±3dB			
Input coupling	DC, GND, AC			
Max. allowable input	400V DC (the maximum voltage that can be applied across input pins without damage)			



FFT ANALOG	UNIT 8938 (Accuracy at 23 ±5°C/73 ±9°F, 35 to 80 % rh after 30 minutes of warm-up time and zero-adjust; accuracy guaranteed for 1 year)		
Measurement functions	Number of channels: 2, for voltage measurement		
Anti-aliasing filter	Integrated filter for suppressing aliasing distortion caused by FFT processing (automatic cutoff frequency setting/OFF)		
Other functions	Other specifications same as the ANALOG UNIT 8936		

Dimensions and mass: approx. 170 (6.69in) W  $\times$  20 (0.79in) H  $\times$  148.5 (5.85in) D mm, approx. 300 g (10.6 oz) Accessories: None



VOLTAGE/TEMP UNIT 8937 (Accuracy at 23 ±5°C/73 ±9°F, 35 to 80 % rh after 1 hour of warm-up time and zero-adjust; accuracy guaranteed for 1 year)			
Measurement functions	Number of channels: 2, for voltage measurement/temperature measurement with thermocouple		
Input connectors	Voltage input: metallic BNC connector (input impedance IMQ, input capacitance 50pF), thermocouple input: terminal connector (input impedance min. 51MQ), Max. rated voltage to earth: 30Vrms or 60V DC (with input isolated from the unit, the maximum voltage that can be applied between input channel and chassis and between input channels without damage)		
Voltage measurement range	500μV to 2V/DIV, 12 ranges, full scale: 20DIV, low-pass filter: 5Hz/ 500Hz/ 5kHz/ 100kHz, Measurement resolution: 1/80 of measurement range (using 12-bit A/D conversion; installed in the 8826)		
Temperature measurement range	10°C to 100°C/DIV, 4 ranges, full scale: 20DIV, low-pass filter: 5Hz/500Hz, Measurement resolution:1/80 of measurement range (using 12-bit A/D conversion; installed in the 8826)		
Thermocouple range	K: -200 to 1350°C, E: -200 to 800°C, J: -200 to 1100°C, T: -200 to 400°C, N: -200 to 1300°C, R: 0 to 1700°C, S: 0 to 1700°C, B: 300 to 1800°C, Reference junction compensation: internal/ external (switchable)		
Highest sampling rate	Voltage input: 1MS/s, Temperature measurement: 4kS/s (simultaneous sampling in 2 channels)		
Accuracy	Voltage input: DC amplitude ±0.4% of full scale, zero position ±0.15% of full scale, Temperature measurement (K, E, J, T, N): ±0.1% of full scale ±1°C, ±0.1% of full scale ±2°C (-200 to 0°C), (R, SS): ±0.1% of full scale ±3°C, (B): ±0.1% of full scale ±4°C (400 to 1800°C), Reference junction compensation accuracy: ±0.1% of full scale ±1.5°C (internal reference junction compensation)		
Frequency characteristics	Voltage input: DC to 400 kHz +1/-3dB Temperature measurement: DC to 1kHz +1/-3dB		
Input coupling	DC, GND, AC		
Max. allowable input	30Vrms or 60V DC (the maximum voltage that can be applied across input pins without damage)		

Dimensions and mass: approx. 170 (6.69in)  $W\times20$  (0.79in)  $H\times148.5$  (5.85in) D mm, approx. 250 g (8.8 oz) Accessories: Conversion cable × 2



STRAIN UNIT 8	(Accuracy at 23 ±5°C/73 ±9°F, 35 to 80 % rh after 1 hour of warm-up time and auto-balance; accuracy guaranteed for 1 year)			
Measurement functions	Number of channels: 2, for distortion measurement (electronic auto-balancing, balance adjustment range within $\pm 10000 \mu s$ )			
Input connectors	Via conversion cable, TAJIMI PRC03-12A10-7M10.5, Max. rated voltage to earth: 30Vrms or 60V DC (with input isolated from the unit, the maximum voltage that can be applied between input channel and chassis and between input channels without damage)			
Suitable transducer	Strain gauge converter, bridge impedance: $120\Omega$ to $1k\Omega$ , bridge voltage $2 \pm 0.05 V$			
Measurement range	20με to 1000με/DIV, 6 ranges, full scale: 20DIV, low-pass filter: 10Hz/30Hz/300Hz/3kHz			
Measurement resolution	1/80 of measurement range (using 12-bit A/D conversion; installed in the 8826)			
Highest sampling rate	1MS/s (simultaneous sampling in 2 channels)			
Accuracy After auto-balancing	DC amplitude: ±(0.5% of full scale +2με), zero position: ±0.5% of full scale			
Frequency characteristics DC to 20 kHz +1/-3dB				
Max. allowable input	10V DC + AC peak (the maximum voltage that can be applied across input pins without damage)			





CONVERSION CABLE 9319 (to connect 3273, 3273-50 and 8940)

Dimensions and mass: approx. 170 (6.69in) W × 20 (0.79in) H × 148.5 (5.85in) D mm, approx. 300 g (10.6 oz) Accessories: None

F/V UNIT 8940	(Accuracy at 23 $\pm$ 5°C/73 $\pm$ 9°F, 35 to 80 % rh after 30 minutes of warm-up time and zero-adjust; accuracy guaranteed for 1 year)		
Measurement functions	Number of channels: 2, for voltage input based frequency measurement, integration, pulse duty ratio, current (with optional clamp-on sensor), and voltage measurement		
Input connectors	Metallic BNC connector (input impedance $IM\Omega$ , input capacitance 60pF), sensor connector (dedicated connector for clamp-on sensor via conversion cable, common ground with recorder), $Max$ . rated voltage to earth: $30V Tms$ or $60V DC$ (with input isolated from the unit, the maximum voltage that can be applied between input channel and chassis and between input channels without damage)		
Compatible current sensors	9270, 9271, 9272, 9277, 9278, 9279, 3273, 3273-50		
Measurement range	Frequency: DC to 100kHz, with 0.05Hz to 5kHz/DIV, 11 ranges, 5 (r/min) to 500 (r/min)/DIV, 5ranges, P50Hz (40 to 60Hz), P60Hz (50 to 70Hz) *Power line frequency measurement requires the DIFFERENTIAL PROBE 9322 or PT 9303, Accuracy: ±0.2% of full scale (except 10kHz/DIV range), ±0.7% of full scale (10kHz/DIV range), ±0.32Hz (P50Hz, P60Hz range)  Integration: DC to 90kHz, with 5counts to 500kcounts/DIV, 11 ranges Pulse duty ratio: 10Hz to 100kHz, with 100% of full scale, 1 range, Accuracy: ±1% of full scale (10Hz to 10kHz)  Threshold: -10 to +10V (settable in 0.2V steps)  Full scale: 10DIV, Max. allowable input: 30Vrms or 60V DC (the maximum voltage that can be applied across input pins without damage)		
Measurement range	Voltage: 0.5mV to 2V/DIV, 12 ranges Current: 5mA to 100A/DIV, 10 ranges, using current sensor (powered from the 8940, max. 4 sensors total) DC amplitude accuracy: ±0.4% of full scale, zero position ±0.15% of full scale (current measurement accuracy dependent on sensor accuracy/characteristics) Frequency characteristics: DC to 400kHz ±3dB Full scale: 20DIV, Max. allowable input: 30Vrms or 60V DC (the maximum voltage that can be applied across input pins without damage)		
Measurement resolution	1/80 of measurement range (installed in the 8826, excluding current range when using 9279)		
Highest sampling rate	1MS/s (simultaneous sampling in 2 channels), (frequency/duty ratio measurement: 1.125µs cycle)		
Other functions	Voltage input pull-up: ON (10kΩ)/OFF, input coupling: DC, GND, AC		

Dimensions and mass: approx. 170 (6.69in) W  $\times$  20 (0.79in) H  $\times$  148.5 (5.85in) D mm approx. 310 g (10.9 oz) Accessories: None

	the E		-	15	
1,	. 6	*	1	Ti.	(0)

CHARGE UNIT	(Accuracy at 23 ±5°C/73 ±9°F, 35 to 80 % rh after 1 hour of warm-up time and zero-adjust; accuracy guaranteed for 1 year)						
Measurement functions	Number of channels: 2, for acceleration measurement						
Input connectors	Voltage input/integrated preamplifier input: metallic BNC connector (for voltage input: input impedance $1M\Omega$ , input capacitance $200pF$ or less) Charge input: miniature connector (#10-32 UNF) Max. rated voltage to earth: $30Vrms$ or $60V$ DC (with input isolated from the unit, the maximum voltage that can be applied between input channel and chassis and between input channels without damage)						
Suitable transducer	Charge input: Charge-output type piezoelectric acceleration pick-up sensor Internal preamp input: Acceleration pick-up sensor with an internal preamp						
Measurement range Charge input (miniature connector) Internal pre-amp input (BNC connector)	$50m~(m/s^3)/DIV~to~10k~(m/s^3)/DIV,~12~ranges \times 6~types,~charge~input~sensitivity:~0.1~to~10~pC/(m/s^3),~integrated~pre-amplifier~input:~0.1~to~10~mV/(m/s^3),~amplitude~accurracy:~\pm 2%~of~full~scale,~frequency~characteristics:~1~to~50kHz,~+1/-3dB,~low-pass~filter:~500Hz/5kHz,~pre-amplifier~drive~power~source:~2mA~\pm 20\%,~\pm 15V~\pm 5\%,~maximum~input~charge:~\pm 500pC~(high-sensitivity~setting,~6~ranges),~\pm 50000pC~(low-sensitivity~setting,~6~ranges),~\pm 50000pC~(low-sensitivity~setting,~6~ranges)$						
Measurement range Voltage input (BNC connector)	$500\mu V$ to $2V/DIV, 12$ ranges, <b>DC amplitude accuracy:</b> $\pm 0.4\%$ of full scale, <b>frequency characteristics:</b> DC to $400kHz, \pm 1/-3$ dB, <b>low-pass filter:</b> $5Hz/500Hz/5kHz/100kHz,$ <b>input coupling:</b> DC, GND, AC, <b>Max. allowable input:</b> $30Vrms$ or $60V$ DC						
Measurement resolution	1/80 to 1/32 of measurement range (depending on measurement sensitivity; installed in the 8826)						
Highest sampling rate	1MS/s (simultaneous sampling in 2 channels)						
Anti-aliasing filter	Integrated filter for suppressing aliasing distortion caused by FFT processing (automatic cutoff frequency setting/OFF)						

Cable length and mass: Main unit cable 1.3 m (4.27 ft), input section cable 46 cm (1.51 ft), approx. 350 g (12.3 oz)



DIFFERENTIAL PROBE 9322 (Accuracy at 23 ±5 °C/73 ±9 °F, 35 to 80 % rh after 30 minutes of warm-up time, accuracy / product guaranteed for 1 year)							
Functions	For high-voltage floating measurement, power line surge noise detection, RMS rectified output measurement						
DC mode	For waveform monitor output, Frequency characteristics: DC to 10 MHz (±3 dB), Amplitude accuracy: ±1 % of full scale (at max. 1000 V DC), ±3% of full scale (at max. 2000 V DC) (full scale: 2000 V DC)						
AC mode	For detection of power line surge noise, Frequency characteristics: 1 kHz to 10 MHz ±3 dB						
RMS mode	DC/AC voltage RMS output detection, Frequency characteristics: DC, 40 Hz to 100 kHz, Response speed: 200 ms or less (400 V AC), accuracy: ±1 % of full scale (DC, 40 Hz to 1 kHz), ±4 % of full scale (1 kHz to 100 kHz) (full scale: 1000 V AC)						
Input	Input type: balanced differential input, Input impedance/capacitance: H-L 9 M $\Omega$ /10 pF, H/L-unit 4.5 M $\Omega$ /20 pF, Max. rated voltage to earth: when using grabber clip 1500V AC/DC (CAT II), 600 V AC/DC (CAT III), when using alligator clip: 1000 V AC/DC (CAT III), 600 V AC/DC (CAT IIII)						
Max. allowable input	2000 V DC, 1000 V AC (CAT II), 600 V AC/DC (CAT III)						
Output	Voltage divider for 1/1000 of input, BNC connectors (output switchable for 3 modes DC, AC, RMS)						
Power source	(1) Use the AC Adapter 9418-15 or (2) Connect to the 8826 logic probe terminal via the Power Cord 9324						

Cable length and mass: Main unit cable 1.5 m  $(4.92\ ft)$ , input section cable 30 cm  $(0.98\ ft)$ , approx. 150 g  $(5.3\ oz)$ Note: The unit-side plug of the 9320 is different from the 9320-01.





LOGIC PROBE 932	(Accuracy at 23 ±5°C/73 ±9°F, 35 to 80% rh, accuracy / product guaranteed for 1 year)						
Function	Detection of voltage signal or relay contact signal for High/Low state recording						
Input	$ \begin{array}{l} 4 \ channels \ (common \ ground \ between \ unit \ and \ channels), \ digital/contact \ input, \\ switchable \ (contact \ input \ an \ detect \ open-collector \ signals) \\ Input \ resistance: 1 \ M\Omega \ (with \ digital \ input, 0 \ to +5 \ V) \\ 500 \ k\Omega \ or \ more \ (with \ digital \ input, +5 \ to +50V) \\ Pull-up \ resistance: 2 \ k\Omega \ (contact \ input: \ internally \ pulled \ up \ to +5 \ V) \\ \end{array} $						
Digital input threshold	1.4V/ 2.5V/ 4.0V						
Contact input detection resistance	$1.4~V:~1.5~k\Omega$ or higher (open) and $500~\Omega$ or lower (short) $2.5~V:~3.5~k\Omega$ or higher (open) and $1.5~k\Omega$ or lower (short) $4.0~V:~25~k\Omega$ or higher (open) and $8~k\Omega$ or lower (short)						
Response speed	500ns or lower						
Max. allowable input	$0\ to\ +50V\ DC$ (the maximum voltage that can be applied across input pins without damage)						

**LAN COMMUNICATOR 9333** 

Distribution media	One CD-R				
Operating environment	Computer equipped with Pentium (133 MHz) or better CPU, running under Windows 95/98/Me or Windows NT 4.0/ 2000/XP operating system, with network adapter installed and configured to use TCP/IP protocol, and at least 64 MB of memory.				
HiCORDER side	Standard LAN connector, LAN card				
Communications	Ethernet, TCP/IP				
Remote control	Remote control of MEMORY HiCORDER (by sending key codes and receiving images on screen), print reports, print images from the screen, receive waveform data in same format as waveform files from the MEMORY HiCORDER (binary only)				
Waveform data acquisition	Accept auto-saves from the MEMORY HICORDER, same format as auto-save files of MEMORY HICORDER (binary only), print automatically with a MEMORY HICORDER from a PC. The MEMORY HICORDER's print key launches printouts on the PC				
Waveform viewer	Simple display of waveform files, conversion to CSV format, Scroll function, enlarge/reduce display, display CH settings.				

 $\begin{tabular}{ll} \textbf{Cable length and mass:} & Main unit cable 1.5 m (4.92 ft), input section cable 1 m (3.28 ft), approx. 320 g (11.3 oz) \\ \hline \textbf{Note:} & The unit-side plug of the MR9321 is different from the MR9321-01. \\ \hline \end{tabular}$ 



	***						
LOGIC PROBE MR	(Accuracy at 23 ±5°C/73 ±9°F, 35 to 80% rh, accuracy / product guaranteed for 1 year)						
Function	Detection of AC or DC relay drive signal for High/Low state recording Can also be used for power line interruption detection						
Input	$4$ channels (isolated between unit and channels), HIGH/LOW range switching Input resistance: $100~k\Omega$ or higher (HIGH range), $30~k\Omega$ or higher (LOW range)						
Output (H) detection	170 to 250 V AC, ±DC 70 to 250 V (HIGH range) 60 to 150 V AC, ±DC 20 to 150 V (LOW range)						
Output (L) detection	0 to 30 V AC, ±DC 0 to 43 V (HIGH range) 0 to 10 V AC, ±DC 0 to 15 V (LOW range)						
Response time	Rising edge 1 ms max., falling edge 3 ms max. (with HIGH range at 200 V DC, LOW range at 100 V DC)						
Max. allowable input	250 Vrms (HIGH range), 150 Vrms (LOW range) (the maximum voltage that can be applied across input pins without damage)						

#### WAVE DROCESSOR 9335

MANE LKOPE220	JR 9550							
Distribution media	One CD-R							
Operating environment	Running under Windows 2000/XP/Vista (32-bit), or Windows 7 (32-bit/64-bit)							
Display functions	Waveform display, X-Y display, Digital value display, Cursor function, Scroll function, Maximum number of channels (32 channels analog, 32 channels logic), Gauge display (time, voltage axes), Graphical display							
File loading	Readable data formats (MEM, REC, RMS, POW)  Maximum loadable file size: Maximum file size that can be saved by a given device (file size may be limited depending on the computer configuration)							
Data conversion	Conversion to CSV format, Tab delimited/Space delimited Data culling (simple), Convert for specified channel, Batch conversion of multiple files							
Print functions	Print formatting (1 up. 2-to-16 up, 2-to-16 rows, X-Y 1-to-4 up), Preview, Hard copy functions usable on any printer supported by operating system							
Other	Parameter calculation, Search, Clipboard copy, Launching of other applications							

■ PC Software Specifications Bundled with the 8826 in the CD-R

Wave Viewer (Wv) Software					
Functions	Simple display of waveform file     Text conversion: convert binary data file to text format, with selectable space or tab separators in addition to CSV, and specifiable section, thinning available     Display format settings: scroll functions, enlarge/reduce display, display channel settings     Others: voltage value trace function, jump to cursor/trigger position function				
Operating environment	Windows 2000/XP/Vista (32-bit), or Windows 7 (32-bit/64-bit)				

Install by inserting into the main unit. Can be replaced by user. 0 12 12 0 ANALOG UNIT 8936 VOLTAGE/TEMP UNIT 8937 0=1 = 0 **FFT ANALOG UNIT 8938** STRAIN UNIT 8939

F/V UNIT 8940 (8826 Ver. 2.10 or later can be used, Current probes with a serial number of No. 1999-0338386 or later can be used, older types cannot be used.)

4ch ANALOG UNIT 8946

(It cannot be used with the 8826)

**CHARGE UNIT 8947** 

.. (Used with the 8826. Ver. 2.20 or later)







4-channel type, for voltage/contact signal ON/OFF detection (response time 0.5 µsec, large terminal type)



Cannot use the smallterminal types 9327, 9320-01, 9321-01 and MR9321-01 with the

LOGIC PROBE MR9321

4 isolated channels, ON/OFF detection of AC/DC voltage (large terminal type)




CONNECTION CORD L9790 Flexible  $\varphi$  4.1 mm (0.16 in) thin dia cable allowing for up to 600 V inpu 1.8 m (5.91 ft) length \* The end clip is sold separately.

6 0 T TO 16

100年的三0年6

· ( ( ) ( )







φ 5 0 mm (0 20 in) dia cable allowing for

up to 300 V input. 1.7 m (5.58 ft) length small alligator clip



10:1 PROBE 9665

Max. rated voltage to earth is same as for Max. rated voltage to earth is same as for input module, max. input voltage 1 kV rms up to 500 kHz), 1.5 m (4.92 ft) length input module, max. input voltage 5 kV peak (up to 1MHz), 1.5 m (4.92 ft) length



φ 5.0 mm (0.20 in) dia.. cable allowing for up to 600 V input. 1.8 m (5.91 ft) length, a detachable

large alligator clips are bundled



**GRABBER CLIP 9243** 

Attaches to the tip of the Cord 9197, Red/ Black set, 196 mm (7.72 in) length

# 100:1 PROBE 9666

#### High-Voltage measurement for use with the power supply



For powering Differential probe 9322. 100 to 240 V AC

POWER CORD 9324

Use to the 9322 from the logic terminal. Note that usage restrictions apply.

POWER CORD 9325 Use to the 9322 from the F/V UNIT

Note that usage restrictions apply.



Insulation transformer, 400 V or 200 V AC input, 10 V AC output, for AC power line measurement. Required along with the Conversion Adapter 9199



RECORDING PAPER 9229

264 mm (10.39 in) × 30 m (98.43 ft), 6 rolls set

**RECORDING PAPER 9229-01** 

perforated type, 264 mm (10.39 in) = 30 m (98.43 ft), 6 rolls set



#### **MEMORY HICORDER 8826**

\* The MEMORY HiCORDER 8826 cannot operate alone. You must install one or more optional input modules in the unit.

Factory-installed option \*Must specify when ordering







WAVE PROCESSOR 9335

Convert data, print and display waveforms. Windows 2000/XP/Vista (32-bit), Windows 7





Power supply unit for the 9272 to the 9279 clamp sensors, except for connecting to the F/V unit 8940, for signal output 9217 is

CONVERSION CABLE 9318 (To connect the 9272 - 9279 and the 8940)

UNIVERSAL CLAMP ON CT 9277

Observe waveforms from DC to distorted AC. DC to 100kHz response, input 20A /

UNIVERSAL CLAMP ON CT

Observe waveforms from DC to distorted AC. DC to 100kHz response, input 200A output 2V AC

UNIVERSAL CLAMP ON CT

Observe waveforms from DC to distorted AC. DC to 20kHz response, input 500A / output 2V AC

#### rrent measurement \* To connect the clamp-on sensor via the conversion cable, The CLAMP ON SENSOR 9272-10

waveforms. Input: 1 to 100kHz, selectable 20 and 200A rms ranges. 2V AC output

#### CONVERSION CABLE 9705

Use with the Conversion Cable 9318 to connect Model 9272-10 to the F/V output wiring specifications
CONVERSION CABLE 9318

To connect the 9272 to 9279 and the 8940



#### CONVERSION CABLE 9319

To connect the 3273-50 and the 8940 Note: cannot be used with the 3274, 3275 3276 to connect the 8940 via this cable

#### CLAMP ON PROBE 3273-50

DC to 50MHz wideband response mA-class current up to 30A rms

## asurement \*co





CLAMP ON PROBE 3274 DC to 10MHz wideband response

#### mA-class current up to 150A rms

CLAMP ON PROBE 3275 DC to 2MHz wideband response, mA-class current up to 500A rms

CLAMP ON PROBE 3276 DC to 100MHz wideband response mA-class current up to 30A rms



## POWER SUPPLY 3272

Connect and power up to one CLAMP ON PROBE to use in combination with voltage input modules

#### POWER SUPPLY 3269

Connect and power up to four CLAMP ON PROBEs to use in combination with voltage input modules

#### CLAMP ON PROBE 9018-50 ut from 10 to 500 A 40 Hz to 3 kHz for

0.2 V AC output. BNC terminal CLAMP ON PROBE 9132-50

## Input from 20 to 1000 A, 40 Hz to 1 kHz for 0.2 V AC output. BNC terminal

PC Communication



Discontinued

Compatible with Windows 95/98/Me Windows NT 4.0/2000/XF

LAN COMMUNICATOR 9333 Application software to create a LAN connection





Discontinued

## CONNECTION CORD L9217

Insulated BNC connectors at both ends, Connects to insulated BNC connectors on input module. 1.7 m (5.58 ft) length

**CONNECTION CORD 9165** Cord has metallic BNC connectors at both ends, and connects to metallic BNC

connectors. 1.5 m (4.92 ft) length




#### CONVERSION ADAPTER 9199 LAN CABLE 9642

Female banana terminals to BNC plug (output), use to connect to BNC terminal on Straight Ethernet cable, supplied with straight to cross conversion adapter, 5 m (16.41 ft) length

## PC Card Preca

Use only PC Cards sold by HIOKI. Compatibility and performance are not guaranteed for PC cards made by other manufacturers. You may be unable to read from or save



PC CARD 512M 9728 (512 MB capacity) PC CARD 256M 9727 (256 MB capacity)

Combination example	Main unit with memory 16 MW	No. of channels	4 ch + logic 32 ch	8 ch + logic 32 ch	12 ch + logic 32 ch	16 ch + logic 32 ch	20 ch + logic 32 ch	24 ch + logic 32 ch	28 ch + logic 32 ch	32 ch + logic 32 ch
(normal choice of the input unit, up to 200V AC direct input.)	8826 × 1	Input module	8936 × 2	8936 × 4	8936 × 6	8936 × 8	8936 × 10	8936 × 12	8936 × 14	8936 × 16
		Input cable	L9198 × 4	L9198 × 8	L9198 × 12	L9198 × 16	L9198 × 20	L9198 × 24	L9198 × 28	L9198 × 32

