

ANALYSIS SUPPLEMENT

8860

8861

MEMORY HiCORDER

Using analysis functions to analyze
measurement data

HIOKI E. E. CORPORATION

Contents

Introduction.....	1
-------------------	---

Chapter 1

Numerical Calculation Functions _____ 3

1.1 Numerical Value Calculation Workflow	4
1.2 Settings for Numerical Value Calculation	6
1.3 Judging Calculation Results	11
1.4 Saving Numerical Calculation Results	14
1.4.1 Automatically Saving Numerical Calculation Results	14
1.4.2 Optionally Selecting Numerical Calculation Results & Saving (SAVE Key)	15
1.4.3 Example of Saving Numerical Calculation Results	16
1.5 Reading Numerical Calculation Results on a PC	17
1.6 Numerical Value Calculation Expressions	19

Chapter 2

Waveform Calculation Functions _____ 23

2.1 Waveform Calculation Workflow	24
2.2 Settings for Waveform Calculation	26
2.3 Calculation Waveform Display	33
2.4 Waveform Processing Calculation Operators and Results	34

Chapter 3

FFT Function _____ 37

3.1 Overview and Features	37
3.2 Screen Organization (FFT Function)	38
3.2.1 Waveform Screen	38
3.2.2 Settings Screen	40
3.3 Operation Workflow	45
3.4 Setting FFT Analysis Conditions	51
3.4.1 Selecting the FFT Function	51
3.4.2 Selecting the Data Source for Analysis	52
3.4.3 Setting the Frequency Range and Number of Analysis Points	53
3.4.4 Setting the Window Function	56
3.4.5 Setting Peak Values of Analysis Results	57

3.4.6	Averaging Waveforms	58
3.4.7	Emphasizing Analysis Results (phase spectra only)	61
3.4.8	Analysis Mode Settings	62
3.4.9	Setting the Display Range of the Vertical Axis (Scaling)	66
3.4.10	Setting and Changing Analysis Conditions on the Waveform Screen	67
3.5	Selecting Channels	69
3.6	Setting the Screen Layout of the Waveform Screen	72
3.7	Saving Analysis Results	75
3.8	Printing Analysis Results	76
3.9	Analysis with the Waveform Screen	78
3.9.1	Selecting the Display Method	78
3.9.2	Selecting Gauges and Values	79
3.9.3	Analyzing after Specifying an Analysis Starting Point	80
3.10	FFT Analysis Modes	85
3.10.1	Analysis Modes and Display Examples	85
3.10.2	Analysis Mode Functions	102
3.11	FFT Definitions	103

Introduction

In this manual, “the instrument” means the Model 8860 or 8861 Memory HiCorder. The following documents are provided with this instrument. Refer to them as appropriate for your application.

Document	Description
1 Quick Start Manual	Read this first. It describes preparations for use, basic operating procedures and usage methods.
2 Input Module Guide	To connect input modules and measurement cables, and when making input channel settings; this Guide describes the optional input modules, related cable connection procedures, and their settings and specifications.
3 Instruction Manual	To obtain setting details; this Manual describes details of the functions and operations of the instrument, and its specifications.
4 Analysis Supplement (This document)	The supplement describes usage of the calculation functions to analyze measurement data.

Before Use

Be sure to read the safety precautions in the *Quick Start Manual*. Also read the precautions regarding input modules and connection cables in the chapter about connections in the *Input Module Guide*.

Registered trademarks

Windows is a registered trademark of Microsoft Corporation in the United States and/or other countries.

Symbols and Indicators in This Manual

The following symbols in this manual indicate the relative importance of cautions and warnings.

NOTE

Indicates advisory items related to performance or correct operation of the instrument.

Other Indicators

(⇒ p.)

Indicates the location of reference information.

*

Indicates that descriptive information is provided below.

A→B

Indicates an operation sequence.

[]

Screen labels such as menu items, page titles, setting items, dialog titles and buttons are indicated by square brackets [].

CURSOR

(Bold characters)

Bold characters within the text indicate operating key labels.

Accuracy

We define measurement tolerances in terms of f.s. (full scale) values, with the following meanings:

f.s. : maximum display value or scale length

In this instrument, the maximum displayable value is the range (V/div) times the number of divisions (20) on the vertical axis.

Example: For the 1 V/div range, f.s. = 20 V

Numerical Calculation Functions


Chapter 1

Numerical calculations can only be used with the Memory function.

Results calculated from the acquired waveform are displayed as numerical values on the Waveform screen.

Judgments can also be made based on calculation results.

Numerical calculation settings are made on the Numerical Calculations Setting screen (Num Calc).

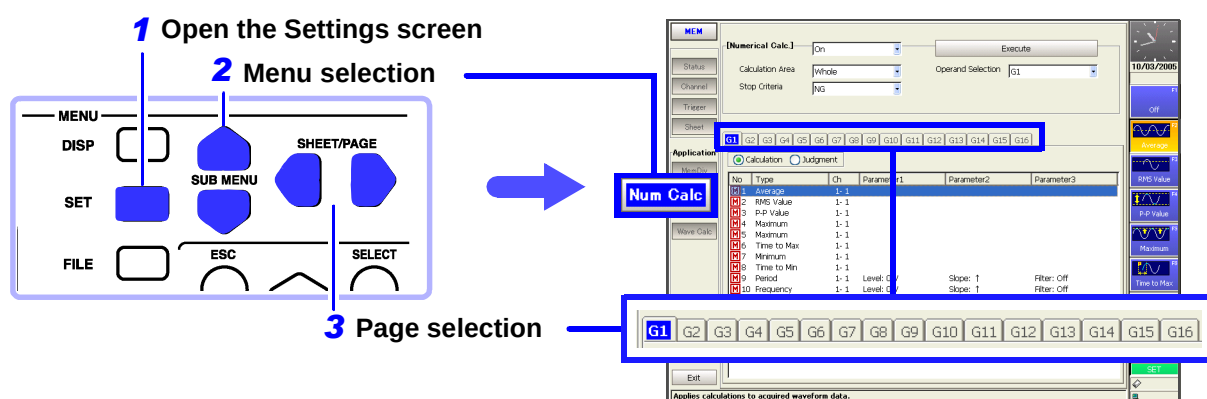

Numerical Calculation Function Capabilities (Numerical Calculation Screen)

Numerical Calculations

- Average value
 - RMS value
 - Peak-to-Peak (p-p) value
 - Maximum value
 - Time to maximum value
 - Minimum value
 - Time to minimum value
 - Period
 - Frequency
 - Rise time
 - Fall time
 - Standard Deviation
 - Area value
 - X-Y Area value
 - Time to specified level
 - Pulse width
 - Duty (%)
 - Pulse count
 - Numerical results of four standard arithmetic operators (Total 19 types)
 - Specified calculation between A/B cursors
- Numerical calculations are available in the range specified by A/B cursors
- Details of calculation expressions:
"1.6 Numerical Value Calculation Expressions" (⇒ p. 19)

Judgments based on Numerical Calculation (⇒ p. 11)

Results of numerical calculations can be compared with a specified range for GO/NG judgments.

Saving and Printing Numerical Calculation Results

- Automatic saving of numerical calculation results
 - Manual saving of existing numerical calculation results
- See** "1.4 Saving Numerical Calculation Results" (⇒ p. 14) in this manual, "Chapter 10 Saving/Loading Data & Managing Files" in the *Instruction Manual*
- Automatic printing
 - Manual printing
- See** "Chapter 11 Printing" in the *Instruction Manual*

Of the nineteen types of numerical calculation available, sixteen types can be applied at the same time.

Up to sixteen groups composed of multiple calculation types (operations) can be defined, with up to sixteen types of calculation per group. By setting up such groups of multiple calculations beforehand, they can be readily selected at calculation time.

See "1.6 Numerical Value Calculation Expressions" (⇒ p. 19)

When Scaling is enabled, numerical calculations are performed on scaled values. Numerical calculation is also available when Memory Division is enabled.

1.1 Numerical Value Calculation Workflow

Before Setting

When specifying a waveform range for calculation: [\[A-B\]](#)

Before executing a calculation, specify the calculation range using the A/B cursors (Vertical or Trace cursors) on the Waveform screen. Set the calculation range on the Num Calc Settings screen to [\[A-B\]](#).

- Horizontal cursors cannot be used to specify the range.
- When one cursor is used, the calculation range is from the cursor to the end of the data.

See "8.7 Specifying a Waveform Range" in the *Instruction Manual*
"1.2 Settings for Numerical Value Calculation" (⇒ p. 6)

To change calculation settings and recalculate


You can make changes to calculation settings and resume calculations from the Waveform screen.

See "To recalculate after changing calculation type settings" (⇒ p. 9)


The following two calculation methods are available:

- Calculate while measuring
Requires making numerical calculation settings beforehand.
- Apply calculations to existing data
Calculations can be applied to data after waveforms are acquired, or after data has been saved to storage media.

Calculating While Measuring

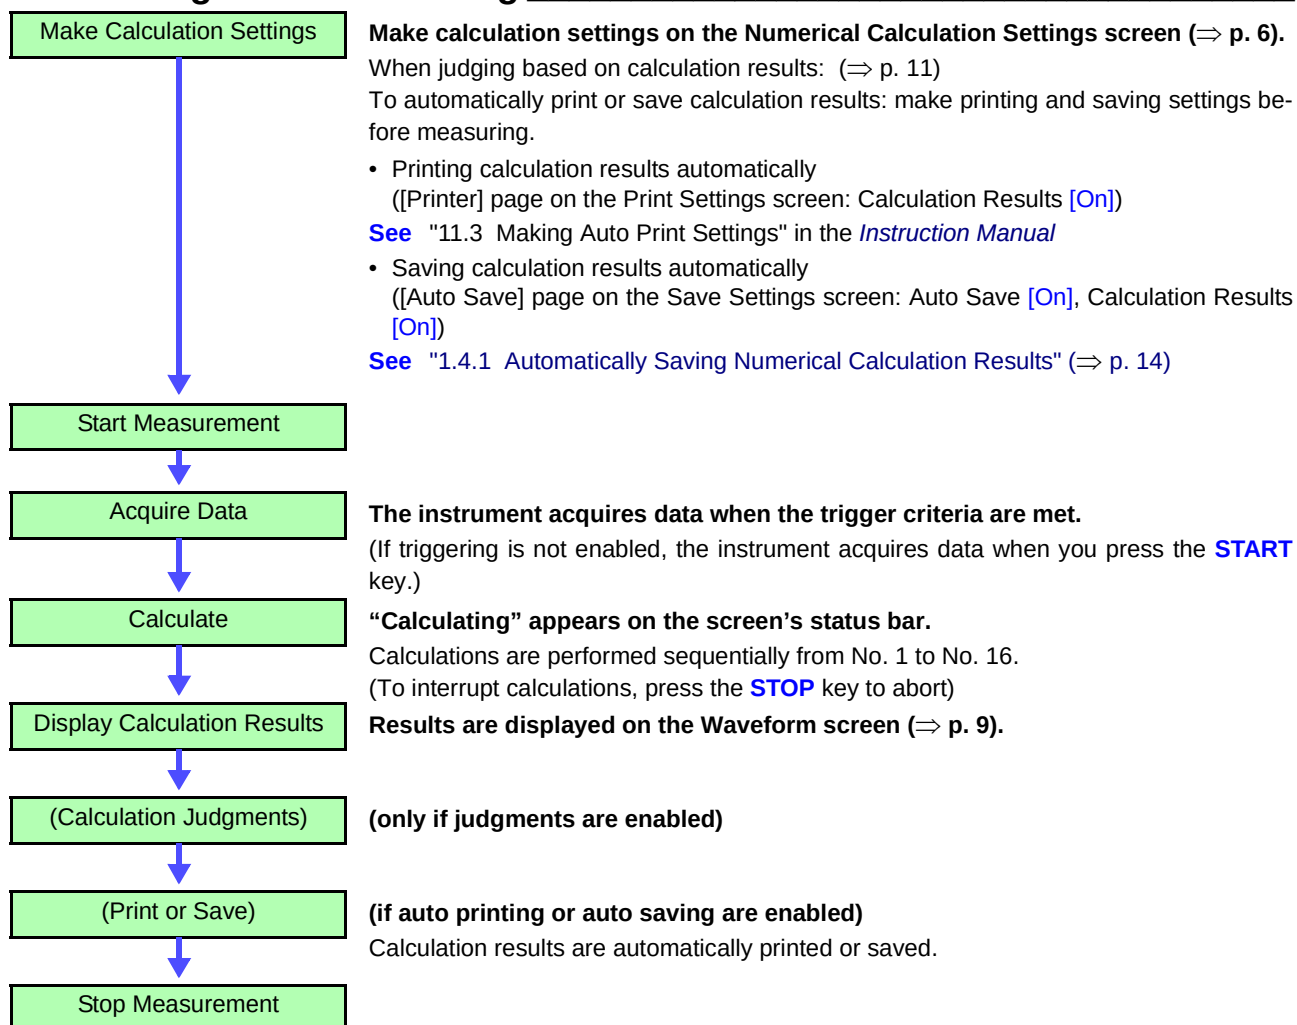

Applying Calculations to Existing Data

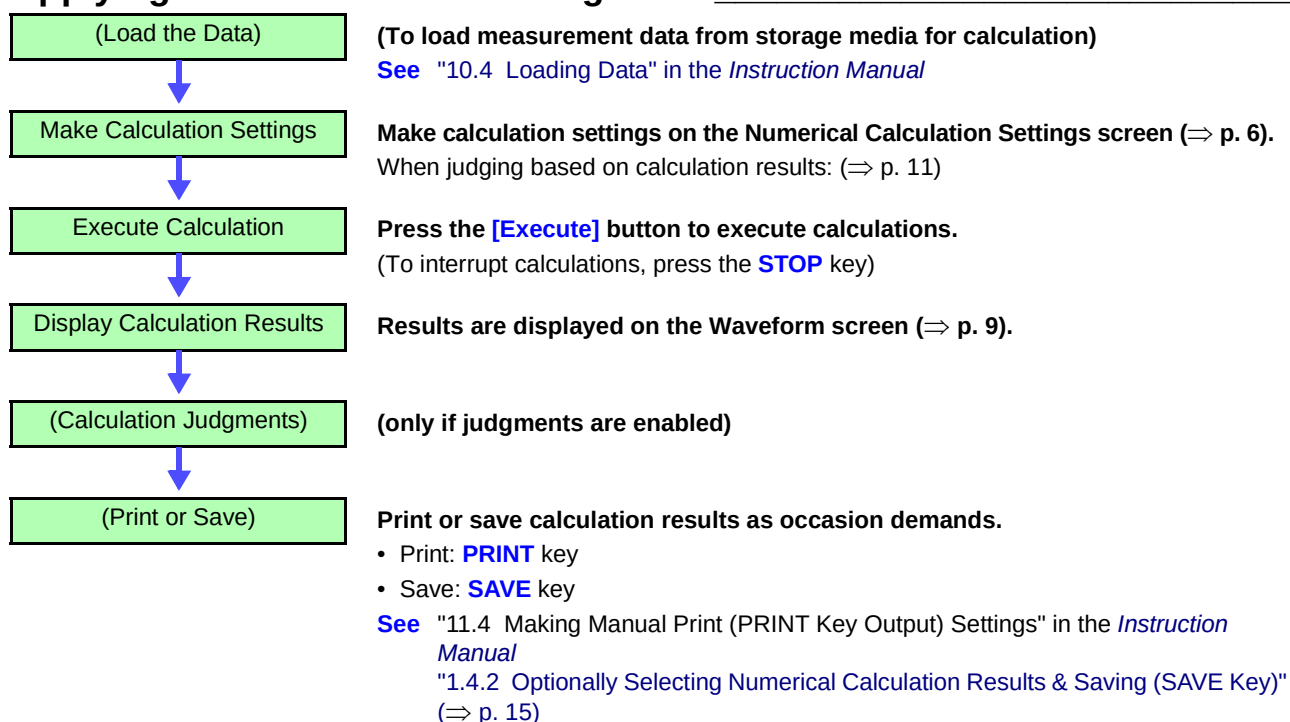

1.2 Settings for Numerical Value Calculation

Numerical Calculations

MEM


To open the screen: Press the **SET** key → Select **Num Calc** with the **SUB MENU** keys → Num Calc Settings screen

Operating Key

Procedure

1 Enable the Numerical Calculation function.

CURSOR Move the cursor to the **[Numerical Calc.]** item.
F2 Select **[On]**.

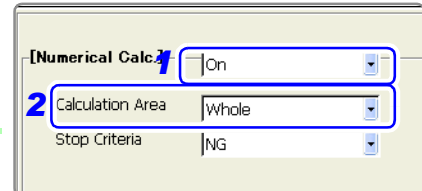

2 Specify the numerical calculation range.

CURSOR Move the cursor to the **[Calculation Area]** item.
F1 to F8 Select either choice.

Whole	Applies calculations to the whole waveform. (default setting)
A-B	Applies calculations to the data between A/B cursors.

When selecting **[A-B]**, specify the calculation range using the A/B cursors on the Waveform screen.
 If no measurement data has been acquired by the instrument, first measure once so that the range can be specified for calculations to be applied to subsequent measurements.


3 Perform calculation settings.

Group of Calculation Settings

Calculation Setting Choices

Calculation No.

Settings can also be made in a dialog (⇒ p. 8).

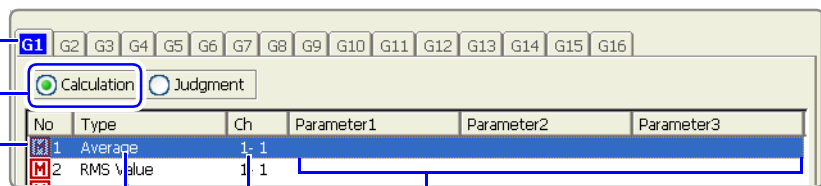

Calculation Type

Channel for Calculation

Calculation Parameters

Setting choices depend on the calculation type.

SHEET/PAGE Select the group for which to set calculations. (G1 to G16)

CURSOR Move the cursor to your setting choice, and select **[Calculation]**.
F1

Also select **[Judgment]** if you require judgment of calculation results. (⇒ p. 11)

4 Select the Calculation type.

CURSOR Move the cursor to the **[Type]** column of the No. row of the calculation to set.

F1 to F8 Select the calculation type.

(Switch Display: F8)

Off	No calculation. (default setting)
Average	Average value of waveform data
RMS Value	RMS value of waveform data
P-P Value	Peak-to-peak value of waveform data
Maximum	Maximum value of waveform data
Time to Max	Time from trigger to maximum value
Minimum	Minimum value of waveform data
Time to Min	Time from trigger to minimum value
Period	Period of signal waveform
Frequency	Frequency of signal waveform

1.2 Settings for Numerical Value Calculation

Operating Key	Procedure
F1 to F8 (Switch Display: F8)	
Rise Time	Rise time of waveform data
Fall Time	Fall time of waveform data
Std Deviation	Standard deviation of waveform data
Area	Area enclosed by zero position and signal waveform
X-Y Area	Area of X-Y composite waveform
Time to Level*	Time from trigger to specified level
Pulse Width*	Pulse width of waveform data
Duty*	Duty of waveform data
Pulse Count*	Pulse count of waveform data
4 Operations	Four arithmetic operations on numerical calculation results

* Applicable to logic channels

5 Select the channel for calculations.

CURSOR	Move the cursor to the [Ch] item.
F1 to F8	Select a channel for calculations. The waveform calculations (Zn) can be selected.

6 Set parameters.

(not required for some calculation types)

CURSOR	Move the cursor to the [Parameter] item.
F1 to F8	Make appropriate parameter settings. About setting choices (⇒ p. 19) See "3.3.3 Entering Text and Numbers" in the <i>Instruction Manual</i>

7 Select a calculation group.

CURSOR	Move the cursor to the [Operand Selection] item.
F1 to F8	Select a calculation group.

Execute the calculations.
(when judging calculations (⇒ p. 12))

Applying Calculations to Existing Data

CURSOR	Move the cursor to the [Execute] button.
F1	Select [Execute].

When calculating automatically after measurement

START	Starts measurement.
--------------	---------------------

To print or save calculation results while measuring


Before measuring, enable Auto Save (⇒ p. 14) or Auto Print. Enable [Calc Results] on the Save Settings or Print Settings screen.

See "10.3.4 Setting Auto Save",
"11.3 Making Auto Print Settings"
in the *Instruction Manual*

To print or save existing data

Press the PRINT or SAVE key (⇒ p. 15).
Manual Print Settings
Manual Save Settings

See "11.4 Making Manual Print (PRINT Key Output) Settings",
"10.3.5 Setting Manual Save (SAVE Key Output)" in the *Instruction Manual*

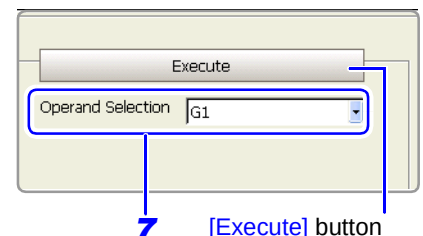

7 [Execute] button

Execute calculation of the displayed group.

Changes made to calculation settings while measuring do not take effect until measurement has been stopped and re-started.

1.2 Settings for Numerical Value Calculation


Making settings in the [Calculation] dialog

Calculation Marker

Markers are displayed next to the calculation No. of enabled calculations.

To copy settings between calculation Nos.:


Select F2 [Copy]. (⇒ p. 10)

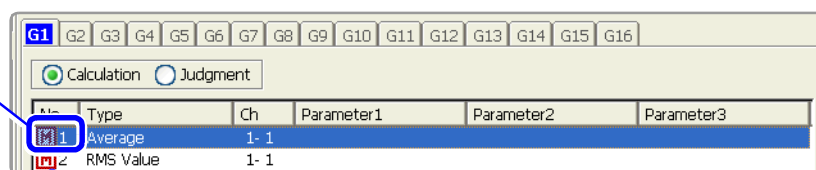

F1 Move the cursor to the [No.] column of the calculation to set, and select **F1 [All Settings]** to open the [Calculation] dialog.

Parameter Settings

(Displayed as required for the selected calculation type)

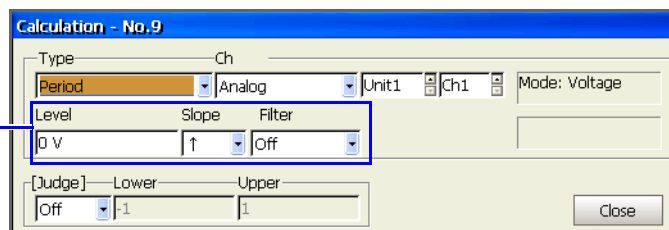

Move the cursor to each item, and make the setting.


See Parameter setting: "1.6 Numerical Value Calculation Expressions" (⇒ p. 19)

After making the appropriate settings, press the **ENTER** key or move the cursor to the **[Close]** button and press the **F1 [Close]** key to accept your settings.

1.2 Settings for Numerical Value Calculation

Numerical Calculation Results

Numerical calculation results are displayed on the Waveform screen.

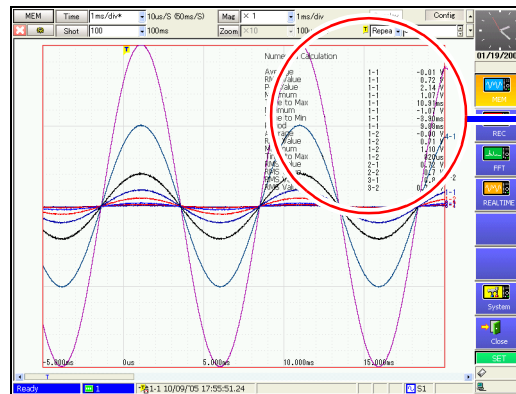


If the display is hard to view because of overlapping numerical values and waveforms



Press the **DISP** key.


Numerical values and waveforms are displayed separately.

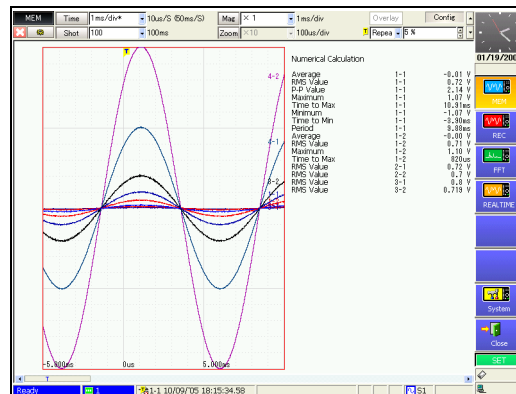

To recalculate after changing calculation type settings

Select your choices for the calculation setting items on the Waveform screen, and execute calculation.

Press the **SUB MENU** keys to switch to the [Num Calc] settings.

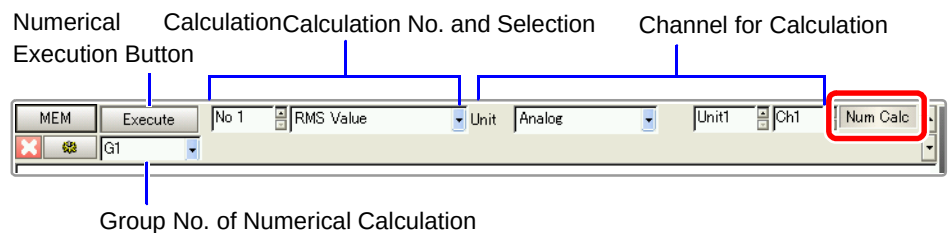

Select a Group No. for calculation or change your choices, and select the **[Execute]** button.

All calculations specified for the selected Group No. are performed.



To save or print calculation results after measuring

When Selection Save (default setting) is enabled, press the **SAVE** key and select **[Calc Results]** for the Save Type.

When Selection Print (default setting) is enabled, press the **PRINT** key and select **F6 [Calc Results]**.

1.2 Settings for Numerical Value Calculation


Copying Settings Between Calculation Nos.

MEM

To open the screen: Press the **SET** key → Select **Num Calc** with the **SUB MENU** keys → Num Calc Settings screen

Operating Key Procedure

- 1 **Open the dialog.**
- CURSOR Move the cursor to the [No.] column of the calculation to copy.
- F2 Select **[Copy]**.
The **[Copy Settings]** dialog appears.

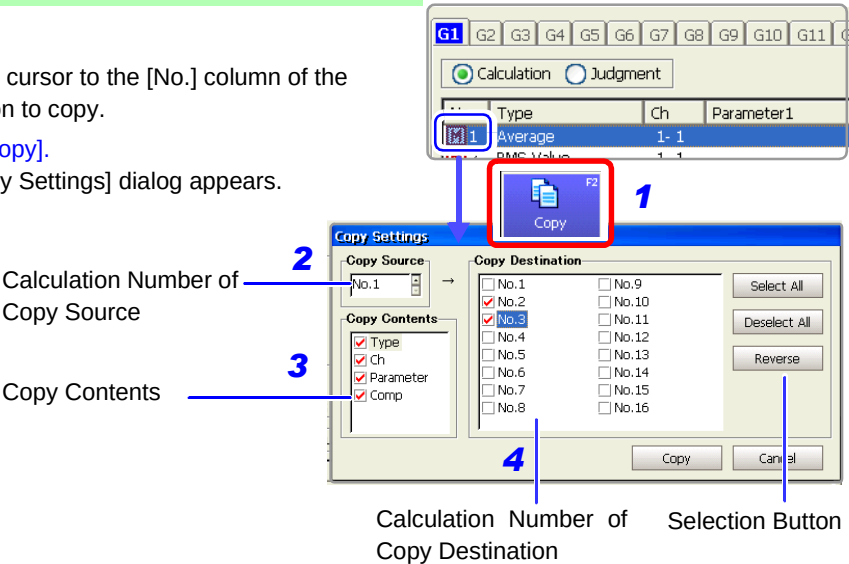

- 2 **Select the copy source.**
- CURSOR Move the cursor to the **[Copy Source]** item.
- F1 to F8 Select the Calculation Number of the copy source.
- 3 **Select the contents to copy.**
- CURSOR Move the cursor to the **[Copy Contents]** item.
- F1 to F8 Select the contents to copy.
- 4 **Select the copy destination.**
- CURSOR Move the cursor to the **[Copy Destination]** item.
- F1 to F8 Select the Calculation Number of the copy destination.

Selections can be made using the buttons in the dialog.

Move the cursor to a button, and press the F1 key.


- **Select All**
Selects all copy destinations.
- **Deselect All**
Deselects all copy destinations.
- **Reverse**
Reverses selected and deselected settings.
- **Copy**
Executes the copy process.
- **Cancel**
Cancels the copy process.

- 5 **Execute copy.**
- F7 Select **[Copy]**.
The selected contents are copied.

1.3 Judging Calculation Results

Set the judgment criteria (upper and lower threshold values) by which to judge numerical calculation results. Judgment criteria can be set for every numerical calculation.

Waveform acquisition processing depends on the trigger mode setting (Single or Repeat) and the criteria specified to stop measuring upon judgment (GO, NG or GO & NG).

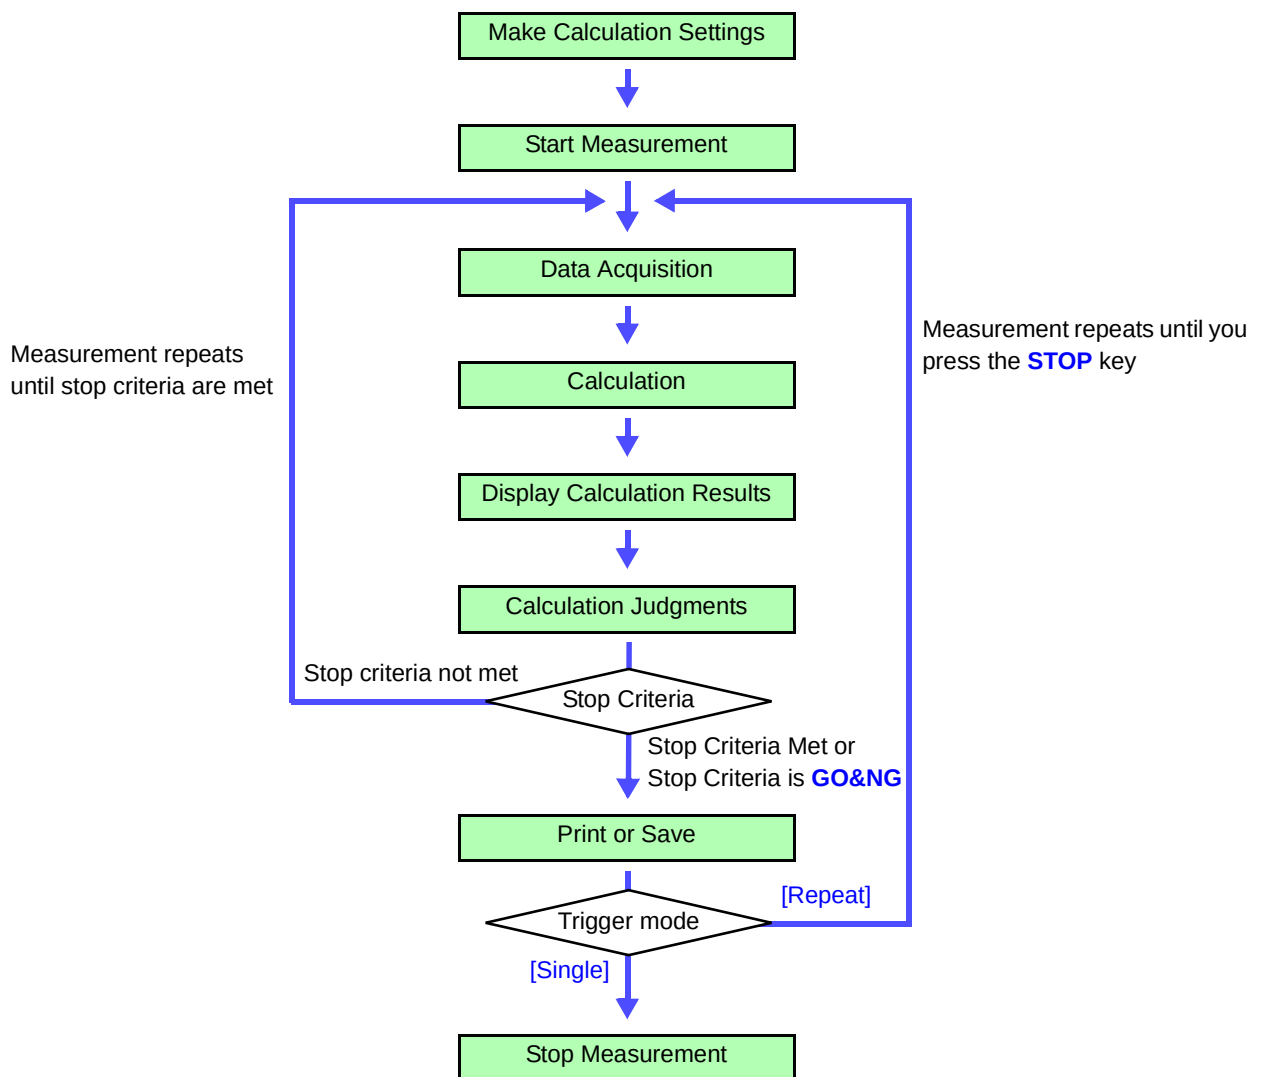

NOTE

Judgment when memory division is enabled

When memory division is enabled, waveform data is retained in the measured block only when stop criteria are met.

When stop criteria are not met, measurement continues to repeat within the same block.

Judging Numerical Value Calculation Results

MEM

To open the screen: Press the **SET** key → Select **Num Calc** with the **SUB MENU** keys → Num Calc Settings screen

Operating Key Procedure

- 1 Make settings for calculation (⇒ p. 6).
- 2 Select the appropriate calculation judgment settings.

Group of Calculation

Calculation Setting

Contents

Calculation No.
Settings can also be made in a dialog (⇒ p. 8).

Calculation Type

Channel for Calculation

Judge or not

Lower and Upper judgment thresholds

No	Type	Ch	Comp	Lower	Upper
1	Average	1- 1	On	-1	1
2	RMS Value	1 1	On	-1	1

SHEET/PAGE Select the group for which to set calculation judgment. (G1 to G16)

CURSOR Move the cursor to your setting choice, and select **[Judgment]**.

F2

- 3 Enable the judgment function.
- CURSOR** Move the cursor to the **[Comp]** setting for Calculation No. to judge

F2 Select **[On]**.

- 4 Specify the judgment thresholds.
- CURSOR** Set the **[Lower]** and **[Upper]**.

F1 to F8 Select an entry method and enter the threshold values.

Input range: -9.9999E+29 to 9.9999E+29

The upper threshold of the period range cannot be set below the lower threshold, and vice-versa.

See "3.3.3 Entering Text and Numbers" in the *Instruction Manual*

- 5 Select the Stop Criteria upon judgment.
- CURSOR** Move the cursor to the **[Stop Criteria]** item.

F1 to F8 Select either choice.
- | | |
|--------------------|--|
| GO | Continue to the next process when within the threshold range (PASS judgment) |
| NG | Continue to the next process when outside of the threshold range (FAIL judgment) |
| GO & NG | Continue to the next process regardless of judgment result. |

[Numerical Calc.] On

Calculation Area Whole

Stop Criteria NG

Execute calculation.

Judging Existing Data

CURSOR Move the cursor to the **[Execute]** button.

F1 Select **[Execute]**.

Execute

Operand Selection G1

When judging automatically after measurement

START Starts measurement.

Processing depends on the Trigger Mode setting.


If calculating while acquiring waveforms, measurement is repeated until the Stop Criteria are met.

Description About judgment results

Judgment results of numerical calculations are displayed on the Waveform screen.

Within the judgment threshold range: GO judgment

Out of the judgment threshold range: NG judgment (displayed in red)

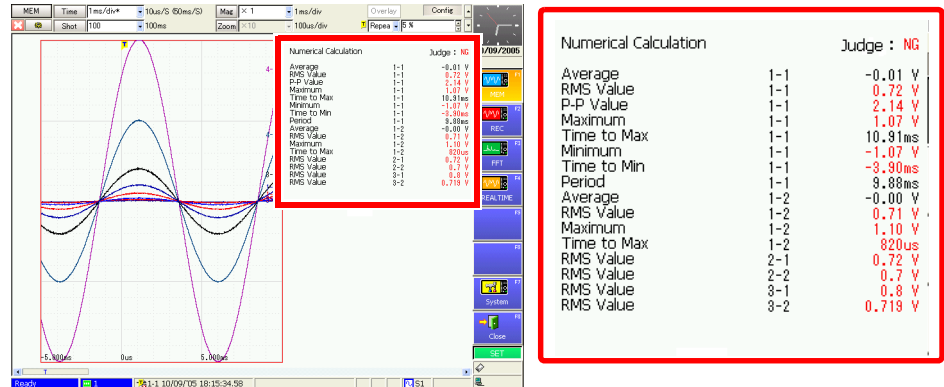

When printing, judgment results for each parameter are also printed.

When performing external control

When the external I/O terminals are enabled, the signal is output from the next sampling period.

See "14.2.5 GO/ NG Evaluation Output (GO/EXT OUT1)/ (NG/EXT OUT2)" in the *Instruction Manual*

When the judgment result is GO

- The GO signal is output at the $\overline{\text{GO/EXT OUT1}}$ external I/O terminal.

When the judgment result is NG

- The NG signal is output at the $\overline{\text{NG/EXT OUT2}}$ external I/O terminal. The NG judgment is asserted when any channel is judged as NG.
- Channels judged as NG are indicated by an "x" in printouts.
- When the beeper is enabled, a beep sounds when a result is out of the threshold range.

1.4 Saving Numerical Calculation Results

1.4.1 Automatically Saving Numerical Calculation Results

Calculate and automatically save during data acquisition.
Before measurement begins, the calculation settings need to be set.



When using auto save during measurement, do not remove the storage media specified as the save destination until the measurement operation is completely finished. Doing so may damage data on the storage media.

Automatically Saving Numerical Calculation Results

MEM

To open the screen: Press the **SET** key → Select **Save** with the **SUB MENU** keys → Save Settings screen

Operating Key Procedure

1 Set auto save .

Set the save destination.

See "10.3.4 Setting Auto Save" in the *Instruction Manual*

2 Enable the saving of numerical calculation results.

CURSOR

Move the cursor to the **[Calc Results]** item.

F2

Select **[On]**. (Default setting: Off)

3 Enter a save name (if you want to use a different name).

CURSOR

Move the cursor to the **[Name]** item.

F1 to F8

Enter the save name. (Default setting: MEAS)

See "3.3.3 Entering Text and Numbers" in the *Instruction Manual*

4 Select the file creation method.

CURSOR

Move the cursor to the **[Save Specified File]** item.

F1 to F8

Select either choice.

New File

Creates a new file for each measurement.

Existing File

Adds calculation results to one file.

Confirm the measurement configuration and numerical calculation result settings, then start measurement (START key).

After the data is acquired and the numerical calculation process completes, the numerical calculation results (text) are saved automatically to the specified storage media.

[Auto Save] Page

Save Name

Up to 40 characters (single byte and double byte) can be used for the save name. A sequential number starting from 0001 is added after save names (if [New File] is selected).

Note that a PC will not be able to handle the following characters if they are used.

- ASCII:
+ = [] \ / | : * ? " < > ; ,
- White space characters

Some saved characters may differ from those used on the instrument. (⇒ p. 16)

1.4.2 Optionally Selecting Numerical Calculation Results & Saving (SAVE Key)

Perform calculations on data saved to storage media and internal memory and save the calculation results by pressing the **SAVE** key.

Before calculation results can be saved, the calculation settings needs to be set and the calculations need to be performed.

Manually Saving Numerical Calculation Results

MEM

To open the screen: Press the **SET** key → Select **Save** with the **SUB MENU** keys → Save Settings screen

Operating Key Procedure

1 Set manual save.

See "10.3.5 Setting Manual Save (SAVE Key Output)" in the *Instruction Manual*

For [Selection Save], press the **SAVE** key after setting the calculation settings and performing the calculations.

(The [Save] dialog box appears.)

Set the save destination.

2 Select the save type.

CURSOR

Move the cursor to the [Save Type] item.

F4

Select [Calc Results].

3 Select the file creation method.

CURSOR

Move the cursor to the [Save Specified File] of the numerical calculation result settings field.

F1 to F8

Select either choice.

New File	Creates a new file each time measurement starts (start operation).
Existing File	Adds calculation results to one file.

[SAVE Key] Page

Some saved characters may differ from those used on the instrument (⇒ p. 16).

For [Quick Save]:

Press the **SAVE** key

The calculation results (text) are saved to the specified storage media upon pressing the key.

For [Selection Save]:

Select the **[OK]** button.

The calculation results (text) are saved to the specified storage media upon selecting the button.

1.4.3 Example of Saving Numerical Calculation Results

NOTE If you save numerical calculation results or data in text format, characters or display items used on the instrument are converted as shown below.
(Characters used on the instrument → Saved characters)
 $^2 \rightarrow ^\wedge 2$, $^3 \rightarrow ^\wedge 3$, $^n \rightarrow ^\wedge n$, $\mu \rightarrow \sim u$, $\Omega \rightarrow \sim o$, $\varepsilon \rightarrow \sim e$, $^\circ \rightarrow \sim c$,
 $\pm \rightarrow \sim +$, μE (display only) $\rightarrow uE$, $^\circ\text{C}$ (display only) $\rightarrow C$

- Calculation No. 1: Maximum value of analog channel 1-1
- Calculation No. 2: Minimum value of analog channel 1-1
- Calculation No. 3: Maximum value of analog channel 1-2
- Calculation No. 4: Minimum value of analog channel 1-2

"Trig Time","No1 Maximum A1_1","No2 Minimum A1_1","No3 Maximum A1_2","No4 Minimum A1_2"
","V","V","V","V"
"04-12-14 11:29:12.530",143,-143,0.0038124997,-0.0038124997
"04-12-14 11:29:15.570",143,-143,0.0038124997,-0.0038124997
"04-12-14 11:29:18.790",143,-142.75,0.0038749997,-0.0038124997
"04-12-14 11:29:21.940",143.25,-143.25,0.0038124997,-0.0038124997

Line 1: Calculation Settings
Line 2: Calculation Result Unit
From Line 3: Calculation Results

Recorded in the order of the calculation settings of line 1.

1.5 Reading Numerical Calculation Results on a PC


The following explains how to import data into Excel on Windows.

The capacity of Excel to import data from a text file is limited to 256 columns and 65,536 rows.

Text files containing data that exceeds these limits cannot be imported into Excel. To avoid exceeding these limits when saving text data, select [Displayed Ch] as the channels to save, or specify the saving range as that between A/B cursors.


1 Start Excel and click [Open] from the [File] menu.

The [Open] dialog box appears.

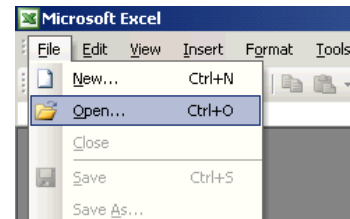

2 Select the file to import.

Select the file and click [Open].

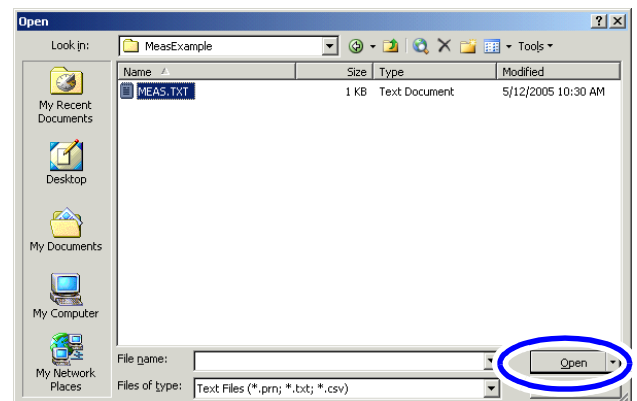


The Text Import Wizard appears.

3 Select the text processing method.


[Text Import Wizard Step 1 of 3]

1. Select [Characters such as commas or tabs separate each field].
2. Click [Next].

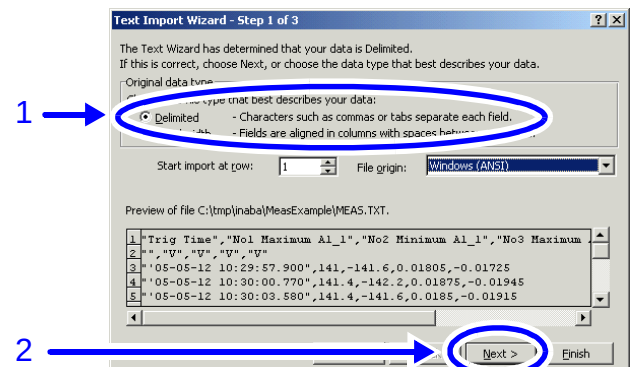

[Text Import Wizard Step 2 of 3]


3. Select [Comma] only for the delimiters.

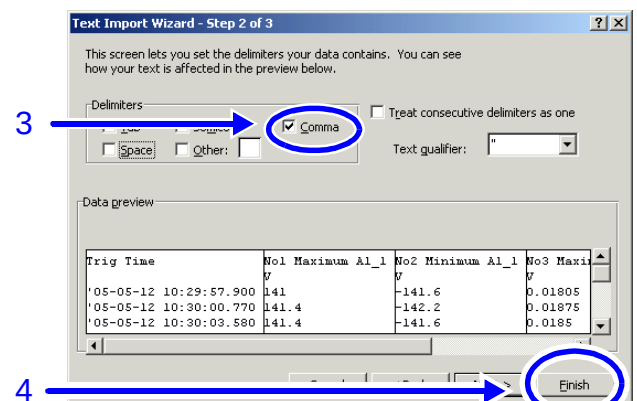

4. Click [Finish].

1.5 Reading Numerical Calculation Results on a PC

Numerical Calculation Results Data Imported into Excel

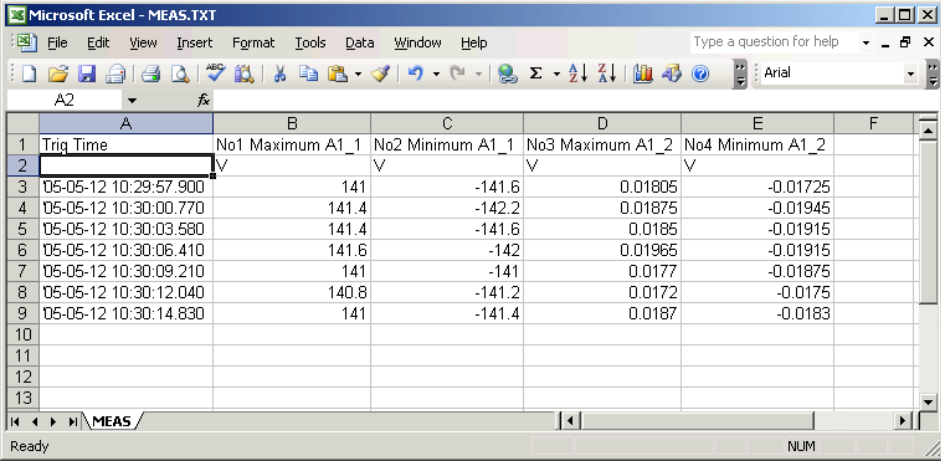

Microsoft Excel - MEAS.TXT

Type a question for help







A2

	A	B	C	D	E	F
1	Trig Time	No1 Maximum A1_1	No2 Minimum A1_1	No3 Maximum A1_2	No4 Minimum A1_2	
2		V	V	V	V	
3	05-05-12 10:29:57.900	141	-141.6	0.01805	-0.01725	
4	05-05-12 10:30:00.770	141.4	-142.2	0.01875	-0.01945	
5	05-05-12 10:30:03.580	141.4	-141.6	0.0185	-0.01915	
6	05-05-12 10:30:06.410	141.6	-142	0.01965	-0.01915	
7	05-05-12 10:30:09.210	141	-141	0.0177	-0.01875	
8	05-05-12 10:30:12.040	140.8	-141.2	0.0172	-0.0175	
9	05-05-12 10:30:14.830	141	-141.4	0.0187	-0.0183	
10						
11						
12						
13						







MEAS





Ready NUM

1.6 Numerical Value Calculation Expressions

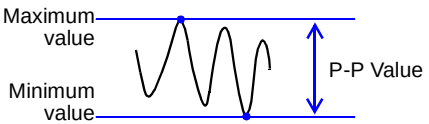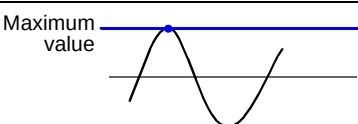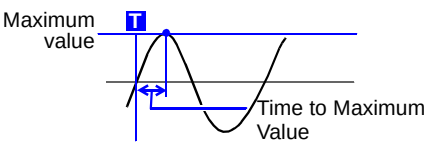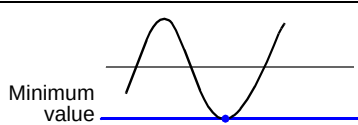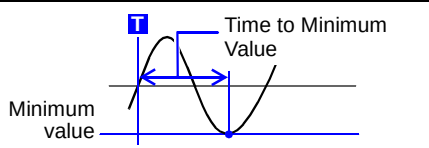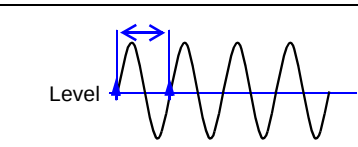Numerical Calculation Type	Description
Average	Obtains the average value of waveform data. $Avg = \frac{1}{n} \sum_{i=1}^n di$ Avg: Average value n: Data count di: Data on channel number i
RMS (Root-Mean-Square) value	Obtains the RMS value of waveform data. If Scaling is enabled, calculations are applied to the waveform after scaling. $RMS = \sqrt{\frac{1}{n} \sum_{i=1}^n di^2}$ RMS: RMS value n: Data count di: Data on channel number i
Peak-to-Peak (P-P) value	Obtains the value of the difference (peak-to-peak value) between maximum and minimum values of waveform data. 
Maximum Value	Obtains the maximum value of waveform data. 
Time to Maximum Value (Time to Max)	Obtains the time (in seconds) from the last trigger point to the maximum value. If the maximum value occurs in two or more instances, the first instance is treated as the maximum value. 
Minimum Value	Obtains the minimum value of waveform data. 
Time to Minimum Value (Time to Min)	Obtains the time (in seconds) from the last trigger point to the minimum value. If the minimum value occurs in two or more instances, the first instance is treated as the minimum value. 
Period and Frequency	Displays the period (in seconds) and frequency (Hz) of the signal waveform. The calculation is based on the interval between two sequential points where the waveform crosses the same level (amplitude) in the same direction (slope). Setting Choices: Level, Slope (↑ or ↓) and Filter 

1.6 Numerical Value Calculation Expressions

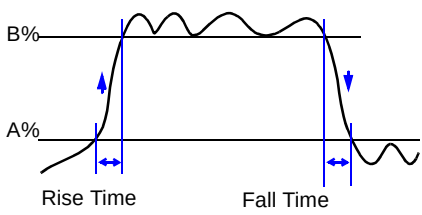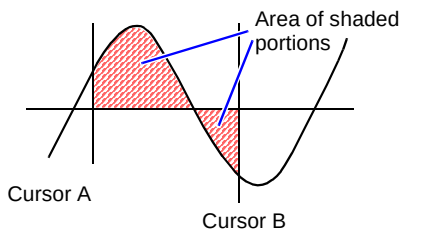Numerical Calculation Type	Description
Rise Time and Fall Time	The rise time of the acquired waveform from A% to B% (or fall time from B% to A%) is obtained by calculation using a histogram (frequency distribution) of the 0 and 100% levels of the acquired waveform. As waveform data is acquired, the rise time (or fall time) is obtained from the first rising (or falling) edge. When calculation of the range specified by the A/B cursors is selected, the obtained rise time (or fall time) is the first rising (or falling) edge between the cursors. Setting Choices: Numerical percentage (%) of rise time (A% → B%) or fall time (B% → A%)  A: 5 to 30% B: 95 to 70%
Standard Deviation (Std Deviation)	Obtains the standard deviation of the waveform data. $\sigma = \sqrt{\frac{1}{n} \sum_{i=1}^n (d_i - \text{Avg})^2}$ σ: Standard Deviation Avg: Average n: Data count di: Data on channel number i
Area	Obtains the area value (V•s) enclosed by the zero position (point of zero potential) and the signal waveform. When calculation of the range specified by the A/B cursors is selected, the calculated area is constrained to the waveform between the cursors.  $S = \sum_{i=1}^n d_i \cdot h$ S: Area n: Data count di: Data on channel number i h=Δt: Sampling period
X-Y Area	Obtains the area (V²) of an X-Y composite waveform. In the following figures, the areas within the lines are calculated. The calculation is available even if the X-Y composite waveform is not intended for display. To enable area calculation, specify the calculation range using the A/B cursors (Vertical or Trace) on the waveform of each channel for X-Y composition. (The area cannot be specified directly by A/B cursors on the X-Y waveform.) See About A/B cursors: "8.8 Cursor Values" in the Instruction Manual When the trace consists of multiple loops  $S = n \times s_0$ S: Area n: Number of loops When the trace is an open curve  $S = s_0$ S: Area (Area enclosed by the curve and line connecting start and end points) When the trace is a figure-8  $S = s_0 - s_1$ S: Area When the trace is a spiral  $S = s_0 \times 2 + s_1$ S: Area (The number of overlapping regions increases with the number of loops) Setting Choices: Set the X- and Y-axis channels. When measuring with Timebase 1 and 2, be sure to select both X- and Y-axis channels from the same Timebase (either Timebase 1 or Timebase 2). The X-Y area value cannot be calculated if the channels are not on the same Timebase.

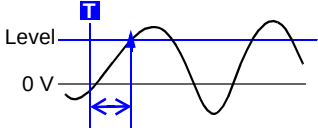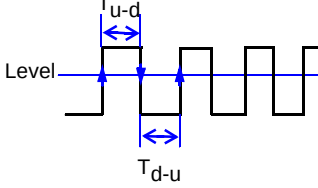Numerical Calculation Type	Description
Time to Level	Finds the point where the signal crosses a specified level from the start of the calculation range, and obtains the time elapsed from the last trigger event. Setting Choices: Level, Slope (↑ or ↓) and Filter 
Pulse Width	Obtains pulse width as the time difference between one rising or falling intersection of the waveform through a specified level to the next intersection (with opposite slope). Setting Choices: Level, Slope (↑ or ↓) and Filter 
Duty (%)	Obtains the duty percentage based upon the ratio of the time from a rising intersection to the next falling intersection at a specified level, to the time from the same falling intersection to the next rising intersection at the same level. $\text{Duty (\%)} = \frac{T_{u-d}}{T_{u-d} + T_{d-u}} \times 100 (\%)$ T_{u-d}: Time (seconds) after rising intersection to falling intersection T_{d-u}: Time (seconds) after falling intersection to the next rising intersection Setting Choices: Level, Filter 
Pulse Count	Obtains the count of pulses from the number of rising or falling intersections with a specified level. One pulse is counted when the signal falls back below the specified level after rising through it (or vice versa) Setting Choices: Level, Slope (↑ or ↓) and Filter 
Four Arithmetic Operations (4 Operations)	Performs arithmetic operations (+, -, ×, ÷) upon arbitrarily selected results of numerical calculations. Setting Choices: Numerical Calculation No., arithmetic operator

NOTE

- Depending on the signal waveform for parameters of period, frequency, rise time and fall time, calculated values may not be displayed.
- When Scaling is enabled, calculations are performed after waveform data has been scaled. Also, the units of parameter values should match the scaling units.

See About Scaling:

"5.4 Converting Input Values (Scaling Function)" in the *Instruction Manual*


Waveform Calculation Functions

Chapter 2

Waveform calculations can only be used with the Memory function.

A pre-specified calculation equation is applied to acquired waveform data, and the calculation results are displayed as a waveform on the Waveform screen.

Waveform calculation settings are made on the Waveform Calculations Setting screen (Wave Calc).

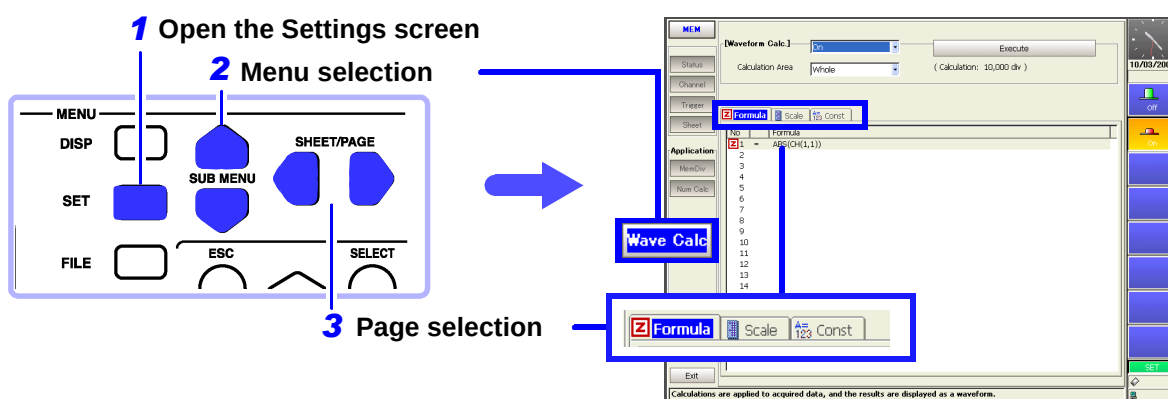

Waveform Calculation Function Capabilities (Waveform Calculation Screen)

Numerical Calculations

- Four Arithmetic Operators (+, -, *, /)
- Absolute Value (ABS)
- Exponent (EXP)
- Common Logarithm (LOG)
- Square Root (SQR)
- Moving Average (MOV)
- Slide along the time axis
- Differential Calculus: 1st derivative (DIF), 2nd derivative (DIF2)
- Integral Calculus: 1st integral (INT), 2nd integral (INT2)
- Trigonometric functions (SIN, COS TAN)
- Inverse Trigonometric functions (ASIN, ACOS ATAN)
(Total 11 types)
- Specified calculation between A/B cursors

Waveform calculations can be limited to data within the range specified by A/B cursors.

Calculation operator details:

"2.4 Waveform Processing Calculation Operators and Results" (⇒ p. 34)

Of the eleven types of waveform calculation available, sixteen types can be applied at the same time.

When Scaling is enabled, numerical calculations are performed on scaled values.

2.1 Waveform Calculation Workflow

Before Setting

When specifying a waveform range for calculation: [\[A-B\]](#)

Before executing a calculation, specify the calculation range using the A/B cursors (Vertical or Trace cursors) on the Waveform screen. Set the calculation range on the Wave Calc Settings screen to [\[A-B\]](#).

- Horizontal cursors cannot be used to specify the range.
- When one cursor is used, the calculation range is from the cursor to the end of the data.

See "8.7 Specifying a Waveform Range" in the *Instruction Manual*
"2.2 Settings for Waveform Calculation" (⇒ p. 26) in this manual

Changing calculation settings while measuring

Changes made to calculation settings while measuring are applied after measurement is finished.

To change calculation settings and recalculate

Make changes to calculation contents on the Waveform Calculation Settings screen, and execute the calculation.

See "2.2 Settings for Waveform Calculation" (⇒ p. 26)

To not display a calculation waveform, or to display only the desired waveform

The displayed sheet and calculation waveform to be displayed can be selected on the Sheet Settings screen.

See "2.3 Calculation Waveform Display" (⇒ p. 33)

NOTE

- Maximum recording length available for waveform calculations

Installed Memory (Word)		Maximum recording length (Divisions)
8860	8861	
32M	64M	2,500
128M	256M	10,000
512M	1G	40,000
1G	2G	80,000

If the recording length is set longer than the above maximum, waveform calculation is not performed.


In this case, reset the recording length so that it is below the maximum, or after performing a partial or divided save, reload a portion of the data into the instrument and apply the calculation.

- Waveform calculation is not available when using Roll Mode and Memory Division.
- When Memory Division is disabled, up to 16 past waveforms can be used for reference. However, waveforms other than the currently referring block (that which includes data for calculation) are deleted when waveform calculation executes.
- If a waveform calculation is interrupted when loading data, the incomplete calculation result is displayed. To repeat the calculation, select the [Execute] button on the Waveform Calculation Settings screen.


The following two calculation methods are available:

- Calculate while measuring
Requires making waveform calculation settings beforehand.
- Apply calculations to existing data
Calculations can be applied to data after waveforms are acquired, or after data has been saved to storage media.

Calculating While Measuring

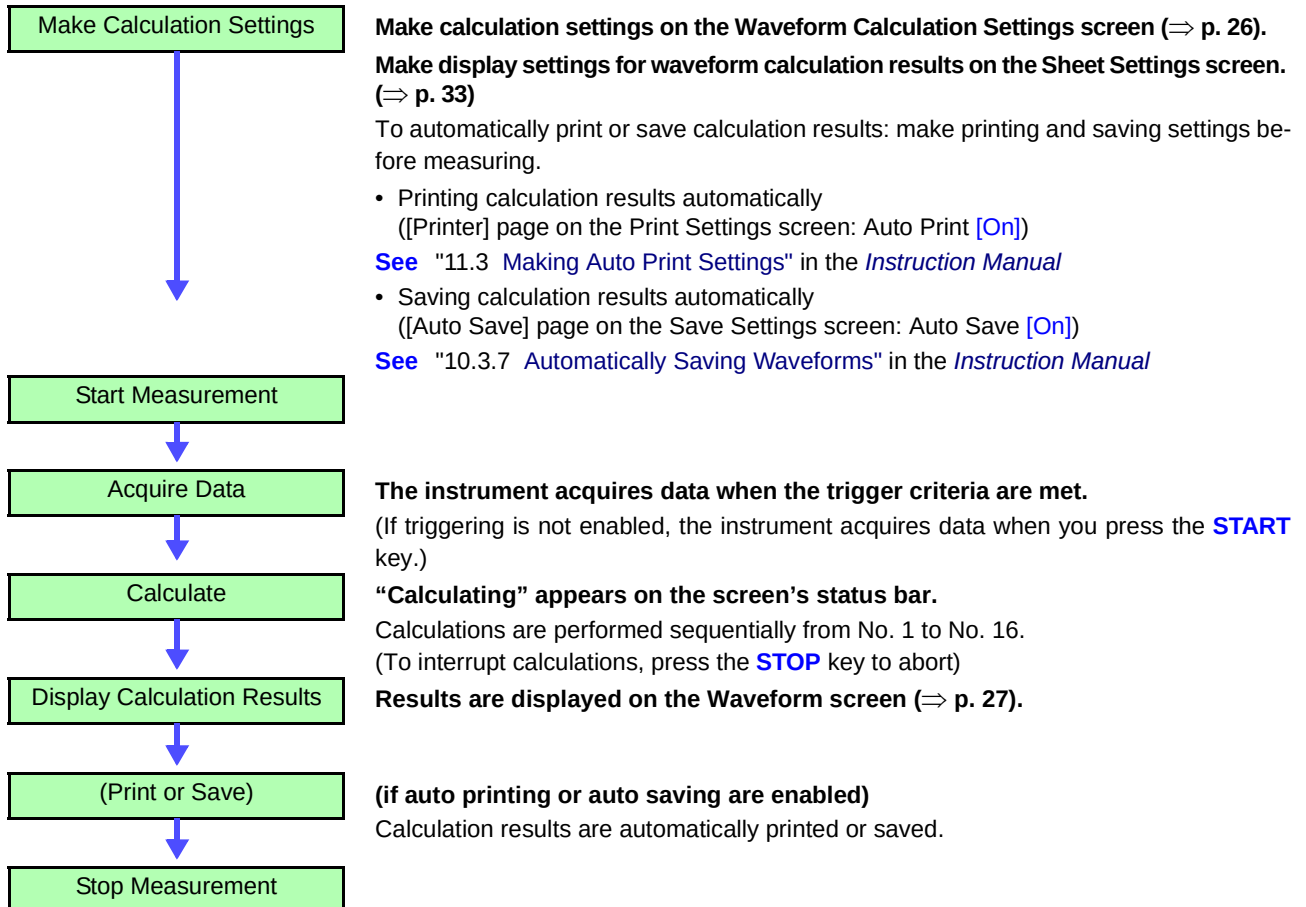

Applying Calculations to Existing Data

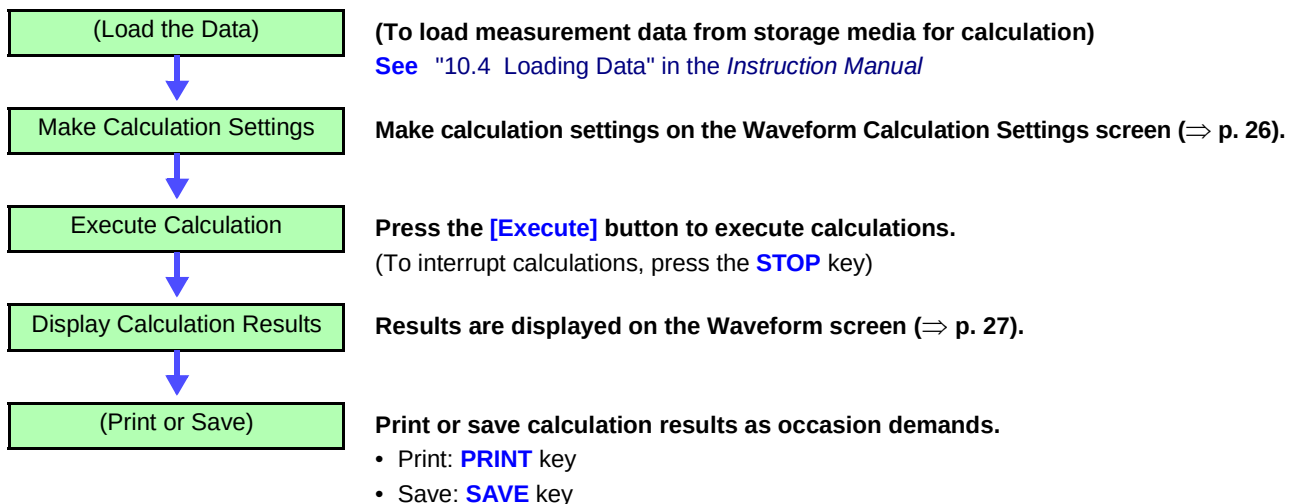

2.2 Settings for Waveform Calculation

Waveform Calculations


MEM

To open the screen: Press the **SET** key → Select **Wave Calc** with the **SUB MENU** keys → Wave Calc Settings screen

Operating Key Procedure

1 Enable the Waveform Calculation function.

CURSOR Move the cursor to the **[Waveform Calc.]** item.
F2 Select **[On]**.

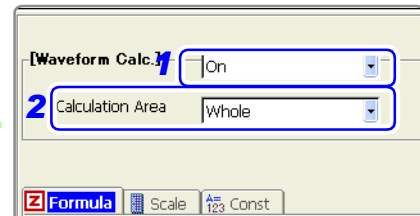

2 Specify the waveform calculation range.

CURSOR Move the cursor to the **[Calculation Area]** item.
F1 to F8 Select either choice.

Whole	Applies calculations to the whole waveform. (default setting)
A-B	Applies calculations to the data between A/B cursors.


When selecting **[A-B]**, specify the calculation range using the A/B cursors on the Waveform screen.

If no measurement data has been acquired by the instrument, first measure once so that the range can be specified for calculations to be applied to subsequent measurements.

3 Perform calculation settings.

CURSOR Move the cursor to your setting choice on the **[Formula]** page.

F1 Select **[Set]**.
 A dialog is displayed for entering a calculation equation.

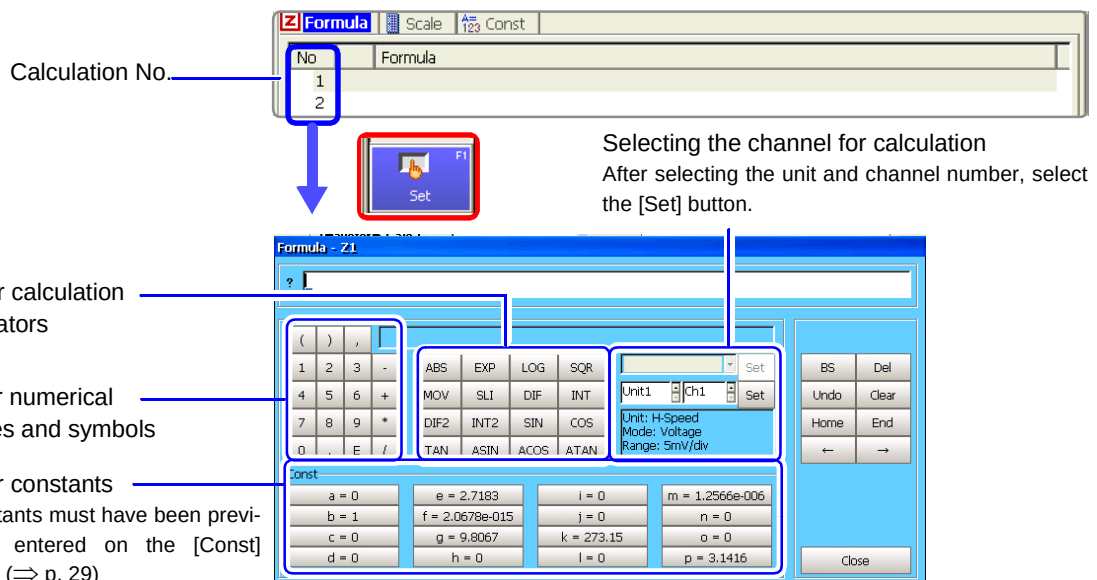

Selecting the channel for calculation
 After selecting the unit and channel number, select the **[Set]** button.

Enter calculation operators

Enter numerical values and symbols

Enter constants
 Constants must have been previously entered on the **[Const]** page. (⇒ p. 29)

CURSOR Select a calculation equation.
F1 to F8 Example of calculation equation entry:(⇒ p. 32)
F7 When finished entry, select **[OK]**.
 The entered equation is displayed in the **[Formula]** field.

The default setting for calculation results display is **[Auto]**.
 To change the display, make settings on the **[Scale]** page.

See "Calculation Waveform Display Settings" (⇒ p. 30)

If "=" is displayed

The entered calculation equation is syntactically correct.

If "?" is displayed

The equation has a syntax error.
 The cursor is placed at the location of the error to facilitate correction.

- Are parentheses correctly matched?
- Has a multiplication operator "*" been omitted?

Operating Key	Procedure
4	(As occasion demands) Make display settings for waveform calculation results on the Sheet Settings screen (⇒ p. 33) Set auto saving and auto printing as needed (<i>Instruction Manual</i>)
5	Execute the calculations.
Applying Calculations to Existing Data	
CURSOR	Move the cursor to the [Execute] button.
F1	Select [Execute].
To calculate while measuring	
START	Starts measurement. Calculation waveforms are displayed after loading waveforms.

4

(As occasion demands)

Make display settings for waveform calculation results on the Sheet Settings screen (⇒ p. 33)

Set auto saving and auto printing as needed (*Instruction Manual*)**5**

Execute the calculations.

Applying Calculations to Existing Data**CURSOR**

Move the cursor to the [Execute] button.



F1

Select [Execute].

To calculate while measuring**START**

Starts measurement.

Calculation waveforms are displayed after loading waveforms.

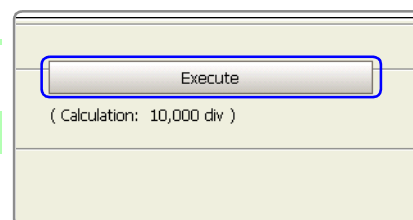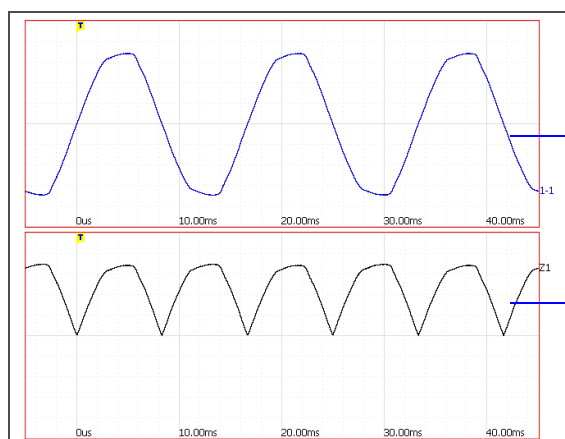**Waveform Calculation Results****Example: Waveform of the calculated absolute value of the waveform of CH1-1. Calculation equation = ABS(CH(1,1))**

CH1-1 Waveform

Absolute Value Waveform

**To copy settings from one calculation to another**

The method is the same as for copying numerical value calculations.

See "Copying Settings Between Calculation Nos." (⇒ p. 10)

**To distribute calculation results onto sheets, or to display in separate Graphs**

Display/non-display of calculation waveforms and graph division can be set on the Sheet Settings screen.

See "2.3 Calculation Waveform Display" (⇒ p. 33)

2.2 Settings for Waveform Calculation

Description About calculation equations

Operators:

Operator	Name	Operator	Name
ABS	Absolute Value	DIF2	2 nd Derivative
EXP	Exponent	INT2	2 nd Integral
LOG	Common Logarithm	SIN	Sine
SQR	Square Root	COS	Cosine
MOV	Moving Average	TAN	Tangent
SLI	Movement parallel to the time axis	ASIN	Inverse Sine
DIF	1 st Derivative	ACOS	Inverse Cosine
INT	1 st Integral	ATAN	Inverse Tangent

See "2.4 Waveform Processing Calculation Operators and Results" ($\Rightarrow$ p. 34)

Entering Calculation Equations

- Each entered calculation equation may contain up to 80 characters.
 - Each constant in a calculation equation may contain up to 30 digits.
 - The multiplication operation (*) must always be explicitly entered.
 - Each calculation expression may contain up to eight instances of the four arithmetic operators.
- Multiplication and division or addition and subtraction of channels within parentheses [e.g., (CH(1,1)*CH(1,2)) or (CH(1,1)+CH(1,2))] each count as one operation.

$$\frac{\text{ABS}(\text{CH}(1,1)) + \text{CH}(1,2) * \text{CH}(2,1) - (\text{CH}(2,2) + \text{CH}(3,2)) * \text{ABS}(\text{CH}(4,1))}{\text{DIF}(\text{CH}(1,1), 1)}$$

1
2
3
4
5

- Division by zero, such as 1/0 (1 $\div$ 0), results in overflow output.
- Channel data is specified in the form CH(u,n), where u = the Unit (input module) number, and n = the number of the channel within input module u. (Example: To specify the data on Channel 2 of Unit 1, enter "CH(1,2)".)
- The result of calculation Z_i can be used in other calculation equations. However, the nth equation can only refer to the results of equations up to Z_{n-1}. (Example: Equation Z4 can include the results of equations Z1 through Z3.)

Using the MOV, SLI, DIF and DIF2 operators in an equation

The number # after a comma within parenthesis (_,#) for each operation is set to the calculation operator.

Operator	Setting Choice	Setting Examples
MOV (Moving Average)	Set the number of points to move. Setting Range	Calculate the 10-point moving average of CH1-1:
SLI (Parallel Movement)	MOV (Moving Average): 1 to 5000 SLI: -5000 to 5000	MOV(CH(1,1),10)
DIF (Derivative)	Specify the sampling interval for differentiation.	Differentiate CH1-2 using a 20-point sampling interval:
DIF2 (2nd Derivative)	"1" is normally acceptable, but this should be set larger to capture fluctuation values of slowly changing waveforms. DIF and DIF2 Setting Range: 1 to 5000	DIF(CH(1,2),20)

2.2 Settings for Waveform Calculation

When calculation results overflow (OVER)

- The displayed A/B cursor values (and those printed when the printer recording type is set to [Numeric]) are incorrect.
- When [Scale] is set to [Auto], waveforms appear at the top or bottom edge of the screen. This makes calculation result overflow obvious.


Waveform calculations with Timebase 2 (measurements using sampling rate 2)

- Calculation equations Z1 to Z8 apply only to Timebase 1, and Z9 to Z16 apply only to Timebase 2.
- Channel data set to use Sampling Rate 1 can only be used in equations Z1 to Z8, and channel data set to use Sampling Rate 2 can only be used in equations Z9 to Z16.
- Inclusion of the results of one calculation (Zn) in another is also limited to only those calculations which apply to the same timebase.
(Example: equation Z8 can include only the results of Z1 to Z7, and Z16 can include only the results of Z9 to Z15.)

Defining Constants

MEM

To open the screen: Press the SET key → Select Wave Calc with the SUB MENU keys → Wave Calc Settings screen

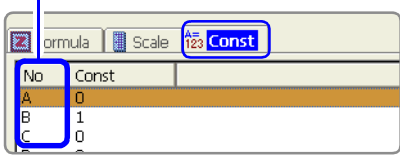Operating Key	Procedure	Constant No.
SHEET/PAGE	Select the [Const] page.	
CURSOR	Move the cursor to the Constant No. to be defined.	
F1 to F8	Select an entry method, and enter the constant. Setting range: -9.9999E+29 to +9.9999E+29	
	See "3.3.3 Entering Text and Numbers" in the Instruction Manual	

Defined constants are shown in the constant display of the calculation equation setting dialog.

2.2 Settings for Waveform Calculation

Calculation Waveform Display Settings

MEM

To open the screen: Press the **SET** key → Select **Wave Calc** with the **SUB MENU** keys → Wave Calc Settings screen


Operating Key Procedure

1 SHEET/PAGE Select the [Scale] page.

Calculation No.

Settings can also be made in a dialog. (⇒ p. 31)

To copy settings between Calculation Nos.:
Select F2 [Copy].

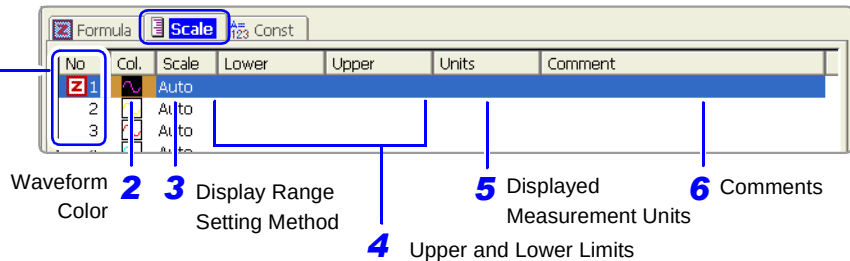

2 Enable waveform display, and display color

CURSOR

Move the cursor to the [Color] column.

F1 to F8

Select whether to display the waveform, and its color (when On)

Off The waveform is hidden.

On The waveform is displayed.
(default setting)

3 Select a method to set scaling

CURSOR

Move the cursor to the [Scale] column for the Calculation No. to be set.

F1 to F8

Set the display range for the calculation waveform.

Auto Automatically sets the display range of the vertical axis. (After calculation, the upper and lower limits are obtained from the results, and set automatically.)

Manual Upper and lower limits of the vertical axis display range are entered manually.

Depending on calculation results, automatic scaling settings may be unsatisfactory, in which case the limits must be entered manually.

4 Set the upper and lower limits of the display range (when [Manual] is selected)

CURSOR

Select [Lower] and [Upper].

F1 to F8

Select an entry method and enter the limit values.
Entry range: -9.9999E+29 to +9.9999E+29

See "3.3.3 Entering Text and Numbers" in the *Instruction Manual*

5 Specify the physical units

CURSOR

Move the cursor to the [Units] column.

F1 to F8

Select an entry method and enter the physical units.

6 Enter a comment (as occasion demands)

CURSOR

Move the cursor to the [Comment] column.

F1 to F8

Enter your comment.

Making settings in the [Calculation] dialog

Calculation No.

F1 Move the cursor to the [No.] column of the calculation to set, and select **F1 [All Settings]** to open the [Calculation] dialog.

Upper and Lower Limit Settings

Set the Value per Division.

Set the Zero Position (same as the Variable Function Setting).

2.2 Settings for Waveform Calculation

Waveform Calculation Example Calculate the RMS waveform from the instantaneous waveform

The RMS values of the waveform input on Unit 1 Channel 1 are calculated and displayed. This example describes the calculation of waveform data measured for one cycle over two divisions.

Operating Key Procedure

- 1 Enable the Waveform Calculation function.
- CURSOR Move the cursor to the [Waveform Calc.] item.
- F2 Select [On].

- 2 Specify the waveform calculation range.
- CURSOR Move the cursor to the [Calculation Area] item.
- F1 Select [Whole].

- 3 Perform calculation settings.
- CURSOR Move the cursor to No. 1 on the [Formula] page.
- F1 Select [Set].
- A dialog is displayed for entering a calculation equation.

Entering the calculation equation

$$\text{SQR}(\text{MOV}(\text{CH}(1,1)*\text{CH}(1,1),200))$$

The number of samples per cycle (1 division = 100 samples) Here, one cycle is two divisions (200 samples)


Enter numerical values and symbols

It is convenient to set constants beforehand on the [Const] page. (⇒ p. 29)




When finished entry, select **F7 [OK]**.
The entered equation is displayed in the [Formula] field.

- 4 Execute the calculations.

- START Starts measurement.
- The calculation waveform is displayed after acquiring the input waveform.

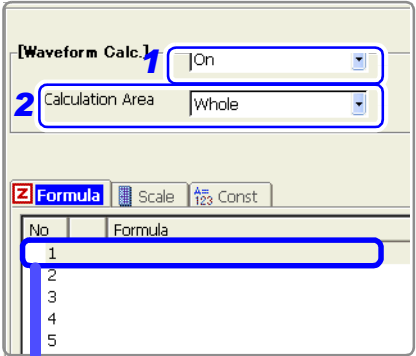

After selecting the unit and channel number, select the [Set] button.

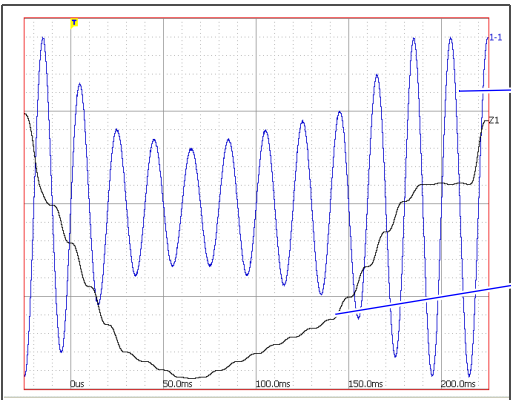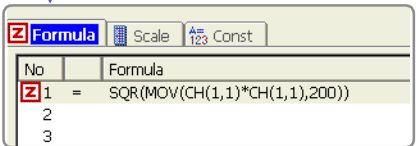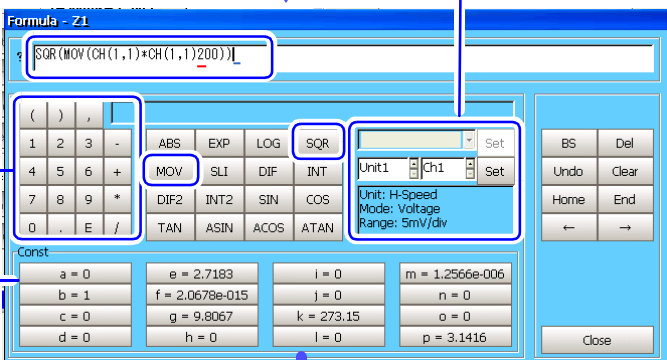

To view the waveform calculated from the acquired data, press the [Execute] button on the Waveform Calculation Settings screen.


2.3 Calculation Waveform Display

Assignment of calculation results and split-screen graph display arrangement can be set.
These settings are effective when Waveform Calculation is enabled.

Waveform Calculation Display Settings MEM

To open the screen: Press the SET key → Select Sheet with the SUB MENU keys →Sheet Settings screen

Operating Key	Procedure
1 SHEET/PAGE	Select the [Wcal] page.
2	Select whether to display calculation waveforms.
CURSOR	Move the cursor to the [Unit-Ch] column for the Calculation No. to be displayed.
F1 to F8	Select the desired calculation equation for display.
	Off The calculation waveform is not displayed.
	Z1 to Z16 Displays the selected calculation waveform.
3	Select a Graph for display. (when [Split-Screen] is set to [2 Graphs] or more, or the [Display Type] is set to [Wave+X-Y])
CURSOR	Move the cursor to [Graph].
F1 to F8	Select the Graph number to be displayed. Graph number samples (G1, G2, ...) are displayed at the left side of the screen.
4	Verify the calculation waveform on the Waveform screen.
DISP	The Waveform screen appears.

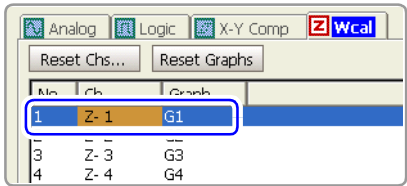

Z1 to Z16 correspond to the calculation equations defined on the Waveform Calculation Setting (Wave Calc) screen.

2.4 Waveform Processing Calculation Operators and Results

b_i : i th member of calculation result data, d_i : i th member of source channel data

Waveform Calculation Type	Description
Four Arithmetic Operators (+, -, *, /)	Executes the corresponding arithmetic operation.
Absolute Value (ABS)	$b_i = d_i $ ($i = 1, 2, \dots, n$)
Exponent (EXP)	$b_i = \exp(d_i)$ ($i = 1, 2, \dots, n$)
Common Logarithm (LOG)	When $d_i > 0$, $b_i = \log_{10} d_i$ When $d_i = 0$, $b_i = -\infty$ (overflow value output) When $d_i < 0$, $b_i = \log_{10} d_i$ ($i = 1, 2, \dots, n$) Note: Use the following equation to convert to natural logarithm calculations. $\ln X = \log_e X = \log_{10} X / \log_{10} e$ $1 / \log_{10} e \approx 2.30$
Square Root (SQR)	When $d_i \geq 0$, $b_i = \sqrt{d_i}$ When $d_i < 0$, $b_i = -\sqrt{ d_i }$ ($i = 1, 2, \dots, n$)
Moving Average (MOV)	When k is odd number: $b_i = \frac{1}{k} \sum_{t=i-\frac{k}{2}}^{i+\frac{k}{2}} dt$ ($i = 1, 2, \dots, n$) When k is even number: $b_i = \frac{1}{k} \sum_{t=i-\frac{k}{2}+1}^{i+\frac{k}{2}} dt$ ($i = 1, 2, \dots, n$) dt: t^{th} member of source channel data k: number of points to move (1 to 5000) 1 div = 100 points. k is specified after a comma. (Ex.) To make Z1 the moving average of 100 points: MOV(Z1,100)
Slides waveform data along the time axis (SLI)	Moves along the time axis by the specified distance. $b_i = d_i - k$ ($i = 1, 2, \dots, n$) k: number of points to move (-5000 to 5000) k is specified after a comma. (Ex.) To slide Z1 by 100 points along the time axis: SLI(Z1,100) Note: When sliding a waveform, if there is no data at the beginning or end of the calculation result, the voltage value becomes zero. 1 div = 100 points.
Sine (SIN)	$b_i = \sin(d_i)$ ($i = 1, 2, \dots, n$) Trigonometric functions employ radian (rad) units.
Cosine (COS)	$b_i = \cos(d_i)$ ($i = 1, 2, \dots, n$) Trigonometric functions employ radian (rad) units.
Tangent (TAN)	$b_i = \tan(d_i)$ ($i = 1, 2, \dots, n$) where $-10 \leq b_i \leq 10$ Trigonometric functions employ radian (rad) units.
Arcsine (ASIN)	When $d_i > 1$, $b_i = \pi / 2$ When $-1 \leq d_i \leq 1$, $b_i = \text{asin}(d_i)$ When $d_i < -1$, $b_i = -\pi / 2$ Trigonometric functions employ radian (rad) units.

2.4 Waveform Processing Calculation Operators and Results

b_i : i th member of calculation result data, d_i : i th member of source channel data

Waveform Calculation Type	Description
Arccosine (ACOS)	When $d_i > 1$, $b_i = 0$ When $-1 \leq d_i \leq 1$, $b_i = \text{acos}(d_i)$ When $d_i < -1$, $b_i = \pi$ ($i = 1, 2, \dots, n$) Trigonometric functions employ radian (rad) units.
Arctangent (ATAN)	$b_i = \text{atan}(d_i)$ ($i = 1, 2, \dots, n$) Trigonometric functions employ radian (rad) units.
First derivative (DIF) Second derivative (DIF2)	The first and second derivative calculations use a fifth-order Lagrange interpolation polynomial to obtain a point data value from five sequential points. d_1 to d_n are the derivatives calculated for sample times t_1 to t_n. Note: Scattering of calculation results increases as input voltage level decreases. If scattering is excessive, apply the moving average (MOV). Calculation formulas for the first derivative Point t_1 $b_1 = (-25d_1 + 48d_2 - 36d_3 + 16d_4 - 3d_5)/12h$ Point t_2 $b_2 = (-3d_1 - 10d_2 + 18d_3 - 6d_4 + d_5)/12h$ Point t_3 $b_3 = (d_1 - 8d_2 + 8d_4 - d_5)/12h$ ↓ Point t_i $b_i = (d_{i-2} - 8d_{i-1} + 8d_{i+1} - d_{i+2})/12h$ ↓ Point t_{n-2} $b_{n-2} = (d_{n-4} - 8d_{n-3} + 8d_{n-1} - d_n)/12h$ Point t_{n-1} $b_{n-1} = (-d_{n-4} + 6d_{n-3} - 18d_{n-2} + 10d_{n-1} + 3d_n)/12h$ Point t_n $b_n = (3d_{n-4} - 16d_{n-3} + 36d_{n-2} - 48d_{n-1} + 25d_n)/12h$ b_1 to b_n: calculation results $h = \Delta t$: Sampling Period Calculation formulas for the second derivative Point t_1 $b_1 = (35d_1 - 104d_2 + 114d_3 - 56d_4 + 11d_5)/12h^2$ Point t_2 $b_2 = (11d_1 - 20d_2 + 6d_3 + 4d_4 - d_5)/12h^2$ Point t_3 $b_3 = (-d_1 + 16d_2 - 30d_3 + 16d_4 - d_5)/12h^2$ ↓ Point t_i $b_i = (-d_{i-2} + 16d_{i-1} - 30d_i + 16d_{i+1} - d_{i+2})/12h^2$ ↓ Point t_{n-2} $b_{n-2} = (-d_{n-4} + 16d_{n-3} - 30d_{n-2} + 16d_{n-1} - d_n)/12h^2$ Point t_{n-1} $b_{n-1} = (-d_{n-4} + 4d_{n-3} + 6d_{n-2} - 20d_{n-1} + 11d_n)/12h^2$ Point t_n $b_n = (11d_{n-4} - 56d_{n-3} + 114d_{n-2} - 104d_{n-1} + 35d_n)/12h^2$

2.4 Waveform Processing Calculation Operators and Results

b_i : ith member of calculation result data, d_i : ith member of source channel data

Waveform Calculation Type	Description
First integral (INT) Second integral (INT2)	First and second integrals are calculated using the trapezoidal rule. d_1 to d_n are the integrals calculated for sample times t_1 to t_n. Calculation formulas for the first integral Point t_1 $I_1 = 0$ Point t_2 $I_2 = (d_1 + d_2)h/2$ Point t_3 $I_3 = (d_1 + d_2)h/2 + (d_2 + d_3)h/2 = I_2 + (d_2 + d_3)h/2$ ↓ Point t_n $I_n = I_{n-1} + (d_{n-1} + d_n)h/2$ I_1 to I_n: calculation results $h = \Delta t$: Sampling Period Calculation formulas for the second integral Point t_1 $II_1 = 0$ Point t_2 $II_2 = (I_1 + I_2)h/2$ Point t_3 $II_3 = (I_1 + I_2)h/2 + (I_2 + I_3)h/2 = II_2 + (I_2 + I_3)h/2$ ↓ Point t_n $II_n = II_{n-1} + (I_{n-1} + I_n)h/2$ II_1 to II_n: calculation results

FFT Function

Chapter 3

3.1 Overview and Features

FFT analysis can only be used with the FFT function.

The FFT (Fast-Fourier Transform) functions provide frequency analysis of input signal data.

Use these functions for frequency analysis of rotating objects, vibrations, sounds and etc.

For details, refer to "3.11 FFT Definitions" ($\Rightarrow$ p. 103).

Analysis can be performed on data as it is being measured, on pre-existing analog waveform data previously acquired with the Memory function, and on data output from waveform calculations.

However, FFT analysis cannot be applied to data acquired with the Model 8958 16-Ch Scanner Unit. Also, FFT analysis cannot be applied to pre-existing waveform data acquired from channels that used Timebase 2 for sampling.

When using an input module equipped with an anti-aliasing filter, the cut-off frequency can be automatically set by linking with the frequency range setting.

(Model 8938 FFT Analog Unit, 8947 Chargin Unit, 8957 High Resolution Unit, 8960 Strain Unit)

Major Features

- FFT analysis frequency range: 133 mHz to 8 MHz
- Frequency resolution: $1/400^{\text{th}}$, $1/800^{\text{th}}$, $1/2000^{\text{th}}$ or $1/4000^{\text{th}}$ of the frequency range
- FFT Analysis Modes (16 types)
 - Storage Waveform
 - RMS Spectrum
 - Power Spectrum Density*
 - Auto-correlation Function
 - Transfer Function
 - Impulse Response
 - 1/1 Octave Analysis*
 - Phase Spectrum
 - Linear Spectrum
 - Power Spectrum
 - Cross-power Spectrum
 - Histogram
 - Cross-correlation Function
 - Coherence Function
 - 1/3 Octave Analysis*
 - Power Spectrum Density (LPC)*

* Not available when using external sampling.

For phase spectra, only the required phase information is highlighted and displayed.

[See "3.4.7 Emphasizing Analysis Results \(phase spectra only\)" \(\$\Rightarrow\$ p. 61\)](#)

Also, when performing FFT analysis with the instrument connected to a sound level or vibration meter, scaling by dB can be set from the Channel Settings screen if you want to read values directly in calibrated units of measurement.

[See "Scaling" \(\$\Rightarrow\$ p. 71\)](#)

NOTE

To suppress the effects of aliasing distortion

We recommend using input modules that are equipped with anti-aliasing filtering to suppress the effects of aliasing distortion when sampling.

[See Aliasing Distortion and Anti-Aliasing Filters](#)
["3.11 FFT Definitions" \(\$\Rightarrow\$ p. 103\)](#)

Refer to the *Instruction Manual* for FFT function specifications.


3.2 Screen Organization (FFT Function)

Measurement-related settings for FFT analysis are made on the Settings screens (Status, Channel, Trigger and Sheet); saving and printing settings are made on the Save Settings and Print Settings screens; and measurement data display settings are made on the Waveform screen. The Channel Settings, Trigger Settings, Save Settings and Print Settings screens are nearly the same as for the other operating functions.

3.2.1 Waveform Screen

To open the Waveform screen

- 1 Press the **DISP** key
(The Waveform screen appears)



Press the **SUB MENU** keys
(To change choices of setting items)

Press the **SHEET/PAGE** keys
(To change sheets)
This is valid only when measurement data has been assigned to multiple sheets.

Data acquired by the instrument can be displayed as any of the following types. The display type can be selected for each Sheet.

Display type:

- FFT
- Nyquist
- FFT+Nyquist
- Wave+FFT
- Wave+Nyquist

See "3.6 Setting the Screen Layout of the Waveform Screen" (⇒ p. 72)

Function Menu
Select a function before measuring.

On-screen changes can be made by clicking the mouse.

Recorded Data
Shows data acquired with this instrument.

Status Bar
This bar indicates the current states of data acquisition, internal processing, settings and display information.

Setting Items and Choices (⇒ p. 39)
Calculation configuration and trigger criteria settings can be changed. These can be changed while measuring. Press the **SUB MENU** keys to select the items to change.

Clock
Shows the current time. You can change the display appearance.

"Key Lock" appears when the key-lock state is enabled.

Setting Choices
The cursor indicates the current setting choice. Select with F keys (F1 to F8). Press the **FUNCTION MODE** key to change the F key functions.


F-Key Function Status
Shows the current F key status.

Internal and External Connection Status

Sheet No.

Input Channel Settings Dialog
Input channel settings can be changed. (Appears when you press the **UNIT** or **CH** keys, or press or turn the **RANGE** knob)


A/B Cursor Settings Dialog
Select the type of cursors. (Appears when you press the **TYPE** key or knob **A**)
Press the **ESC** key to remove the dialog.

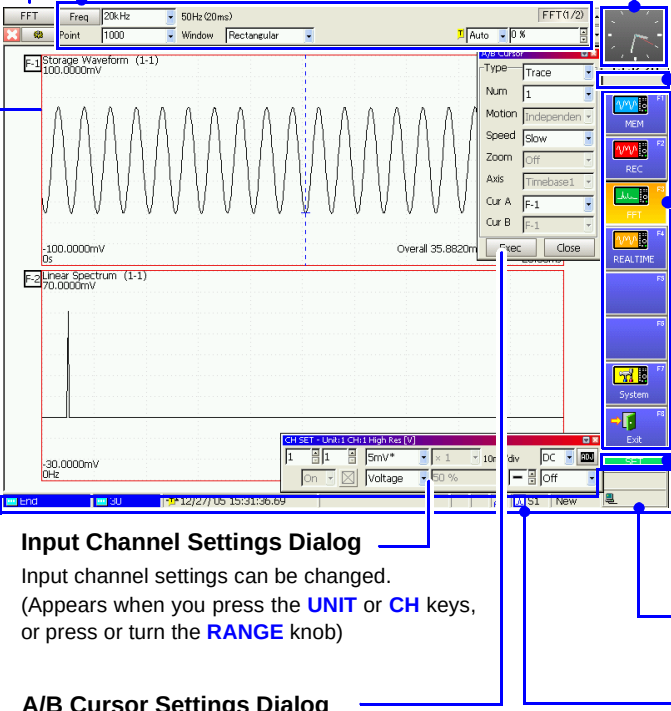

Setting Items and Choices

FFT Function Settings [FFT(1/2)]


See "3.4.10 Setting and Changing Analysis Conditions on the Waveform Screen" (⇒ p. 67)

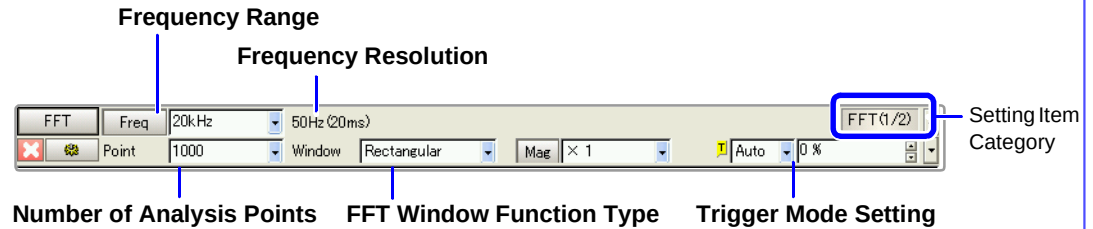

↕ Switch with the **SUB MENU** keys

FFT Function Settings [FFT(2/2)]

See "3.4.10 Setting and Changing Analysis Conditions on the Waveform Screen" (⇒ p. 67)

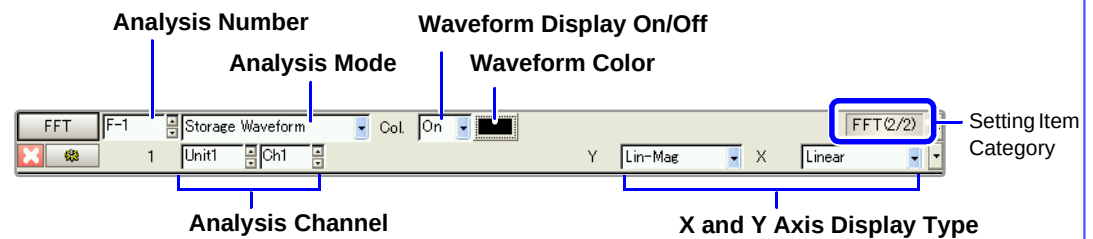


↕ Switch with the **SUB MENU** keys

Analog Trigger Settings [Trigger]

See "6.7 Triggering by Analog Signals" in the *Instruction Manual*

(When using Level Triggering) **Type of Analog Trigger**

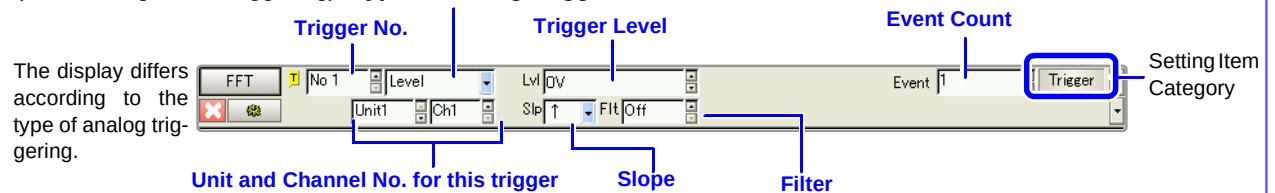

3.2.2 Settings Screen

To open the Settings screen

- 1 Press the **SET** key. (The Settings screen appears.)

MENU

DISP

SET

FILE

SUB MENU

E

SELECT

SHEET/PAGE

2 Press the **SUB MENU** keys to select from the Settings menu.

3 Press the **SHEET/PAGE** keys to select a page.
- Status

Status Settings Screen
- Make settings here for FFT analysis.
- Input Data Selection (⇒ p. 52)
- Select whether FFT analysis is to be applied to newly acquired data, or to a pre-existing waveform (Memory waveform).
- Frequency Range and Number of Calculation Points (⇒ p. 53)
- More calculation points provide greater frequency resolution.
- Window Function Settings (⇒ p. 56)
- Selects a window function and correction for acquiring input signals.
- FFT Analysis Settings (⇒ p. 62)
- | No. | Analyze | Col. | Parameter | Ch1 | Ch2 | Yaxis | Xaxis |
|-----|------------------------|------|----------------|-----|-----|---------|--------|
| 1 | Storage Waveform | A | Normal | 1-1 | | Lin-Mag | Linear |
| 2 | Linear Spectrum | A | | 1-1 | | Lin-Mag | Linear |
| 3 | RMS Spectrum | A | | 1-1 | | Lin-Mag | Linear |
| 4 | Power Spectrum | A | | 1-1 | | Lin-Mag | Linear |
| 5 | Power Spectrum Density | A | | 1-1 | | Lin-Mag | Linear |
| 6 | Auto Correlation | A | | 1-1 | | Lin-Mag | Linear |
| 7 | Histogram | A | | 1-1 | | Lin-Mag | Linear |
| 8 | 1/1 Octave | A | Filter: Normal | 1-1 | | Lin-Mag | Log |
- Peak Value Display Setting (⇒ p. 57)
- Selects whether to display the peaks (maximal or maximum) of analysis results.
- Averaging Settings (⇒ p. 58)
- Noisy or unstable values can be averaged to clarify the waveform display. When averaging is enabled, select the method and count for averaging.
- Phase Spectra Highlighting
- For the maximum value of a power spectrum or cross-power spectrum, data exceeding the specified ratio can be displayed with emphasis (highlighted).
- [Analyze] Page
- | No. | Analyze | Col. | Parameter | Ch1 | Ch2 | Yaxis | Xaxis |
|-----|------------------------|------|-----------|-----|-----|---------|--------|
| 1 | Storage Waveform | A | Normal | 1-1 | | Lin-Mag | Linear |
| 2 | Linear Spectrum | A | | 1-1 | | Lin-Mag | Linear |
| 3 | RMS Spectrum | A | | 1-1 | | Lin-Mag | Linear |
| 4 | Power Spectrum | A | | 1-1 | | Lin-Mag | Linear |
| 5 | Power Spectrum Density | A | | 1-1 | | Lin-Mag | Linear |
- Selects the analysis mode, analysis channels, x and y axes and display parameters. (⇒ p. 62)
- [Scale] Page
- | No. | Scale | Lower | Upper | Units | Comment |
|-----|-------|-------|-------|-------|---------|
| 1 | Auto | | | V | |
| 2 | Manu | -70m | 30m | V | |
| 3 | Auto | | | V | |
| 4 | Auto | | | V² | |
- Sets the display scale of the vertical (y) axis. (⇒ p. 66)

Channel

Channel Settings Screen

Set analog channels.

All Channel Settings List
(The Logic page is not accessible)

Setting Unit (Module)
and Channel Nos.

Level Monitor

Indicates the value and range of input relative to the area displayed on the waveform screen for verification.

Input Waveform Settings

Set the waveform display color, zero position, vertical axis magnification and display area. These settings are also available on the [All Ch] page.

Comment Setting


Make this setting to enter channel-specific comments. This setting is also available on the [Comment] page. Comments can be displayed on the Waveform screen.

Input Module Settings

Set the input channels for the installed input modules. See "Chapter 3 Input Channel Settings" in the *Input Module Guide*. These settings are also available on the [All Ch] page.

Scaling Settings (⇒ p. 71)

Make these settings to convert measurement units for display as physical values when using a clamp or external sensor. These settings are also available on the [Scaling] page.

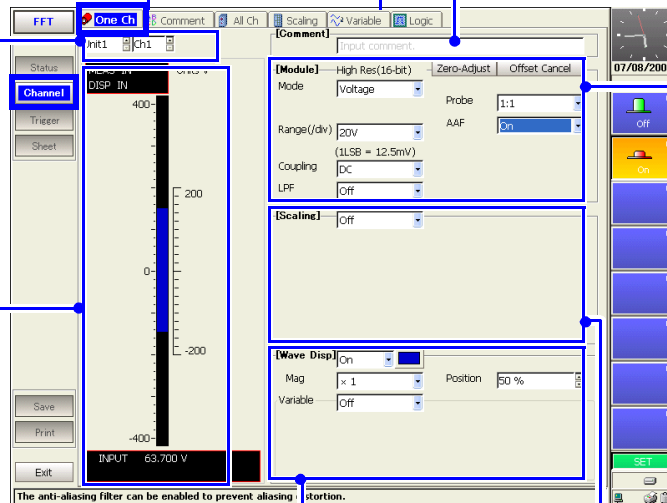

Trigger

Trigger Settings Screen

Set trigger criteria.

Trigger Mode Setting

Sets trigger activation criteria.

Combining Method
(AND/OR) for Multiple
Trigger Sources

Pre-Trigger Settings

Make these settings to record prior to triggering. When Trigger Priority is On, triggering is allowed during the Pre-Trigger Wait.

Analog Trigger Settings


Timer Trigger Settings

Set recording start and end times, and set timing when desired to apply a trigger within a specified period.

External Trigger
Settings

Set this to accept triggering from a signal input on the External Trigger terminal.

Logic Trigger Settings

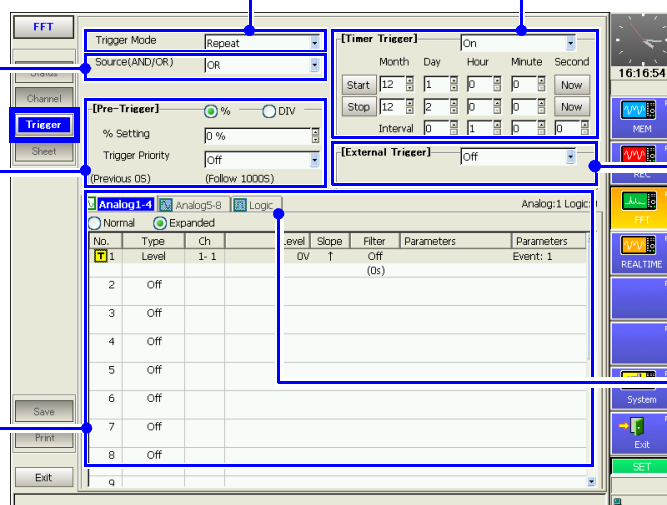

3.2 Screen Organization (FFT Function)

Settings on the [Analog] and [Wcal] pages are the same as for the Memory function.

Sheet


Sheet Settings Screen

Set the display method for the Waveform screen.

Screen Layout Setting (⇒ p. 72)

Set the data type and display arrangement for each sheet to be displayed.

- Sheet Name setting
- Display type
- Split screen

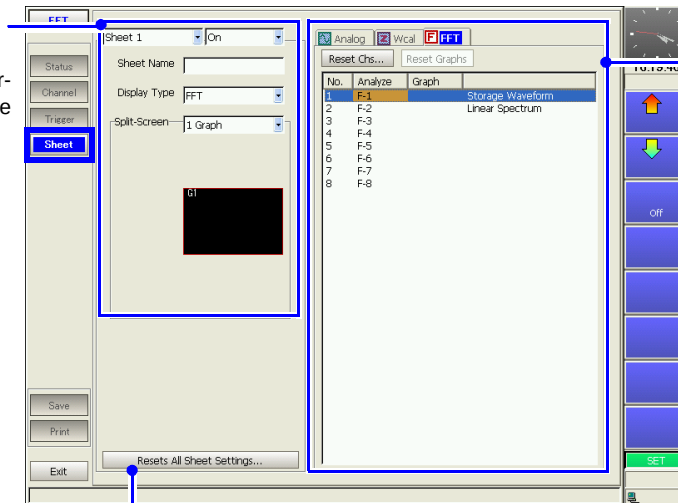


Assigning Channels to Sheets

Assigns the channel, calculation results and waveform display position for each display sheet.

Resets all sheet settings

[Analog] Page

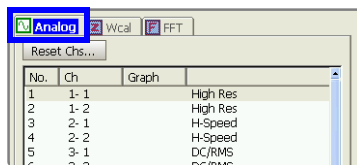

Assign analog channels.

See "7.2.6 Assigning Display Channels to Graphs (Analog Channels)" in the *Instruction Manual*


[Wcal] Page



Arrange waveform calculation results.

See "2.3 Calculation Waveform Display" (⇒ p. 33)

[FFT] Page

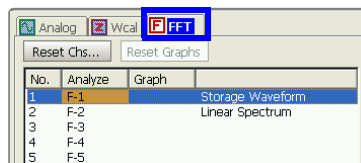

Assigns FFT analysis results and sets graph arrangement for split-screen display.

Setting procedures on the Save Settings screen are the same for all functions.

See "Chapter 10 Saving/Loading Data & Managing Files" in the *Instruction Manual* for details.

Save

Save Settings Screen [Auto Save] Page

Make these settings to specify automatic saving.

The factory default setting for auto save is [Off].

Auto-Save Settings

Select the action to take when the save destination or storage media becomes full during automatic saving, such as whether to create new directories. (Default setting: [Off])

Settings for Saving Waveform Data

Select the saving format, area to save and related settings for automatic saving.

Settings for Saving Screen Images

Make these setting to automatically save Waveform screens.

Save

Save Settings Screen [SAVE Key] Page

These settings determine the operation of the **SAVE** key.

Manual Save Settings (Saving by SAVE key)

Set the save destination, file name and related settings for saving with the **SAVE** key.

Settings for Saving Waveform Data

Select the saving format, area to save and related settings for waveform saving.

Save settings are also available for saving settings data and display images.

Save Type Settings

Select what to save with the **SAVE** key. Display contents depend on the selections.

3.2 Screen Organization (FFT Function)

Setting procedures on the Print Settings screen are the same for all functions.
See "Chapter 11 Printing" in the *Instruction Manual* for details.

Print

Print Settings Screen [Printer] Page

Select the printing method and printer for automatic or manual printing.

The factory default setting for auto print is [Off].

Auto Print Settings

Make these setting to print automatically.

Manual Print Settings

Set the printing method (Quick or Selection Print) and items you want to print when pressing the **PRINT** key.

Internal Printer Settings

Set the printer's print density and quality.

External Printer Settings

Set the paper orientation and margins.

Print

Print Settings Screen [Print Items] Page

Select the items to be printed (printout contents).

Print Item Common Settings

Select the printout type, print area and horizontal axis display value.

Waveform Printing Settings

Select the items to print when printing waveforms.


- Grid Type
- List & Gauge
- Print Upper and Lower Limits
- Print Counter

Numerical Printing Settings

Select the thinning method for numerical data.

Printing Settings for Comments, Title and Settings Data

3.3 Operation Workflow

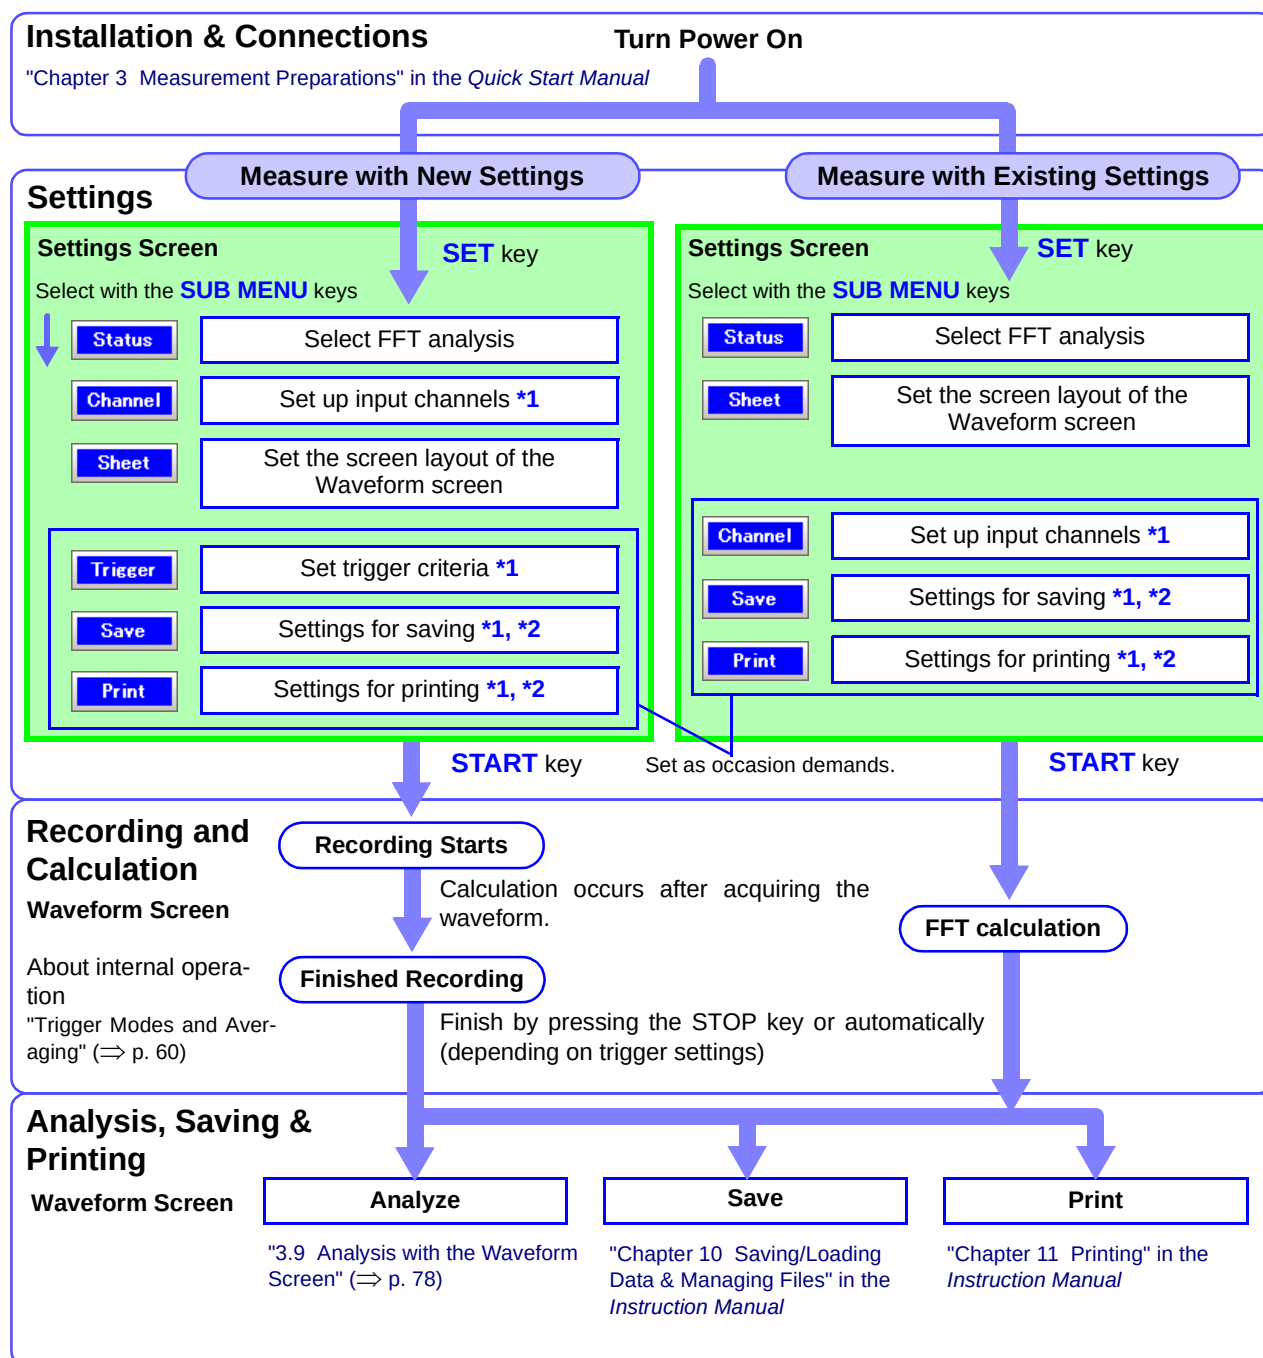

*1. Settings are the same as for the Memory and Recorder functions. Refer to the *Instruction Manual* for details about each setting.


*2. When saving or printing manually, settings can be changed after calculation.

Settings Procedure for FFT Analysis

Function Selection


Opening screen:

Press the F3 [FFT] key.

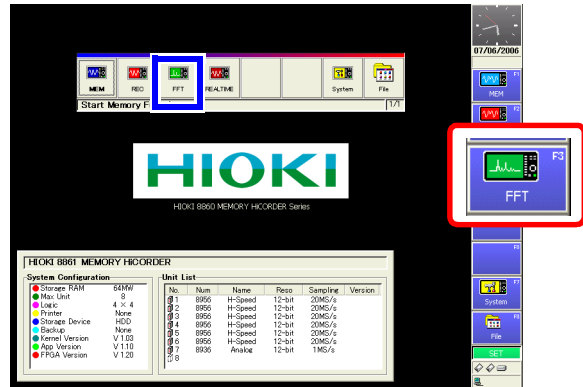
Select the FFT function ($\Rightarrow$ p. 51).

Waveform screen or Settings screen:

Using the CURSOR keys, move the cursor to the Function menu, and press the F3 [FFT] key.

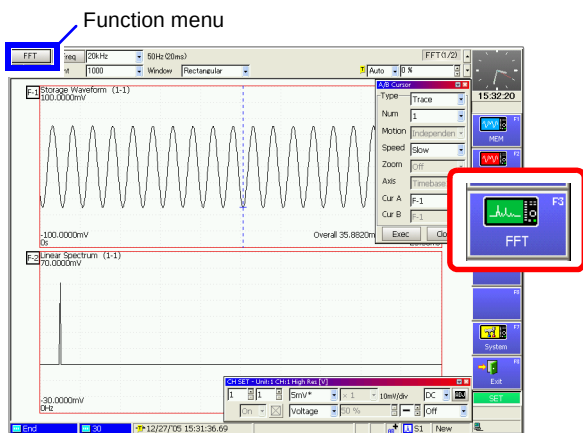

Waveform screen

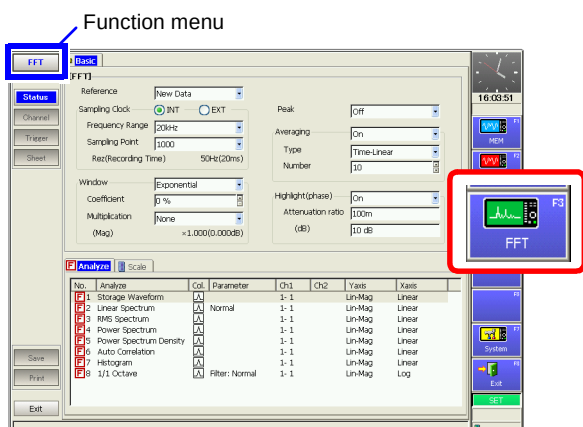

Settings screen

Measurement Configuration Settings

Press the **SET** key to open the Settings screen.
Press the **SUB MENU** keys to select the **Status** menu

1 Select the input data
Select whether to analyze newly acquired data, or existing data.

2 Select the frequency range and number of points for FFT analysis

3 Select the desired window function
Set the window function to be applied to the input signal.

4 Select the peak value display
Select whether to display local or global maximum result values (maximal/ maximum).


5 Set averaging
If averaging is desired, select the method and count for averaging.

6 Set highlighting (attenuation correction rate, for phase spectrum analysis only)
Select whether a spectrum is to be displayed with highlighting. If highlighting, sets the attenuation correction ratio to the maximum value of the power spectrum (or cross-power spectrum).



7 Select the analysis type
Select the analysis type, x axis, y axis, waveform color and channels to be analyzed (up to eight).

8 Set scaling
Set the display scale of the vertical (y) axis.

Make settings on the Status Settings screen.

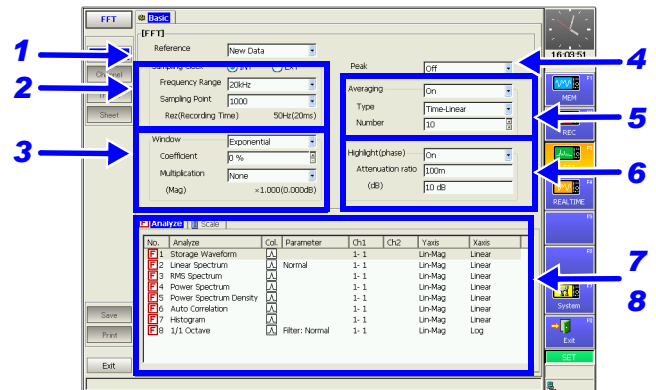

See "3.4 Setting FFT Analysis Conditions" (⇒ p. 51)

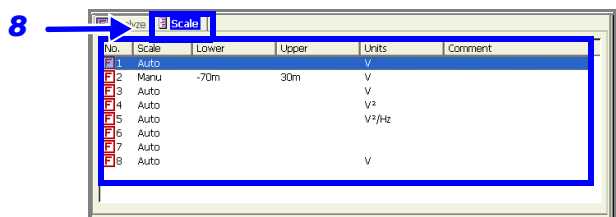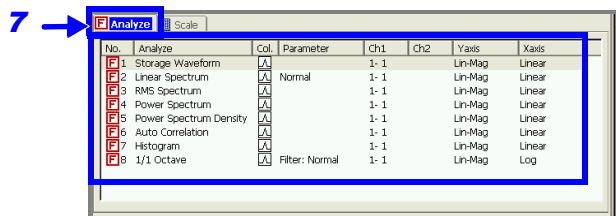

Input Channel Settings

Press the **SUB MENU** keys to select the **Channel** menu

Press the **SHEET/PAGE** keys to select the **[One Ch]** page


- 9 Select the Unit (module) and Channel
- 10 Select the measurement range (vertical axis)
Make input-module-related settings
- 11 Perform zero adjustment
(after warm-up)
- 12 (As occasion demands) Set the scaling

Trigger Settings

Press the **SUB MENU** keys to select the **Trigger** menu

- 13 Set the trigger mode
Default setting: **[Auto]**
- 14 Set the trigger criteria (AND/OR)
Default setting: **[OR]**
- 15 (As occasion demands) Set pre-trigger
- 16 Set each trigger source
Default setting: All **[Off]**


Make settings on the Channel Settings screen.

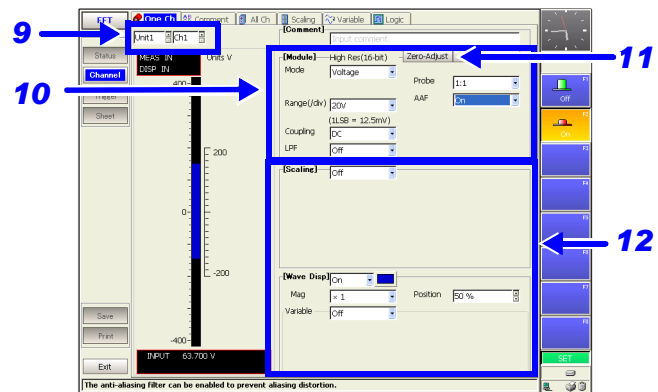

See "3.5 Selecting Channels" (⇒ p. 69)


(If you want to record a specific waveform, such as an anomaly)

Set on the Trigger Settings screen.

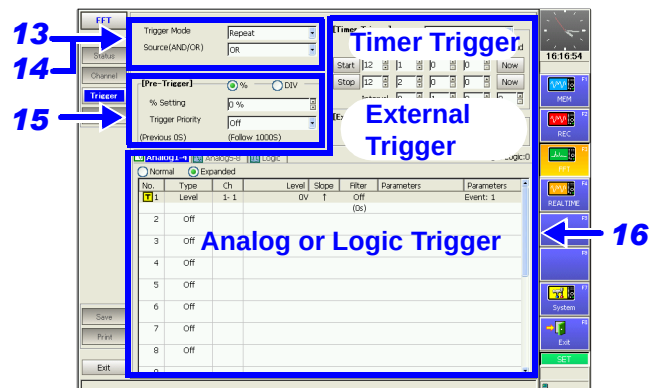


Settings are the same as for the Memory function.

See "Chapter 6 Trigger Settings" in the *Instruction Manual*

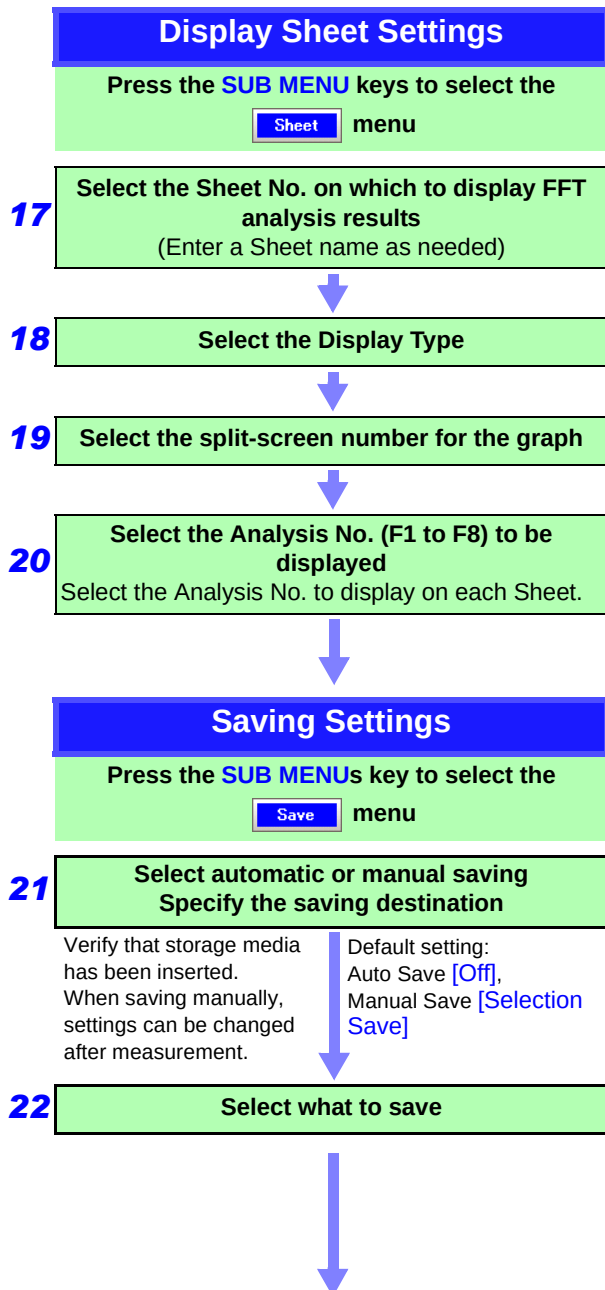


(Configure the Waveform screen display layout)
Set on the Sheet Settings screen.

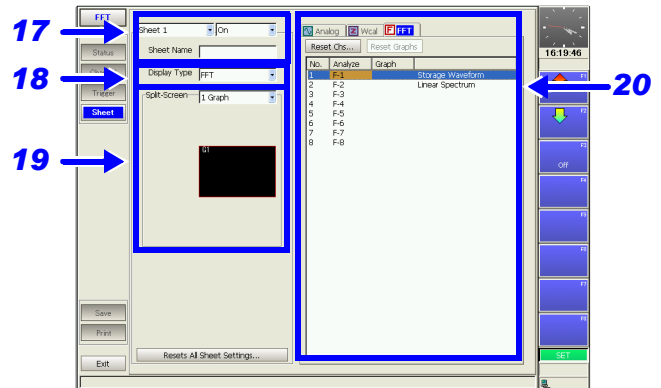

See "3.6 Setting the Screen Layout of the Waveform

(If you want to save data)
Set on the Save Settings screen.

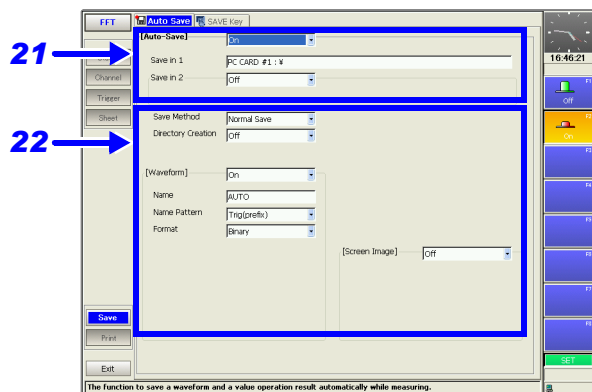

(Example: Auto Save)

See "Chapter 10 Saving/Loading Data & Managing Files" in the *Instruction Manual*

Printing Settings

Press the **SUB MENU** keys to select the

Print menu

Press the **SHEET/PAGE** keys to select the **[Printer]** page

23 Select automatic or manual printing

Verify that the paper is loaded correctly. When printing manually, settings can be made after measurement.

Default setting:
Auto Print **[Off]**
Manual Print **[Selection Print]**

Press the **SHEET/PAGE** keys to select the **[Print Items]** page

24 Select what you want to print

Start of Measurement

Data acquisition
Save & Print (when Auto enabled)

End of Measurement


Data Analysis

Optionally Save and Print

Power OFF

(If you want to print data)

Set on the Print Settings screen.

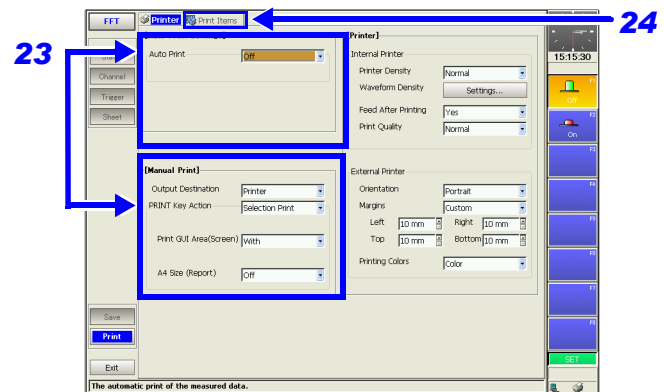

See "Chapter 11 Printing" in the *Instruction Manual*

Press the **START** key. (the green LED lights)



Press the **STOP** key.

Recording stops after acquiring the specified length (the green LED goes off).



Press twice to stop immediately.

If **[Single]** trigger is selected, recording stops automatically after acquiring the specified data length.


Analysis on the waveform screen.

See "3.9 Analysis with the Waveform Screen" (⇒ p. 78)

Press the **SAVE** key to save. (Manual saving)


Press the **PRINT** key to print. (Manual printing)

Remove the cables from the measurement object, and turn the power off.

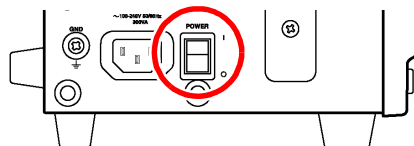

3.4 Setting FFT Analysis Conditions

Basic measurement configuration settings are performed on the Status Settings screen. Measurement configuration can be performed from the Waveform screen ($\Rightarrow$ p. 67).

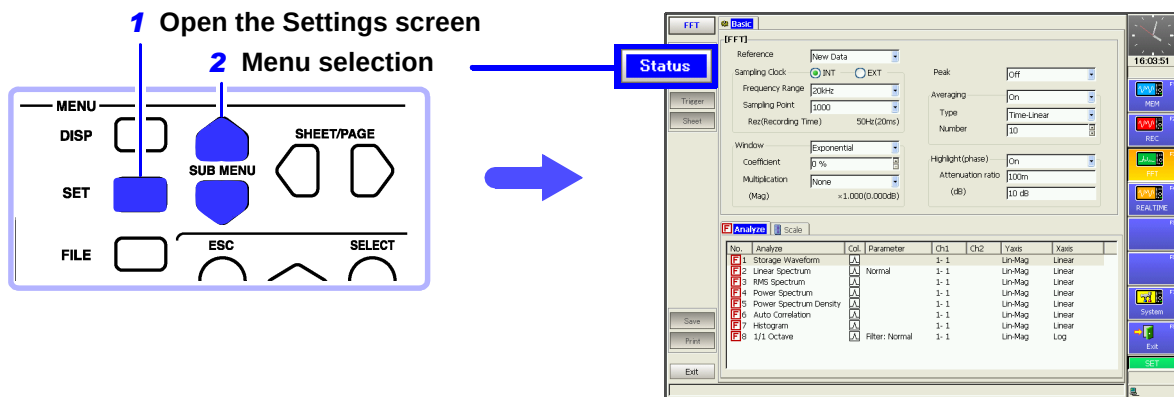

3.4.1 Selecting the FFT Function


The FFT function can be selected from the Opening, Waveform or Settings screen.

Function Selection: From the Opening Screen

Operating Key Procedure

- 1** **CURSOR** Move to the desired function.
- 2** **F1 to F8** Select the appropriate function.

Opening Screen

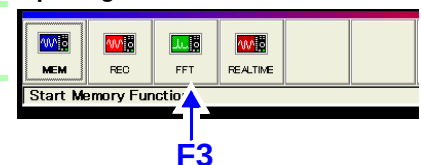


Function Selection: From the Waveform or Settings Screen


Operating Key Procedure

- 1** **CURSOR** Move to the function menu (at the top left).
- 2** **F3** Select the FFT function.

Waveform Screen

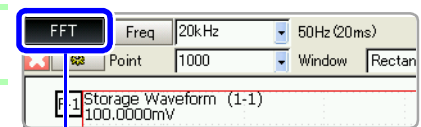

Function Menus

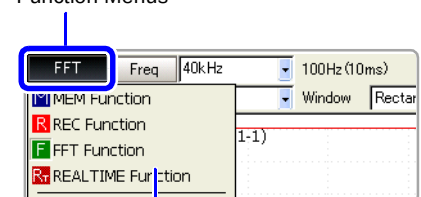

Pull-Down Menu

(Select from the pull-down menu)

- SELECT** The pull-down menu appears.
- CURSOR** Select the appropriate function.
- ENTER** Accepts the setting.

3.4.2 Selecting the Data Source for Analysis


Select the data to be used for FFT analysis.
Analysis can be applied either to new data as it is measured, or to existing data (previously recorded to memory).

Selecting Input Data

FFT

To open the screen: Press the **SET** key → Select **Status** with the **SUB MENU** keys → Status Settings screen
See Screen Layout (⇒ p. 40), To set from the Waveform screen (⇒ p. 67)

Operating Key	Procedure
1	Select the input data source.
CURSOR	Move the cursor to the [Reference] item.
F1 to F8	Selects the data to be analyzed.
New Data	Acquire a new waveform for analysis.
From Mem	Analyze a waveform recorded in memory.

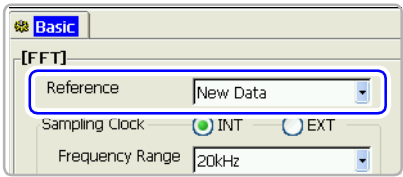

- 2** When finished making settings, press the **START** key
- For the [New Data] case**
Measurement starts to acquire data for the number of analysis points specified as the [Sampling Point], and FFT analysis is performed.
- For the [From Mem] case**
Analysis is performed on the number of specified points from data previously recorded in memory (Memory function data).
The analysis starting point can also be specified.
See "3.9.3 Analyzing after Specifying an Analysis Starting Point" (⇒ p. 80)

The frequency range is selected automatically.
See "Relationship Between Frequency Range, Resolution and Number of Analysis Points" (⇒ p. 55)

When the trigger mode is [Repeat] or [Auto], and the input data [Reference] is [From Mem]

Analysis is performed until the specified number of FFT analysis points have been processed, then the data is shifted by that amount and analysis repeats until all of the previously acquired data has been processed. (If the amount of data is less than the specified number of FFT analysis points, no analysis occurs.)
See "Trigger Modes and Averaging" (⇒ p. 60)

When no trace is displayed after pressing the START key

Analysis is impossible if [From Mem] is selected as the input data source and no recorded data exists in the instrument's memory.
Either select [New Data] as the input data source, or load the data to be analyzed before pressing the START key again.

3.4.3 Setting the Frequency Range and Number of Analysis Points

About the frequency range and number of analysis points

The settings for the frequency range and number of analysis points determine the input signal acquisition time and frequency resolution.

The frequency range setting for the FFT function corresponds to the timebase (time/division) setting of the Memory function. Changing the frequency range also changes the data sampling period.

See "Relationship Between Frequency Range, Resolution and Number of Analysis Points" (⇒ p. 55)

The cut-off frequency of the anti-aliasing filter is the same as the frequency range setting.

The set number of analysis points specifies the amount of data to be analyzed with each measurement. Increasing the number of analysis points increases the frequency resolution, but also increases the time required for calculations.

See "Number of Analysis Points" (⇒ p. 105)

When using the external sampling to calculate:

Set the Sampling Clock to [EXT] (External sampling).

In this case, octave analysis, power spectrum density and LPC power spectrum density are not available.

The following two methods are available for setting the frequency range:



- Using the operating keys
- Using the **TIME/DIV** key (settable regardless of cursor position)

Frequency Range Setting: Using the TIME/DIV Key

FFT

To open the screen: Press the **SET** key → Select **Status** with the **SUB MENU** keys → Status Settings screen

See Screen Layout (⇒ p. 40), To set from the Waveform screen (⇒ p. 67)

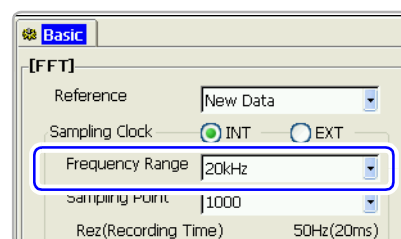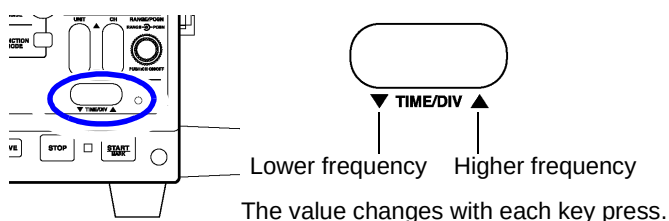


Frequency Range and No. of Analysis Points Settings:
Using the Operating Keys

FFT

To open the screen: Press the **SET** key → Select **Status** with the **SUB MENU** keys → Status Settings screen
See Screen Layout (⇒ p. 40), To set from the Waveform screen (⇒ p. 67)

Operating Key	Procedure
1	Select the sampling clock.
CURSOR	Move the cursor to the [Sampling Clock] item.
F1	Select [INT] (Internal). (default setting)
2	Select the frequency range.
CURSOR	Move the cursor to the [Frequency Range] item.
F1 to F8 (Switch Display: F8)	Select the frequency range. 8 (default setting), 4, 2 MHz 800, 400, 200, 80, 40, 20, 8, 4, 2 kHz 800, 400, 200, 80, 40, 20, 8, 4, 1.33 Hz 800, 667, 400, 333, 133 mHz
3	Set the number of FFT analysis points.
CURSOR	Move the cursor to [Sampling Point]
F1 to F8 (Switch Display: F8)	Select the number of points for analysis. 1000(default setting), 2000, 5000, 10000
	See "Number of Analysis Points" (⇒ p. 105)

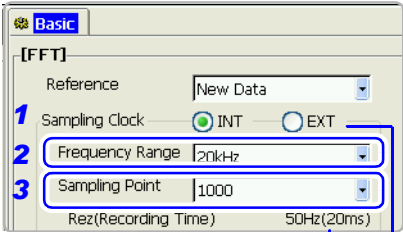

Frequency Resolution (during acquisition)
The resolution is affected by settings of frequency range and the number of analysis points. Not displayed for external sampling.

Normally, select [INT].

To control sampling by an external signal, select [EXT]
In this case, set only the number of analysis points.

When [From Mem] is selected as the input data source
The frequency range is set automatically when analysis is started.

Relationship Between Frequency Range, Resolution and Number of Analysis Points

Range [Hz]	Sampling frequency [Hz]	Timebase [div] (MEM)	Sampling period	Number of FFT Analysis Points							
				1,000		2,000		5,000		10,000	
				Resolution [Hz]	Acquisition interval	Resolution [Hz]	Acquisition interval	Resolution [Hz]	Acquisition interval	Resolution [Hz]	Acquisition interval
8 M * ¹	20 M	5 μ s	50 ns	20 k	50 μ s	10 k	100 μ s	4 k	250 μ s	2 k	500 μ s
4 M * ¹	10 M	10 μ s	100 ns	10 k	100 μ s	5 k	200 μ s	2 k	500 μ s	1 k	1 ms
2 M * ¹	5 M	20 μ s	200 ns	5 k	200 μ s	2.5 k	400 μ s	1 k	1 ms	500	2 ms
800 k * ¹	2 M	50 μ s	500 ns	2 k	500 μ s	1 k	1 ms	400	2.5 ms	200	5 ms
400 k * ¹	1 M	100 μ s	1 μ s	1 k	1 ms	500	2 ms	200	5 ms	100	10 ms
200 k * ¹	500 k	200 μ s	2 μ s	500	2 ms	250	4 ms	100	10 ms	50	20 ms
80 k * ¹	200 k	500 μ s	5 μ s	200	5 ms	100	10 ms	40	25 ms	20	50 ms
40 k	100 k	1 ms	10 μ s	100	10 ms	50	20 ms	20	50 ms	10	100 ms
20 k	50 k	2 ms	20 μ s	50	20 ms	25	50 ms	10	100 ms	5	200 ms
8 k	20 k	5 ms	50 μ s	20	50 ms	10	100 ms	4	250 ms	2	500 ms
4 k	10 k	10 ms	100 μ s	10	100 ms	5	200 ms	2	500 ms	1	1 s
2 k	5 k	20 ms	200 μ s	5	200 ms	2.5	400 ms	1	250 ms	500 m	2 s
800	2 k	50 ms	500 μ s	2	500 ms	1	1 s	400 m	2.5 s	200 m	5 s
400	1 k	100 ms	1 ms	1	1 s	500 m	2 s	200 m	5 s	100 m	10 s
200	500	200 ms	2 ms	500 m	2 s	250 m	4 s	100 m	10 s	50 m	20 s
80	200	500 ms	5 ms	200 m	5 s	100 m	10 s	40 m	25 s	20 m	50 s
40	100	1 s	10 ms	100 m	10 s	50 m	20 s	20 m	50 s	10 m	100 s
20	50	2 s	20 ms	50 m	20 s	25 m	40 s	10 m	100 s	5 m	200 s
8 * ²	20	5 s	50 ms	20 m	50 s	10 m	100 s	4 m	250 s	2 m	500 s
4 * ²	10	10 s	100 ms	10 m	100 s	5 m	200 s	2 m	500 s	1 m	1 ks
1.33 * ²	3.33	30 s	300 ms	3.33 m	300 s	1.66 m	600 s	666 μ	1.5 ks	333 μ	3 ks
800 m * ²	2	50 s	500 ms	2 m	500 s	1 m	1 ks	400 μ	2.5 ks	200 μ	5 ks
667 m * ²	1.67	60 s	600 ms	1.66 m	600 s	833 μ	1.2 ks	333 μ	3 ks	166 μ	6 ks
400 m * ²	1	100 s	1 s	1 m	1 ks	500 μ	2 ks	200 μ	5 ks	100 μ	10 ks
333 m * ²	833 m	120 s	1.2 s	833 μ	1.2 ks	416 μ	2.4 ks	166 μ	6 ks	83.3 μ	12 ks
133 m * ²	333 m	300 s	3 s	333 μ	3 ks	166 μ	6 ks	66.6 μ	15 ks	33.3 μ	30 ks


The cut-off frequency of the anti-aliasing filter is the same as the frequency range.

*1. The anti-aliasing filter is turned off.


*2. Cut-off frequency is 20 Hz.

3.4.4 Setting the Window Function


The window function defines the segment of the input signal to be analyzed. Use the window function to minimize leakage errors. There are three general types of window functions:



• Rectangular window



- Hann window
- Hamming window
- Blackman window
- Blackman-Harris window
- Flat top window



• Exponential window

The non-rectangular window functions generally produce lower-level analysis results. By applying attenuation correction, the attenuation introduced by the non-rectangular window functions can be corrected to bring analysis results back to similar levels.


Selecting the Window Function and Correction

FFT


To open the screen: Press the **SET** key → Select **Status** with the **SUB MENU** keys → Status Settings screen

See Screen Layout (⇒ p. 40), To set from the Waveform screen (⇒ p. 67)

Operating Key	Procedure
1	Select the window function.
CURSOR	Move the cursor to the [Window] item.
F1 to F8	Select the appropriate window function type.
	Rectangular (default setting), Hanning, Exponential, Hamming, Blackman, BlackmanHarris, Flat-Top
	See "Window Function" (⇒ p. 110)

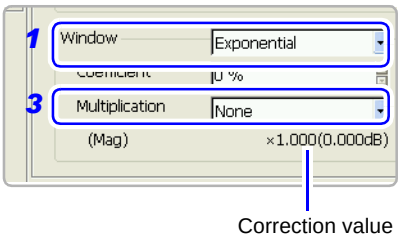


2	If [Exponential] is the selected type
	Set the attenuation coefficient (percentage).
CURSOR	Move the cursor to the [Coefficient] item.
F1 to F8	Set the attenuation coefficient as a percentage. Setting the attenuation coefficient to 0% results in the same processing as a setting of 0.1%.

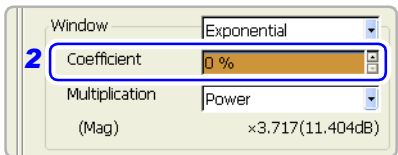

For the exponential window function Noise is suppressed in the attenuated waveform.

3	Set attenuation correction.
CURSOR	Move the cursor to the [Multiplication] item.
F1 to F8	Select the correction method.
None	Attenuated window function values are not corrected. (default setting)
Power	The window function multiplies the power levels of the time-domain waveform so that output levels are comparable to those of a rectangular window.
Average	The window function multiplies the average value of the time-domain waveform so that output levels are comparable to those of a rectangular window.

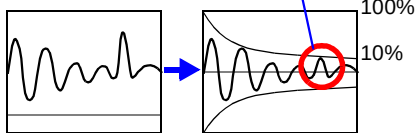

When the attenuation rate is 10%

For the rectangular window function:
The correction value is always 1 (0 dB).
For the exponential window function:
The correction value depends on the attenuation coefficient.

Power correction
$$\sqrt{\frac{2 \ln (x / 100)}{(x / 100)^2 - 1}}$$

Average correction
$$\frac{\ln (x / 100)}{(x / 100) - 1}$$

x: Attenuation coefficient (%)

3.4.5 Setting Peak Values of Analysis Results

Either local or global maxima ([maximal]/ [maximum]) of the input signal and analysis results can be displayed on the Waveform screen. However, if Nyquist display is selected on the Sheet Settings screen, no peak values are displayed.

Selecting Displayed Values

FFT

To open the screen: Press the **SET** key → Select **Status** with the **SUB MENU** keys → Status Settings screen
See Screen Layout (⇒ p. 40)

Operating Key Procedure

Selecting peak value display.



CURSOR

Move the cursor to the **[Peak]** item.

F1 to F8

Select the type of numerical value to be displayed.


Off	Not displayed.(default setting)
Maximal	(local maxima) When the value of data at a point is greater than that of the adjacent points, that data is considered a local maxima. The ten largest local maxima are displayed.
Maximum	(global maxima) Among all data values, the ten points with the greatest values are displayed.

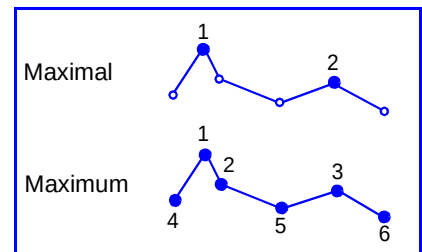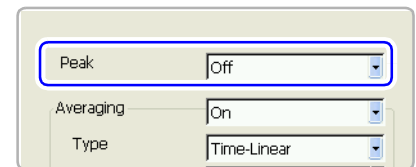

NOTE

- Peak values on the Waveform screen can be displayed and printed, but cannot be saved as peak values in text files.
- Depending on split-screen settings, there may be insufficient space to display all ten maxima. In this case, only the number of maxima that can be displayed are shown, from the largest.

Example: 4-Section Split-Screen

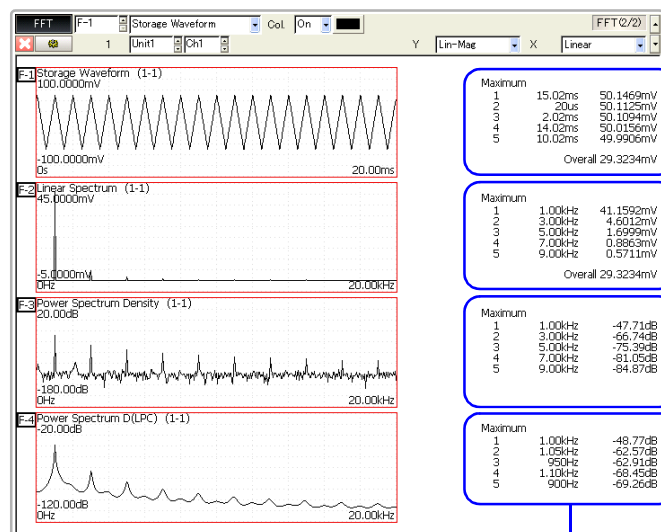

Peak value display
From 1 to 5

3.4.6 Averaging Waveforms

The averaging function calculates the average of the values obtained from multiple measurements of a periodic waveform. This can reduce noise and other non-periodic signal components. Averaging can be applied to a time-domain waveform or to a spectrum.


Averaging Settings

FFT

To open the screen: Press the **SET** key → Select **Status** with the **SUB MENU** keys → Status Settings screen

See Screen Layout (⇒ p. 40)

Operating Key	Procedure
1	Enable averaging.
CURSOR	Move the cursor to the [Averaging] item.
F1 to F8	Select whether to enable or disable averaging.
Off	Averaging is disabled (default setting)
On	Averaging is enabled.

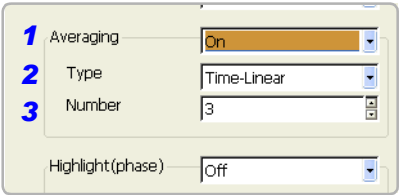

2	Select the type of averaging.
CURSOR	Move the cursor to the [Type] item.
F1 to F8	Select from the following types:
Time-Linear	Perform simple (linear) averaging of time-domain waveform values.
Time-Exponential	Perform exponential averaging of time-domain waveform values.
Freq-Linear	Perform simple (linear) linear averaging of (frequency-domain) spectrum values.
Freq-Exponential	Perform exponential averaging of (frequency-domain) spectrum values.
Freq-Peak Hold	Retain the maximum value of (frequency-domain) spectrum values.

About averaging calculation formulas
See "Averaging" (⇒ p. 109)

When averaging and auto saving or auto printing are enabled at the same time
Data is saved or printed after the specified count of values have been averaged. After calculating the average, changing the analysis channel does not cause re-calculation.

3	Select the count for averaging.
CURSOR	Move the cursor to the [Number] item.
F1 to F8	Select the number of measurements to be averaged. Setting range: 2 to 10,000

- NOTE**

- After measuring with averaging enabled, display is not available when the channel is changed. Also, when the analysis mode is changed, the analysis modes that can be displayed are limited.
 - When averaging is performed with the analysis mode disabled (Off), no trace is displayed when the analysis mode is changed after measurement.

Description See "Trigger Modes and Averaging" (⇒ p. 60)

When averaging time-domain waveform values

Waveforms are acquired and averaged within the time domain. After averaging, FFT calculation is performed.

When the trigger mode is [Auto]: Data is acquired when the START key is pressed, even if trigger criteria are not met after a certain interval. So if averaging is applied to an asynchronous signal, the resulting data is meaningless.

Synchronous signals have better SNR (signal-to-noise ratio) and are more suitable for analysis.

When averaging spectrum values

Acquired data is first subject to FFT analysis. After analysis, averaging is performed within the frequency range, and the result is displayed. This differs from time-domain averaging in that averaging can be performed without trigger synchronization. However, if the characteristics of the input waveform allow triggering, using the trigger for synchronization is recommended.

Spectrum peak hold

After performing FFT calculations on the acquired waveform, peak values are retained (held) and displayed within the frequency range.

FFT Analysis Modes and Averaging

●: Settable, ×: Unsettable, ○: Partially settable

Analysis Mode	Averaging				
	Waveform Averaging		Spectrum Averaging		
	Simple	Exponential	Simple	Exponential	Peak Hold
OFF	×	×	×	×	×
Storage Waveform	●	●	×	×	×
Linear Spectrum	●	●	○ *2	○ *2	○ *2
RMS Spectrum	●	●	○ *2	○ *2	○ *2
Power Spectrum	●	●	●	●	●
Power Spectrum Density *1	●	●	●	●	●
Auto-correlation Function	●	●	●	●	●
Histogram	●	●	×	×	×
1/1 Octave Analysis *1	●	●	●	●	●
1/3 Octave Analysis *1	●	●	●	●	●
Transfer Function	●	●	○ *2	○ *2	○ *2
Cross Power Spectrum	●	●	○ *2	○ *2	○ *2
Cross-correlation Function	●	●	●	●	●
Impulse Response	●	●	●	●	●
Coherence Function	×	×	●	●	×
Phase Spectrum	●	●	×	×	×
Power Spectrum Density (LPC) *1	●	●	×	×	×


*1. Not available for external sampling

*2. Not available when the y axis is real (linear) or imaginary (linear), or for Nyquist plots

Trigger Modes and Averaging

When the trigger mode is [Single]

Measurements continue until the specified number of averaging points is acquired.

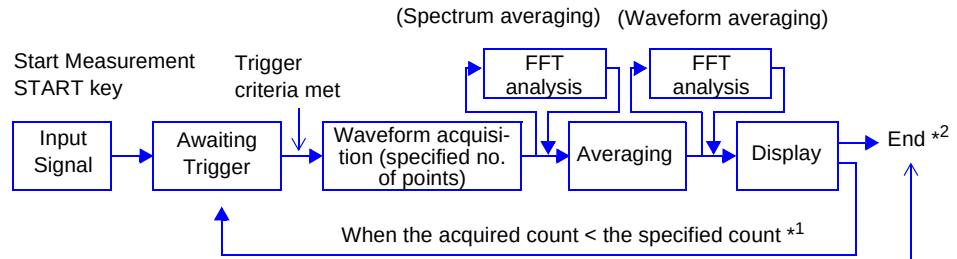


*1. Awaiting trigger continues until the specified count is reached.

*2. Measurement stops automatically when the specified count is reached. If measurement was interrupted by the STOP key, the averaging result up to that point is displayed.

When the acquired count = the specified count

When the trigger mode is [Repeat]


Measurement continues after the specified averaging count has been acquired. When the specified averaging count is exceeded, averaging is repeated and measurement continues until the STOP key is pressed.

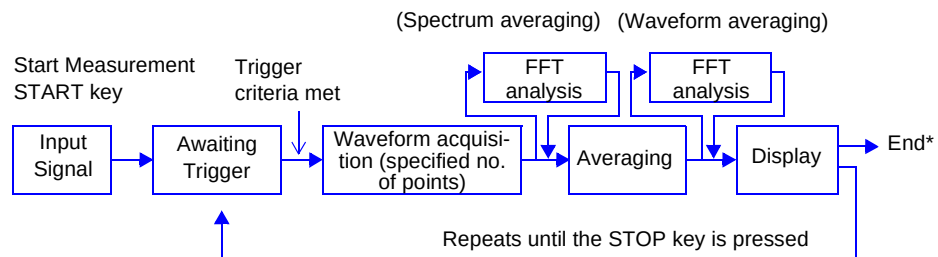

* When stopped before the specified count, the average up to that point is displayed.

When the trigger mode is [Auto]

- For time-domain waveforms:
Data is acquired when the START key is pressed, even if trigger criteria are not met after a certain interval. So if averaging is applied to an asynchronous signal, the resulting data is meaningless.
- For spectrum values:
When the START key is pressed, measurement starts. Even if the trigger criteria are not met, the specified amount of data is acquired, and after FFT analysis, the results are averaged.
When the specified averaging count is exceeded, averaging is repeated and measurement continues until the STOP key is pressed.

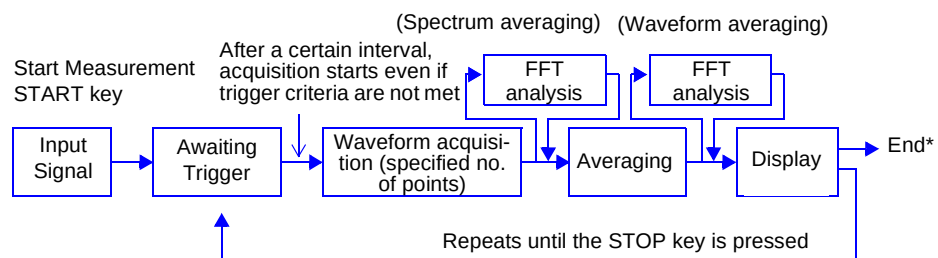


* When stopped before the specified count, the average up to that point is displayed.

3.4.7 Emphasizing Analysis Results (phase spectra only)

By specifying a setting factor (rate) to be applied to the input signal, the display of data exceeding the resulting threshold can be emphasized. This feature is useful for viewing waveforms that may otherwise be obscured by noise.

The reliability of phase spectrum values is poor when discrete Fourier transform values are extremely small. For example, in the case of a pure sine wave, almost all phase values at frequencies other than the input frequency result from calculation errors. By treating the maximum value of the power (or cross-power) spectrum of the input signal, $P_{\max}$, as a reference value, data that exceeds that value multiplied by rate R can be displayed with emphasis.

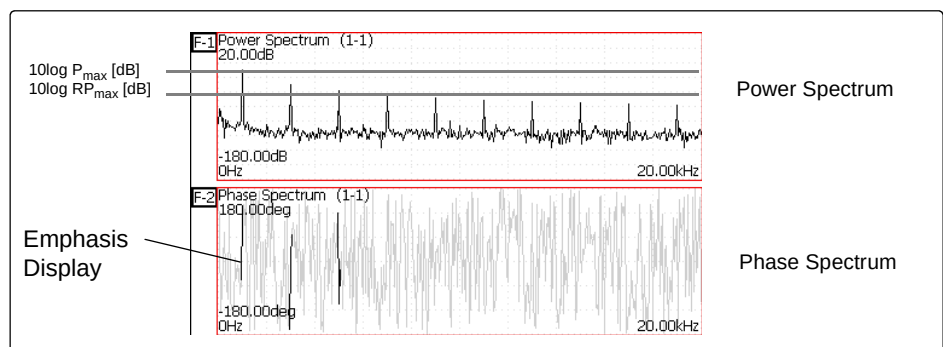

Setting Phase Spectrum Highlighting

FFT

To open the screen: Press the **SET** key → Select **Status** with the **SUB MENU** keys → Status Settings screen
See Screen Layout (⇒ p. 40)

Operating Key Procedure

1 Enable the highlighting function.

- CURSOR** Move the cursor to the **[Highlight (phase)]** item.
- F1 to F8** Select whether to enable or disable the highlighting function.
- | | |
|------------|---|
| Off | Emphasis display disabled.(default setting) |
| On | Emphasis display enabled. |

1 Highlight(phase) On
2 Attenuation ratio 1
3 (dB) 0 dB

2 Set the attenuation rate or attenuation value.

To set an attenuation rate

- CURSOR** Move the cursor to the **[Attenuation ratio]** item.
- F1 to F8** Enter the attenuation rate.

To set an attenuation value [dB]

- CURSOR** Move the cursor to the **[(dB)]** item.
- F1 to F8** Enter the attenuation value.

Attenuation Rate and Value

Attenuation value: A [dB]
Attenuation rate: R

$$-A = 10\log_{10}R$$

$$1 \times 10^{-6} \leq R \leq 1$$

$$0 \leq A \leq 60$$

3.4.8 Analysis Mode Settings

Select the type of FFT analysis, channel(s), waveform display color and x and y axes.

Analysis Content Settings

FFT

To open the screen: Press the **SET** key → Select **Status** with the **SUB MENU** keys → Status Settings screen
See Screen Layout (⇒ p. 40), To set from the Waveform screen (⇒ p. 67)

Operating Key	Procedure
---------------	-----------

- 1
- Open the [Analyze] page.
- SHEET/PAGE Select the [Analyze] page.

1

Analysis Setting Contents

Analysis No. Settings can be made from the dialogs, or copied from another Analysis No. (⇒ p. 65)

No.	Analyze	Col.	Parameter	Ch1	Ch2	Yaxis	Xaxis
1	Storage Waveform			1- 1		Lin-Mag	Linear
2	Linear Spectrum		Normal	1- 1		Lin-Mag	Linear

2 Analysis Type

3 Display Color

4

5 Channel for Analysis

6 X/Y Axes Display


- 2
- Select the FFT analysis mode.
- CURSOR Move the cursor to the [Analyze] column of the Analysis No. to set.
- F1 to F8 (Switch Display: F8) Select the analysis mode.

OFF	No analysis. (default setting)	1/1 Octave*	Example (⇒ p. 91)
Storage Waveform	Example (⇒ p. 85)	1/3 Octave*	Example (⇒ p. 91)
Linear Spectrum	Example (⇒ p. 86)	Phase Spectrum	Example (⇒ p. 95)
RMS Spectrum	Example (⇒ p. 87)	Transfer Function	Example (⇒ p. 96)
Power Spectrum	Example (⇒ p. 88)	Cross Power Spectrum	Example (⇒ p. 97)
Pow.Spectrum Density*	(Power spectrum density) Example (⇒ p. 89)	Cross Correlation	Example (⇒ p. 98)
Auto Correlation	Example (⇒ p. 90)	Impulse Response	Example (⇒ p. 99)
Histogram	Example (⇒ p. 90)	Coherence	Example (⇒ p. 100)
		Pow.Spectrum Density (LPC)*	(Power spectrum density LPC) Example (⇒ p. 101)

* Not available with external sampling enabled.

See "3.10.2 Analysis Mode Functions" (⇒ p. 102)

- 3
- Select whether to display the waveform, and its color.
- CURSOR Move the cursor to the [Col.] column.
- F1 to F8 Select whether the waveform is to be displayed (On) or not, and its color if displayed.

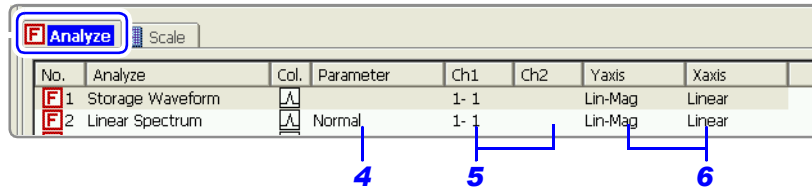

Operating Key Procedure

4 When [Parameter] setting contents are displayed

Set the parameter.

CURSOR Move the cursor to the [Parameter] column of the Analysis No. to set.

F1 to F8 Select the desired type of analysis or display.

Analyze mode	Parameter	Setting Contents
Linear Spectrum, Transfer Function, Cross Power Spectrum	Normal	Analysis results are displayed as amplitude vs. frequency.
	Nyquist	Analysis results are displayed as imaginary vs. real components.
1/1 Octave, 1/3 Octave	Filter: Normal	Enables the octave filter.
	Filter: Sharp	See "Octave Filter Setting" (⇒ p. 64)
Phase Spectrum	1ch FFT	Calculates the phase of [Channel 1].
	2ch FFT	Calculates the phase difference between [Channel 1] and [Channel 2].
Pow.Spectrum Density (LPC)	Order:2 to 64	Larger numerical values make finer spectrum components visible.

5 Select the channel for analysis.

CURSOR Move the cursor to the [Ch1] item.

F1 to F8 Select which channel number to use.

6 Set the x and y axes for display of analysis results.

CURSOR Move the cursor to the [X axis] or [Y axis] item.

F1 to F8 Select the analysis result components to display on the x and y axes.
(Selectable display components depend on the analysis mode)
See "Analysis Modes and X/Y Axis Display" (⇒ p. 64)

Y-axis display

Lin-Mag	Analysis results are displayed as amplitude values.
Log-Mag	Analysis results are displayed as dB values.
Lin-Real	The real-number component of analysis results are displayed.
Lin-Imag	The imaginary component of analysis results are displayed.

X-axis display

Linear	Frequency is displayed linearly.
Log	Frequency is displayed logarithmically. This is convenient when the data of interest is at the lower end of the frequency range, such as for sound and vibration.

Analysis channel setting

For any of the following analysis modes, set both channels 1 and 2.

Transfer Function, Impulse Response, Cross-correlation Function, Cross Power Spectrum, Coherence Function, Phase Spectrum (2ch FFT)

To analyze without the influence of aliasing distortion

The following input modules are recommended for channels to be subject to FFT analysis:

- Model 8938 FFT Analog Unit
- Model 8947 Chargin Unit
- Model 8957 High Resolution Unit
- Model 8960 Strain Unit

To analyze using external sampling


The x axis displays the number of data points.

For Nyquist display

When the [Nyquist Display] parameter settings is selected, x- and y-axis display settings are not available.


Octave Filter Setting

Filter characteristics comply with tolerance standards for IEC61260 filters.



Normal

Filter characteristics approximate those of an analog filter.



Sharp

Only those spectral component within the octave band are used for analysis. Spectral components outside of the octave band are totally ignored.

After determining the entire power spectrum, the instrument performs octave analysis on the spectral bands defined by the above filter characteristics. Analog filtering is not used for analysis.

See "Octave Filter Characteristics" (⇒ p. 114)

Analysis Modes and X/Y Axis Display

O: Selectable, x: Unselectable

Analysis Mode	X axis		Y axis				Nyquist display
	Linear	Log	Lin-Mag	Log-Mag	Lin-Real	Lin-Imag	
OFF	x	x	x	x	x	x	x
Storage Waveform	O	x	O	x	x	x	x
Linear Spectrum	O	O	O	O	O	O	O
RMS Spectrum	O	O	O	O	O	O	x
Power Spectrum	O	O	O	O	x	x	x
Power Spectrum Density	O	O	O	O	x	x	x
Auto-correlation Function	O	x	O	x	x	x	x
Histogram	O	x	O	x	x	x	x
1/1 Octave	O	O	O	O	x	x	x
1/3 Octave	O	O	O	O	x	x	x
Transfer Function	O	O	O	O	O	O	O
Cross Power Spectrum	O	O	O	O	O	O	O
Cross-correlation Function	O	x	O	x	x	x	x
Impulse Response	O	x	O	x	x	x	x
Coherence Function	O	O	O	x	x	x	x
Phase Spectrum	O	O	O	x	x	x	x
Power Spectrum Density (LPC)	O	O	O	O	x	x	x

The x/y axes cannot be set when Nyquist Display is selected.

To Set from a Dialog

No.	Analyze	Col.	Parameter	Ch1	Ch2	Yaxis	Xaxis
F1	Storage Waveform	⌘		1- 1		Lin-Mag	Linear
F2	Linear Spectrum	⌘	Normal	1- 1		Lin-Mag	Linear
F3	MS Spectrum	⌘		1- 1		Lin-Mag	Linear



Move the cursor to the [No.] column of the Analysis to set, and press F1 [All Settings].

A dialog box appears. Items that cannot be set for the particular analysis mode are grayed out.

Move the cursor to each item, and select with the F1 to F8 keys.

FFT Analyze Settings - No:1

Analyze: コスト
Power Spectrum

Ch Mode: Ch1 Ch2 Y X

1ch FFT: Unit1 Ch1 Unit1 Ch1 Log-Mag Linear

Color: On

Octave: Normal Nyquist: Normal Order: 2

[Scale]: Lower Upper Units
Auto 0 0 dB

Close


These are the same as the setting contents on the [Analyze] page.

These are the same as the setting contents on the [Scale] page.

Parameter Settings

To copy settings between Calculation Nos.

No.	Analyze	Col.	Parameter	Ch1	Ch2	Yaxis	Xaxis
F1	Storage Waveform	⌘		1- 1		Lin-Mag	Linear
F2	Linear Spectrum	⌘	Normal	1- 1		Lin-Mag	Linear
F3	MS Spectrum	⌘		1- 1		Lin-Mag	Linear



Move the cursor to the [No.] column of the Analysis to copy, and press F2 [Copy].

A dialog box appears.

Make settings in the dialog with the F keys or dialog buttons.

Copy Settings

Copy Source: No.1

Copy Contents:

- ☒ Analyze
- ☒ Channel
- ☐ Col.
- ☒ Scale
- ☐ Comment

Copy Destination:

- ☒ No.1
- ☐ No.2
- ☐ No.3
- ☐ No.4
- ☐ No.5
- ☐ No.6
- ☐ No.7
- ☐ No.8

Select All Deselect All Reverse

Copy Cancel

Select the Analysis No. of the copy source.

Select the contents to copy.

Select the Analysis No. of the copy destination.

Make the desired settings, and click Copy (or F7 [Copy]).

3.4.9 Setting the Display Range of the Vertical Axis (Scaling)

The display range of the vertical (y) axis can be set to automatically suit analysis results, and can be freely expanded and compressed.

Vertical Axis (Scaling) Setting

FFT

To open the screen: Press the **SET** key → Select **Status** with the **SUB MENU** keys → Status Settings screen

See Screen Layout (⇒ p. 40)

Operating Key	Procedure
---------------	-----------

- 1
- Open the [Scale] page.
- SHEET/PAGE Select the [Scale] page.

Analysis Setting Contents

Calculation No. Settings can be made from the dialogs, or copied from another Analysis No. (⇒ p. 65)

- 2
- Select automatic or manual scaling of the y-axis display.

CURSOR Move the cursor to the [Scale] column of the Analysis No. to set.

F1 to F8 Select the scaling display type.

Auto	Scaling of the vertical (y) axis is automatically set according to analysis results. (default setting)
Manu (manual)	Scaling of the vertical (y) axis can be set as desired, to suit the purpose of the measurement. This is useful for magnifying or reducing the displayed amplitude, and for shifting the displayed waveform up or down.

About displayed units (y axis)
The selected units for the scaled channel are displayed. When scaling is disabled [Off], the measurement range units are displayed.
To convert to other units, set the scaling units on the Channel Settings screen.
See "5.4 Converting Input Values (Scaling Function)" in the *Instruction Manual*

Input values can be converted to dB.
See "Scaling" (⇒ p. 71)

- 3
- When [Manu] is selected

Set the upper and lower limits to display.

CURSOR Move the cursor to the [Lower] or [Upper] item.

F1 to F8 Set the upper and lower limits to display the analysis results.
Setting range: -9.9999E+29 to +9.9999E+29 (with exponent from E-29 to E+29)

To display comments on the Waveform screen

Enable the [Comment] setting on the System Settings screen.

When comments are entered on both the Channel Settings screen and the [Analyze] page, both comments are displayed. When no channel comment has been entered, unit (module) and channel number are displayed.

- 4
- To enter a comment for an analysis result

CURSOR Move the cursor to the [Comment] item.

F1 Enter your comment.
The entry method is the same as for channel comments.
See "5.2.2 Adding Channel Comments"; "Comment Entry Example" in the *Instruction Manual*

3.4.10 Setting and Changing Analysis Conditions on the Waveform Screen

The following settings can be made on the Waveform screen.

Press the **SUB MENU** keys to switch the displayed measurement items.

Changes to the displayed analysis results become effective when the settings are changed.

- **[FFT(1/2)]**
Available settings are frequency range, number of analysis points, type of window function, trigger mode and pre-triggering
- **[FFT(2/2)]**
Available settings are analysis number, analysis mode, waveform color, analysis channel and x/y axis display type
- **[Trigger]**
Available settings are trigger number and analog trigger settings

To change the analysis number to be displayed on the current Sheet, press the F5 [Channel Set] key in the FN mode, and make settings in the dialog (⇒ p. 68).

Changes can be made to frequency range, number of analysis points, type of window function, trigger mode and pre-triggering

2 Use the CURSOR keys to move the cursor to each setting item, and select your choice with the F keys.

1 Press the SUB MENU key to display [FFT(1/2)].



The screenshot shows the FFT settings interface. At the top left is the 'FFT' label. Below it are icons for 'Freq' (frequency), 'Point' (analysis points), and 'Window' (window function). The 'Freq' section shows '20kHz' and '50Hz (20ms)'. The 'Point' section shows '1000'. The 'Window' section shows 'Rectangular'. To the right of these are 'Mag' (magnitude) set to '× 1' and 'Auto' (auto-trigger) set to '0 %'. On the far right, a button labeled 'FFT(1/2)' is highlighted with a red box. Blue lines connect text labels to specific controls: 'Frequency Range' points to the '20kHz' field; 'Frequency Resolution' points to the '50Hz (20ms)' field; 'FFT Window Function Type' points to the 'Rectangular' dropdown; 'Number of Analysis Points' points to the '1000' field; and 'Trigger mode and Pre-trigger' points to the 'Auto' and '0 %' fields.

Frequency Range (⇒ p. 53)
Select whether to sample from an internal (input module) or external (External Control terminal) source.
Select the frequency range (133 mHz to 8 MHz).

Frequency Resolution (during acquisition)

FFT Window Function Type (⇒ p. 56)

Number of Analysis Points (⇒ p. 53)
(1000, 2000, 5000, 10000)

Trigger mode and Pre-trigger
Select the trigger mode and pre-triggering (same as for the Memory function).
Trigger Mode: Single, Repeat, Auto
Pre-trigger: -100 to 100% (1% or 1div step)
See "6.3 Setting the Trigger Mode" and "6.5 Pre-Trigger Settings" in the *Instruction Manual*

3.4 Setting FFT Analysis Conditions

Changing analysis number, analysis mode, waveform color, analysis channel and x/y axis display type

1 Press the SUB MENU key to display [FFT(2/2)].

2 Use the CURSOR keys to move the cursor to each setting item, and select your choice with the F keys.

Analysis Number (⇒ p. 62)
This is linked to the setting on the [Analyze] page of the Status Settings screen.

Analysis Mode

Waveform Display On/Off

Waveform Color

Analysis Channel

X and Y Axis Display Type



Changing Analog Trigger Settings

See "6.12 Making Trigger Settings on the Waveform Screen" in the Instruction Manual

1 Press the SUB MENU key to display [Trigger].

2 Use the CURSOR keys to move the cursor to each setting item, and select your choice with the F keys.

(When using Level Triggering)

Type of Analog Trigger

Trigger No.

Trigger Level

The display differs according to the type of analog triggering.

Unit and Channel No. for this trigger

Slope

Filter



Changing the Analysis No. for Display


This setting is the same as that on the Display page of the Sheet Settings screen.

See "3.6 Setting the Screen Layout of the Waveform Screen" (⇒ p. 72)

3 Select [FFT].

5 Select the graph(s) for display.

4 Select the Analysis Nos. for display

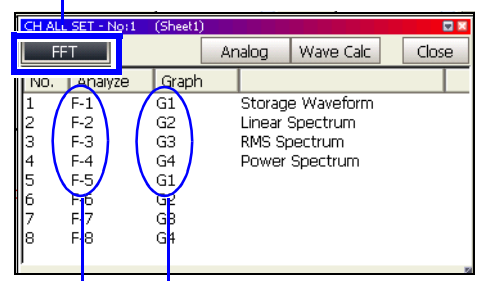

No.	Analyze	Graph
1	F-1	G1
2	F-2	G2
3	F-3	G3
4	F-4	G4
5	F-5	G1
6	F-6	G2
7	F-7	G3
8	F-8	G4

Channel Set

F5

FN

(FN: FUNCTION MODE)

3.5 Selecting Channels

Channel selection is the same for all functions. The setting examples here describe operation with the Model 8957 High Resolution Unit.

Channel Settings

MEM


REC

FFT


To open the screen: Press the **SET** key → Select **Channel** with the **SUB MENU** keys → Channel Settings screen
See Screen Layout (⇒ p. 41)

Operating Key	Procedure	Module (Unit) No.	Channel No.
1 SHEET/PAGE	Select the [One Ch] page.		
2	Select the module (Unit) and channel number to be set.		
CURSOR	Move the cursor to each [Unit (no.)] and [Ch (no.)].		
F1 to F8	Select the module (Unit) number (Unit 1, 2, ...) and channel. (The type of the selected module is indicated beside the [Unit].)		
3	Verify the module type and measurement mode to be set.		
	Verify that the [Mode] is set to [Voltage].		
4	Set the measurement range.		
CURSOR	Move the cursor to the [Range (/div)] item.		
F1 to F8	Set the vertical axis (voltage axis range).		
	5 m, 10 m, 20 m, 50 m, 100 m, 200 m, 500 mV/div, 1, 2, 5, 10, 20 V/div		
	The setting is the amplitude per division on the vertical axis. This setting can also be made with the RANGE/ POSN knobs.		
5	Select the input signal coupling method (as occasion demands).		
CURSOR	Move the cursor to the [Coupling] item.		
F1 to F8	Select either choice.		
DC	DC Coupling Select this to acquire both DC and AC components of an input signal.		
AC	Select this to eliminate any DC component from an input signal. Use this to measure only the ripple component superimposed on pulsating current.		
GND	The input signal is disconnected. Zero position can be confirmed.		

Module (Unit) No. Channel No.

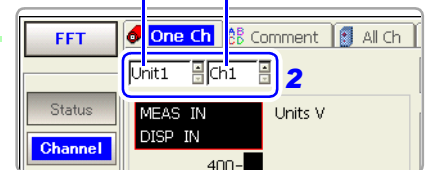

Comments can be entered for each channel.


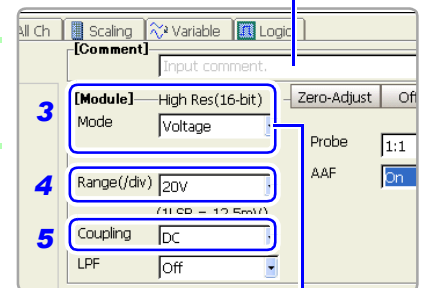


Measurement Mode

When using an input module that can provide multiple types of measurement, select the type of measurement to be performed.

See "3.10.2 Setting Input Coupling" in the *Input Module Guide*

Operating Key	Procedure								
6	Set low-pass filtering (as occasion demands).								
CURSOR	Move the cursor to the [LPF] item.								
F1 to F8	Set the low-pass filter in the input module. (For Model 8957) OFF, 5Hz, 50Hz, 500Hz, 5kHz, 50Hz								
7	Select the probe attenuation.								
CURSOR	Move the cursor to the [Probe] item.								
F1 to F8	Select according to the connection cables being used.								
	<table><tr><td>1:1</td><td>Select when measuring using Model 9197, 9198 or 9217 Connection Cords.</td></tr><tr><td>10:1</td><td>Select when measuring using the Model 9665 10:1 Probe.</td></tr><tr><td>100:1</td><td>Select when measuring using the Model 9666 100:1 Probe.</td></tr><tr><td>1000:1</td><td>Select when measuring using the Model 9322 Differential Probe.</td></tr></table>	1:1	Select when measuring using Model 9197, 9198 or 9217 Connection Cords.	10:1	Select when measuring using the Model 9665 10:1 Probe.	100:1	Select when measuring using the Model 9666 100:1 Probe.	1000:1	Select when measuring using the Model 9322 Differential Probe.
1:1	Select when measuring using Model 9197, 9198 or 9217 Connection Cords.								
10:1	Select when measuring using the Model 9665 10:1 Probe.								
100:1	Select when measuring using the Model 9666 100:1 Probe.								
1000:1	Select when measuring using the Model 9322 Differential Probe.								
8	Set the anti-aliasing filter.								
CURSOR	Move the cursor to the [AAF] item.								
F1 to F8	Select either choice.								
	<table><tr><td>Off</td><td>The anti-aliasing filter is disabled. (default setting)</td></tr><tr><td>On</td><td>The anti-aliasing filter is enabled. (When the external sampling is used, the anti-aliasing filter (AAF) is not available.)</td></tr></table>	Off	The anti-aliasing filter is disabled. (default setting)	On	The anti-aliasing filter is enabled. (When the external sampling is used, the anti-aliasing filter (AAF) is not available.)				
Off	The anti-aliasing filter is disabled. (default setting)								
On	The anti-aliasing filter is enabled. (When the external sampling is used, the anti-aliasing filter (AAF) is not available.)								
9	Perform zero adjustment (after warm-up).								
CURSOR	Move the cursor to the [Zero-Adjust] button.								
F1	Select [Execute] . When executed, all channels are zero adjusted. (Except in the Model 8958 16-Ch Scanner Unit)								
10	Perform Offset Cancel (as occasion demands).								
CURSOR	Move the cursor to the [Offset Cancel] button.								
F1	Select [Execute] . When executed, only the selected channel is corrected.								

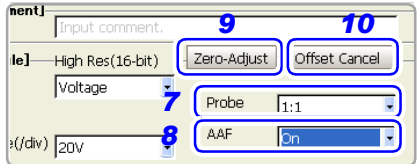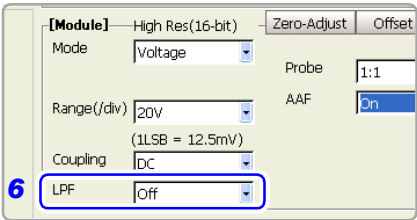

About low-pass filtering
See "3.10.3 Low-Pass Filter (LPF) Settings" in the *Input Module Guide*

About probe attenuation
Matching the probe attenuation setting to that of the input channel's probe enables automatic conversion of voltage axis range measurements for direct reading of numerical values.
See "3.10.15 Probe Attenuation Selection" in the *Input Module Guide*

Anti-Aliasing Filter
Enable to prevent aliasing distortion.
See "Anti-Aliasing Filters" (⇒ p. 107)


About zero adjustment
Adjusts the zero position of an input module. Warm-up time depends on the type of input module.
See "3.10.17 Executing Zero Adjustment" in the *Input Module Guide*

About offset canceling
Executing Offset Cancel when using a sensor corrects for external signal bias.
See "3.10.18 Executing Offset Cancellation" in the *Input Module Guide*


Scaling

The scaling setting allows values displayed on this instrument to match the actual values read directly on a sound level meter or vibration meter.

Without Scaling


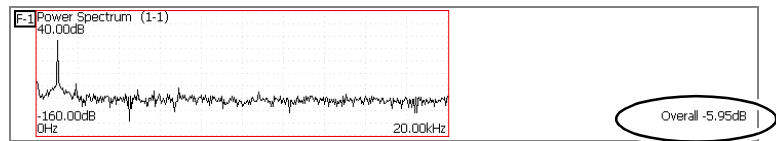


With Scaling

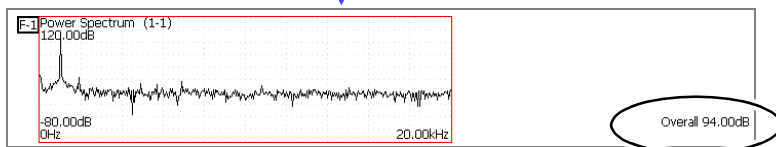


Setting example: To display measurement data on this instrument so that it corresponds to that on a sound level meter.

In a case where a sound level meter displays 94 dB and the overall value displayed on the Waveform screen of this instrument is -5.95 dB.

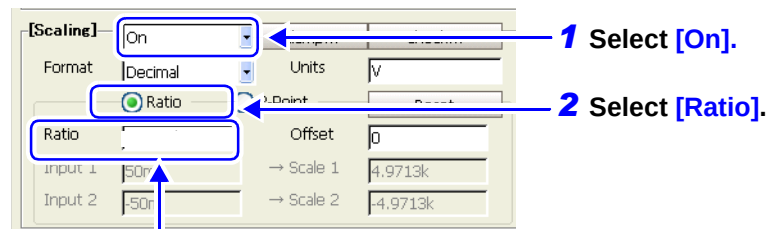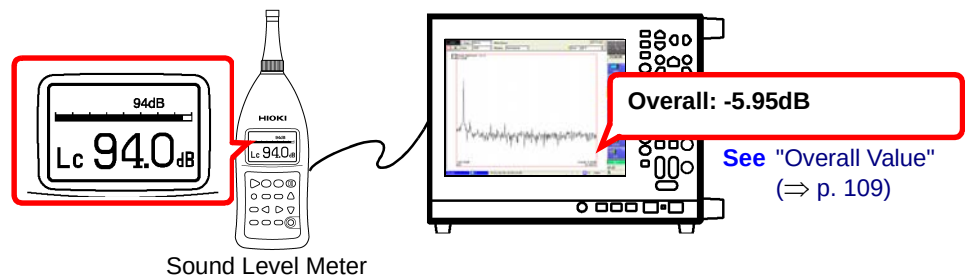

3 Move the cursor to [Ratio], and press the **F7 [dB]** key.

The dB Scaling dialog appears.

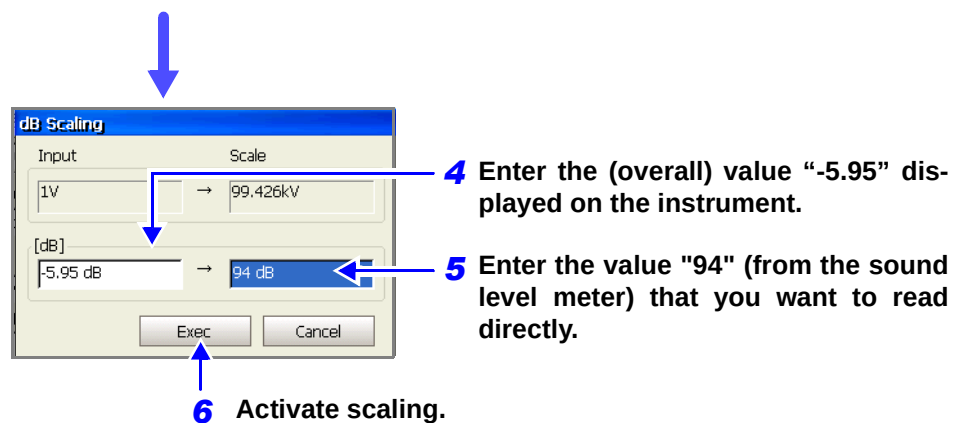

Scaling is performed automatically, and the corresponding values appear in the conversion ratio fields.

3.6 Setting the Screen Layout of the Waveform Screen

Measurement data can be split and displayed on up to 16 sheets on the Waveform screen.

Assigning the Results of FFT Analysis to a Sheet

FFT

To open the screen: Press the **SET** key → Select **Sheet** with the **SUB MENU** keys → Sheet Settings screen
See Screen Layout (⇒ p. 42)

Operating Key Procedure

1 Sheet Assignment.


CURSOR
F1 to F8

Move the cursor to the **[Sheet 1]** item.
Select the number of the Sheet to set.

CURSOR
F1 to F8

Move the cursor to the **[On]** or **[Off]** item.
Select whether to display the selected sheet on the Waveform screen.

Off	The selected sheet is not displayed.
On	The selected sheet is displayed.

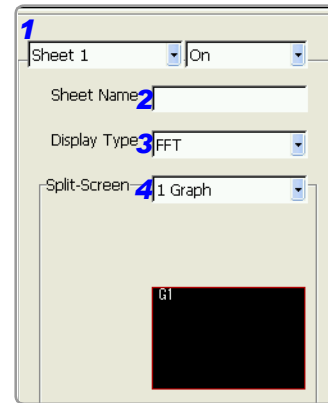

2 Enter a Sheet Name (if you want to change it).

CURSOR
F1 to F8

Move the cursor to the **[Sheet Name]** item.
Enter a name. (up to 8 characters)
(When you enter a sheet name other than the default, it is displayed to the right of the waveform.)

3 Select the Display Type.

CURSOR
F1 to F8

Move the cursor to the **[Display Type]** item.
Select the type of data to be displayed.
The display type depends on the input data selected for analysis.

FFT	Displays a plot of FFT analysis results.
Nyquist	(When the analysis mode is Linear Spectrum, Transfer Function or Cross-Power Spectrum) The real-number part is displayed on the x axis, and the imaginary part on the y axis.
FFT+Nyquist	Analysis results and the Nyquist plot are displayed at the same time.
Wave+FFT *	A memory waveform and FFT analysis results are displayed.
Wave+Nyquist *	The Memory waveform and Nyquist plot are displayed at the same time.

* Input data source [Reference]: selectable only when [From Mem] is selected.

To use an existing memory waveform for analysis

Select [From Mem] as the input data source [Reference].

See "3.4.2 Selecting the Data Source for Analysis" (⇒ p. 52)

To specify the analysis starting point

Specify the starting point on the memory waveform.

See "3.9.3 Analyzing after Specifying an Analysis Starting Point" (⇒ p. 80)

4 Select split-screen display (as occasion demands).


The number of possible screen partitions depends on the selected display type.

See "Display Types and Split-Screen Settings" (⇒ p. 74)


3.6 Setting the Screen Layout of the Waveform Screen

Operating Key	Procedure
5	Select the data to display on the Sheet.
SHEET/PAGE	Select the [FFT] page.
CURSOR	Move the cursor to the [Analyze] column.
F1 to F8	Select the desired calculation number for display. (This becomes the Analysis No. setting on the Status Settings screen.)
(When using split-screen display)	
CURSOR	Move the cursor to the [Graph] column.
F1 to F8	Select the Graph number to be displayed.


Press the DISP key to display the Waveform screen.
The displayed sheet changes each time you press the SHEET/PAGE keys.

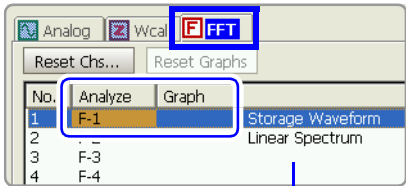

The analysis mode is displayed.

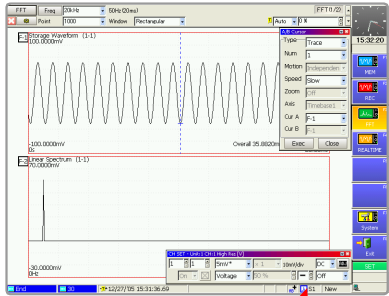

Waveform screen



The sheet number is displayed.



When "Drawing failed"

- **NG: Nyquist Display**
There is a mismatch between the display type setting on the Sheet Settings screen and a parameter setting on the Status Settings screen.
The normal display and Nyquist display cannot be combined. To display both, set the display type to [FFT+Nyquist].
- **NG: X-Axis Setting**
Increase the number of split screen sections, or change the x-axis display.
Linear x-axis and logarithmic displays cannot be combined in the same graph.
- **NG: Analysis Mode Error**
Octave analysis (1/1 or 1/3) cannot be overlaid with another analysis. Increase the number of split screen sections, or set display on another sheet.

Display Types and Split-Screen Settings

Fourteen display arrangements are available.

	1 Graph	2 Graphs	4 Graphs	4 (Print 8)
FFT	G1	G1 G2	G1 G2 G3 G4	G1 G2 G3 G4
Nyquist	G1	G1 G2	G1 G2 G3 G4	G1 G2 G3 G4
FFT+Nyquist	FFT Nyquist G1	FFT Nyquist G1 Nyquist G2		
Wave+FFT *	ANALOG FFT G1	ANALOG FFT G1 FFT G2		
Wave+Nyquist*	ANALOG Nyquist G1	ANALOG Nyquist G1 Nyquist G2		

* Selectable only when the [Reference] setting on the Status Settings screen is [From Mem].

3.7 Saving Analysis Results

The saving procedure is the same as for the Memory and Recorder functions.

See "Chapter 10 Saving/Loading Data & Managing Files" in the *Instruction Manual*

The size of saved files depends on the file format.

See "Appendix 2.2 Waveform File Sizes" in the *Instruction Manual*

When FFT Analysis Results are Saved as Text

A file is created for each analysis mode. One of the following text strings is appended to the file name.


Example: When the Name Pattern setting is [Trig (prefix)] and the save name is "TEST"

150000_051201_TEST_LIN.TXT

(15:00:00, Dec. 1, 2005, "TEST" Linear Spectrum text data)

Analysis Mode	Save Name	Analysis Mode	Save Name
Storage Waveform	STR	Cross Power Spectrum	CSP
Linear Spectrum	LIN	Cross-correlation Function	CCR
RMS Spectrum	RMS	Impulse Response	IMP
Power Spectrum	PSP	Coherence Function	COH
Power Spectrum Density	PSD	Phase Spectrum (1ch / 2ch)	PHASE
Auto-correlation Function	ACR	Power Spectrum (LPC)	LPC
Histogram	HIS	1/1 Octave	1_1_OCT
Transfer Function	TRF	1/3 Octave	1_3_OCT

Text Saving Example

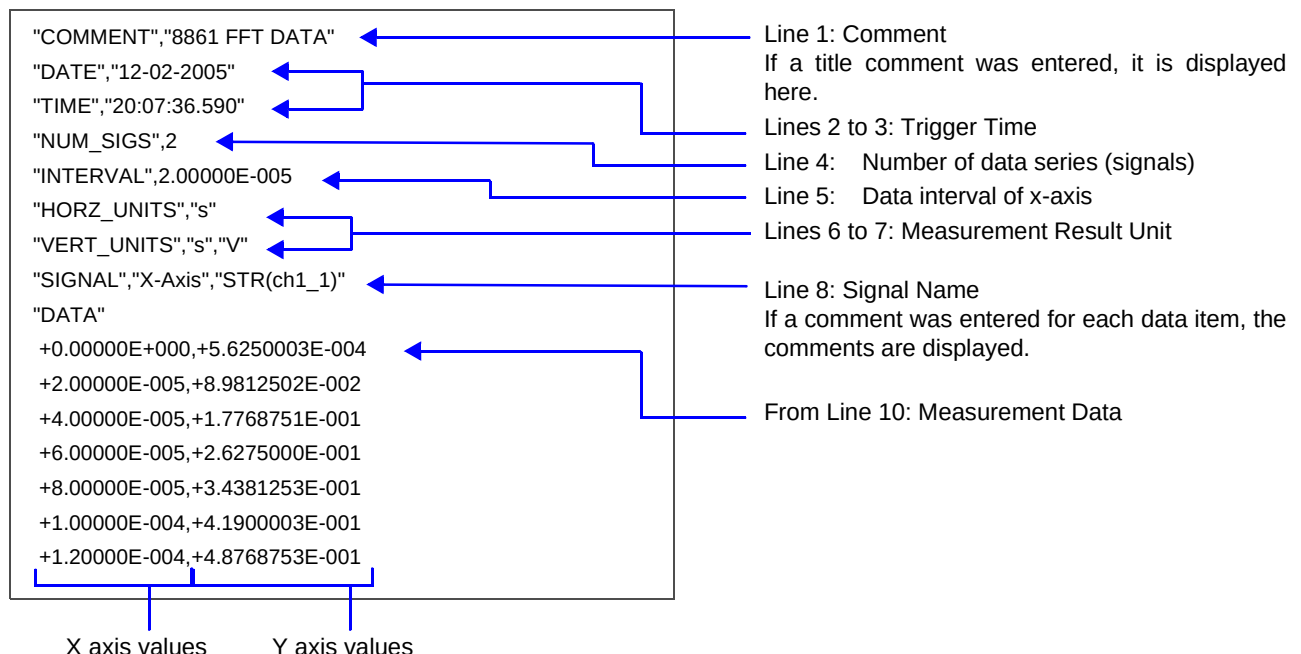


3.8 Printing Analysis Results

The printing procedure is the same as for the Memory and Recorder functions.

See "Chapter 11 Printing" in the *Instruction Manual*

Example of Waveform Printout

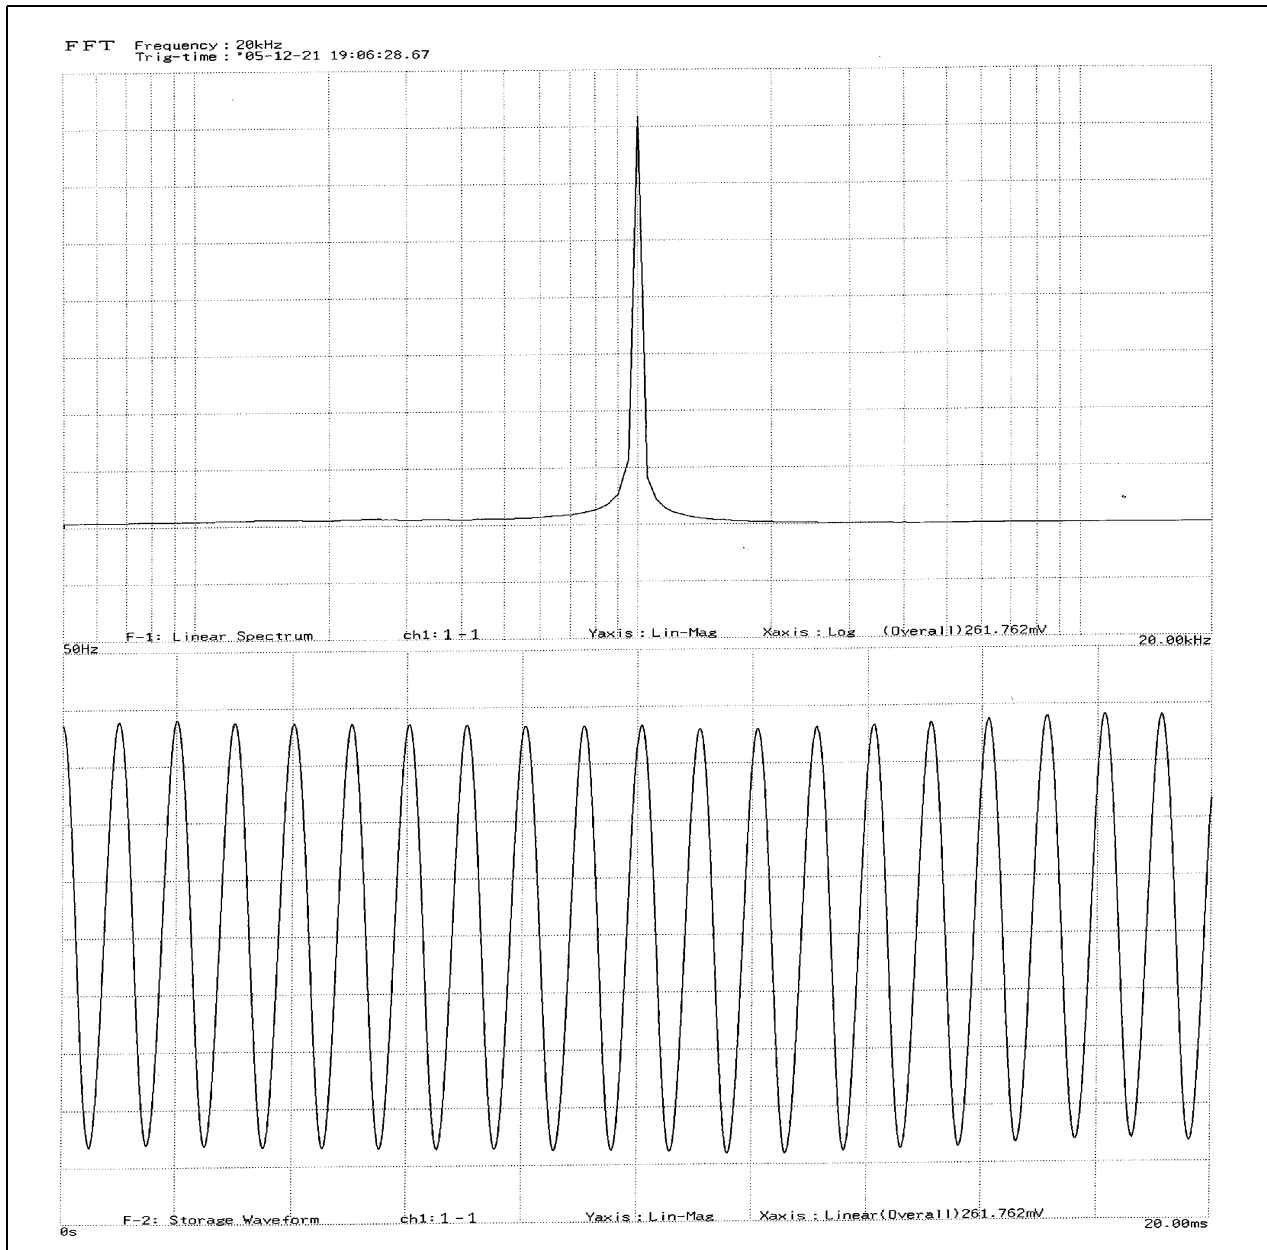

FFT *05-12-21 19:06:28.67

F-1 Linear Spectrum		w1:1-1		Yaxis: Lin-Mag	Xaxis: Log	(Overall)1261.762m									
90Hz	0.553mW	50Hz	0.317mW	100Hz	4.881mW	150Hz	5.766mW	200Hz	5.247mW	250Hz	6.366mW	300Hz	5.278mW	350Hz	5.736mW
40Hz	0.554mW	50Hz	0.829mW	500Hz	0.805mW	550Hz	0.636mW	600Hz	0.721mW	650Hz	0.263mW	700Hz	0.355mW	750Hz	0.117mW
80Hz	0.815mW	85Hz	0.898mW	1.00Hz	0.135mW	1.05Hz	0.136mW	1.10Hz	0.358mW	1.15Hz	0.472mW	1.20Hz	22.856mW	1.25Hz	1.173mW
1.20kHz	11.854mW	1.25kHz	6.785mW	1.30kHz	7.251mW	1.35kHz	6.153mW	1.40kHz	5.435mW	1.45kHz	4.764mW	1.50kHz	4.282mW	1.55kHz	3.821mW
1.60kHz	3.478mW	1.65kHz	3.110mW	1.70kHz	2.870mW	1.75kHz	2.749mW	1.80kHz	2.442mW	1.85kHz	2.365mW	1.90kHz	2.168mW	1.95kHz	2.055mW
2.00kHz	1.948mW	2.05kHz	1.836mW	2.10kHz	1.761mW	2.15kHz	1.665mW	2.20kHz	1.632mW	2.25kHz	1.545mW	2.30kHz	1.471mW	2.35kHz	1.404mW
2.40kHz	1.325mW	2.45kHz	1.272mW	2.50kHz	1.261mW	2.55kHz	1.205mW	2.60kHz	1.131mW	2.65kHz	1.074mW	2.70kHz	1.206mW	2.75kHz	1.063mW
2.80kHz	1.941mW	2.85kHz	0.967mW	2.90kHz	0.963mW	2.95kHz	0.934mW	3.00kHz	0.933mW	3.05kHz	0.906mW	3.10kHz	0.881mW	3.15kHz	0.855mW
3.20kHz	0.836mW	3.25kHz	0.825mW	3.30kHz	0.791mW	3.35kHz	0.734mW	3.40kHz	0.740mW	3.45kHz	0.768mW	3.50kHz	0.787mW	3.55kHz	0.702mW
3.60kHz	0.678mW	3.65kHz	0.685mW	3.70kHz	0.688mW	3.75kHz	0.647mW	3.80kHz	0.617mW	3.85kHz	0.621mW	3.90kHz	0.501mW	3.95kHz	0.620mW
4.00kHz	0.636mW	4.05kHz	0.567mW	4.10kHz	0.557mW	4.15kHz	0.571mW	4.20kHz	0.586mW	4.25kHz	0.552mW	4.30kHz	0.518mW	4.35kHz	0.538mW
4.40kHz	0.546mW	4.45kHz	0.538mW	4.50kHz	0.543mW	4.55kHz	0.521mW	4.60kHz	0.486mW	4.65kHz	0.505mW	4.70kHz	0.483mW	4.75kHz	0.461mW
4.80kHz	0.468mW	4.85kHz	0.472mW	4.90kHz	0.479mW	4.95kHz	0.447mW	5.00kHz	0.448mW	5.05kHz	0.433mW	5.10kHz	0.439mW	5.15kHz	0.416mW
5.20kHz	0.411mW	5.25kHz	0.425mW	5.30kHz	0.437mW	5.35kHz	0.426mW	5.40kHz	0.421mW	5.45kHz	0.403mW	5.50kHz	0.391mW	5.55kHz	0.383mW
5.60kHz	0.426mW	5.65kHz	0.382mW	5.70kHz	0.377mW	5.75kHz	0.400mW	5.80kHz	0.384mW	5.85kHz	0.356mW	5.90kHz	0.347mW	5.95kHz	0.379mW
6.00kHz	0.382mW	6.05kHz	0.353mW	6.10kHz	0.349mW	6.15kHz	0.352mW	6.20kHz	0.345mW	6.25kHz	0.328mW	6.30kHz	0.356mW	6.35kHz	0.343mW
6.40kHz	0.283mW	6.45kHz	0.362mW	6.50kHz	0.358mW	6.55kHz	0.285mW	6.60kHz	0.359mW	6.65kHz	0.349mW	6.70kHz	0.267mW	6.75kHz	0.332mW
6.80kHz	0.334mW	6.85kHz	0.311mW	6.90kHz	0.371mW	6.95kHz	0.277mW	7.00kHz	0.313mW	7.05kHz	0.362mW	7.10kHz	0.268mW	7.15kHz	0.301mW
7.20kHz	0.298mW	7.25kHz	0.278mW	7.30kHz	0.352mW	7.35kHz	0.282mW	7.40kHz	0.261mW	7.45kHz	0.319mW	7.50kHz	0.278mW	7.55kHz	0.288mW
7.60kHz	0.368mW	7.65kHz	0.281mW	7.70kHz	0.275mW	7.75kHz	0.257mW	7.80kHz	0.330mW	7.85kHz	0.293mW	7.90kHz	0.274mW	7.95kHz	0.274mW
8.00kHz	0.276mW	8.05kHz	0.254mW	8.10kHz	0.248mW	8.15kHz	0.248mW	8.20kHz	0.248mW	8.25kHz	0.281mW	8.30kHz	0.256mW	8.35kHz	0.269mW
8.40kHz	0.251mW	8.45kHz	0.245mW	8.50kHz	0.253mW	8.55kHz	0.313mW	8.60kHz	0.266mW	8.65kHz	0.282mW	8.70kHz	0.225mW	8.75kHz	0.256mW
8.80kHz	0.277mW	8.85kHz	0.213mW	8.90kHz	0.264mW	8.95kHz	0.265mW	9.00kHz	0.250mW	9.05kHz	0.220mW	9.10kHz	0.216mW	9.15kHz	0.294mW
9.20kHz	0.287mW	9.25kHz	0.224mW	9.30kHz	0.226mW	9.35kHz	0.199mW	9.40kHz	0.281mW	9.45kHz	0.278mW	9.50kHz	0.188mW	9.55kHz	0.269mW
9.60kHz	0.159mW	9.65kHz	0.167mW	9.70kHz	0.248mW	9.75kHz	0.213mW	9.80kHz	0.235mW	9.85kHz	0.283mW	9.90kHz	0.133mW	9.95kHz	0.161mW
10.00kHz	0.210mW	10.05kHz	0.224mW	10.10kHz	0.241mW	10.15kHz	0.168mW	10.20kHz	0.115mW	10.25kHz	0.186mW	10.30kHz	0.207mW	10.35kHz	0.189mW
10.40kHz	0.211mW	10.45kHz	0.179mW	10.50kHz	0.213mW	10.55kHz	0.175mW	10.60kHz	0.195mW	10.65kHz	0.192mW	10.70kHz	0.158mW	10.75kHz	0.184mW
10.80kHz	0.175mW	10.85kHz	0.171mW	10.90kHz	0.189mW	10.95kHz	0.157mW	11.00kHz	0.183mW	11.05kHz	0.186mW	11.10kHz	0.173mW	11.15kHz	0.176mW
11.20kHz	0.179mW	11.25kHz	0.168mW	11.30kHz	0.196mW	11.35kHz	0.226mW	11.40kHz	0.142mW	11.45kHz	0.131mW	11.50kHz	0.196mW	11.55kHz	0.235mW
11.60kHz	0.188mW	11.65kHz	0.219mW	11.70kHz	0.186mW	11.75kHz	0.133mW	11.80kHz	0.204mW	11.85kHz	0.198mW	11.90kHz	0.203mW	11.95kHz	0.178mW
12.00kHz	0.159mW	12.05kHz	0.182mW	12.10kHz	0.154mW	12.15kHz	0.183mW	12.20kHz	0.227mW	12.25kHz	0.222mW	12.30kHz	0.185mW	12.35kHz	0.159mW
12.40kHz	0.190mW	12.45kHz	0.181mW	12.50kHz	0.195mW	12.55kHz	0.218mW	12.60kHz	0.134mW	12.65kHz	0.165mW	12.70kHz	0.160mW	12.75kHz	0.164mW
12.80kHz	0.185mW	12.85kHz	0.198mW	12.90kHz	0.158mW	12.95kHz	0.158mW	13.00kHz	0.182mW	13.05kHz	0.182mW	13.10kHz	0.151mW	13.15kHz	0.164mW
13.20kHz	0.149mW	13.25kHz	0.140mW	13.30kHz	0.197mW	13.35kHz	0.181mW	13.40kHz	0.166mW	13.45kHz	0.147mW	13.50kHz	0.160mW	13.55kHz	0.182mW
13.60kHz	0.209mW	13.65kHz	0.169mW	13.70kHz	0.148mW	13.75kHz	0.162mW	13.80kHz	0.105mW	13.85kHz	0.188mW	13.90kHz	0.176mW	13.95kHz	0.127mW
14.00kHz	0.131mW	14.05kHz	0.170mW	14.10kHz	0.155mW	14.15kHz	0.174mW	14.20kHz	0.143mW	14.25kHz	0.154mW	14.30kHz	0.145mW	14.35kHz	0.149mW
14.40kHz	0.201mW	14.45kHz	0.150mW	14.50kHz	0.110mW	14.55kHz	0.169mW	14.60kHz	0.170mW	14.65kHz	0.155mW	14.70kHz	0.142mW	14.75kHz	0.145mW
14.80kHz	0.165mW	14.85kHz	0.164mW	14.90kHz	0.149mW	14.95kHz	0.130mW	15.00kHz	0.164mW	15.05kHz	0.176mW	15.10kHz	0.161mW	15.15kHz	0.139mW
15.20kHz	0.137mW	15.25kHz	0.188mW	15.30kHz	0.188mW	15.35kHz	0.152mW	15.40kHz	0.132mW	15.45kHz	0.139mW	15.50kHz	0.139mW	15.55kHz	0.151mW
15.60kHz	0.171mW	15.65kHz	0.128mW	15.70kHz	0.153mW	15.75kHz	0.185mW	15.80kHz	0.122mW	15.85kHz	0.141mW	15.90kHz	0.117mW	15.95kHz	0.147mW
16.00kHz	0.178mW	16.05kHz	0.092mW	16.10kHz	0.188mW	16.15kHz	0.200mW	16.20kHz	0.097mW	16.25kHz	0.175mW	16.30kHz	0.177mW	16.35kHz	0.097mW
16.40kHz	0.159mW	16.45kHz	0.137mW	16.50kHz	0.141mW	16.55kHz	0.163mW	16.60kHz	0.104mW	16.65kHz	0.167mW	16.70kHz	0.175mW	16.75kHz	0.091mW
16.80kHz	0.146mW	16.85kHz	0.180mW	16.90kHz	0.170mW	16.95kHz	0.135mW	17.00kHz	0.168mW	17.05kHz	0.161mW	17.10kHz	0.138mW	17.15kHz	0.162mW
17.20kHz	0.139mW	17.25kHz	0.165mW	17.30kHz	0.163mW	17.35kHz	0.142mW	17.40kHz	0.129mW	17.45kHz	0.174mW	17.50kHz	0.160mW	17.55kHz	0.155mW
17.60kHz	0.157mW	17.65kHz	0.151mW	17.70kHz	0.157mW	17.75kHz	0.142mW	17.80kHz	0.155mW	17.85kHz	0.155mW	17.90kHz	0.137mW	17.95kHz	0.099mW
18.00kHz	0.149mW	18.05kHz	0.156mW	18.10kHz	0.120mW	18.15kHz	0.140mW	18.20kHz	0.102mW	18.25kHz	0.163mW	18.30kHz	0.191mW	18.35kHz	0.091mW
18.40kHz	0.134mW	18.45kHz	0.189mW	18.50kHz	0.138mW	18.55kHz	0.124mW	18.60kHz	0.145mW	18.65kHz	0.115mW	18.70kHz	0.104mW	18.75kHz	0.172mW
18.80kHz	0.166mW	18.85kHz	0.103mW	18.90kHz	0.150mW	18.95kHz	0.130mW	19.00kHz	0.133mW	19.05kHz	0.155mW	19.10kHz	0.122mW	19.15kHz	0.140mW
19.20kHz	0.129mW	19.25kHz	0.133mW	19.30kHz	0.127mW	19.35kHz	0.087mW	19.40kHz	0.163mW	19.45kHz	0.140mW	19.50kHz	0.117mW	19.55kHz	0.164mW
19.60kHz	0.076mW	19.65kHz	0.130mW	19.70kHz	0.183mW	19.75kHz	0.120mW	19.80kHz	0.125mW	19.85kHz	0.091mW	19.90kHz	0.131mW	19.95kHz	0.122mW
20.00kHz	0.177mW														

3.9 Analysis with the Waveform Screen


3.9.1 Selecting the Display Method

The display of FFT analysis data can be switched between waveform and numerical views.

Press the **DISP** key repeatedly to change the display method.

Pressing the **DISP** key opens the Display dialog in which to select a display method. Selections in this dialog are available using the F keys.

Press the **ESC** key or an F key to close the dialog.

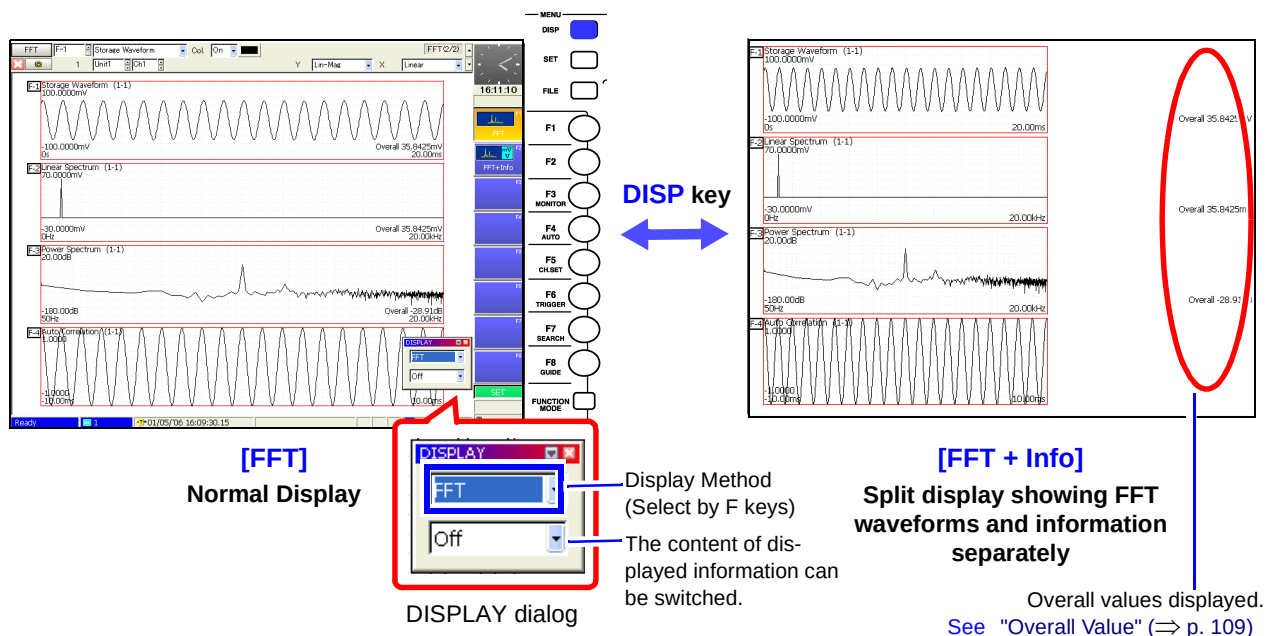

NOTE

When the display type on the Sheet Settings screen is [Nyquist], [FFT+Nyquist] or [Wave+Nyquist], the display cannot be switched.

3.9.2 Selecting Gauges and Values

Display of upper and lower limits and peak values [maximal/ maximum] can be selected by analysis number. However, selection is not possible when Nyquist display is enabled.

Press the **FUNCTION MODE** key to enable the FN mode, then press **F2 [Gauge & Value]**.

The Gauge dialog appears.

Select an analysis number as occasion demands to display gauge and measurement values.

Press the **ESC** key or the **F8 [Close]** key to close the dialog.

The diagram illustrates the process of selecting gauges and values in the waveform screen. It shows the main screen with a waveform, the 'Gauge & Value' dialog box, and the 'GAUGE & VALUE' dialog box. Arrows indicate the sequence of actions: pressing F2 (Gauge & Value) and then FN (FUNCTION MODE). The resulting screen shows the waveform with upper and lower limits and peak values displayed.

GAUGE & VALUE dialog

Using the CURSOR keys, move the cursor into the dialog and select the channels for which to display a gauge.

When the analysis number that was set on the Status screen is selected, upper and lower limits and the local maxima values are displayed.

3.9.3 Analyzing after Specifying an Analysis Starting Point

A starting point for FFT analysis can be specified on an existing memory waveform before analyzing.

The procedure depends on the Trigger Mode setting.

See "Trigger Modes and Averaging" (⇒ p. 60)

- When the Trigger Mode is [Single]
Analysis is performed once on the specified number of analysis points beginning with the specified starting point, and analysis results are displayed. This is convenient for analyzing only a specific range. However, if averaging is enabled, analysis repeats for the specified averaging count.
- When the Trigger Mode is [Auto] or [Repeat]
Analysis is performed repeatedly on the specified number of analysis points beginning with the specified starting point and ending with end of waveform data, and final analysis results are displayed (because analysis is only performed on the specified number of analysis points, final analysis results may be determined and become available before the end of the waveform data).


The starting point can be specified by one of the following methods:

(1) Verifying the analysis starting point while viewing analysis data
(⇒ p. 81)

The memory waveform and analysis results are displayed at the same time on the Waveform screen (Sheet Settings screen: Display type [Wave+FFT] or [Wave+Nyquist]) and the analysis starting point is specified on the memory waveform.


(2) Performing FFT analysis after specifying a starting point on an existing memory waveform using the A/B cursors (⇒ p. 83)

The analysis starting point is specified using the A/B cursors with the Memory function. If the cursors are not displayed, analysis begins at the start of the data. The starting position cannot be verified while the FFT function is enabled.

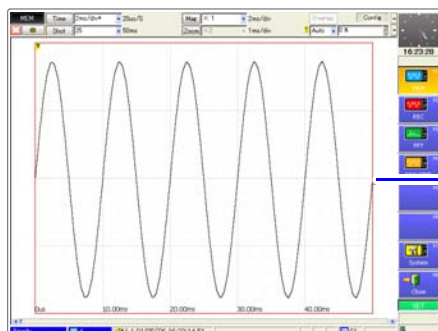Procedure 1. Verifying the analysis starting point while viewing analysis data

1 Display the waveform to be analyzed.


2 Select the FFT function (F3 [FFT]) to display the Status Settings screen.

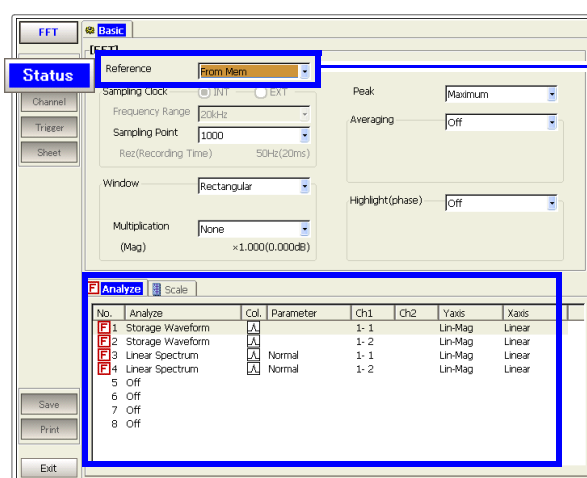

3 Set the analysis input data source to [From Mem].

Set analysis conditions such as the analysis mode and number of analysis points (these can also be set on the Waveform screen).

4 Press the SUB MENU keys to display the Sheet Settings screen.

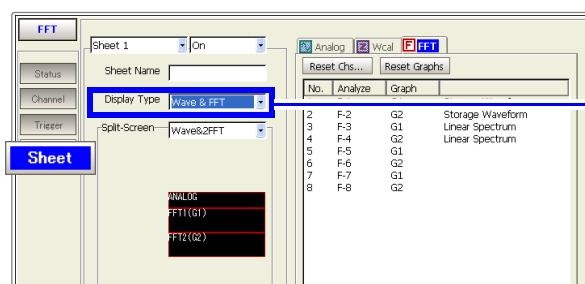

5 Set the display type to [Wave+FFT] or [Wave+Nyquist].

To use split-screen display, set graph assignments on the [FFT] page.

6 Press the DISP key to display the Waveform screen.

3.9 Analysis with the Waveform Screen

Analysis segment for one pass (the number of analysis points)

Specify the location of the analysis input data using the jog and shuttle controls.

Jog
Moves the analysis starting point.

Shuttle
Scrolls the Memory waveform.

A/B CURSOR
TYPE SPEED

Press the **SPEED** key to adjust the movement and scrolling speed.

To change the number of analysis points

The setting can be changed at the top of the Waveform screen.
The range is determined by the number of analysis points.
If the analysis range (number of points) is larger than the memory waveform as shown below, analysis is not performed.

Analysis Segment Display

To analyze only a certain portion

At the top of the Waveform screen, set the trigger mode to **[Single]**, so that only the currently displayed analysis segment will be analyzed.
When the trigger mode is other than **[Single]**, analysis continues for the specified number of analysis points, or to the end of data. To interrupt analysis in progress, press the **STOP** key.

To change analysis conditions

Press the **SUB MENU** keys to select **[FFT (1/2)]** or **[FFT (2/2)]**, and change the settings.

9 Press the START key to begin analyzing.


Shows the last analysis segment.



Analysis results are displayed on the lower graphs.

When the trigger mode is **[Auto]** or **[Repeat]**, the number of analysis points up to the end of the waveform data is analyzed, and the last data is displayed.

Shows the number of times analysis was performed.

Procedure 2. Performing FFT analysis after specifying a starting point on an existing memory waveform using the A/B cursors

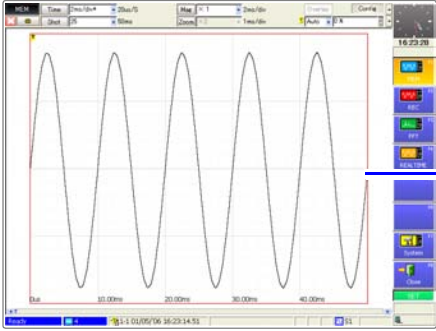
- 

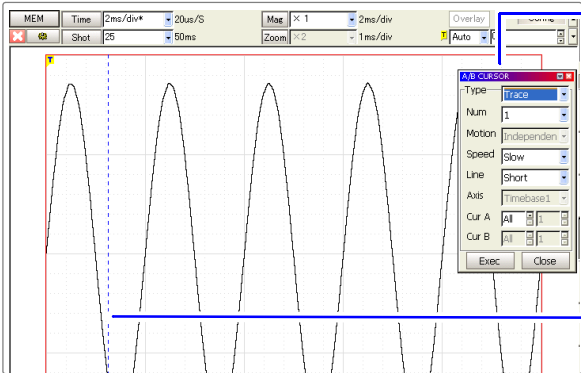1 Display the waveform with the Memory function.
- 


2 Press the **TYPE** key and select **[Vertical]** or **[Trace]**.

TYPE key **A/B** knob
-

3 Specify the analysis starting point with the **A/B** knobs.

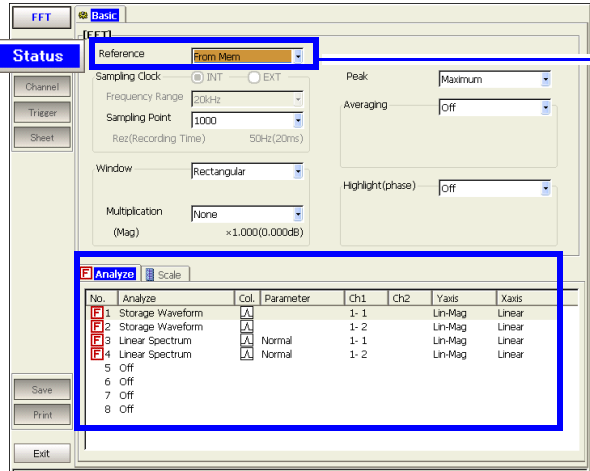
When both A/B cursors are enabled, the analysis starting point is determined by the earliest (leftmost) cursor. The length of the waveform segment for FFT analysis cannot be specified using the cursors.
- 4** Select the FFT function (**F3 [FFT]**) to display the Status Settings screen.
- 

5 Set the analysis input data source to **[From Mem]**.

Set analysis conditions such as the analysis mode and number of analysis points (these can also be set on the Waveform screen).

No.	Analyze	Col	Parameter	Ch1	Ch2	Yaxis	Xaxis
1	Storage Waveform	LA		1-1		Lin-Mag	Linear
2	Storage Waveform	LA		1-2		Lin-Mag	Linear
3	Linear Spectrum	LA	Normal	1-1		Lin-Mag	Linear
4	Linear Spectrum	LA	Normal	1-2		Lin-Mag	Linear
5	Off						
6	Off						
7	Off						
8	Off						
- 6** Press the **DISP** key to display the Waveform screen.

3.9 Analysis with the Waveform Screen

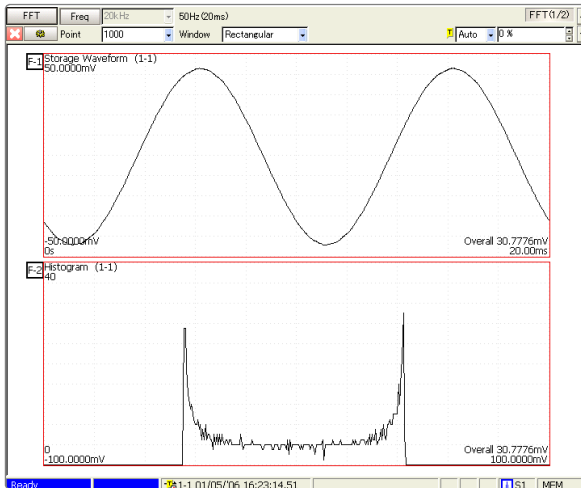

- 7 Make other settings as occasion demands, then press the **START** key to begin analyzing.

3.10 FFT Analysis Modes

3.10.1 Analysis Modes and Display Examples

For the functions of each analysis mode, see "3.10.2 Analysis Mode Functions" (⇒ p. 102).

Storage


STR

Displays the time axis waveform of the input signal.

When the window function setting is other than rectangular, the window function is applied to the waveform and displayed.

Axis	Display Type	Description
X axis	Linear	Time-domain display Displays the value of the time-domain waveform corresponding to the set frequency range. See "Relationship Between Frequency Range, Resolution and Number of Analysis Points" (⇒ p. 55)
Y axis	Lin-Mag	Displays the input module waveform.

Waveform Example

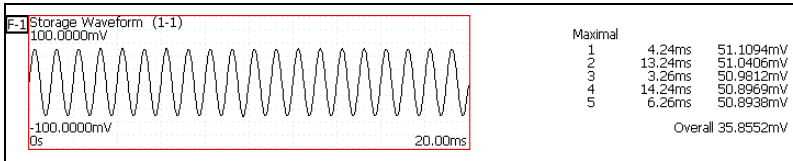

Window: Rectangular
X axis: Linear
Y axis: Lin-Mag

Linear Spectrum

LIN

The linear spectrum plots the input signal frequency. It can be displayed as a Nyquist plot.

Main uses:


- To inspect the peak frequency contents of a waveform
- To inspect signal amplitudes at each frequency

See About the Functions "3.10.2 Analysis Mode Functions" (⇒ p. 102)


Axis	Display Type	Description
X axis	Linear	Frequency is displayed with equal spacing Display Range: DC to the top of the frequency range
	Log	Frequency is displayed logarithmically Display Range: 1/400 th to 1/4000 th (depending on the number of analysis points) to the top of the frequency range
	Nyquist display	The real-number component of analysis values are displayed linearly.
Y axis	Lin-Mag	Analysis values are displayed linearly.
	Log-Mag	Analysis values are displayed as dB values. (0 dB reference value: 1eu)*
	Lin-Real	The real-number component of analysis values are displayed.
	Lin-Imag	The imaginary component of analysis values are displayed.
	Nyquist display	The imaginary component of analysis values are displayed.

* eu: engineering units that are currently set are the standard (e.g., when the unit settings is volts, 0 dB = 1 V)


Waveform Example

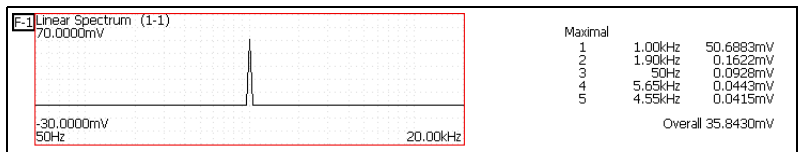


Normal display
X axis: Log
Y axis: Lin-Mag

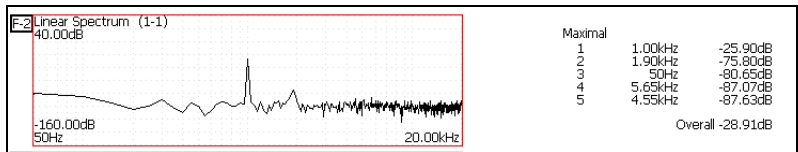


Normal display
X axis: Log
Y axis: Log-Mag

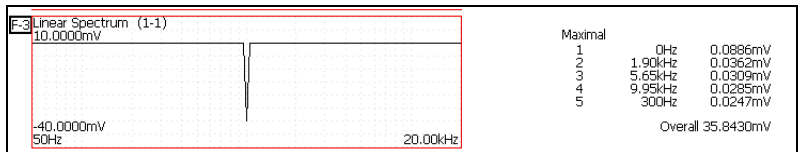

Normal display
X axis: Log
Y axis: Lin-Real

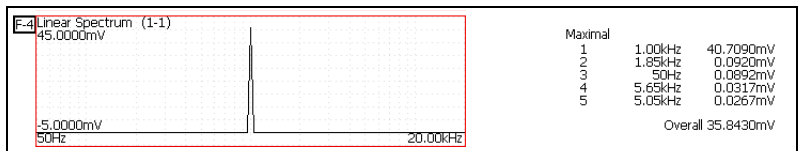

Normal display
X axis: Log
Y axis: Lin-Imag

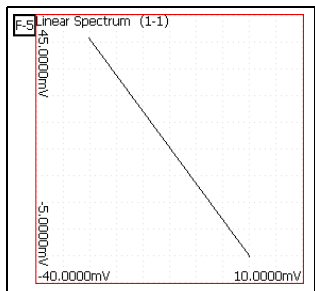

Nyquist display

RMS Spectrum

RMS

Amplitudes (RMS values) are calculated along the frequency axis from the input signal waveform. RMS and power spectra displays use the same analysis results displayed logarithmically (amplitude in dB).

Main uses:


- To inspect the peak frequency contents of a waveform
- To inspect the RMS value at each frequency

See About the Functions "3.10.2 Analysis Mode Functions" (⇒ p. 102)

Axis	Display Type	Description
X axis	Linear	Frequency is displayed with equal spacing Display Range: DC to the top of the frequency range
	Log	Frequency is displayed logarithmically Display Range: 1/400 th to 1/4000 th (depending on the number of analysis points) to the top of the frequency range
Y axis	Lin-Mag	Analysis values are displayed linearly.
	Log-Mag	Analysis values are displayed as dB values. (0 dB reference value: 1eu)*
	Lin-Real	The real-number component of analysis values are displayed.
	Lin-Imag	The imaginary component of analysis values are displayed.

* eu: engineering units that are currently set are the standard (e.g., when the unit settings is volts, 0 dB = 1 V)


Waveform Example

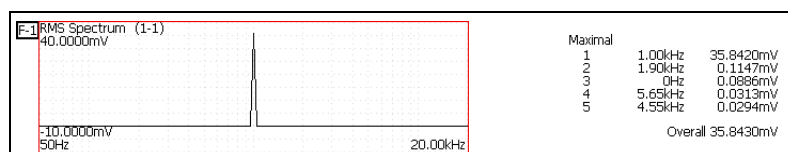

Normal display

X axis: Log


Y axis: Lin-Mag

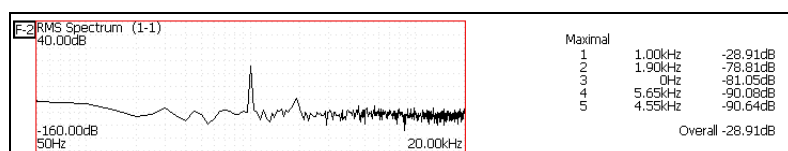

Normal display

X axis: Log


Y axis: Log-Mag

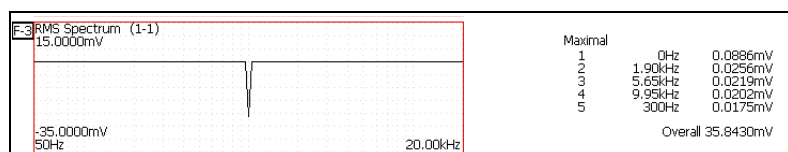

Normal display

X axis: Log

Y axis: Lin-Real

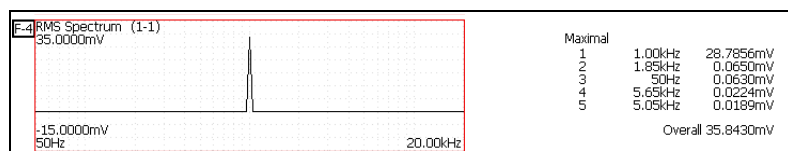

Normal display

X axis: Log

Y axis: Lin-Imag

Power Spectrum

PSP

Displays input signal power as the amplitude component.

Main uses:


- To inspect the peak frequency contents of a waveform
- To inspect the power level at each frequency

See About the Functions "3.10.2 Analysis Mode Functions" (⇒ p. 102)


Axis	Display Type	Description
X axis	Linear	Frequency is displayed with equal spacing Display Range: DC to the top of the frequency range
	Log	Frequency is displayed logarithmically Display Range: 1/400 th to 1/4000 th (depending on the number of analysis points) to the top of the frequency range
Y axis	Lin-Mag	Analysis data is displayed linearly as squared values. Indicates the power component.
	Log-Mag (logarithm)	Analysis values are displayed as dB values. (0 dB reference value: 1eu ²)*

* eu: engineering units that are currently set are the standard (e.g., when the unit settings is volts, 0 dB = 1 V²)

Waveform Example

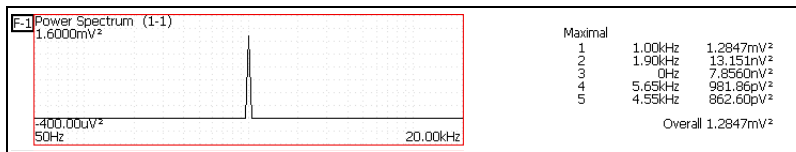

Normal display
X axis: Log
Y axis: Lin-Mag

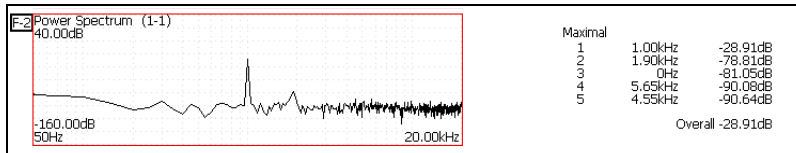

Normal display
X axis: Log
Y axis: Log-Mag

Power Spectrum Density

PSD

Indicates the power spectrum density of the input signal with only the amplitude component included. This is the power spectrum divided by the frequency resolution.

Not available with external sampling enabled.

Main uses:


To acquire a power spectrum with 1-Hz resolution for highly irregular waveforms such as white noise

See About the Functions "3.10.2 Analysis Mode Functions" ($\Rightarrow$ p. 102)

Axis	Display Type	Description
X axis	Linear	Frequency is displayed with equal spacing Display Range: DC to the top of the frequency range
	Log	Frequency is displayed logarithmically Display Range: 1/400 th to 1/4000 th (depending on the number of analysis points) to the top of the frequency range
Y axis	Lin-Mag	Analysis values are displayed linearly.
	Log-Mag (logarithm)	Analysis values are displayed as dB values. (0 dB reference value: 1eu ² /Hz)*

* eu: engineering units that are currently set are the standard (e.g., when the unit settings is volts, 0 dB = 1 V²/Hz)


Waveform Example

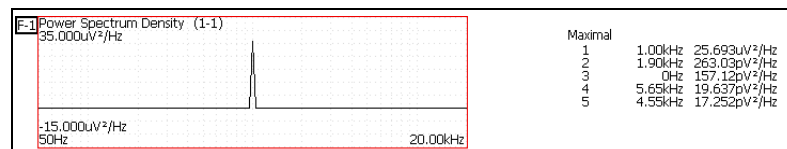

Normal display

X axis: Log

Y axis: Lin-Mag

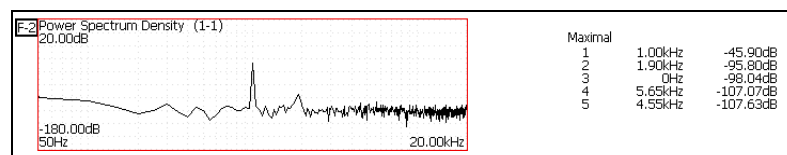

Normal display

X axis: Log

Y axis: Log-Mag

Auto Correlation Function

ACR

Shows the correlation of two points on the input signal at time differential t .


Main uses:

- To detect periodicity in irregular signals (improving and detecting SNR)
- To inspect periodic components in a noisy waveform.

See About the Functions "3.10.2 Analysis Mode Functions" ($\Rightarrow$ p. 102)

Axis	Display Type	Description
X axis	Linear	Time display The center ($t = 0$) is the reference. To the right is lag time ($+t$), and to the left is lead time ($-t$)
Y axis	Lin-Mag	+1 to -1 (dimensionless units) The closest correlation at time differential t is +1, and the least correlation is 0. -1 indicates completely reversed polarity. Because of the characteristics of the function, $t = 0$ becomes +1.

Waveform Example

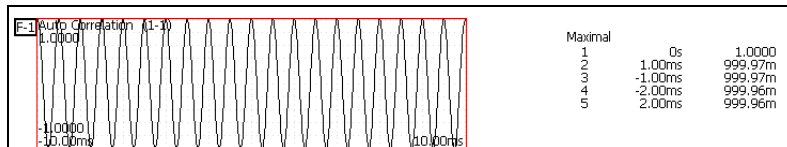

X axis: Linear
Y axis: Lin-Mag

This instrument provides a circular auto-correlation function.
Analysis results are normalized to the maximum value.

Histogram

HIS

Acquires the amplitude distribution of the input signal.


Main uses:

- To inspect deviations in the amplitude range of a waveform
- With analysis point distribution, to ascertain whether a waveform is artificial or natural (natural forms exhibiting regular distribution)

See About the Functions "3.10.2 Analysis Mode Functions" ($\Rightarrow$ p. 102)

Axis	Display Type	Description
X axis	Linear	Displays input level of the input signal.
Y axis	Lin-Mag	Displays analysis data distribution.

Waveform Example

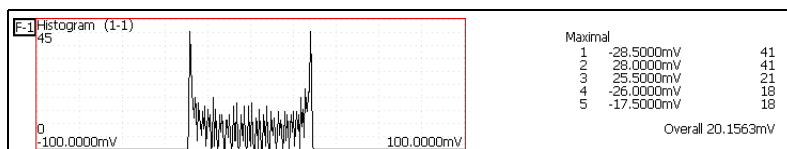

Normal display
X axis: Log
Y axis: Lin-Mag

1/1 and 1/3 Octave Analysis

OCT

The sound pressure level of the spectrum of a signal such as noise is displayed through a fixed-width one- or one-third octave band-pass filter.

Not available with external sampling enabled.

Main uses:


To analyze frequency components of noise

See About the Functions "3.10.2 Analysis Mode Functions" (⇒ p. 102), "Octave Filter Characteristics" (⇒ p. 114)

Axis	Display Type	Description
X axis	Log	Displays the center frequency of each band.
Y axis	Lin-Mag	Octave analysis values are displayed linearly.
	Log-Mag (logarithm)	Octave analysis values are displayed as dB values. (0 dB reference value: 1eu)*

* eu: engineering units that are currently set are the standard (e.g., when the unit settings is volts, 0 dB = 1 V)

Waveform Example

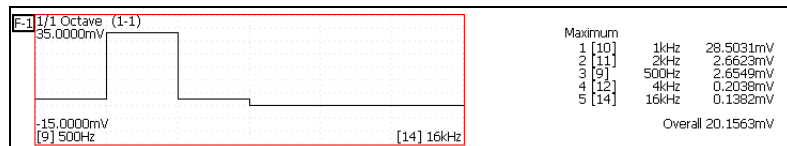


1/1 Octave

X axis: Log

Y axis: Lin-Mag

Filter: Normal

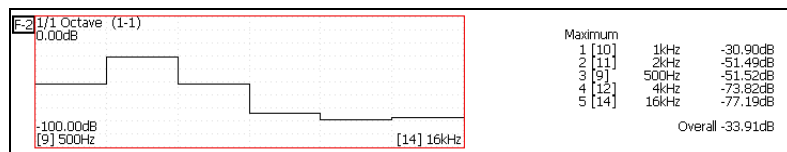


1/1 Octave

X axis: Log

Y axis: Log-Mag

Filter: Normal

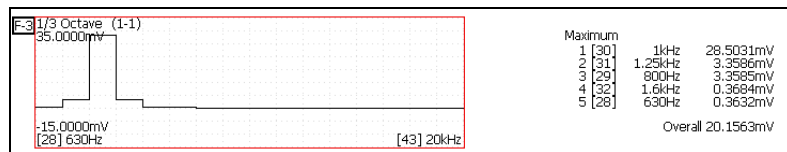


1/3 Octave

X axis: Log

Y axis: Lin-Mag

Filter: Normal

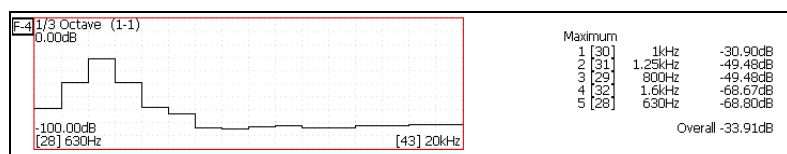

1/3 Octave

X axis: Log

Y axis: Log-Mag

Filter: Normal

Octave Analysis

Octave analysis consists of frequency analysis of the signal passed through a constant-width band-pass filter. The power spectrum displays the power level in each subband after dividing the spectrum into fixed-width segments (subbands), while octave analysis scales the spectrum logarithmically and displays each octave (subband) as a bar graph.

The center frequency of the octave bands and filter characteristics are determined according to IEC61260 standards. With this instrument, 1/1- and 1/3-octave analyses are calculated using power spectrum Analysis results.

1/1 Octave Analysis: 6 subbands

1/3 Octave Analysis: 16 subbands

(●: 1/1 OCT, ○: 1/3 OCT)

[illegible]

[illegible]

Phase Spectrum

PHA

Shows the phase characteristics of the input signal.

Main uses:


- To inspect the phase spectrum of channel 1. Displays the phase of a cosine waveform as a reference (0°).
- To inspect the phase difference between channels 1 and 2.

See About the Functions "3.10.2 Analysis Mode Functions" (⇒ p. 102)


- 1 Ch FFT: Displays the phase of the signal on channel 1. Displays the phase of a cosine waveform as a reference (0°). Unless the waveform is synchronous, phase values are unstable.
- 2 Ch FFT: Displays the phase difference between channels 1 and 2. Positive values indicate that the phase of channel 2 is leading.

Axis	Display Type	Description
X axis	Linear	Frequency is displayed with equal spacing Display Range: DC to the top of the frequency range
	Log	Frequency is displayed logarithmically Display Range: 1/400 th to 1/4000 th (depending on the number of analysis points) to the top of the frequency range
Y axis	Lin-Mag	Analysis values are displayed linearly.

Waveform Example

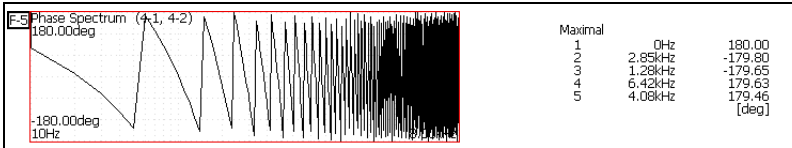

1chFFT
X axis: Log
Y axis: Lin-Mag

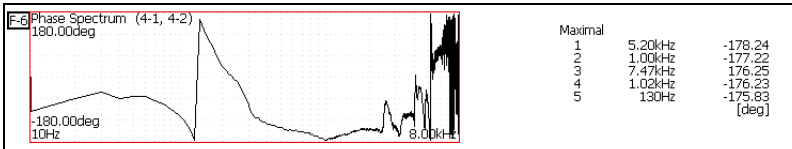

2chFFT
X axis: Log
Y axis: Log-Mag

Emphasizing only a Specific Portion (Highlighted Display)

A specific portion of a phase spectrum can be emphasized and displayed.

See "3.4.7 Emphasizing Analysis Results (phase spectra only)" (⇒ p. 61)

Transfer Function

TRF

From the input and output signals, the transfer function (frequency characteristic) of a measurement system can be obtained. It can also be displayed as a Nyquist plot.


Main uses:

- To inspect a filter's frequency characteristic
- To inspect the stability of a feedback control system (using the Nyquist plot)
- To inspect the resonance characteristic of an object using an impulse hammer and pick-up sensor

See About the Functions "3.10.2 Analysis Mode Functions" (⇒ p. 102), "Linear Time-Invariant Systems" (⇒ p. 104)

Axis	Display Type	Description
X axis	Linear	Frequency is displayed with equal spacing Display Range: DC to the top of the frequency range
	Log	Frequency is displayed logarithmically Display Range: 1/400 th to 1/4000 th (depending on the number of analysis points) to the top of the frequency range
	Nyquist display	Displays the real-number component of the input-output ratio.
Y axis	Lin-Mag	Displays the input-output ratio linearly (dimensionless units).
	Log-Mag (logarithm)	Displays the input-output ratio as dB values.
	Lin-Real	Displays the real-number component of the input-output ratio (dimensionless units).
	Lin-Imag	Displays the imaginary component of the input-output ratio (dimensionless units).
	Nyquist display	Displays the imaginary component of the input-output ratio.


Waveform Example

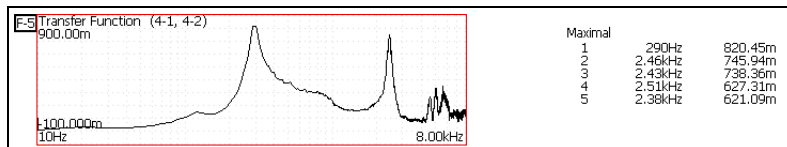

Normal display

X axis: Log


Y axis: Lin-Mag

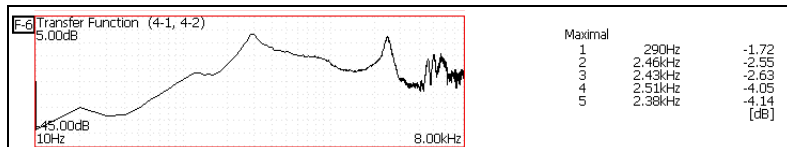

Normal display

X axis: Log


Y axis: Log-Mag

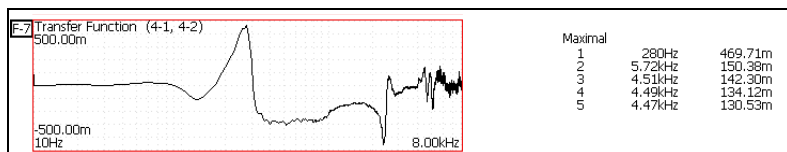

Normal display

X axis: Log


Y axis: Lin-Real

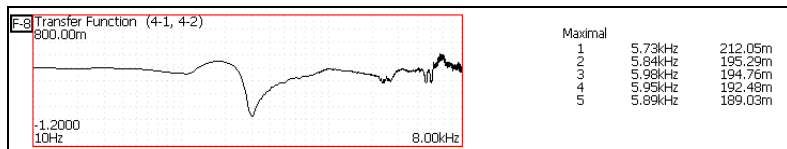

Normal display

X axis: Log

Y axis: Lin-Imag

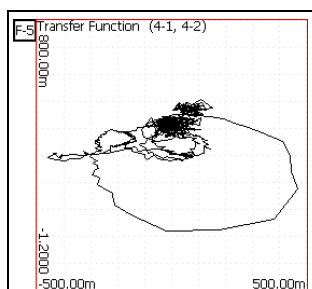

Nyquist display

Cross Power Spectrum

CSP

The product of the spectra of two input signals can be obtained. The common frequency components of two signals can be obtained.

Using the voltage and current waveforms as input signals, active power, reactive power and apparent power can be obtained at each frequency.

Main uses:


To inspect common frequency components of two signals

See About the Functions "3.10.2 Analysis Mode Functions" (⇒ p. 102)


Axis	Display Type	Description
X axis	Linear	Frequency is displayed with equal spacing Display Range: DC to the top of the frequency range
	Log	Frequency is displayed logarithmically Display Range: 1/400 th to 1/4000 th (depending on the number of analysis points) to the top of the frequency range
	Nyquist display	Displays the real-number component of the input-output ratio linearly.
Y axis	Lin-Mag	Displays the squared value of amplitude contents of analysis data linearly.
	Log-Mag (logarithm)	Displays the amplitude contents of analysis data as dB values. (0 dB reference value: 1eu ²)*
	Lin-Real	Displays the squared values of the real component of analysis data linearly.
	Lin-Imag	Displays the squared values of the imaginary component of analysis data linearly.
	Nyquist display	Displays the imaginary component of analysis data linearly.

* eu: engineering units that are currently set are the standard (e.g., when the unit settings is volts, 0 dB = 1 V²)


Waveform Example

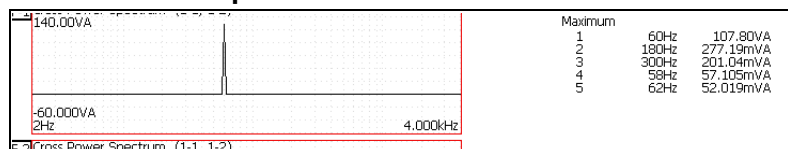


Normal display
X axis: Log
Y axis: Lin-Mag

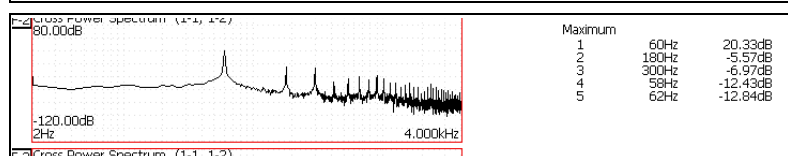


Normal display
X axis: Log
Y axis: Log-Mag

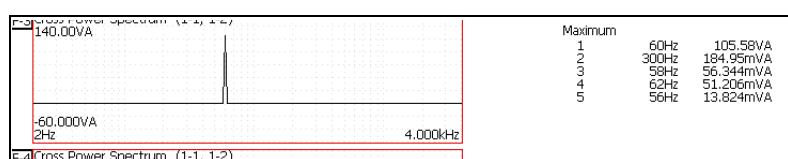

Normal display
X axis: Log
Y axis: Lin-Real

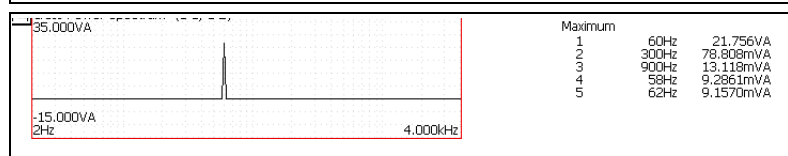

Normal display
X axis: Log
Y axis: Lin-Imag

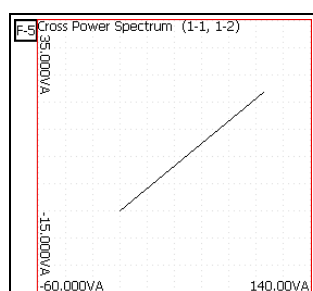

Nyquist display

Cross-Correlation FunctionCCR

Using two input signals, shows the correlation of two points on the input signal at time differential t . Output is displayed as a function of differential time t .


Main uses:

- To determine the phase shift of two signals per unit of time
- To determine the speed and distance of time lag between two signals

See About the Functions "3.10.2 Analysis Mode Functions" (⇒ p. 102)

Axis	Display Type	Description
X axis	Linear	Time display The center ($t = 0$) is the reference. To the right is lag time ($+t$), and to the left is lead time ($-t$)
Y axis	Lin-Mag	+1 to -1 is displayed in dimensionless units. At time differential t , this value is +1 when the correlation of input and output signals is the closest, and 0 when correlation is the least. -1 indicates completely reversed polarity.

Waveform Example

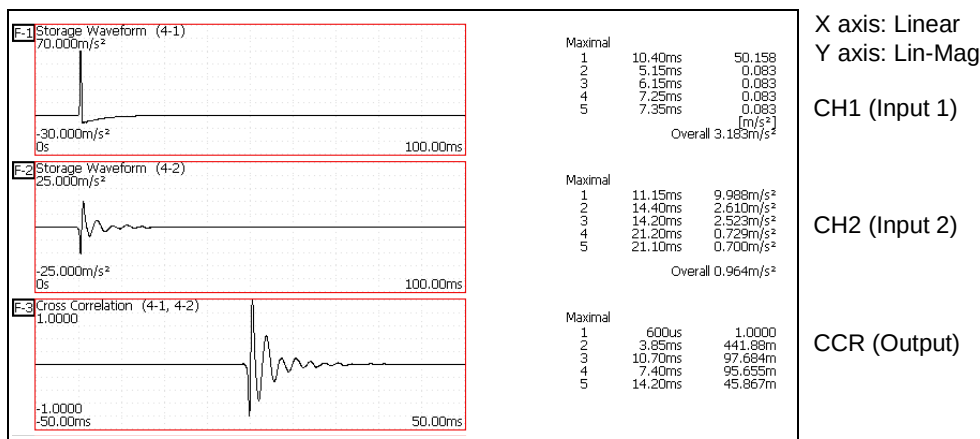

This instrument provides a circular cross-correlation function. Analysis results are normalized to the maximum value.

Impulse Response

IMP

The transfer characteristic of a system is obtained as a time-domain waveform.

Utilizing both output and input signals of the measurement system, a unit impulse is applied to the system and the corresponding response waveform is obtained.


Main uses:

To inspect circuit time constants

See About the Functions "3.10.2 Analysis Mode Functions" ($\Rightarrow$ p. 102), "Linear Time-Invariant Systems" ($\Rightarrow$ p. 104)

Axis	Display Type	Description
X axis	Linear	Time display The center ($t = 0$) is the reference. To the right is lag time ($+t$), and to the left is lead time ($-t$)
Y axis	Lin-Mag	This value is the transfer function provided by inverse Fourier transformation.

Waveform Example

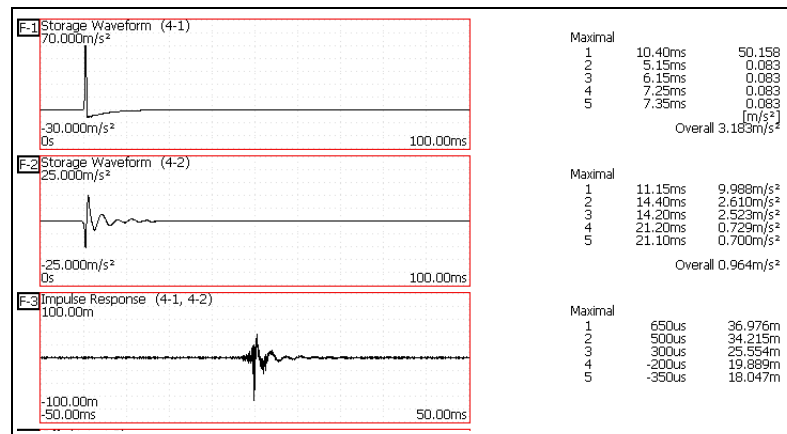

Normal display

X axis: Linear

Y axis: Lin-Mag

CH1

CH2

IMP

Coherence Function

COH

This function gives a measure of the correlation (coherence) between input and output signals. Values obtained are between 0 and 1.

With a single measurement, the coherence function gives a value of one for all frequencies. Spectrum (frequency-domain) averaging should always be performed before measurement (analysis is not available with time-domain averaging).


Main uses:

- To evaluate transfer functions
- In a system with multiple inputs, to inspect the effect of each input on the output

See About the Functions "3.10.2 Analysis Mode Functions" (⇒ p. 102)

Axis	Display Type	Description
X axis	Linear	Frequency is displayed with equal spacing Display Range: DC to the top of the frequency range
	Log	Frequency is displayed logarithmically Display Range: 1/400 th to 1/4000 th (depending on the number of analysis points) to the top of the frequency range
Y axis	Lin-Mag	Displays the causal relationship and degree of relationship between two input signals, as a value between 0 and 1 (dimensionless units).

Waveform Example

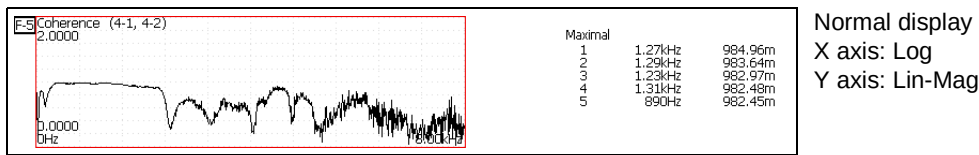

The coherence function has two general definition formulas. For the definition formulas, see "3.10.2 Analysis Mode Functions" (⇒ p. 102)

Power Spectrum Density (Linear Predictive Coding)

LPC

When the spectrum shape is complex and hard to comprehend with either linear or power spectra, a rough spectrum structure can be obtained.

Not available with external sampling enabled.

Main uses:


To obtain a spectral envelope using statistical methods

See About the Functions "3.10.2 Analysis Mode Functions" (⇒ p. 102)


Axis	Display Type	Description
X axis	Linear	Frequency is displayed with equal spacing Display Range: DC to the top of the frequency range
	Log	Frequency is displayed logarithmically Display Range: 1/400 th to 1/4000 th (depending on the number of analysis points) to the top of the frequency range
Y axis	Lin-Mag	Analysis values are displayed linearly.
	Log-Mag (logarithm)	Analysis values are displayed as dB values. (0 dB reference value: 1eu ² /Hz)*

* eu: engineering units that are currently set are the standard (e.g., when the unit settings is volts, 0 dB = 1 V²/Hz)

Waveform Example

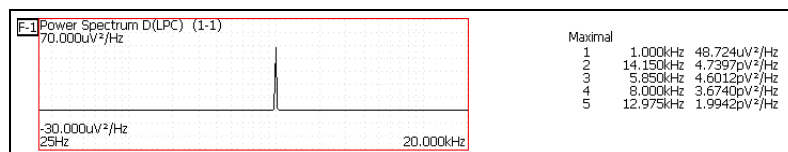

X axis: Log
Y axis: Lin-Mag

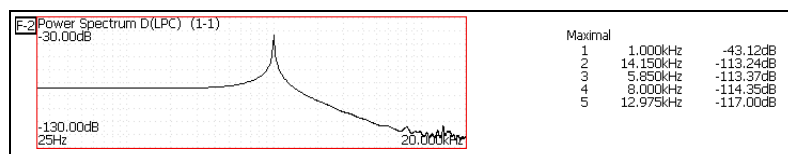

X axis: Log
Y axis: Log-Mag

NOTE

- Always specify the order (from 2 to 64). Higher orders can expose finer spectral details.
- Amplitude values provided by LPC are not always the same as the power spectrum density.
- If an error occurs during analysis, no waveform is displayed.
- Noise-like phenomena can strongly affect the spectrum shape.

3.10.2 Analysis Mode Functions

Analysis Mode	Internal analysis formula (linear, real, imag [imaginary], log [logarithm])
No Analysis	No analysis.
Storage Waveform	A waveform obtained by applying the window function to a time-domain waveform.
Linear Spectrum (LIN)	$X(k) = \sum_{n=0}^{N-1} x(n)W^{kn} \quad F(k) = CX(k) \quad C = \begin{cases} 1/N(DC) \\ 2/N(AC) \end{cases}$ $linear = F(k) \quad real = \text{Re}\{F(k)\} \quad imag = \text{Im}\{F(k)\} \quad log = 20 \log F(k) $
RMS Spectrum (RMS)	$F'(k) = C'F(k) \quad C' = \begin{cases} 1(DC) \\ 1/\sqrt{2}(AC) \end{cases}$ $linear = F'(k) \quad real = \text{Re}\{F'(k)\} \quad imag = \text{Im}\{F'(k)\} \quad log = 20 \log F'(k) $
Power Spectrum (PSP)	$P(k) = a F(k) ^2 \quad a = \begin{cases} 1(DC) \\ 1/2(AC) \end{cases}$ $linear = P(k) \quad log = 10 \log P(k) $
Power Spectrum Density (PSD)	$P'(k) = P(k) / \delta f \quad \delta f: \text{Frequency resolution}$ $linear = P'(k) \quad log = 10 \log P'(k) $
Auto-correlation Function (ACR)	$R_{xx}(n) = \frac{1}{N} \sum_{k=0}^{N-1} X(k) ^2 W^{-kn} \quad (\text{recursive convolution})$
Histogram (HIS)	Counts amplitude data.
Transfer Function (TRF)	$H(k) = Y(k) / X(k)$ $linear = H(k) \quad real = \text{Re}\{H(k)\} \quad imag = \text{Im}\{H(k)\} \quad log = 20 \log H(k) $
Cross Power Spectrum (CSP)	$S_{yx}(k) = X^*(k)Y(k) : \text{Cross Spectrum}$ $X_{power}(k) = AS_{yx}(k) \quad A = \begin{cases} 1/N^2 \\ 2/N^2 \end{cases}$ $linear = X_{power}(k) \quad real = \text{Re}\{X_{power}(k)\}$ $mag = \text{Im}\{X_{power}(k)\} \quad log = 10 \log X_{power}(k) $
Cross-correlation Function (CCR)	$R_{yx}(n) = \frac{1}{N} \sum_{k=0}^{N-1} S_{yx}(k)W^{-kn} \quad (\text{recursive convolution})$
Impulse Response (IMP)	$h(n) = \frac{1}{N} \sum_{k=0}^{N-1} \frac{Y(k)}{X(k)} W^{-kn}$
Coherence Function (COH)	$coh(k) = \sqrt{\frac{S_{yx}(k)S_{yx}^*(k)}{S_{xx}(k)S_{yy}(k)}}$
Phase Spectrum (1ch / 2ch) (PHA)	$\theta(k) = 180 / \pi \times \tan^{-1}(\text{Im}(F'(k)) / \text{Re}(F'(k)))$ $\theta(k) = 180 / \pi \times \tan^{-1}(\text{Im}(S_{yx}(k)) / \text{Re}(S_{yx}(k)))$
Power Spectrum (LPC)	(Abbr.) Spectrum approximation from Linear Predictive Coding. See "Linear Predictive Coding (LPC)" ($\Rightarrow$ p. 115)


3.11 FFT Definitions

What is FFT?

FFT is the abbreviation for Fast Fourier Transform, an efficient method to calculate the DFT (Discrete Fourier Transform) from a time-domain waveform. Also, the reverse process of transforming frequency data obtained by the FFT back into its original time-domain waveform is called the IFFT (Inverse FFT). The FFT functions perform various types of analysis using FFT and IFFT.

Time and Frequency Domain Considerations

All signals are input to the instrument as a function of the time domain. This function can be considered as a combination of sine waves at various frequencies, such as in the following diagram. The characteristics of a signal that may be difficult to analyze when viewed only as a waveform in the time domain can be easier to understand by transforming it into a spectrum (the frequency domain).

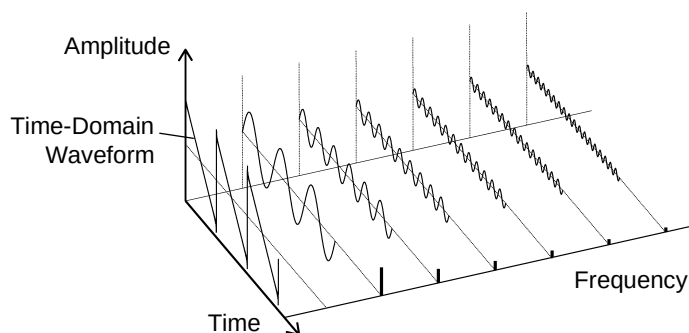

Discrete Fourier Transforms and Inverse FFT

For a discrete signal $x(n)$, the DFT is $X(k)$ and the number of Analysis points is N , which relate as follows:

$$X(k) = DFT\{x(n)\} = \sum_{n=0}^{N-1} x(n)W_N^{kn} \quad \dots \dots \dots (1)$$

$$x(n) = IDFT\{X(k)\} = \frac{1}{N} \sum_{k=0}^{N-1} X(k)W_N^{-kn} \quad \dots \dots \dots (2)$$

$$W_N = \exp\left(-j \frac{2\pi}{N}\right) \quad \dots \dots \dots (3)$$


$X(k)$ is typically a complex number, so expression (1) can be transformed again and written as follows:

$$F(k) = |F(k)| \exp\{j\phi(k)\} = |F(k)| \angle \phi(k) \quad \dots \dots \dots (4)$$

$$\phi(k) = \tan^{-1} \frac{\text{Im}\{X(k)\}}{\text{Re}\{X(k)\}} \quad \dots \dots \dots (5)$$

$|F(k)|$: Amplitude spectrum, $\phi(k)$: Phase spectrum

Representing the above relationship on a complex flat surface produces the following figure.

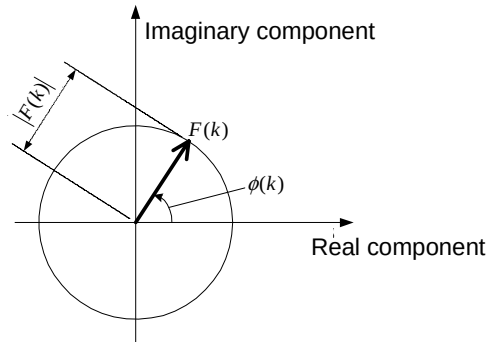

Linear Time-Invariant Systems

Consider a linear time-invariant (LTI) system $y(n)$ that is a response to discrete time-domain signal $x(n)$.

In such an LTI system, the following expression applies to any integer A_i when the response to $x_i(n)$ is $y_i(n) = L[x_i(n)]$.

$$L[A_1 x_1(n) + A_2 x_2(n)] = A_1 y_1(n) + A_2 y_2(n) \quad \text{----- (6)}$$

If the system function of an LTI system is $h(n)$, the input/output relationship can be obtained by the next expression.

$$y(n) = \sum_{m=0}^{\infty} h(n)x(n-m) = \sum_{m=-\infty}^{\infty} h(n-m)x(m) \quad \text{----- (7)}$$

Therefore, when a unit impulse $\delta(n)$ (which is 1 when $n = 0$, and 0 when $n \neq 0$) is applied to $x(n)$, the input/output relationship is:

$$y(n) = h(n) \quad \text{----- (8)}$$


This means that when the input signal is given as a unit impulse, the output is the LTI system characteristic itself.

The response waveform of a system to a unit impulse is called the **impulse response**.

On the other hand, when the discrete Fourier transforms of $x(n)$, $y(n)$ and $h(n)$ are $X(k)$, $Y(k)$ and $H(k)$, respectively, expression (7) gives the following:

$$Y(k) = X(k)H(k) \quad \text{----- (9)}$$

$H(k)$ is also called the transfer function, calculated from $X(k)$ and $Y(k)$. Also, the inverse discrete Fourier transform function of $H(k)$ is the unit impulse response $h(n)$ of the LTI system. The impulse response and transfer function of this instrument are calculated using the relationships of expression (9).

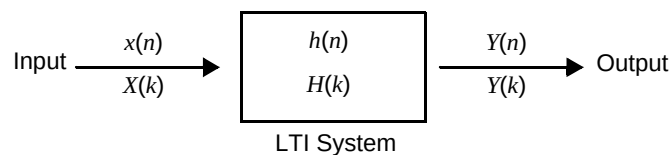

Number of Analysis Points


The FFT functions of this instrument can perform frequency analysis of time-domain waveforms consisting of 1000, 2000, 5000 or 10,000 points. However, when the following conditions are satisfied, previously analyzed data can be reanalyzed with a different number of analysis points.

- A. When measurements are made with the averaging function disabled (Off)
- B. When measurements are made with the averaging function enabled for time-domain averaging (simple or exponential).

When the number of analysis points at measurement time is N_1 and the number of analysis points is changed to N_2 after measurement, the instrument performs as follows.


(1) When $N_1 < N_2$

- Because not enough data has been collected, zero is inserted for time after the end of the measured waveform.
- The window function applies only to the N_1 segment.
- Frequency resolution is increased. For example, if $N_1 = 1000$ and $N_2 = 2000$, frequency resolution is doubled.
- The average energy of the time-domain waveform is reduced, so the amplitude of the linear spectrum is also reduced.

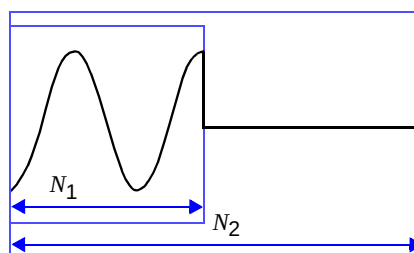

(2) When $N_1 > N_2$

- The specified (N_2) segment is extracted from the head of the (N_1) data.
- The window function applies only to the N_2 segment.
- Frequency resolution is decreased. For example, if $N_1 = 2000$ and $N_2 = 1000$, frequency resolution is halved.
- The average energy of the time-domain waveform is unchanged, so the amplitude of the linear spectrum is not significantly affected.

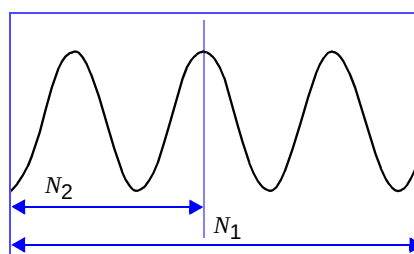

Aliasing



When the frequency of a signal to be measured is higher than the sampling rate, the observed frequency is lower than that of the actual signal, with certain frequency limitations. This phenomena occurs when sampling occurs at a lower frequency than that defined by the Nyquist-Shannon sampling theorem, and is called **aliasing**.

If the highest frequency component of the input signal is $f_{\max}$ and the sampling frequency is f_s , the following expression must be satisfied:

$$f_s = 2 f_{\max} \quad \text{-----} \quad (10)$$

Therefore, if the input includes a frequency component higher than $f_s/2$, it is observed as a lower frequency (alias) that does not really exist.

The following diagrams show the results of spectrum analysis of composite waveforms having components of 1 kHz and 3 kHz, and of 1 kHz and 7 kHz. If sampling frequency f_s is 10 kHz, the spectral component of an input frequency above 5 kHz (in this case, 7 kHz) is observed as an alias at 5 kHz or below. In this example the difference between the 3 and 7 kHz components is indiscernible.

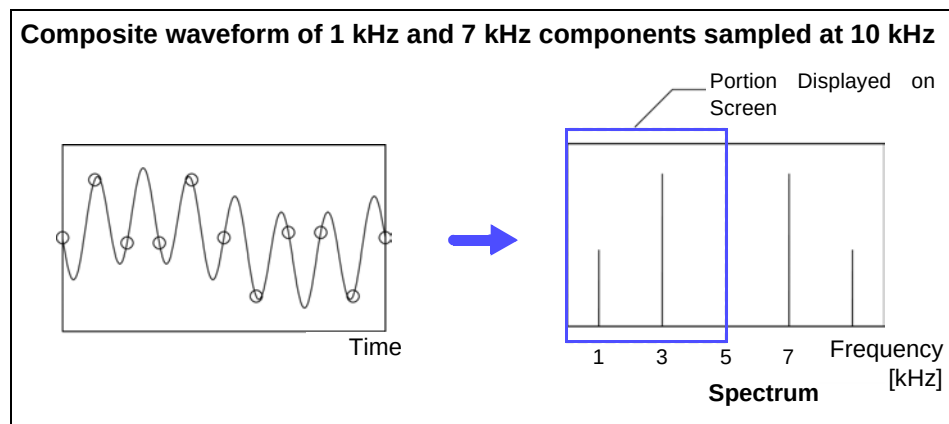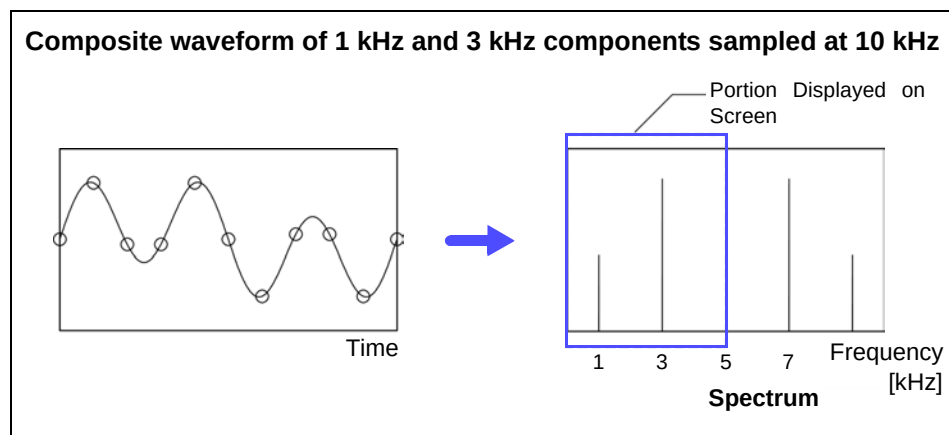


Anti-Aliasing Filters

When the maximum frequency component of the input signal is higher than one-half of the sampling frequency, aliasing distortion occurs. To eliminate aliasing distortion, a low-pass filter can be used that cuts frequencies higher than one-half of the sampling frequency. Such a low-pass filter is called an anti-aliasing filter.


The following figures show the effect of application of an anti-aliasing filter on a square wave input waveform.

Without an anti-aliasing filter

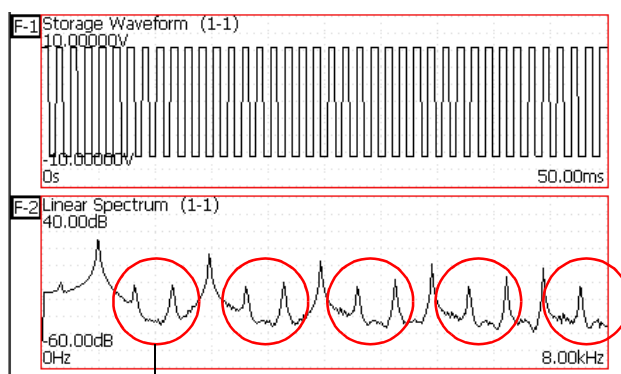

Non-existent frequency components are observed.



With an anti-aliasing filter

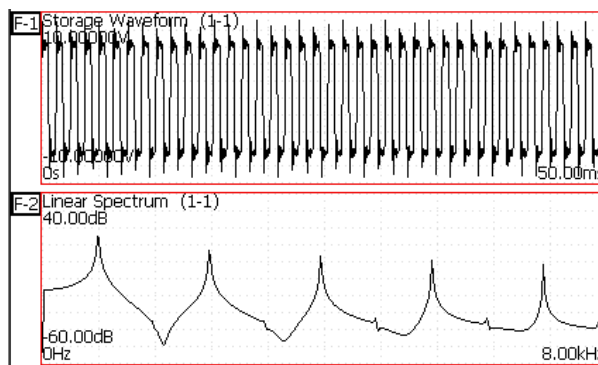

Imaging

When the instrument is set to a measurement frequency range that requires a higher sampling rate than the maximum capability of the input module, intermediate data points are interpolated between successive data samples. In this case, the time-domain waveform exhibits a stair-step shape. When FFT analysis is performed in this situation, non-existent high frequency spectral components appear. This phenomena is called zero-order hold characteristic **imaging**.

The following figures show the time-domain waveform and spectrum of a sine wave applied to the Model 8959 DC/RMS Unit.

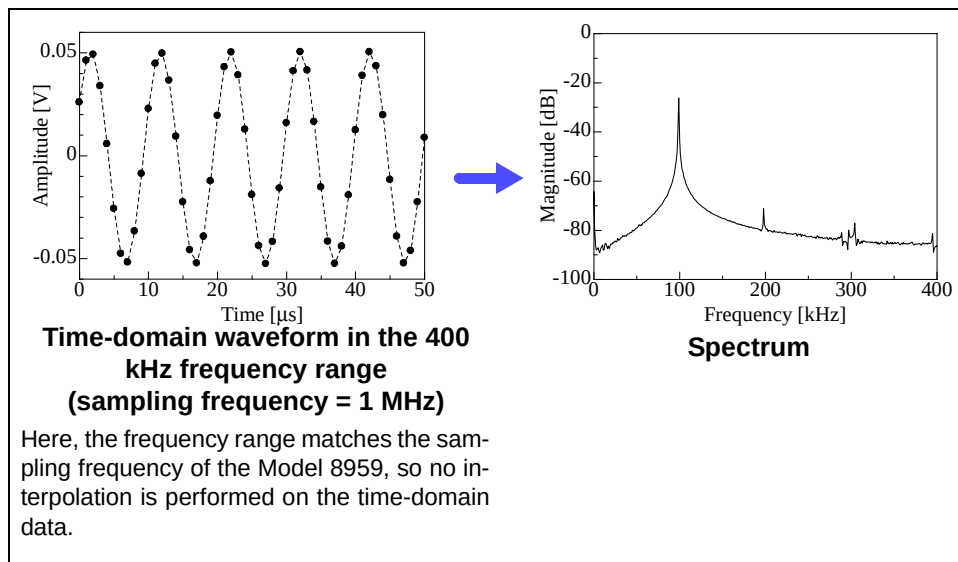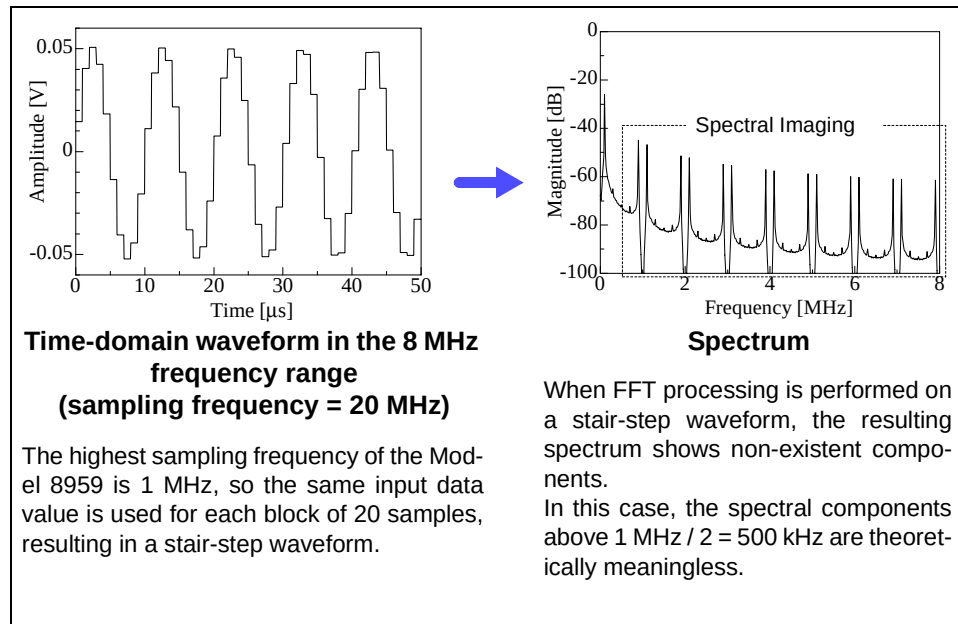

To avoid imaging phenomena when analyzing waveforms with the FFT function, verify the maximum sampling frequency of the input module before measuring.

Averaging

With the FFT function, averaging is performed according to the following analytical expressions. Averaging in the time domain produces meaningless data if performed with inconsistent trigger criteria.

1. Simple Averaging (Time and Frequency Domains)

Sequences of acquired data are summed and divided by the number of acquisitions.

$$A_n = \frac{(n-1)A_{n-1} + Z_n}{n} \dots \dots \dots (11)$$

n : count of measurements to average

A_n : averaging results of n counts

Z_n : measurement data of n counts

2. Exponential Averaging (Time and Frequency Domains)

Before averaging, newer data is given exponentially greater significance than older data.

$$A_n = \frac{(N-1)A_{n-1} + Z_n}{N} \dots \dots \dots (12)$$

N : Specified number of counts to average

n : count of measurements to average

A_n : averaging results of n counts

Z_n : measurement data of n counts

Overall Value

The overall value is the sum of the power spectrum at each frequency. This value is equal to the positive sum of the squares of the (RMS) input signals, except when frequency averaging is performed. The FFT function of this instrument calculates and displays the RMS values for stored waveforms and the overall value from the sum of the power spectrum for the frequency domain.

$$(Over\ all) = \sum_{i=0} P_i \dots \dots \dots (13)$$


P_i : power spectrum of value i

Window Function



The Fourier transform of a continuous system is defined by the integral Calculus in expression (14) for the time range from minus infinity to plus infinity.

$$X(f) = \int_{-\infty}^{\infty} x(t)\varepsilon^{-2\pi ft} dt \dots\dots\dots (14)$$

However, because expression (14) cannot be calculated with actual measurements, the Analysis is performed on a segment between finite limits. Processing the waveform segment within these limits is called window processing. For FFT analysis, the waveform segment within these limits is assumed to repeat periodically (as shown below).

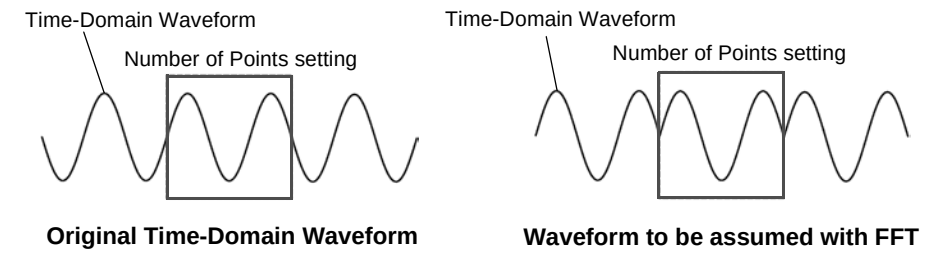

When the number of points for FFT analysis is an integer multiple of the input signal frequency, a single-line spectrum is obtained. However, if it is not an integer multiple of the frequency (when the waveform assumed with FFT includes discontinuous points), the spectrum is scattered, and a line spectrum cannot be obtained. This phenomena is called leakage error (as shown below).

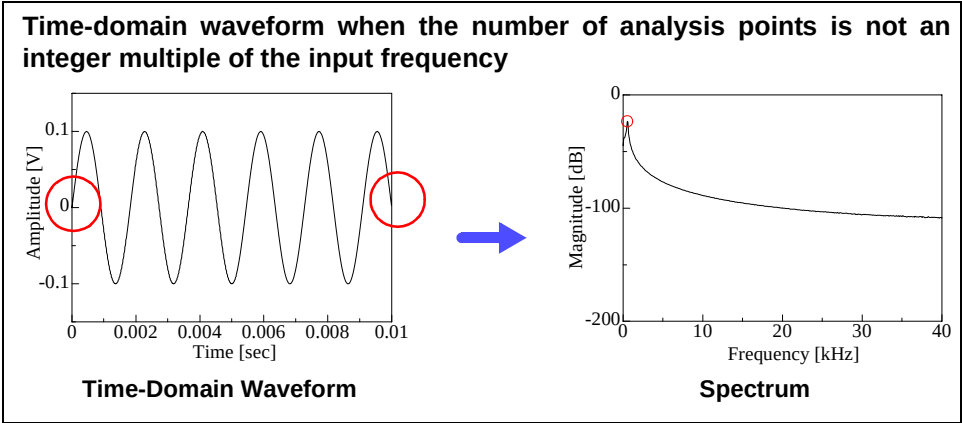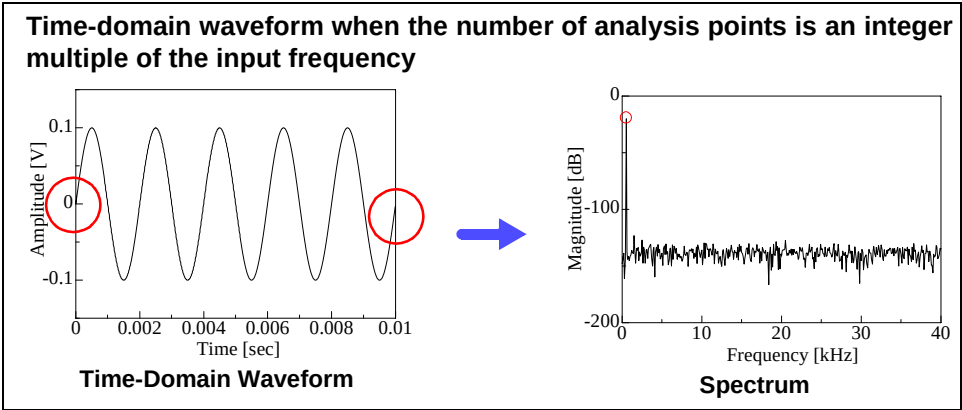


The window function was created to suppress such leakage errors. The window function smoothly connects each end of the time-domain waveform where it is cut off.

The following figure presents an example of spectral analysis by applying a window function to a time-domain waveform.

Using the window function, discontinuous points on the time-domain waveform are eliminated, so the wave shape approaches a line spectrum.

When a Blackman-Harris window function is applied to a time-domain waveform ($\Rightarrow$ p. 110) in which the number of analysis points is not an integer multiple of the input frequency

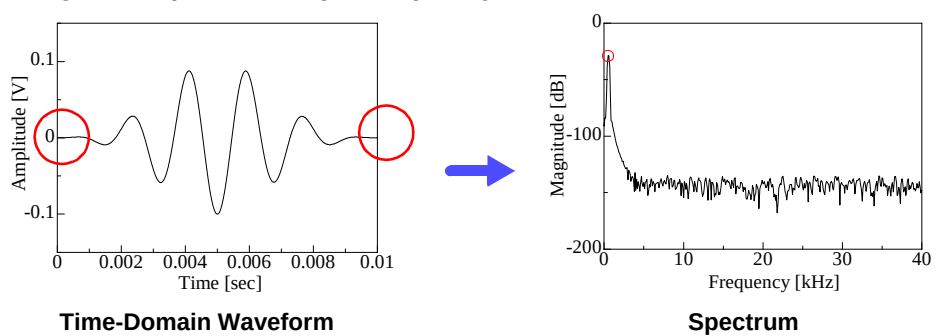

The following figure shows the time-domain waveform of the window function and its spectrum.


Each spectrum shows a large peak at a low frequency, and many smaller peaks at higher frequencies. The largest peak is called the **main lobe**, and the smaller peaks are the **side lobes**.

The most accurate results of the FFT function are obtained when the width of the main lobe and the amplitude of the side lobes are minimized, although both conditions cannot be satisfied at the same time.


Therefore, a window function having a wide main lobe is used when amplitude values are important, while a window function having a small main lobe is used to observe fine spectral details, and a window function having small side lobe amplitudes is used to exclude the effects of the surrounding spectrum.









However, because the main lobe width is proportional to the width ($1/W$) of the window, increasing the number of analysis points increases the frequency resolution.

Rectangular window

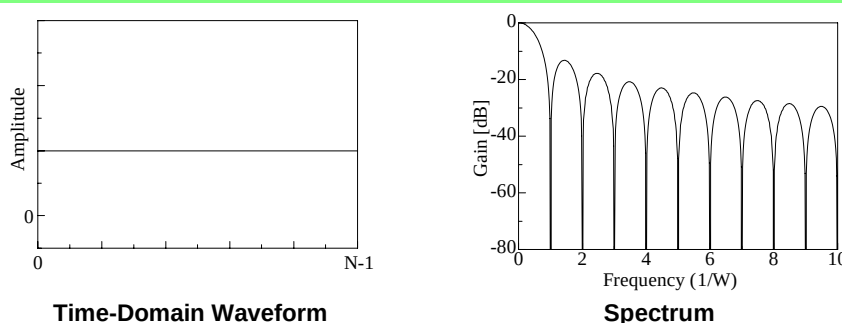


Hann window

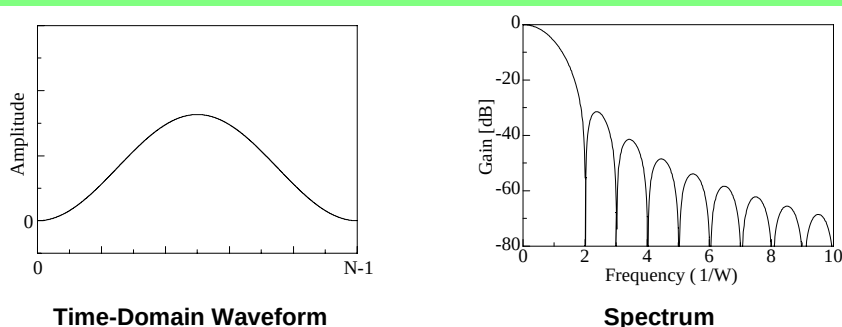


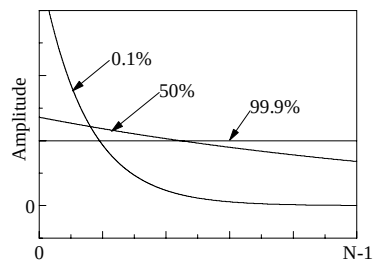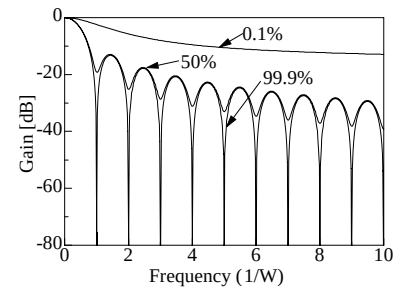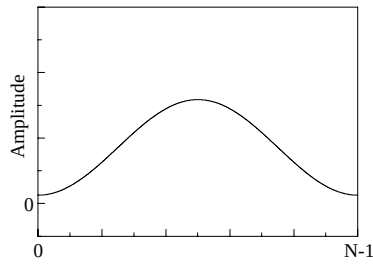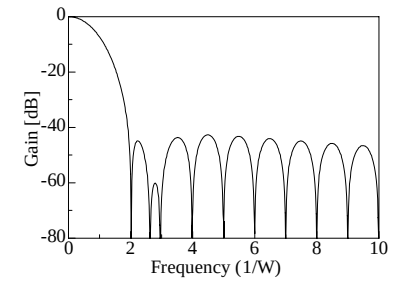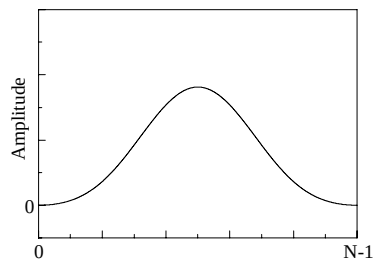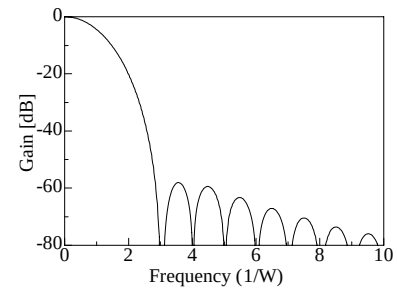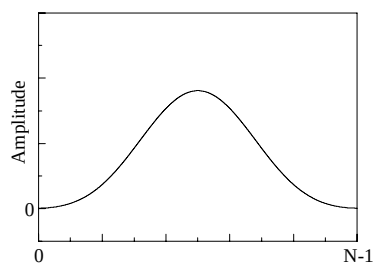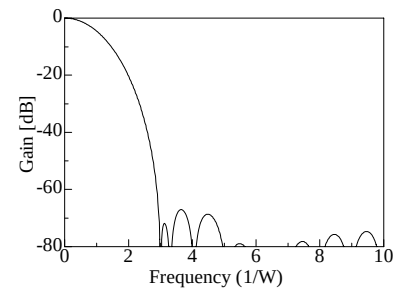Exponential window**Time-Domain Waveform****Spectrum****Hamming window****Time-Domain Waveform****Spectrum****Blackman window****Time-Domain Waveform****Spectrum****Blackman-Harris window****Time-Domain Waveform****Spectrum**

Flat top window

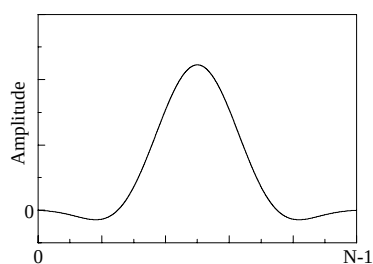


Time-Domain Waveform

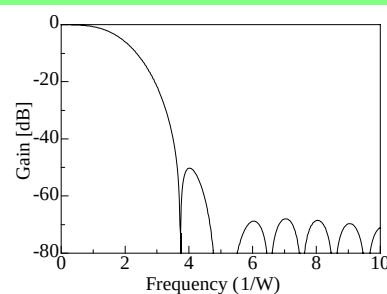


Spectrum

The following example shows input sine waves of 1050 and 1150 Hz analyzed with different window functions. Because the frequencies in this example are close to one another, a rectangular window with a narrow main lobe is able to separate and display both frequencies, but a Hann window with a wide main lobe displays the two as a single spectral component.

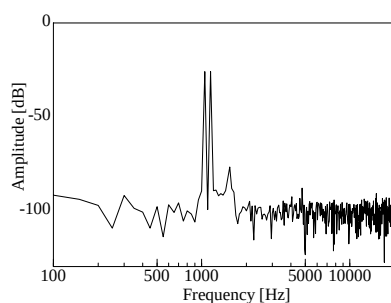

Analysis Using a Rectangular Window

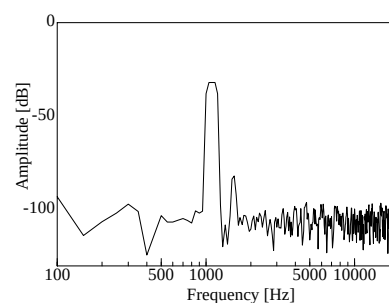


Analysis Using a Hann Window


Octave Filter Characteristics

Octave filter characteristics are determined according to IEC61260 standards. The figures below show these standards and the filter characteristics of this instrument.

1/1 Octave Filter Characteristic

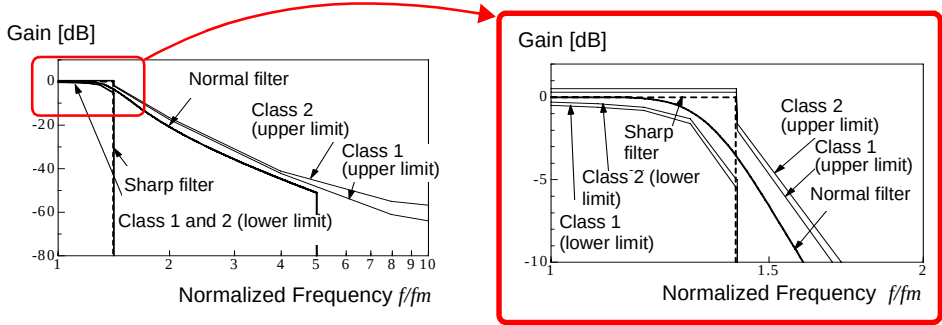


1/3 Octave Filter Characteristic

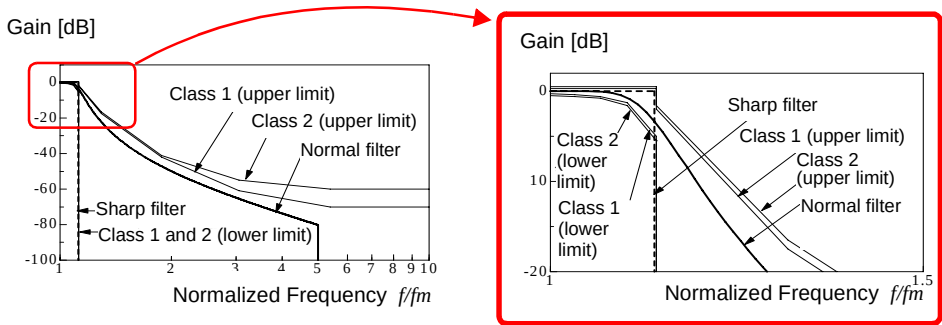

Linear Predictive Coding (LPC)

In the following figure, linear predictive coding is implemented by passing a sample of the input signal through the prediction filter while altering the filter so as to minimize errors in the original signal.

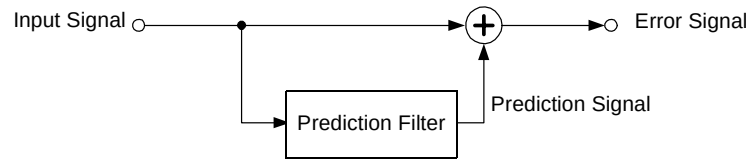

Given a time-discrete signal $\{x_t\}$ (t is an integer) where the input signal is sampled at interval ΔT , LPC analysis presumes the following relationship between current sample value x_t and the value of previous sample p .

$$x_t + \alpha_1 x_{t-1} + \alpha_2 x_{t-2} + \cdots + \alpha_p x_{t-p} = \varepsilon_t \quad (15)$$

However, $\{\varepsilon_t\}$ is an uncorrelated random variable with average value 0 and the dispersion σ^2 .

Expression (15) shows how current sample value x_t can be “linearly predicted” from previous sample values. If the predicted value of x_t is actually $\hat{x}_t$, expression (15) can be transformed as follows.

$$x_t = \hat{x}_t + \varepsilon_t = -\sum_{i=1}^p \alpha_i x_{t-i} + \varepsilon_t \quad (16)$$

Here, α_i is called the **linear predictor coefficient**.

For LPC analysis, this coefficient is calculated using the Levinson-Durbin algorithm, and a spectrum is obtained. In this instrument, the order of the coefficient can be set from 2 to 64. Larger orders reveal fine spectral components, while small orders reveal the overall spectrum shape.

Index

A

A/B cursor	80, 83
Acquisition interval	55
ACR	90
Aliasing	106
Analysis modes	59, 62, 64, 102
Analysis starting point	80
Analyze page	62
Anti-aliasing filter	37, 107
Area	7, 20
Auto correlation function	90
Average value	6, 19
Averaging	58, 109

B

Blackman	56, 112
Blackman Harris	56, 112

C

Calculation dialog	31
Calculation No.	62
CCR	98
Channel settings	69
Channel settings screen	41
One Ch page	69
COH	100
Coherence Function	100
Color	62
Comment	66
Cross Power Spectrum	97
Cross-correlation function	98
CSP	97

D

dB input	71
Display color	
Calculation waveforms	30
DISPLAY dialog	78
Display Method	78
Display sheet settings	49
Display type	72
Display types and split-screen settings	74
Duty	7, 21

E

Exponential	56, 112
Exponential averaging	58, 109
External sampling	53

F

Fall Time	7, 20
Flat-Top	56, 113
Four arithmetic Operations (4 Operations)	21
Fourier transforms	103
Frequency range	53, 54, 67
Frequency resolution	55
Function selection	46

G

Gauge	79
GAUGE&VALUE dialog	79

H

Hamming	56, 112
Hanning	56, 111
Highlight	95
Attenuation ratio	61
dB	61
HIS	90
Histogram	90, 102

I

Imaging	108
IMP	99
Impulse response	99, 104
Input channel settings	48
Input coupling	69

L

LIN	86
Linear predictive coding	115
Linear spectrum	86
Linear time-invariant systems	104
Low-pass filter	70
LPC	101, 115
LPF (low-pass filter)	70
LTI system	104

Index 2

Index

M

Maximum value	19
Measurable ranges with octave analysis	92
Measurement	
End of measurement	50
Start of measurement	50
Measurement configuration settings	47
Measurement range	48
Memory waveform	80
Minimum value	19
Mode (measurement mode)	69

N

NG	
Analysis Mode Error	73
Nyquist Display	73
X-Axis Setting	73
Number of analysis points	53, 54, 67, 105
Numerical calculations	3
Calculation expressions	19
Calculation results	9
Calculation type	6
Copying settings	10
Judging	11
Settings	6
Nyquist	64, 74

O

OCT	91
Octave analysis	91, 92
Octave filter	64, 114
Offset Cancel	70
Opening screen	51
Overall	71, 109

P

Parameter	63
Peak value display	57
Peak-to-peak value (P-P value)	6, 19
Period and Frequency	19
PHA	95
Phase spectrum	95
Highlight	61
Power spectrum	88
Power spectrum density	89, 101
Pre-trigger	48, 67
Print settings screen	44, 50
Printing	76
Printing settings	50
Probe attenuation	70
PSD	89
PSP	88
Pulse count	7, 21

Pulse width	21
-------------------	----

R

Range	
Measurement range	69
Rectangular	56, 111
Reference	52
Rise Time	7, 20
RMS	87
RMS (Root-Mean-Square) value	6, 19

S

Sampling clock	54
Save	
Example of saving numerical calculation results	16
Numerical calculation results(Auto Save)	14
Numerical calculation results(Manual Save) ..	15
Save Settings Screen	43
Saving	75
Saving settings	49
Scale page	66
Sheet settings screen	49
Simple averaging	109
Standard deviation (Std. Deviation)	7, 20
Status settings screen	40
Storage	85
STR	85

T

Time to Level	21
Time value	
Time to maximum value (Time to Max)	19
Time to minimum value (Time to Min)	19
TIME/DIV key	53
Timebase	55
Transfer Function	96
TRF	96
Trigger	45, 48
Trigger criteria	48
Trigger mode	60, 67
Trigger settings	48
Trigger Settings Screen	41

W

Waveform calculation	
Operators	34
Settings	26
Waveform Calculations	23
Waveform color	68
Waveform screen	38, 78
Setting items	39
Window	

Coefficient	56
Window function	56, 67, 110
Multiplication	56

X

X axis	63
X-Y area	20

Y

Y axis	63
--------------	----

Z

Zero adjustment	48, 70
-----------------------	--------

HIOKI 8860/8861 MEMORY HiCORDER
Analysis Supplement

Publication date: July 2006 Revised edition 1

Edited and published by HIOKI E.E. CORPORATION
Technical Support Section

All inquiries to International Sales and Marketing Department
81 Koizumi, Ueda, Nagano, 386-1192, Japan

TEL: +81-268-28-0562 / FAX: +81-268-28-0568

E-mail: os-com@hioki.co.jp

URL <http://www.hioki.co.jp/>

Printed in Japan 8860A987-01

-
-
- All reasonable care has been taken in the production of this manual, but if you find any points which are unclear or in error, please contact your supplier or the International Sales and Marketing Department at HIOKI headquarters.
 - In the interests of product development, the contents of this manual are subject to revision without prior notice.
 - Unauthorized reproduction or copying of this manual is prohibited.
-
-

HIOKI

HIOKI E. E. CORPORATION

HEAD OFFICE

81 Koizumi, Ueda, Nagano 386-1192, Japan

TEL +81-268-28-0562 / FAX +81-268-28-0568

E-mail: os-com@hioki.co.jp / URL <http://www.hioki.co.jp/>

HIOKI USA CORPORATION

6 Corporate Drive, Cranbury, NJ 08512, USA

TEL +1-609-409-9109 / FAX +1-609-409-9108

8860A987-01 06-07H



Printed on recycled paper
