




# FC S Series

## Flocculators

Independent positions to allow optimal analysis conditions  
and highly reproducible results

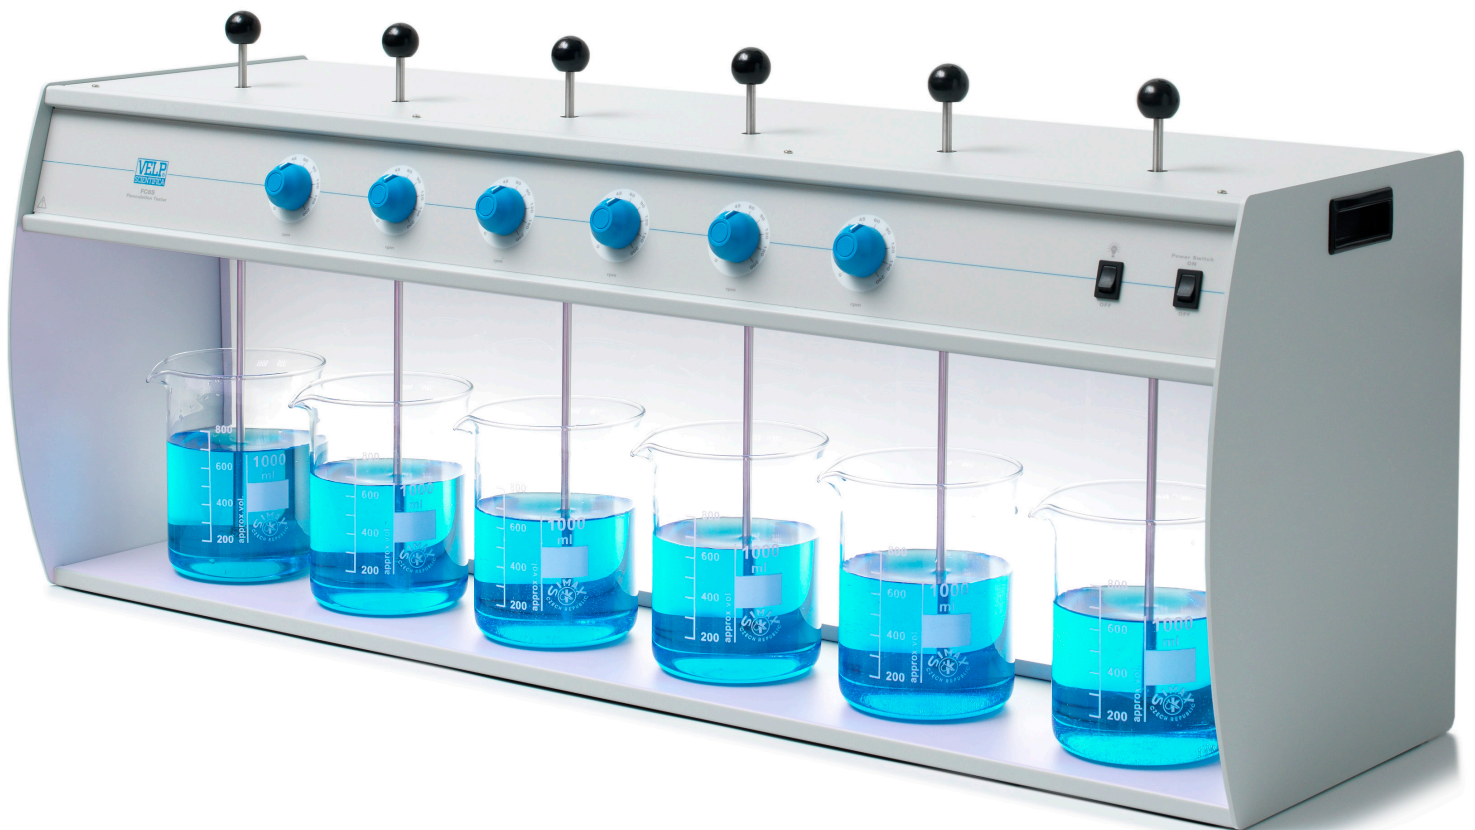

# Independent Control and Easy to use

Flocculators in 4 and 6 positions with independent stirring speed setting and illuminated back panel to allow standard conditions to be met during Jar Testing for water treatment plants.

- Independently selectable speeds 10-15-30-45-60-90-120-150-200-300 rpm
- Manage and simulate different conditions in parallel in one single instrument
- Stirring rods adjustable in height without tools
- Illuminated back panel to simplify sample observation
- Strong resistance to chemical and mechanical corrosion



## INSTRUMENT - CODE

FC4S	100-240 V / 50-60 Hz	F105A0111
FC6S	100-240 V / 50-60 Hz	F105A0112

## TECHNICAL DATA

	FC4S	FC6S
CONSTRUCTION MATERIAL	Epoxy painted metal structure	Epoxy painted metal structure
NUMBER OF SAMPLES	4 positions	6 positions
BACK PANEL	Disconnectable illuminated	Disconnectable illuminated
STAINLESS STEEL STIRRING RODS	Adjustable in height by a selflocking chuck	Adjustable in height by a selflocking chuck
PLURISELECTOR	Settable individual speed for each rod	Settable individual speed for each rod
ELECTRONIC SPEED CONTROL	10 - 15 - 30 - 45 - 60 - 90 -120 - 150 - 200 - 300 rpm	10 - 15 - 30 - 45 - 60 - 90 -120 - 150 - 200 - 300 rpm
POWER	18 W	23 W
DIMENSIONS (WXHXD)	645x347x260 mm (25.4x13.7x10.2 in)	935x347x260 mm (36.8x13.7x10.2 in)
WEIGHT	12.5 kg (27.5 lb)	18 kg (39.6 lb)



We reserve the right to make technical alterations  
We do not assume liability for errors in printing, typing or transmission

VELP Official Partner

## DESIGNED AND MANUFACTURED IN ITALY



**ITALY - HQ**  
Via Stazione 16  
20865 Usmate (MB) Italy  
Tel. +39 039 628811  
velpitalia@velp.com

**INDIA**  
velpindia@velp.com

**USA**  
155 Keyland Court, Bohemia  
NY 11716 - U.S.  
Tel. +1 631 573 6002  
velpusa@velp.com

**CHINA**  
Xinlong Rd Building 28, Lane 1333  
Shanghai city - China  
Tel. +86 18017557329  
velpchina@velp.com