

Supplement

| | | | |
|----------------|-------------|-------------------|----------|
| Title: | 365 Users | Supplement Issue: | 8 |
| Part Number: | 3622684 | Issue Date: | 7/16 |
| Print Date: | August 2010 | Page Count: | 6 |
| Revision/Date: | | | |

This supplement contains information necessary to ensure the accuracy of the above Users Manual.

Change #1, #2, 520

On page 3, under **Warning** add:

- **When the white wear indicator insulation shows through the clamp cable jacket, replace the clamp cable .**
- **When batteries are changed, ensure that the calibration seal in the battery compartment is not damaged. If damaged, the Meter may not be safe to use. Return the Meter to Fluke for replacement of the seal.**
- **Use Product-approved measurement category (CAT), voltage, and amperage rated accessories (probes, test leads, and adapters) for all measurements.**
- **Do not exceed the Measurement Category (CAT) rating of the lowest rated individual component of a Product, probe, or accessory.**
- **Do not use a current measurement as an indication that a circuit is safe to touch. A voltage measurement is necessary to know if a circuit is hazardous.**

- **Do not use the Product above its rated frequency.**
- **Do not use in CAT III or CAT IV environments without the protective cap installed on test probe. The protective cap decreases the exposed probe metal to <4 mm. This decreases the possibility of arc flash from short circuits.**




Change #3

On page 4, add:

- **Measure a known voltage to verify product operation.**

Change #4, 64918, 486, 105, 524, 316

On page 5, add the following to the **Symbols** table:

| | |
|---|--|
|  | Conforms to relevant South Korean EMC Standards. |
| CAT II | Measurement Category II is applicable to test and measuring circuits connected directly to utilization points (socket outlets and similar points) of the low-voltage MAINS installation. |
| CAT IV | Measurement Category IV is applicable to test and measuring circuits connected at the source of the building's low-voltage MAINS installation. |
|  | Conforms to relevant Australian Safety and EMC standards. |
|  | Consult user documentation. |

On page 17, delete **Safety Compliance** and **Agency Approvals** and replace with:

Safety IEC 61010-1 Pollution Degree 2, IEC 61010-2-033
IEC 61010-2-032, CAT III 600 V,

Electromagnetic Compatibility (EMC)

International..... IEC 61326-1: Portable Electromagnetic
Environment

CISPR 11: Group 1, Class A

Group 1: Equipment has intentionally generated and/or uses conductively-coupled radio frequency energy that is necessary for the internal function of the equipment itself.

Class A: Equipment is suitable for use in all establishments other than domestic and those directly connected to a low-voltage power supply network that supplies buildings used for domestic purposes. There may be potential difficulties in ensuring electromagnetic compatibility in other environments due to conducted and radiated disturbances.

Caution: This equipment is not intended for use in residential environments and may not provide adequate protection to radio reception in such environments.

Emissions that exceed the levels required by CISPR 11 can occur when the equipment is connected to a test object.

Korea (KCC) Class A Equipment (Industrial Broadcasting & Communication Equipment)

Class A: Equipment meets requirements for industrial electromagnetic wave equipment and the seller or user should take notice of it. This equipment is intended for use in business environments and not to be used in homes.

USA (FCC) 47 CFR 15 subpart B. This product is considered an exempt device per clause 15.103.

Change #5, 105, 524, 316

On page 6, replace CAT III with the following and remove the TUV:

| | |
|----------------|--|
| CAT III | Measurement Category III is applicable to test and measuring circuits connected to the distribution part of the building's low-voltage MAINS installation. |
|----------------|--|

Change #6, 524

On page 1, under "The Meter ships with", replace the first bullet with:

- Test leads

On page 7, replace the Figure with:

The Meter

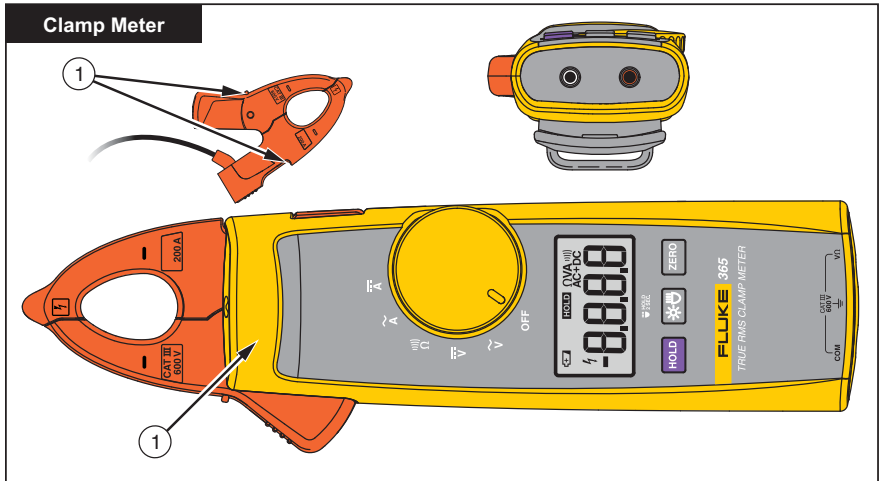


fig01.eps