

User Manual

PCE-TTC 30 Thermocouple Calibrator



User manuals in various languages (français, taliano, español, português, nederlands, türk, polski, русский, 中文) can be found by using our

product search on: www.pce-instruments.com

Last change: 10 August 2018 v1.0

© PCE Instruments



1 2 2.1 2.2 2.3 2.4 3 Start Up and Basic Operations9 3.1 3.2 4 4.1 4.2 4.3 4.4 4.5 4.6 4.7 5 Maintenance and Troubleshooting41 5.1 Common Problems41 Replacing the Battery41 5.2 6 Technical Specifications 42 7 8

1 Safety notes

Please read this manual carefully and completely before you use the device for the first time. The device may only be used by qualified personnel and repaired by PCE Instruments personnel. Damage or injuries caused by non-observance of the manual are excluded from our liability and not covered by our warranty.

• The device must only be used as described in this instruction manual. If used otherwise, this can cause dangerous situations for the user and damage to the meter.

PCE

- The instrument may only be used if the environmental conditions (temperature, relative humidity, ...) are within the ranges stated in the technical specifications. Do not expose the device to extreme temperatures, direct sunlight, extreme humidity or moisture.
- Do not expose the device to shocks or strong vibrations.
- The case should only be opened by qualified PCE Instruments personnel.
- Never use the instrument when your hands are wet.
- You must not make any technical changes to the device.
- The appliance should only be cleaned with a damp cloth. Use only pH-neutral cleaner, no abrasives or solvents.
- The device must only be used with accessories from PCE Instruments or equivalent.
- Before each use, inspect the case for visible damage. If any damage is visible, do not use the device.
- Do not use the instrument in explosive atmospheres.
- The measurement range as stated in the specifications must not be exceeded under any circumstances.
- To prevent electrical shocks or damage to the instrument, do not connect more than 30 V between the terminals, or between the terminals and the ground.
- This instrument uses a Lithium-Ion battery pack. To prevent an explosion or fire, do not short circuit, do not disassemble and keep it safe from damage.
- To prevent battery leakage or heat generation, only use the battery charger in the temperature range 0 ... 45 °C (32 ... 113 °F).
- To make sure the display shows the correct data, disconnect the test leads before you set the power to on or change to another measure or source function.
- To prevent damage to the display, do not use sharp objects on the screen.
- Only sufficiently skilled persons may use the meter. Qualifications from an approved training establishment may be necessary.
- Follow good engineering practice at all times.
- Non-observance of the safety notes can cause damage to the device and injuries to the user.

We do not assume liability for printing errors or any other mistakes in this manual.

We expressly point to our general guarantee terms which can be found in our general terms of business.

If you have any questions please contact PCE Instruments. The contact details can be found at the end of this manual.



2 PCE-TTC 30 Hardware Parts and Accessories

2.1 Unpacking and Inspection

At the factory each new PCE-TTC 30 passes a careful inspection. It should be free of scrapes and scratches and in proper operation order upon receipt. The receiver should, however, inspect the unit for any damage that may have occurred during transit. If there are signs of obvious mechanical damage, package contents are incomplete, or the instrument does not operate according to specifications, contact the purchasing sales office as soon as possible.

Delivery contents:

- 1 x Temperature sensor PCE-TTC 30 2 x Laboratory cables with 2 mm plug 1 x Thermocouple adapter to 2 mm plug 2 x Adapter 2 mm on 4 mm laboratory cable 2 x Alligator clips 1 x Mini USB cable
- 1 x Power supply 5 V / 1 A
- 1 x Carrying bag
- 1 x User manual

The software can be downloaded here: <u>https://www.pce-instruments.com/english/download-win_4.htm</u>

If you have to return the instrument to the factory for any reason, use the original packing whenever possible. Include a detailed description of the reason for the return.



2.2 Operational Sections and Connections

All sections and connections are presented in detail on the next pages.

Note: Keep in mind that the next picture (as well as all pictures of the PCE-TTC 30 in this manual) has an example configuration of modules. The configuration of your PCE-TTC 30 may vary significantly from the one in the picture.




- 1 Terminal Connection for TC Measure and Source
- and EM Measure
- 2 Keypad Section
- 3 Color Display
- 4 USB Connection Slot for PC Communication and
- Charging





2.2.1 Terminal Connections



EM Measure Terminals

Input Terminal for measuring voltage, current and supplying loop power.

EM Measure Terminals		
mA	Range: 0.000 24.000 mA Resolution: 0.001 mA	
mA(24V)	Range: 0.000 24.000 mA Resolution: 0.001 mA	
v	Range: 0.000 30.000 V Resolution: 0.001 V	


Current Measurement

The PCE-TTC 30 supports current measurement using either PCE-TTC 30 as the loop power supply while at the same time measuring the current or simply measuring the current while an external power supply is used.

The following picture displays the connection for Current Measurement for different mode. And also different ways of providing the supply power to the loop.

mA Current Measurement


In this mode, the PCE-TTC 30 does not provide any supply voltage. For proper measurement the external device should capable of providing the voltage supply. If the external device should not capable, an external Power Supply should be connected in series.





mA Read Power Current Measurement


In this mode, the PCE-TTC 30 works as Loop Power Supply while at the same time measuring the current.



Voltage Measurement

The PCE-TTC 30 is capable of voltage Measurement with two voltage measurement ranges.

The following picture displays the connection for Voltage Measurement for different mode.




TC Terminals

Terminal for measuring and simulating thermocouples and mV. This terminal accepts a miniature polarized thermocouple plug with flat, inline blades spaced 7.9 mm (0.312 in) center to center.

	TC Terminal (Measure and Source)				
ТС Туре	Range	Display Resolution	Accuracy		
E	-200.0 1000.0 °C	0.1 °C	± 0.3 °C		
J	-200.0 1200.0 °C	0.1 °C	± 0.3 °C		
К	-200.0 1372.0 °C	0.1 °C	± 0.3 °C		
Т	-200.0 400.0 °C	0.1 °C	± 0.3 °C		
В	450.0 1800.0 °C	0.1 °C	± 0.5 °C		
R	0.0 1750.0 °C	0.1 °C	± 0.5 °C		
S	0 1750.0 °C	0.1 °C	± 0.5 °C		
N	-200.0 1300.0 °C	0.1 °C	± 0.3 °C		
	-10 80 mV	0.001 mV	<u>+</u> 0.02 % of reading <u>+</u> 2µV		
mV	-10 250 mV	0.01mV	<u>+</u> 0.02 % of reading <u>+</u> 0.02mV		

The PCE-TTC 30 supports measurement and simulation of Thermocouple and mV.



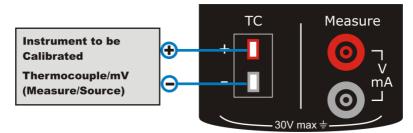

2.2.2 KeyPad



The PCE-TTC 30 has six different keys. The key description is given below.

F1	This key has different functionalities in different menus. These are shown in the bottom left part of the display.
F2	This key has different functionalities in different menus. These are shown in the bottom left part of the display.
	 Scroll down to next parameter Decrease value of digit in Editbox
	 Scroll down to previous parameter Increase value of digit in Editbox
	 Enter menu when in Run mode Save edited parameter to memory
LOG	 Log current reading in memory if device is in Run mode and log mode is manual When not in Run mode, this key is used to enter Run mode Press and hold (approx. 2 s) to turn meter on/off



2.2.3 Display



- LCD with a 2.4" color display
- Resolution of 240x320 pixels
- Supporting 262K colors

2.2.4 USB Connection

- The USB connection is located at the top of the PCE-TTC 30. It is a USB mini B-Type female connector.
- It can be used for PC communication and for charging the device.
- The USB cable supplied with the device is USB A-type male to USB B-type male. It is used for connecting charger and PC.

2.2.5 Stand for Table Top Use

- This stand offers the best support for table top use which gives good viewing angle when the PCE-LOC 20 is placed on a table.
- Procedure to open stand:




is being engraved on the top of the stand. You should pull a bit first.

2

a is being engraved on the bottom of the stand. Now during first pull of above you release this lower part easily so that you

can can

maneuver the stand as you like.





2.3 Power Options

There are three power options:

- Lithium-Ion battery: All the instrument functions are available with a charged battery.
- 5 V DC charging adaptor: It supplies power to the instrument and charges the battery at the same time. It charges the battery when the instrument is on or off.
- USB mini Type B connection: This charges the battery when the instrument is off and increases the battery life when the instrument is on.

2.4 Battery

The Device uses 2300mAh Lithium-Ion Battery. When you set the power on, the battery symbol at the top of the display shows the charge status. To get more information on Battery go to Battery Info Page in Setting Menu.

2.4.1 Charging time

Charging method	Charging time (to full capacity)
External Charging Adaptor	≈ 5 hours

Note:

USB mini Type B connector charges the battery when the instrument is off and increases the battery life when the instrument is on.

2.4.2 Operating Time

Operation	Battery Duration
Continuous operation (measure or source)	>18 hours
Continuous operation (12mA (24V) measure)	> 8 hours

These are typical operating times for a new, fully charged Li-Ion battery pack with these settings:

- Backlight Intensity set to 5% (Default: 100%)
- Backlight Timeout set to 0 (0=Infinite) (Default: 0)

Power save options: To get the best battery duration, set a low value for the *Backlight Intensity* (40%) and a short *Timeout*.

The maximum operating time without recharging varies depending on the usage and brightness setting of the display light. Also the generated output and the usage of the 24 V transmitter supply affect the maximum operating time.



Notes:

- The PCE-TTC 30's memory and the internal clock/calendar use a small amount of power although the calibrator is switched off. Remember to check the capacity of the batteries from time to time although the PCE-TTC 30 is not in use.
- Do not leave the PCE-TTC 30 without a Battery Pack or an Empty Battery for a long time. The PCE-TTC 30 may lose its settings if it is left without a support voltage for an extended period.

3 Start Up and Basic Operations

3.1 Power On or Off

To set the instrument power ON, press and release this button down until the display comes on. During the power on sequence, the instrument shows a Startup Message and then shows the applicable data.

To set the instrument power off, press and hold (\approx 2 seconds) this button again. When the power is off, the last set of configuration options stays in memory.

3.2 User Interface

Every time the PCE-TTC 30 is switched on, the startup message ends in RUN Page. 3 display modes are available in RUN Page.

- 1. TC Measure/Source Mode
- 2. EM Measure Mode
- 3. TC Measure/Source + EM Measure Mode

This Display Mode can be selected from MENU→DISPLAY Page.

In case of Dual Mode Display Screen is divided into two parts. Due to that only few additional info will appear on RUN Page. The information to be shown can be selectable in Display Mode Menu.

3.2.1 The Status Bar



The status bar at the top of the display is visible only in RUN Page. It is divided into five main sections.

1	Time in HH:MM:SS f	ormat			
	Available in two formats				
	1. 24 hour (default)				
	2. 12 hour				
	This setting is available	ble in Date/Time in Settings Men			
2	Error Code Indicator				
	This ison is visible if	any on board parinharela like DTC ADC DAC ate are not working			
		any on-board peripherals like RTC, ADC, DAC, etc. are not working 5 Maintenance and Troubleshooting.			
	property, see chapter	o Maintenance and Troubleshooting.			
	The List of error code	es available in this device is given below.			
		,			
	Error code	Description			
	0	Memory corrupted or device unable to read/write it			
	1	RTC not working properly			
	2	Device unable to read battery information			
	3	Measure mode not working			
	4	Device unable to get source feedback reading			
	5	Data log memory corrupt			
	6	Source mode not working			
	9 More than one error from above list is occurring				
3	3 USB Connection Status Icon				
Ŭ					
	Icon is visible if USB charging adaptor or USB data cable is connected to the device. Icon				
	is different for both in	dications, see below.			
		data cable is connected and communication with PC			
		ailable			
	USB charging adaptor is connected.				
	Batt	ery starts charging.			
4	Battery Charge Percentage Indicator				
	Always visible in Run page; battery % is shown in the centre of the icon and the icon				
	background is filled v	vith green, yellow or red color if battery % is >= 50%, >= 20 and <20			
	respectively.				
5	Data Logging Enable	Status Indicator			
	Less la challet d'altre	la présente provide de la destructura d			
		logging is enabled and will flash when a data log is stored to the			
	memory				




3.2.2 Function Key Bar



The function key bar at the bottom of the display is visible all the time. 2 function keys are available. The meaning of the function keys varies depending on the situation. A blank function key text means that the function is disabled at the moment.

3.2.3 Display Mode

1. TC Mode

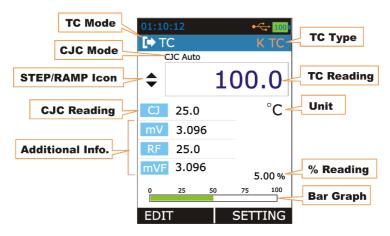



TC Display Mode					
TC Mode	Shows the Current Thermocouple Mode				
	I	TC Measure Mode	е		
	[→	TC Source Mode			
ТСТуре	Shows the curren	t Thermocouple/mV	Туре.		
CJC Mode	Shows the CJC Mode				
	CJC Auto	CJC Auto Mode			
	CJC Manual	CJC Manual Mod	е		
TC Reading	Shows the Thermocouple/mV Measure/Source reading according to display mode and TC Type			cording to display	
Unit	Shows the Unit of the TC Reading, CJC				
	°C			d TC Unit is <i>Celsius</i> .	
	°F	Shows If TC Display mode is <i>Actual</i> and TC Unit is <i>Fahrenheit</i> .			
	К	Shows If TC Displa	Shows If TC Display mode is Actual and TC Unit is Kelvin.		
	mV	Shows If TC Display mode is <i>Actual.</i> And TC Type is -10 80 or -10 250mV.			
	%	Shows If TC Display mode is <i>Percentage</i> .			
STEP/RAM P lcon	Shows the Icon in SOURCE.	Shows the Icon indicating STEP/RAMP mode. Only applicable if TC mode is			
		Manual Step	5	Rising Ramp	
	_	Step UP	$\mathbf{\lambda}$	Falling Ramp	
	\mathcal{L}	Step DOWN		Ramp Hold @ 0%	
			\frown	Ramp Hold @ 100%	
CJC Reading	and shows the us	erature of the Cold Ju er entered CJC Tem is same as TC Unit.		is selected as <i>AUTO</i> C mode is <i>MANUAL</i> .	
Additional Info		on Information accord lected in $MENU \rightarrow D$			

Bar Graph	Horizontal Bar graph according to TC Percentage Value $(0.00\%)^{\frac{1}{2}}$ 100.00%). The value scales according to TC reading and Input 0% and 100% value as set in <i>MENU</i> \rightarrow <i>DISPLAY</i> \rightarrow <i>TC terminal</i> Menu.
Percentage Value	The Percentage Value in according to TC Reading.

2. EM Measure Mode

	01:10:12	100	
EM Measure Window 🛌	E EM	mA(24V)-	Input Type
HART Icon		Scaled	EM Display Mode
Measure Reading	12	2.000	
Bar Graph	0 25 5	0 75 100	
		50.00%	Percentage Value
Tare	T 0.000	A 12.000	Actual Value
Min	_ ↓ 5.000	↑ 16.000	Мах
Max-Min	_	X 12.000	Cumulative
	RESET		Average

Measure Window				
Input Type	The Input Type.			
	mA mA Current Input			
	mA(24V)	mA Current (Read Power-24V) Input		
	V	V Voltage Input		
EM Display Mode	The Measure Reading Display Mode			
	Actual	Displays the Raw Input Value without any scaling		
	Percentage	Displays the Percentage Value		
	Scaled	Displays the Scaled Value		



The Reading as per the Measure Display Mode
HART Enable Status Icon
This icon will appear if HART is enabled from $MENU \rightarrow SETTING \rightarrow HART$ page. (This icon is visible for mA (24V) Input Type only. For other Input Types this will invisible regardless of HART settings)
Horizontal Bar graph according to Input Percentage Value (0.00% 100.00%).
The Percentage Value in Percentage according to Input Value.
The Tare Value Set from $MENU \rightarrow DISPLAY \rightarrow EM$ Terminal Tare page
The Raw Input Value without any scaling
This will appear only if Main Display in $MENU \rightarrow DISPLAY \rightarrow EM$ Terminal is set to PERCENTAGE/SCALED .
Displays the minimum value found after a measurement was started or minimum was reset.
Displays the maximum value found after a measurement was started or maximum was reset.
Displays the Maximum-Minimum value found after a measurement was started or Maximum-Minimum was reset.
Displays the Cumulative Average value found after a measurement was started or Cumulative Average was reset.

3. TC + EM Mode

CJC Reading CJ 25 Additional Info. mVF 3.0 HART Icon % EM Display Mode EDIT	10 SE	°C Unit (24V) EM Input Type .00 EM Reading ETTING	
	TC + EN	/ Mode	
TC Mode TC Type CJC Mode TC Reading STEP/RAMP Icon CJC Reading Additional Info. Unit	Refer to TC	Display Mode on previous pages.	
EM Input Type EM Reading HART Icon	Refer to EM	I Display Mode on previous pages.	
EM Display Mode	The Measure Reading Display Mode		
	"" (Blank) % S	Displays the Raw Input Value without any scaling Displays the Percentage Value Displays the Scaled Value	



3.2.4 Display Operations

Mainly, four types of widgets are available in the Device Menu.

- i. ListBox
- ii. EditBox
- iii. CheckBox
- iv. RadioButtonBox


The below section will show how to change the value of different widgets.

i. ListBox

ListBox are used when there is a limited amount of preset values. You have to select one of the available options. The list of available options is displayed in the centre part.

A ListBox list opens when you press the **F1** key. Use the **UP/DOWN** key to scroll through the available options. Select one of the options with the **ENTER** key.

Example: How to change of Input Type (I/P Type) from mA to V. This option is available in $MENU \rightarrow EM SETUP$ Page.

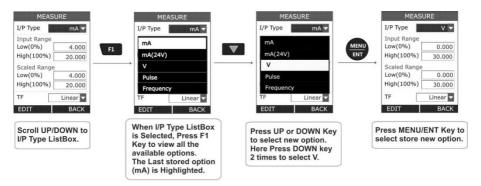




ii. EditBox

EditBox is used where a large range of values is possible for a parameter.


To edit the value of an EditBox, press F1 key. After that EditBox enters Edit mode where F1 and F2 keys work as shifter. User can shift to desired digit and using UP or DOWN key digit value can be incremented or decremented. The modified value can be saved using MENU/ENT key.

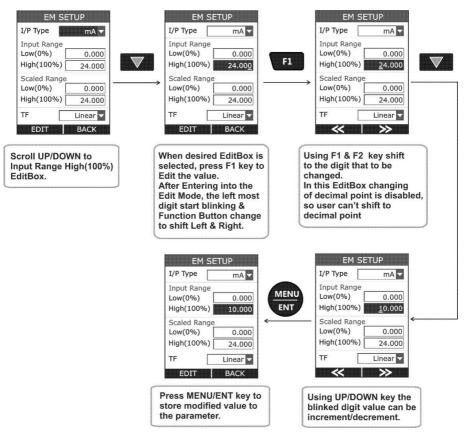

The above figure shows the example how to change Input High (100%) Range from 24.000 to 10.000 mA.

There are mainly 2 types of EditBox in this device. In most of the EditBox changing of decimal point & changing of sign is not allowed. But there are few EditBox, where these are allowed. Examples Scaled Low (0%) & High (100%) etc.

The below figure shown the example how to change decimal point of the Input Scaled High (100%) Range.

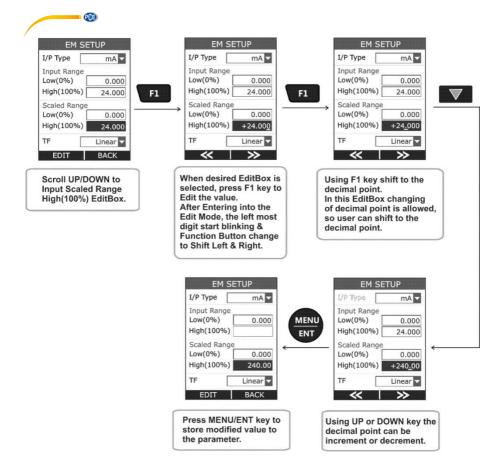

To change the sign of the value, shift to the sign digit and pressing UP or DOWN key will toggle the sign.



iii. CheckBox

CheckBox is used where Binary Value (1/0, True/False) is available for any parameter.

To change the CheckBox status, press **F1** key. This will enter edit mode. In this mode, status can be toggled by pressing **F1** key. Press **MENU/ENT** key to store new status.

STEP	STEP	STEP	STEP
Low(%) -200.0	Low(%) -200.0	Low(%) -200.0	Low(%) -200.0
High(%) 1372.0	High(%) 1372.0	High(%) 1372.0 MEN	U High(%) 1372.0
Manual	Manual	Manual 🗹 EN	Manual 🗹
Step Time(s) 10	Step Time(s) 10	Step Time(s) 10	Step Time(s) 10
Step Defination	Step Defination	Step Defination	Step Defination
Step Value	Step Value	Step Value	Step Value 🔽
Step(°C) 20.0	Step(°C) 20.0	Step(°C) 20.0	Step(°C) 20.0
EDIT BACK	СНЕСК ВАСК	UNCHECK BACK	EDIT BACK
Scroll UP/DOWN to Step Manual CheckBox.	When desired CheckBox is selected, press F1 key to enter into Edit mode.	Press F1 key to change CheckBox status.	Press MENU/ENT key to store new CheckBox status.
	After Entering into the Edit Mode, F1 Function Button change to CHECK/UNCHECK according to current status		sidus.

iv. RadioButtonBox

Radio Button Box is used where very few values can be possible and all the available values need to be visible.

In this device, two types of Radio Button Box are available. One with 1 value can be selectable & the other where 1 or 2 values can be selectable at a time.

In Radio Button Box the other option can be selected by pressing **MENU/ENT** key on that option. When pressing this key the new option will be selected and the other option will be disabled. Below an example is given, How to change TC Source Mode from STEP to RAMP.

TC SETUP		TC SE	TUP
TC Mode MEASURE		TC Mode MEASURE	-
hereal	MEN	U	
SOURCE	ENT	SOURCE	
TC Select		TC Select	
Unit Celsius	-	Unit	Celsius 🔻
Source Mode		Source Mode	
STEP 🔳		STEP	
RAMP		RAMP	
EDIT BAC	ĸ	EDIT	BACK
Scroll UP/DOWN to Desired RadioButton option.	Box	Press MENU to select the Now the new selected and	option. option is
		option will b	e disabled.




4 Menu Layout

4.1 MENU page

There are mainly six Menus in this device.

To enter into the MENU page press **MENU/ENT** key and press **F2** key to come out from Menu page.

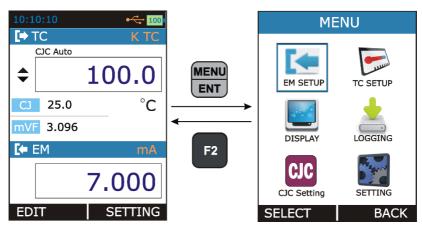


EM SETUP	Contains Parameters related to EM Measure Mode like Input Type, Range etc.
TC SETUP	Contains Parameters related to Thermocouple like TC Mode, TC Type etc.
DISPLAY	Contains Parameters related to different display mode for RUN page
LOGGING	Contains Parameters related to Data Logging.
CJC Setting	Contains Parameters related to Alarm & Alarm Set-Points.
SETTINGS	Contains Parameters related to General Settings of the device like display, Date/Time, Calibration, Reset, etc.



4.2 MEASURE Page

This page appears when you select $RUN \rightarrow MENU \rightarrow EM SETUP$.

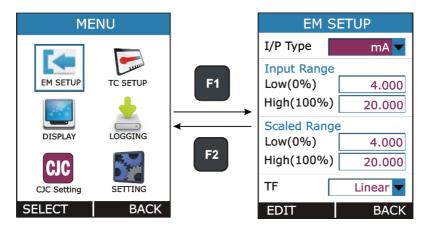

This page contains parameters related to EM Measure like Input Type, Input Range, Scaling and Transfer Function. The Description of the Parameters appear on this page is given below.


Parameter Name	Description / Options
I/P Type (Input Type)	Measure Input Type <u>Available Options</u> : mA: 0.000 24.000 mA DC mA (24 V): 0.000 24.000 mA DC V: 0.000 30.000 V DC
Input Range Low (0%)	Low Range for Measure Input Range: Default Input Low to Input Range High (100%) This parameter is enabled, if Main Display in MENU → DISPLAY → EM SETUP is set to Percentage or Scaled.
Input Range High (100%)	 High Range for Measure Input <u>Range:</u> Input Range Low (0%)to Default Input High This parameter is enabled, if Main Display in <i>MENU → DISPLAY → EM</i> <i>SETUP</i> is set to Percentage or Scaled

Scaled Input	Scaling Low Range for Measure Input
Range Low (0%)	Range: -99999 to Scaled Input Range High (100%)
	Decimal Point for this Edit Box is changeable
	This parameter is enabled, if Main Display in <i>MENU</i> → <i>DISPLAY</i> → <i>EM SETUP</i> is set to Scaled
Scaled Input	Scaling High Range for Measure Input
Range High (100%)	Range: Scaled Input Range Low (0%) to 99999
	Decimal Point for this EditBox is changeable.
	This parameter is enabled, if Main Display in $MENU \rightarrow DISPLAY \rightarrow EM$ SETUP is set to Scaled.
TF (Transfer	Transfer Function for Scaling
Function)	<u>Available Options:</u> Linear
	x^2 (x²) x^(1/2) (√x)
	This parameter is enabled, if Main Display in MENU \rightarrow DISPLAY \rightarrow EM SETUP is set to Scaled .



4.3 SOURCE Page

This page appears when you select $RUN \rightarrow MENU \rightarrow TC SETUP$.

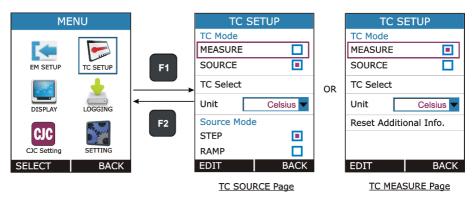


This page contains parameters related to Thermocouple like TC Mode Type, TC Type, Unit, TC Source Mode etc. The Description of the Parameters appear on this page is given below.

Parameter Name	Description / Options		
TC Mode	Thermocouple Mode		
	Available Options: MEASURE SOURCE		
TC Select	Select the Thermocoup Simulation	ble/mV Type for Measurement /	
	Available Options:		
	ТС Туре	Range	
	E TC	-200.0 1000.0 °C	
	J TC	-200.0 1200.0 °C	
	КТС	-200.0 1372.0 °C	
	T TC	-200.0 400.0 °C	
	B TC	450.0 … 1800.0 °C	
	R TC 0.0 , 1750.0 °C		
	S TC	0.0 1750.0 °C	
	N TC	-200.0 1300.0 °C	
	-10 to 80 mV	-10.000 80.000 mV	
	-10 to 250 mV	-10.00 250.00 mV	
TC Unit Unit	Measure/Source Reading Unit		
	<u>Available Options:</u> Celsius Fahrenheit Kelvin		


Source Mode	TC Source Output Format This option appears only if TC Mode is SOURCE
	<u>Available Options:</u> STEP RAMP
	At a time one can be selected. Press F1 key on one of the options for more settings.
Reset Additional Info	Reset the Additional Information of Measure mode like Minimum and Maximum This option appear only if TC Mode is <i>MEASURE</i> .

4.3.1 STEP Page

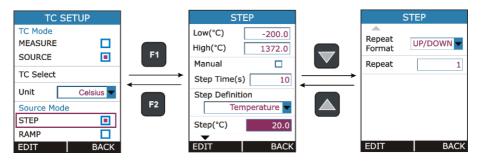

Parameter Name	Description / Options
Low	Starting Value of Step Enter value according to TC Display Mode. If display mode is actual, enter value in temperature/mV and if display mode is %, enter value in %.
High	Ending Value of Step Enter value according to TC Display Mode. If display mode is actual, enter value in temperature/mV and if display mode is %, enter value in %.
Manual (Output Type)	Step Manual Mode Selection CheckBox
	Ticking this checkbox will enable Step Manual Mode and Un-ticking will enable Auto Step Mode.

Step Time (s)	Enter the time for a single step in seconds
	Range: 1 9999
	This parameter is enabled only for Auto Step Mode (Manual CheckBox is Un-Checked)
Step Definition	Step Definition for the Step function
	Available Options: Temperature (Appear only if TC Display mode is Actual) Percentage (Appear only if TC Display mode is Percentage) User Defined
Step	Step Value in Temperature/mV/% according to TC Display Mode and TC unit Only appears if Step Definition is Temperature or Percentage.
Define Steps	User Defined Step value for Manual and Auto Step Mode. This option appears only if Step Definition is User Defined. Maximum 10 step value can be configured. First enter the no. of step and then define step value in serial order.
Repeat Format	How the stepping should be done.
	Available Options: UP DOWN UP/DOWN DOWN/UP
	This parameter is enabled only for Auto Step Mode (Manual CheckBox is Un-Checked)
Repeat Repeat Counts	Defines how many times the steps are repeated
	Range: 1 9999
	This parameter is enabled only for Auto Step Mode (Manual CheckBox is Un-Checked)

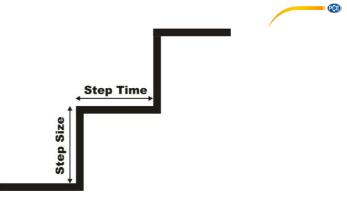

Manual Stepping

To Enable Manual Stepping, select Source Type as STEP and Check the Manual CheckBox.

If this mode is enabled, **V** icon will appear in Source Display Window in RUN Page.

Pressing UP or DOWN key in RUN Page will Increment or Decrement Source Value by Step specified in STEP Page.

In RUN Page, Source Value can directly change by Pressing F1 key (EDIT) and modifying value like in EditBox. And STEP Setting can be accessed directly by F2 key (SETTING).

Auto Stepping

To Enable Auto Stepping, select Source Type as STEP & UnCheck the Manual Check Box.

If this mode is enabled, I (Step UP) or (Step Down) icon will appear in Source Display Window in RUN Page and F1 & F2 Button change to START and SETTING respectively.

Automated Step can be started by Pressing F1 key (START). After that F1 and F2 key will change to PAUSE&STOP respectively. So by pressing F1 & F2 key running STEP can be PAUSE or STOP at any time in RUN Page.

STEP Setting can be accessed directly by F2 key (SETTING).

NOTE: While STEP is running STEP settings can't be accessible and Source Page Parameter settings can't be change. Stop STEP before changing any settings.




4.3.2 RAMP Page

TC SETUP		RAMP	R	AMP
TC Mode MEASURE	F1	Low(°C) -200.0 High(°C) 1372.0	Repeat Format	UP/DOWN
TC Select	\rightarrow	Hold@0%(s) 10	Repeat	1
Unit Celsius 🗸		Rise Time(s) 10		
Source Mode	F2	Hold@ 100%(s) 10		
STEP		Fall Time(s) 10		
RAMP 🔳		▼		
EDIT BACK		EDIT BACK	EDIT	BACK

Parameter Name	Description / Options
Low	Starting Value of Ramp Enter value according to TC Display Mode. If display mode is actual, enter value in temperature/mV and if display mode is %, enter value in %.
High	Ending Value of Ramp Enter value according to TC Display Mode. If display mode is actual, enter value in temperature/mV and if display mode is %, enter value in %.
Hold@0%(s)	Time to wait at Low (0%) level in second This parameter is used for Repeat Format UP/DOWN or DOWN/UP .
	<u>Range:</u> 0 9999
Rise Time (s)	Time to Increase from Low to High Level.
	<u>Range:</u> 1 9999
Hold@100%(s)	Time to wait at High (100%) level in second This parameter is used for Repeat Format UP/DOWN or DOWN/UP .
	<u>Range:</u> 0 9999

Fall Time (s)	Time to decrease from High to Low Level
	<u>Range:</u> 1 9999
Repeat Format	How the Ramp should be done
	<u>Available Options:</u> UP DOWN UP/DOWN DOWN/UP
Repeat Repeat Counts	Defines how many times the steps are repeated
	<u>Range:</u> 1 9999

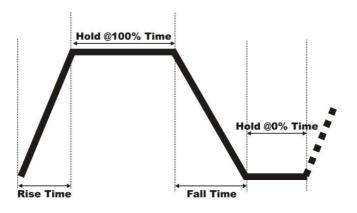



Starting the RAMP To Enable Ramp, select Source Type as RAMP.




Source Display Window according to current RAMP mode in RUN Page and F1 & F2 Button change to **START** and **SETTING** respectively.

RAMP can be started by Pressing F1 key (START). After that F1 & F2 key will change to **PAUSE** and **STOP** respectively. So by pressing F1 and F2 key running RAMP can be PAUSE or STOP at any time in RUN Page.

<u>NOTE:</u> While RAMP is running RAMP settings can't be accessible and Source Page Parameter settings can't be change. Stop RAMP before changing any settings.

4.4 DISPLAY Page

This page appears when you select $RUN \rightarrow MENU \rightarrow DISPLAY$.

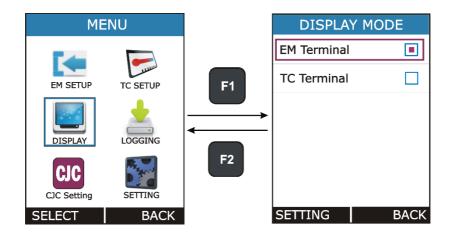


There are mainly Four RUN Display Modes possible in this device. And this mode can be selected from the above Page. What information to be shown in each RUN Display Mode can be defined by this page.

In this page there is one RadioButtonBox. At a time one or two option can be selected. The possible combinations are given below.



4.4.1 EM Display Settings

This page appears when you select $RUN \rightarrow MENU \rightarrow DISPLAY \rightarrow EM$ Terminal.

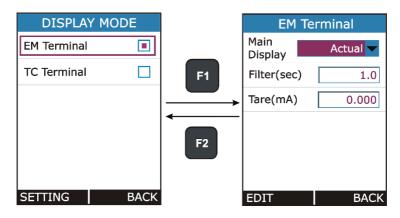

Parameter Name	Description / Options		
Main Display	Select which Reading to be displayed as a Main Reading (Reading Displays in Box in RUN Page).		
	Available Options:		
	Actual	Display the Actual Input Value	
	Percentage	Display the Percentage Value of the Input	
		The Value depends on Input Range. These settings are available from $MENU \rightarrow EM SETUP$.	
	Scaled	Display the Scaled Value of the Input	
		The Scale Value depends on Input Range, Input Scaled Range and Transfer Function. These settings are available from $MENU \rightarrow EM SETUP$.	
Filter (sec)	1 st Order IIR Low Pass Filter for Input Reading Filter is useful when a measurement signal contains unwanted noise.		
	<u>Range:</u> 0.0 60.0 sec		



Г

Tare (unit)	The Tare value is subtracted from the reading of the measured value. Here unit is changed according to current Input Type and Measure Display Mode.
	Range: In accordance with Input Range & Measure Display Mode.
	Note: Beware of the problems that may result in not seeing the true measurement value.

4.4.2 TC Display Settings

This page appears when you select $RUN \rightarrow MENU \rightarrow DISPLAY \rightarrow TC$ Terminal.

DISPLAY MODE		TC Term	inal		TC T	erminal
EM Terminal		Main Display	Actual 🔽		Main Display	Percentage 🤜
TC Terminal		Range 0% 100%	-200.0 1372.0	OR	Range 0% 100%	-200.0 1372.0
	F2	Additional Info.	dback 🔽		Additional I Filter(sec)	nfo. Actual mV 🔽
SETTING BACK		EDIT	BACK		EDIT	BACK

TC SOURCE Mode

TC MEASURE Mode

Parameter Name	Description / Options			
Main Display	Select which Reading to be display as a Main Reading (Reading Displays in Box in RUN Page).			
	Available Option	<u>ıs:</u>		
	Actual	Actual Display the Actual Thermocouple/mV Value		
	Percentage Display the Percentage Value of Thermocouple/mV according to value set in 0% and 100%.			
0%	Low Value in Temperature/mV for (0 100%) scaling.			
100%	High Value in Temperature/mV for (0 100%) scaling.			

Additional Info.1	Choose which information to be shown as TC Mode Additional Information on RUN Page.			
	Available Options for TC Measure Mode:			
	Options	Description		
	None	-	No info is visible.	
	Actual Value	AV	Shows the Actual Thermocouple Temperature/mV value without any scaling. This option is available only if TC Display Mode is Percentage.	
	mV	mV	Shows the Thermovoltage which is measured through TC terminals.	
	mV w/o CJC	mV₀	Shows the Thermovoltagea ccording to TC Temperature with adding CJ Temperature mV.	
	Maximum	Υ	Shows the Maximum measured reading from the time when info last reset.	
	Minimum	¥	Shows the Minimum measured reading from the time when info last reset.	
	Min & Max	-	Shows the Minimum (in place of mV_0) and Maximum value both together. This option available only for only TC Display mode.	
	Available Options	s for TC Sou	rce Mode:	
	Options	Icon	Description	
	None	-	No info is visible.	
	Actual Value	AV	Shows the Actual Thermocouple Temperature/mV value without any scaling. This option is available only if TC Display Mode is Percentage.	
	mV	mV	Shows the Thermovoltage according to Temperature including CJ temperature mV. The mV which is sourced through TC Terminal.	


	Reading Feedback	RF	Shows the Feedback Temperature/mV Reading. When TC-12 generate mV, it uses its own measurement function to control the generated value. This feedback measurement is shows if this option is selected.
	%Error	%E	Shows the error in % between the Desired Source Value and Feedback value.
	mV Feedback	mVF	Shows the Feedback mV Reading.
	mV w/o CJC	mV₀	Shows the Thermovoltage according to Temperature (for CJ Temperature = 0 °C)
Filter(sec)	1 st Order IIR Low Pass Filter for TC Measure Reading. This option is available only for TC mode is Measure. Filter is useful when a measurement signal contains unwanted noise.		
	Range: 0.0 60.0 sec		

4.5 DATA LOGGING Page

PCE

This section gives examples of how to log Readings with time and date over a set time period or on a key press. Logged data is stored in a user defined file in internal memory.

This Page appears when you select $RUN \rightarrow MENU \rightarrow LOGGING$.

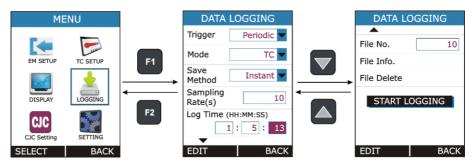

		/	
Parameter Name	Description / Options		
Trigger	Data Logging Trigger Mode Selection.		
	Available Options		
	Key Press	Log Data on pressing from RUN key Page	
	Periodic	Log Data periodically at every Sampling Rate for total time specified by Logging Time.	
Mode	Data Mode Select	ion for Logging	
	Available Options		
	EM	Log only EM Measure Readings	
	тс	Log only TC Terminal Readings	
	EM+TC	Log EM Measure and TC Terminal both Readings	
	This parameter is enabled only for Periodic Trigger.		
Save Method	Reading Type selection for Logging		
	<u>Available Options:</u> Instant Min Max Average All		
	This parameter is enabled only for Periodic Trigger.		
Sampling Rate(s)	Sampling Rate for Periodic Data Logging in seconds		
	<u>Range:</u> 1 9999		
	This parameter is	enabled only for Periodic Trigger.	
Logging Time (HH:MM:SS)	Total Logging Tim	e in HH:MM:SS Format for Periodic Logging	
	This parameter is	enabled only for Periodic Trigger.	



File No.	File Number.
	Range: 1 25
	This parameter is enabled only for Periodic Trigger.
File Info.	Shows the information of stored files. This information contains Logging Start Time & Date and No of Samples stored in the file.
File Delete	Delete stored file.
START LOGGING	Press F1 key while selecting this button to start the Logging.

Notes:

• Maximum No. of Readings that can be stored in

Logging Mode	Max. Reading
Periodic	150000
Key Press	484

- In Periodic mode, changing of any Measure or Source parameter is not allowed. So While Periodic Logging is Running, the úser can't enter *MEASURE*, *SOURCE* and *DISPLAY* menu. But in Key Press Logging mode, there is no restriction.
- In Periodic Mode, if error message like "*Not Sufficient Memory*" comes while starting the Logging. Try to Reduce Logging Time or Increase Sampling Period or try deleting some existing files.
- In Key Press Mode, If No of Samples reach its maximum limit that is 484, the next sample will start from the first overwriting the memory.
- While Logging is running, entering into the *LOGGING* menu shows below page.

IOI Periodic Mode	
DATA LO	OGGING
Logging Runn	ning
No of Sample Taken	20 out of 100
Time Remaining	00:10:45
STOP L	OGGING
	BACK

- For Periodic Mode, this page contains information of Number of Samples Taken and Time Remaining for Logging in HH:MM:SS.
- Both Periodic and Key Press logging can be stop manually by pressing F1 key on STOP LOGGING Button. For Periodic Mode, Logging will automatically stopped when defined log time ends and a message "LOGGING DONE" pop ups.

Transferring the Results to a Personal Computer:


fan Daniadia Mada

A 32-bit Windows® software called **mCAL+.exe** can be downloaded here: <u>https://www.pce-instruments.com/english/download-win_4.htm</u>. Start this software just as any other Windows® software.

All communication between the PC and PCE-TTC 30 is initiated from **mCAL+.exe**. More information on the software can be found in the separate software manual.

4.6 CJC Setting Page

This page appears when you select $RUN \rightarrow MENU \rightarrow CJC$ Settings.

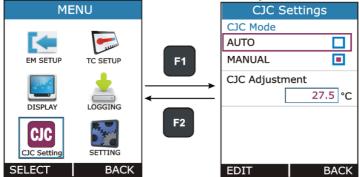




Parameter Name	Description / Options		
CJC Mode	CJ (Cold Junction) Temperature Mode		
	Available Options:		
	AUTO CJ Temperature is TC Terminal's temperature.		
	MANUAL	CJ Temperature is user selectable irrespective of TC Terminal temperature.	
CJC Adjustment	CJ Temperature adjustment for Manual CJC Temperature.		

4.7 SETTING Page

This page appears when you select $RUN \rightarrow MENU \rightarrow SETTING$.

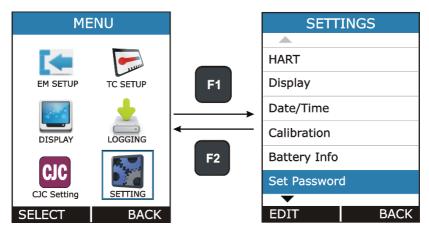

All the available Settings Options are given below.

i. HART ii. Display iii. Date/Time iv. Calibration v. Battery Info vi. Set Password vii. Factory Reset viii. About Us

Press F1 key to Enter into the settings of any option. Description of all settings is given below.



4.7.1 HART Settings

HART	
HART (250 ohms)	
NO	
YES	
EDIT	BACK

Select YES to add a Series resistor (250Ω) into the mA circuit. You can then use this instrument together with a HART® communicator to set up and calibrate HART® devices. This option is applicable for mA(24V) Read Power Input Type Only.


4.7.2 Display Settings

DISP	LAY
Display Intensity(%)	100
Display Off Time(s) (0=Infinite)	10
EDIT	BACK

Display Intensity	Display Brightness Settings.
	<u>Range:</u> 5 to 100
Display Off Time	Standby Time in second after which display will turn Off. To turn the display off press any key.
	Range: 0 to 9999 sec
	Setting 0 will disable this feature. That means display will never turn off automatically.



4.7.3 Date/Time Settings



To set the Time + Date of the device.

2 date formats are supported in this device: **DD/MM/YY** and **MM/DD/YY**. This is useful only in Data Logging, to decide in which format the Date is to be stored.

2 time formats are supported in this device: **24 Hour** and **12 Hour**. This is to select in which format the time should be displayed on Run page and time to be stored in Data Logging.

AM/PM selection is enabled only for 12 Hour Time Format.

4.7.4 Calibration

The instrument is factory calibrated for the specified range, but due to long term drift of components, re-calibration may be necessary in some cases. For calibrating the instrument, a reliable source is required. This source should be at least ten times accurate compared to the range of the instrument.

Note: PCE Instruments can provide a calibration service that is traceable to international standards.

We recommend that you return the instrument to the manufacturer or an approved service agent for calibration. If you use an alternative calibration facility, make sure that it uses these standards.

4.7.5 Battery Info

This page shows the basic battery Information.

- Battery Level (Percentage)
- Battery Voltage (in mV)
- Current (in mA)
- Battery Status
- Time to Full (in min)
- Time to Empty (in min)

4.7.6 About Calibrator

This Page illustrates the Connection diagrams for valid connections to this device.



5 **Maintenance and Troubleshooting**

5.1 **Common Problems**

Problem	Possible Causes
Device Not Starting Up	Battery DischargedBattery Connection Loose
Reading Fluctuation/ Reading OPEN	Wrong / Loose Connections
Error Code on status bar	One of the peripheral not working properly. (Solution: Restart the Device if still error code showing contact PCE Instruments)
Calibration Out	 Distortion in due to external noise connection (Solution: Check connection. If still out, contact PCE Instruments or Recalibrate Device in authorized calibration laboratory.)
Battery Not Charging	Battery Connection LooseBattery Dead

Replacing the Battery 5.2





Take out the old battery and stick new battery same as old one with double sided tap & connect battery connector to J3 connector



OPEN 3 Screws to remove battery holder sheet



6 Technical Specifications

Voltage DC V				
Measuring range		Resolution	Accuracy	
0 30V		0.001V	± 0.02% v.Mw. + 2 Dgt	
Current DC mA				
Measuring range		Resolution	Accuracy	
0 24-mA		0.001-mA	± 0.02% v.Mw. + 2 Dgt	
Measurement / Si	imulation			
Thermocouples	Measuring range	Resolution	Accuracy	
е	-200 1200°C / -328	0.1°C /	± 0.3°C / 0.54°F	
	2192°F	0.18°F		
J	-200 1200°C / -328	0.1°C /	± 0.3°C / 0.54°F	
	2192°F	0.18°F		
K	-200 1372°C / -328	0.1°C /	± 0.3°C / 0.54°F	
	2501°F	0.18°F		
Т	-200 400°C / -328	0.1°C /	± 0.3°C / 0.54°F	
	752°F	0.18°F		
В	450 1800°C / 842	0.1°C /	± 0.3°C / 0.54°F	
	3272°F	0.18°F		
R	0 1750°C / 32	0.1°C /	± 0.3°C / 0.54°F	
	3182°F	0.18°F		
S	0 1750°C / 32	0.1°C /	± 0.3°C / 0.54°F	
	3182°F	0.18°F		
N	-200 1300°C / -328	0.1°C /	± 0.3°C / 0.54°F	
	2372°F	0.18°F		
mV	10 80 mV	0.001 mV	± 0.02% of the displayed	
	-10 250 mV	0.01 mV	value + 2µV	
			± 0.02% of reading + 0.02	
			mV	
Note: The specific	Note: The specifications refer to the temperature standard ITS-90			

Display modesMeasurement: mA / V / thermocouple / mV Simulation: thermocouple / mVtemperature units°C / °F / KColdjunction $\leq \pm 0.5^{\circ}C$ / 0.9°FMaximum input voltage30V DCTemperature coefficient<30 ppmInputimpedanceMeasurementCurrent measurement: 10 ΩResponse time<100 msImpedance> 4,7 kΩ with thermocouple / mVResponse time<100 msImpedance> 4,7 kΩ with thermocouple / mVRefresh rate display10 HzIsolation500V DCData storageInternal memory 150000 readingsInterfaceUSB 2.0Display2.4° TFT LCD 240 x 320 pixels LED illuminatedOutput voltage current250 Ω ± 20%Power supply3.7V / 230mAh Li-ion batteryCharging timeabout 5 hPower supply3.7V / 230mAh Li-ion batteryCharging timeabout 5 hPower adapterInput: 100 240V AC / 50/60 Hz Output: SV / 1 A DCBattery lifeApprox. 8 h: Measurement with low LCD illumination Approx. 8 h: Measurement with low LCD illuminationDimensions162 x 82 x 40 mm Main operation: 0 45°C / 32 113, 30 90% RH Main operation: 0 45°C / 32 113, 30 90% RH Main operation: 0 45°C / 32 113, 30 90% RH Main operation: 0 45°C / 32 113, 30 90% RH Main operation: 0 45°C / 32 113, 30 90% RH	General specifications		
Simulation: thermocouple / mVtemperature units $\mbox{C}/\mbox{F}/\mbox{K}$ Coldjunction $\le \pm 0.5^{\circ}\mbox{C}/0.9^{\circ}\mbox{F}$ compensation errorMaximum input voltage30V DCTemperature coefficient<30 pm		Measurement: mA / V / thermocouple / mV	
temperature units °C / °F / K Cold junction compensation error 30V DC Temperature coefficient <30 ppm			
Coldjunction $\leq \pm 0.5^{\circ}C / 0.9^{\circ}F$ Maximum input voltage30V DCTemperature coefficient<30 ppm	temperature units		
Maximum input voltage 30V DC Temperature coefficient <30 ppm		≤ ± 0.5°C / 0.9°F	
Temperature coefficient <30 ppm Input impedance Thermocouple / mV / V:> 1 MΩ Response time <100 ms	compensation error		
Input impedance measurement Thermocouple / mV / V:> 1 MΩ Current measurement: 10 Ω Response time <100 ms	Maximum input voltage	30V DC	
measurement Current measurement: 10 Ω Response time <100 ms	Temperature coefficient	<30 ppm	
measurement Current measurement: 10 Ω Response time <100 ms	Input impedance	Thermocouple / mV / V:> 1 MΩ	
Impedance > 4,7 kΩ with thermocouple / mV Refresh rate display 10 Hz Isolation 500V DC Data storage Internal memory 150000 readings Interface USB 2.0 Display 2.4" TFT LCD 240 x 320 pixels LED illuminated Output voltage current 24V DC / 24mA loop 250 Ω ± 20% resistance Step and ramp function Special features Step and ramp function Automatic and manual mode \sqrt{x} , x2: For the measuring function 2.7V / 2300mAh Li-ion battery Continuity test Adjustable threshold up to 100 Ω Power supply 3.7V / 2300mAh Li-ion battery Charging time about 5 h Power adapter Input: 100 240V AC / 50/60 Hz Output: 5V / 1 A DC Battery life Battery life Approx. 15 h: Simulation and measurement with low LCD illumination Dimensions 162 x 82 x 40 mm Weight About 300 g / < 1 lb	measurement		
Refresh rate display10 HzIsolation500V DCData storageInternal memory 150000 readingsInterfaceUSB 2.0Display2.4" TFT LCD 240 x 320 pixels LED illuminatedOutput voltage current loop24V DC / 24mAIoop250 $\Omega \pm 20\%$ HARTmA loopKarton Markow250 $\Omega \pm 20\%$ Special featuresStep and ramp function Automatic and manual mode \sqrt{x} , x2: For the measuring functionContinuity testAdjustable threshold up to 100 Ω Power supply3.7V / 2300mAh Li-ion batteryCharging timeabout 5 hPower adapterInput: 100 240V AC / 50/60 Hz 	Response time	<100 ms	
Isolation500V DCData storageInternal memory 150000 readingsInterfaceUSB 2.0Display2.4" TFT LCD 240 x 320 pixels LED illuminatedOutput voltage current loop24V DC / 24mAIoop250 Ω ± 20%FesistanceStep and ramp function Automatic and manual mode $√x$, x2: For the measuring functionContinuity testAdjustable threshold up to 100 ΩPower supply3.7V / 2300mAh Li-ion batteryCharging timeabout 5 hPower adapterInput: 100 240V AC / 50/60 Hz Output: 5V / 1 A DCBattery lifeApprox. 15 h: Simulation and measurement with low LCD illumination Approx. 8 h: Measurement with low LCD illuminationDimensions162 x 82 x 40 mmWeightAbout 300 g / < 1 lb	Impedance	> 4,7 k Ω with thermocouple / mV	
Data storageInternal memory 150000 readingsInterfaceUSB 2.0Display2.4" TFT LCD 240 x 320 pixels LED illuminatedOutput voltage current24V DC / 24mAloop250 $\Omega \pm 20\%$ HART mA loop resistance250 $\Omega \pm 20\%$ Special featuresStep and ramp function Automatic and manual mode \sqrt{x} , x2: For the measuring functionContinuity testAdjustable threshold up to 100 Ω Power supply3.7V / 2300mAh Li-ion batteryCharging timeabout 5 hPower adapterInput: 100 240V AC / 50/60 Hz Output: 5V / 1 A DCBattery lifeApprox. 15 h: Simulation and measurement with low LCD illumination Approx. 8 h: Measurement with low LCD illuminationDimensions162 x 82 x 40 mmWeightAbout 300 g / < 1 lb			
InterfaceUSB 2.0Display2.4" TFT LCD 240 x 320 pixels LED illuminatedOutput voltage current loop24V DC / 24mAOutput voltage current loop250 $\Omega \pm 20\%$ HARTmAloop 250 $\Omega \pm 20\%$ Special featuresStep and ramp function Automatic and manual mode \sqrt{x} , x2: For the measuring functionContinuity testAdjustable threshold up to 100 Ω Power supply3.7V / 2300mAh Li-ion batteryCharging timeabout 5 hPower adapterInput: 100 240V AC / 50/60 HzOutput: 5V / 1 A DCBattery lifeApprox. 15 h: Simulation and measurement with low LCD illumination Approx. 8 h: Measurement with low LCD illuminationDiegree of protectionIP20Operating conditions62 x 82 x 40 mmWeightAbout 300 g / < 1 lb	Isolation	500V DC	
Display 2.4° TFT LCD 240×320 pixels LED illuminatedOutput voltage current loop $24V$ DC / 24mADop $24V$ DC / 24mAHART mA loop $250 \Omega \pm 20\%$ FesistanceStep and ramp function Automatic and manual mode \sqrt{x}, x^2 : For the measuring functionContinuity testAdjustable threshold up to 100 Ω Power supply $3.7V / 2300mAh$ Li-ion batteryCharging timeabout 5 hPower adapterInput: 100 240V AC / 50/60 Hz Output: 5V / 1 A DCBattery lifeApprox. 15 h: Simulation and measurement with low LCD illumination Approx. 8 h: Measurement with low LCD illuminationDimensions $162 \times 82 \times 40$ mmWeightAbout 300 g / < 1 lb	9		
240 x 320 pixels LED illuminatedOutput voltage current loop24V DC / 24mAIoop24V DC / 24mAHART mA loop resistance250 $\Omega \pm 20\%$ Special featuresStep and ramp function Automatic and manual mode \sqrt{x} , x2: For the measuring functionContinuity testAdjustable threshold up to 100 Ω Power supply3.7V / 2300mAh Li-ion batteryCharging timeabout 5 hPower adapterInput: 100 240V AC / 50/60 Hz Output: 5V / 1 A DCBattery lifeApprox. 15 h: Simulation and measurement with low LCD illumination Approx. 8 h: Measurement with low LCD illuminationDimensions162 x 82 x 40 mmWeightAbout 300 g / < 1 lb	Interface		
LED illuminatedOutput voltage current loop $24V DC / 24mA$ HART mA resistance250 $\Omega \pm 20\%$ Special featuresStep and ramp function Automatic and manual mode \sqrt{x} , x^2 : For the measuring functionContinuity testAdjustable threshold up to 100 Ω Power supply $3.7V / 2300mAh$ Li-ion batteryCharging timeabout 5 hPower adapterInput: 100 240V AC / 50/60 Hz Output: $5V / 1 A DC$ Battery lifeApprox. 15 h: Simulation and measurement with low LCD illumination Approx. 8 h: Measurement with low LCD illuminationDimensions $162 x 82 x 40 mm$ WeightAbout 300 g / < 1 lb	Display		
Output voltage current loop $24V DC / 24mA$ loopHART mA resistanceloopSpecial featuresStep and ramp function Automatic and manual mode \sqrt{x} , x^2 : For the measuring functionContinuity testAdjustable threshold up to 100 Ω Power supply $3.7V / 2300mAh$ Li-ion batteryCharging timeabout 5 hPower adapterInput: 100 240V AC / 50/60 Hz Output: 5V / 1 A DCBattery lifeApprox. 15 h: Simulation and measurement with low LCD illumination Approx. 8 h: Measurement with low LCD illuminationDimensions $162 \times 82 \times 40 mm$ WeightAbout 300 g / < 1 lb			
loopInterventionHARTmAloopresistanceStep and ramp function Automatic and manual mode \sqrt{x} , x2: For the measuring functionSpecial featuresStep and ramp function Automatic and manual mode \sqrt{x} , x2: For the measuring functionContinuity testAdjustable threshold up to 100 ΩPower supply3.7V / 2300mAh Li-ion batteryCharging timeabout 5 hPower adapterInput: 100 240V AC / 50/60 Hz Output: 5V / 1 A DCBattery lifeApprox. 15 h: Simulation and measurement with low LCD illumination Approx. 8 h: Measurement with low LCD illuminationDimensions162 x 82 x 40 mmWeightAbout 300 g / < 1 lb			
HART resistanceIoop loop $250 \Omega \pm 20\%$ Special featuresStep and ramp function Automatic and manual mode \sqrt{x} , x^2 : For the measuring functionContinuity testAdjustable threshold up to 100Ω Power supply $3.7V / 2300$ mAh Li-ion batteryCharging timeabout 5 hPower adapterInput: $100 \dots 240V$ AC / $50/60$ Hz Output: $5V / 1$ A DCBattery lifeApprox. 15 h: Simulation and measurement with low LCD illumination Approx. 8 h: Measurement with low LCD illuminationDimensions $162 \times 82 \times 40$ mmWeightAbout $300 \text{ g} / < 1$ lbDegree of protectionIP20Operating conditionsBattery operation: $0 \dots 55^{\circ}C / 32 \dots 131^{\circ}F$, $30 \dots 90\%$ RH Main operation: $0 \dots 45^{\circ}C / 32 \dots 113$, $30 \dots 90\%$ RH		24V DC / 24mA	
Special featuresStep and ramp function Automatic and manual mode √x, x2: For the measuring functionContinuity testAdjustable threshold up to 100 ΩPower supply $3.7V / 2300$ mAh Li-ion batteryCharging timeabout 5 hPower adapterInput: 100 240V AC / 50/60 Hz Output: 5V / 1 A DCBattery lifeApprox. 15 h: Simulation and measurement with low LCD illumination Approx. 8 h: Measurement with low LCD illuminationDimensions162 x 82 x 40 mmWeightAbout 300 g / < 1 lb		250 Ω ± 20%	
Automatic and manual mode \sqrt{x} , x2: For the measuring functionContinuity testAdjustable threshold up to 100 Ω Power supply $3.7V / 2300$ mAh Li-ion batteryCharging timeabout 5 hPower adapterInput: 100 240V AC / 50/60 Hz Output: 5V / 1 A DCBattery lifeApprox. 15 h: Simulation and measurement with low LCD illumination Approx. 8 h: Measurement with low LCD illuminationDimensions162 x 82 x 40 mmWeightAbout 300 g / < 1 lb	resistance		
mode \sqrt{x} , x2: For the measuring functionContinuity testAdjustable threshold up to 100 Ω Power supply $3.7V / 2300$ mAh Li-ion batteryCharging timeabout 5 hPower adapterInput: 100 240V AC / 50/60 Hz Output: 5V / 1 A DCBattery lifeApprox. 15 h: Simulation and measurement with low LCD illumination Approx. 8 h: Measurement with low LCD illuminationDimensions162 x 82 x 40 mmWeightAbout 300 g / < 1 lbDegree of protectionIP20Operating conditionsBattery operation: 0 55°C / 32 131°F, 30 90% RH Main operation: 0 45°C / 32 113, 30 90% RHStorage conditions-20 60°C / -4 140°F, 30 90% rh non-condensing	Special features		
Continuity testAdjustable threshold up to 100 ΩPower supply $3.7V / 2300$ mAh Li-ion batteryCharging timeabout 5 hPower adapterInput: 100 240V AC / 50/60 Hz Output: 5V / 1 A DCBattery lifeApprox. 15 h: Simulation and measurement with low LCD illumination Approx. 8 h: Measurement with low LCD illuminationDimensions162 x 82 x 40 mmWeightAbout 300 g / < 1 lb			
Power supply 3.7V / 2300mAh Li-ion battery Charging time about 5 h Power adapter Input: 100 240V AC / 50/60 Hz Output: 5V / 1 A DC Output: 5V / 1 A DC Battery life Approx. 15 h: Simulation and measurement with low LCD illumination Approx. 8 h: Measurement with low LCD illumination Dimensions 162 x 82 x 40 mm Weight About 300 g / < 1 lb			
Charging timeabout 5 hPower adapterInput: 100 240V AC / 50/60 Hz Output: 5V / 1 A DCBattery lifeApprox. 15 h: Simulation and measurement with low LCD illumination Approx. 8 h: Measurement with low LCD illuminationDimensions162 x 82 x 40 mmWeightAbout 300 g / < 1 lb			
Power adapter Input: 100 240V AC / 50/60 Hz Output: 5V / 1 A DC Battery life Approx. 15 h: Simulation and measurement with low LCD illumination Approx. 8 h: Measurement with low LCD illumination Dimensions 162 x 82 x 40 mm Weight About 300 g / < 1 lb			
Output: 5V / 1 A DC Battery life Approx. 15 h: Simulation and measurement with low LCD illumination Approx. 8 h: Measurement with low LCD illumination Dimensions 162 x 82 x 40 mm Weight About 300 g / < 1 lb			
illumination Approx. 8 h: Measurement with low LCD illumination Dimensions 162 x 82 x 40 mm Weight About 300 g / < 1 lb	Power adapter		
illumination Approx. 8 h: Measurement with low LCD illumination Dimensions 162 x 82 x 40 mm Weight About 300 g / < 1 lb	Battery life	Approx. 15 h: Simulation and measurement with low LCD	
Dimensions 162 x 82 x 40 mm Weight About 300 g / < 1 lb			
Dimensions 162 x 82 x 40 mm Weight About 300 g / < 1 lb		Approx. 8 h: Measurement with low LCD illumination	
Degree of protection IP20 Operating conditions Battery operation: 0 55°C / 32 131°F, 30 90% RH Main operation: 0 45°C / 32 113, 30 90% RH Storage conditions -20 60°C / -4 140°F, 30 90% rh non-condensing	Dimensions		
Operating conditions Battery operation: 0 55°C / 32 131°F, 30 90% RH Main operation: 0 45°C / 32 113, 30 90% RH Storage conditions -20 60°C / -4 140°F, 30 90% rh non-condensing	Weight	About 300 g / < 1 lb	
Operating conditions Battery operation: 0 55°C / 32 131°F, 30 90% RH Main operation: 0 45°C / 32 113, 30 90% RH Storage conditions -20 60°C / -4 140°F, 30 90% rh non-condensing	Degree of protection	IP20	
Storage conditions -20 60°C / -4 140°F, 30 90% rh non-condensing		Main operation: 0 45°C / 32 113, 30 90% RH	
	Storage conditions	-20 60°C / -4 140°F, 30 90% rh non-condensing	



You can read our Contact terms in our General Business Terms which you can find here: https://www.pce-instruments.com/english/terms.

8 Disposal

For the disposal of batteries in the EU, the 2006/66/EC directive of the European Parliament applies. Due to the contained pollutants, batteries must not be disposed of as household waste. They must be given to collection points designed for that purpose.

In order to comply with the EU directive 2012/19/EU we take our devices back. We either re-use them or give them to a recycling company which disposes of the devices in line with law.

For countries outside the EU, batteries and devices should be disposed of in accordance with your local waste regulations.

If you have any questions, please contact PCE Instruments.





FC

PCE Instruments contact information

Germany

PCE Deutschland GmbH Im Langel 4 D-59872 Meschede Deutschland Tel.: +49 (0) 2903 976 99 0 Fax: +49 (0) 2903 976 99 29 info@pce-instruments.com www.pce-instruments.com/deutsch

United States of America

PCE Americas Inc. 711 Commerce Way suite 8 Jupiter / Palm Beach 33458 FL USA Tel: +1 (561) 320-9162 Fax: +1 (561) 320-9176 info@pce-americas.com www.pce-instruments.com/us

The Netherlands

PCE Brookhuis B.V. Institutenweg 15 7521 PH Enschede Nederland Telefoon: +31 (0)53 737 01 92 Fax: +31 53 430 36 46 info@pcebenelux.nl www.pce-instruments.com/dutch

China

PCE (Beijing) Technology Co.,Ltd 1519 Room, 6 Building Men Tou Gou Xin Cheng, Men Tou Gou District 102300 Beijing China Tel: +86 (10) 8893 9660 info@pce-instruments.cn www.pce-instruments.cn

France

PCE Instruments France EURL 23, rue de Strasbourg 67250 SOULTZ-SOUS-FORETS France Téléphone: +33 (0) 972 3537 17 Numéro de fax: +33 (0) 972 3537 18 info@pce-france.fr www.pce-instruments.com/french

United Kingdom

PCE Instruments UK Ltd Unit 11 Southpoint Business Park Ensign Way, Southampton Hampshire United Kingdom, SO31 4RF Tel: +44 (0) 2380 98703 0 Fax: +44 (0) 2380 98703 9 info@industrial-needs.com www.pce-instruments.com/english

Chile

PCE Instruments Chile S.A. RUT: 76.154.057-2 Santos Dumont 738, local 4 Comuna de Recoleta, Santiago, Chile Tel. : +56 2 24053238 Fax: +56 2 2873 3777 info@pce-instruments.cl www.pce-instruments.com/chile

Turkey

PCE Teknik Cihazları Ltd.Şti. Halkalı Merkez Mah. Pehlivan Sok. No.6/C 34303 Küçükçekmece - İstanbul Türkiye Tel: 0212 471 11 47 Faks: 0212 705 53 93 info@pce-cihazlari.com.tr www.pce-instruments.com/turkish

Spain

PCE Ibérica S.L. Calle Mayor, 53 02500 Tobarra (Albacete) España Tel. : +34 967 543 548 Fax: +34 967 543 542 info@pce-iberica.es www.pce-instruments.com/espanol

PCE

Italy

PCE Italia s.r.l. Via Pesciatina 878 / B-Interno 6 55010 LOC. GRAGNANO CAPANNORI (LUCCA) Italia Telefono: +39 0583 975 114 Fax: +39 0583 974 824 info@pce-italia.it www.pce-instruments.com/italiano

Hong Kong

PCE Instruments HK Ltd. Unit J, 21/F., COS Centre 56 Tsun Yip Street Kwun Tong Kowloon, Hong Kong Tel: +852-301-84912 jyi@pce-instruments.com www.pce-instruments.cn