



SP-UV1000

USER'S MANUAL

Contents

Safety	1
Package Contents	1
Unpacking	1
Installation	2
1. <i>Environment Required</i>	2
2. <i>Install Spectrophotometer</i>	2
Overview	2
Symbols	3
Main Specifications	3
Description of Appearance and Keys	4
1. <i>Appearance</i>	4
2. <i>Keypad</i>	5
3. <i>Description of Keys</i>	5
Functions	6
Getting Started	6
Important Guidelines	7
General Operating	7
Measuring	8
1. <i>Photometry</i>	8
2. <i>Quantitation</i>	9
3. <i>Utility</i>	9
Troubleshooting	15
Repair and Maintenance	16
1. <i>Daily Maintain</i>	16
2. <i>Spare Parts Replacement</i>	16

Warranty	20
Equipment Disposal	20

Safety

Please follow the guidelines below, and read this manual in its entirety to ensure safe operation of the unit.

We recommends against the use of SP-UV1000 Spectrophotometer.



- Do not open the device.
- Disconnect the device from the mains supply before carrying out maintenance work or changing the fuses.
- The inside of the device is a high-voltage area Danger!
- Do not use the device if it is damaged, especially if the main power cable is in any way damaged or defective.
- Repairs may only be carried out by the service technicians from us and authorized contractual partners.
- The device must be connected to a power outlet that has a protective ground connection.
- If the equipment is used in a manner not specified by the manufacturer, the protection provided by the equipment may be impaired.



- Do not allow any liquid to enter into the device.
- Do not operate the device in a hazardous location or potentially explosive environment.

Package Contents

Description	Quantity
Spectrophotometer	1PC
10mm Glass Cuvette	4PCS
10mm QuartzCuvette	2PCS
Power Cord	1PC
User's Manual	1PC
Dust Cover	1PC

Unpacking

Open the package, according to carefully check the packaging packing list items, if found inside the packaging are missing or damaged items please

contactus and authorized contractual partners.

Installation

1. Environment Required

To ensure the best performance, the following conditions are required:

- The best working temperature range is 16—35°C and the humidity is 45—80%.
- Keep it as far as possible away from the strong magnetic or electrical fields or any electrical device that may generate high-frequency fields.
- Set the unit up in an area that is free of dust, corrosive gases and strong vibrations.
- Remove any obstructions or materials that could hinder the flow of air under and around the instrument.
- The power requirement is 110±11V/60±1Hz or 220±22V/50±1Hz.
- Use the appropriate power cord and plug into a grounded outlet.
- If the local voltage is not stable, a voltage regulator is required.
- Be away from direct sunlight.

2. Install Spectrophotometer

Placement

Place the instrument on the stable table carefully.

Install Printer (Printer is Optional Accessories)

Check to confirm instrument power switch is turned off, connect the printer's data cable to the instrument's parallel port.

Link the Power Cord

Check to confirm instrument power switch is turned off, the power cord plug into two separate power interface and power supply socket apparatus.

Overview

SP-UV1000 Spectrophotometer is an electrical measure instrument which is widely used in the laboratories.

- Use Frequency: Intermittence
- Excessive Voltage(Current): No
- Pollution Class: Class 1

Symbols

The following chart is an illustrated glossary of the symbols that are used in this manual.



Caution, Danger!



Caution, High Voltage!



Caution, Hot!



Ground



Fuse



Recycle, this instrument will be called back by the appointed Electrical Treatment Department or by the original Manufacturer when wasted.

Main Specifications


· Optical System	Single beam
· Wavelength Range	200—1000nm
· Wavelength Accuracy	±2nm
· Wavelength Repeatability	0.8nm
· Photometric Range	-0.3—3A, 0—200%T
· Photometric Accuracy	±0.5%T
· Photometric Repeatability	0.3%T
· Spectral Bandwidth	4nm
· Stray Light	0.3%T@220nm&360nm
· Stability	±0.002A/h@500nm
· Work Mode	Photometry, Quantitation
· Interface	USB, Parallel(printer)
· Power Requirement	AC 110/220V, 50/60Hz

· Dimensions	490x360x210
· Weight	14kg
· Work Environment	15—35℃, 15—70% relative humidity
· StoreEnvironment	-10—50℃, 15—70% relative humidity

Description of Appearance and Keys

1. Appearance

Front View

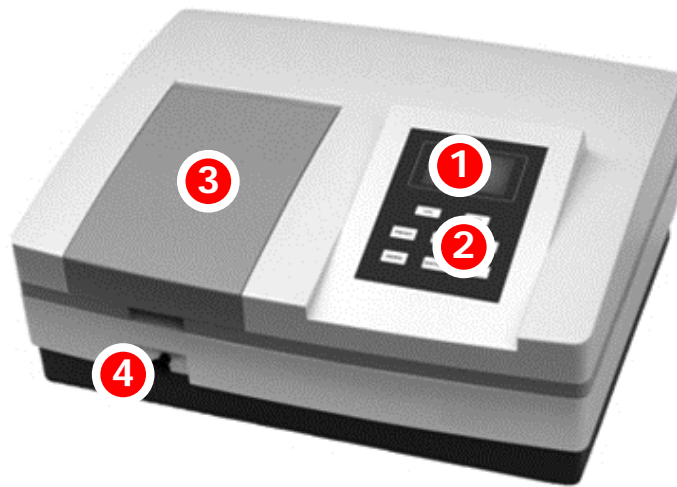

Back View



- | | |
|-----------------------|---------------------------|
| 1 LCD Display | 7 USB port |
| 2 Keypad | 8 Cover of Fan |
| 3 Lid of Sample Room | 9 Power Socket |
| 4 Rod | 10 Power Switch |
| 5 LCD Contrast Adjust | 11 Cover of Cooling Vents |
| 6 Printer port | |

2. Keypad



3. Description of Keys

SET

SET Key: Set Parameters

GOTO λ


GOTO λ Key: Set Wavelength

ZERO

ZERO Key: Blank

PRINT

PRINT Key: Print measuring result



Function Key: Functions according to the screen



UP, DOWN Keys: Scroll menu/data and set Y scale

Functions

Photometry

Display results as Abs, %T or Energy.

Quantitation

Use a Standard Sample to establish Standard Curve.

Getting Started

The following chart describes the basic operation of the instrument.

Turn On and Self-check

Switch on the power. Then the instrument begins to self-check and 20 minutes' warm up. Self-check includes the following steps: Turn on lamps → Check Sensor → Initialize AD → System position → Get Dark Current → Warm up.

Self-test...

Warm up 20 minutes,
Any key to skip

After warm up, instrument displays Main Interface.


WL: 500.0nm		0.000A
100.0%T		
Basic		Quantitative

Important Guidelines





- Reagents and dilution buffers can cause cauterization and other damage to health.
- Samples (nucleic acids, proteins, bacteria cultures) can be infectious and cause serious damage to health.
- During sample preparation, measuring procedures and maintenance and cleaning work, observe all local laboratory safety precautions (e.g. wear protective clothing and gloves, use of disinfectant) regarding the handling of sample material.
- Dispose of measuring solutions and cleaning and disinfectant materials in accordance with the relevant local laboratory regulations.

General Operating

Select Application





Main interface, press the key  (left) to enter into.

Set Wavelength




Test interface, press key  to set wavelength, ,  to modify wavelength value, then press key  (left) to go to wavelength and blank.

WL: 500.0nm	
Please enter WL. :	
500.0 nm	
OK	

Set Parameters

Press  enter into setup interface, ,  to select items or input parameters,  (left) to confirm.

Delete the test result and stored data

Test Interface, press the key , then press key ,  to select

"Clear Data, not Print ", (left) to delete.

Blank

Put the Reference in the light path, press to do blank.

Measure Samples

Put the samples in the light path, press (left) to measure.

Print the test results

Test Interface, press the key , , select "Print, clear data", press the key (left) to print.

Store the Standard Curve

After got the Standard Curve by Marked, press , input the file name and press (left) to save.

Load the Standard Curve


"Quantitative" interface, press , to select "Load Curve", press , to choose the curve you want, press (left) to open.

Measuring

1. Photometry

Step 1. StartPhotometry

MainInterface, press key (left) to choose "Basic".

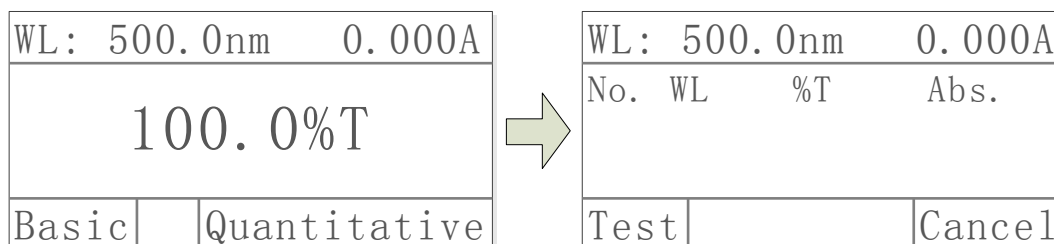

Step 2. Set Wavelength

Press to set wavelength, press , to input wavelength value, press (left) to go to wavelength.

Step 3. Blank

Put the Reference in the light path and press to do blank.

Step 4. Measuresamples

Put the sample in the light path, and then the result displays on the screen automatically, press (left) to record.


WL: 500.0nm 0.000A			
No.	WL	%T	Abs.
1	500.0	100.0	0.000
2	500.0	100.0	0.000
Test			Cancel

2. Quantitation

Step 1. Start Quantitation

Main Interface, press key (left) to choose "Quantitative".


WL: 500.0nm 0.000A	
100.0%T	
Basic	Quantitative



<input checked="" type="radio"/> Create Curve		
<input type="radio"/> Load Curve		
<input type="radio"/> Clear Curve		
OK		Cancel

Step 2. Establish or call Standard Curve




<input checked="" type="radio"/> Create Curve		
<input type="radio"/> Load Curve		
<input type="radio"/> Clear Curve		
OK		Cancel







WL: 500.0nm		
<input checked="" type="radio"/> Coefficient		
<input type="radio"/> Standard Curve		
OK		Cancel




2 methods to establish Standard Curve:


Method 1: Establish Standard Curve by inputting coefficients

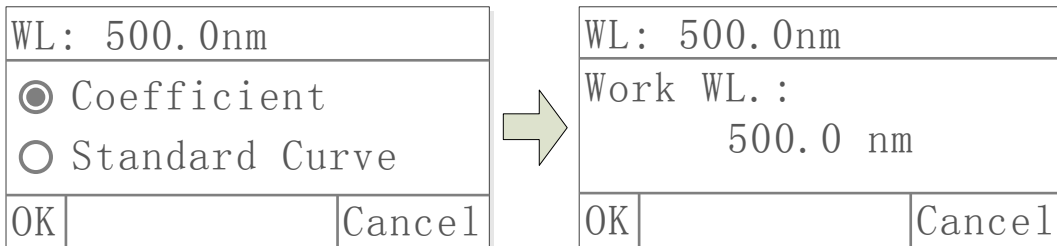- 1) **Starts establish.** Press ,  to select "Coefficient", then press  (left) to confirm.







- 2) **Set wavelength.** Press ,  to input test wavelength value, press  (left) to confirm.

- 3) **Set coefficient K and B.** Press ,  to input coefficient K, press  (left), same way set B.

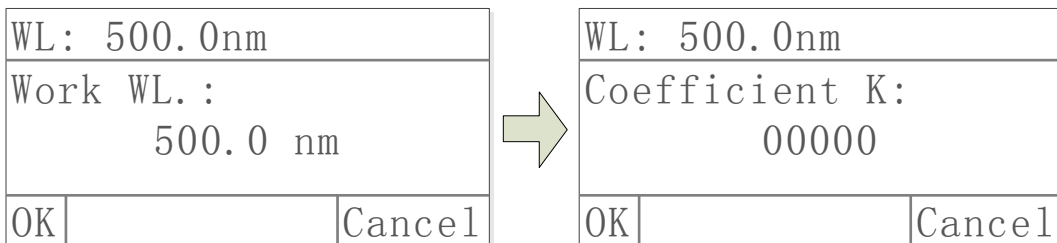


Method 2: Establish Standard Curve by using Standard Samples


- 1) **Starts establish.** Press ,  to select "Standard Curve", then press  (left).

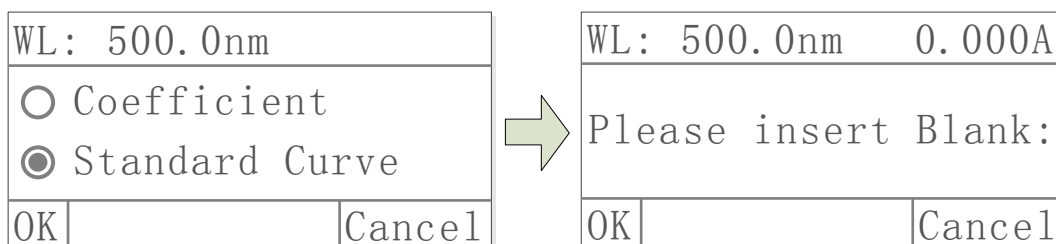

- 2) **Set Wavelength.** Press to enter to set wavelength, Press , to input wavelength value, press (left) to go the setting value.
- 3) **Blank.** Put the Reference in the light path, press (left) to do blank.
- 4) **Setup number of Standard Samples.** Press , to input the quantity of standard sample (No more than 9 standard curve.), press (left) to confirm.

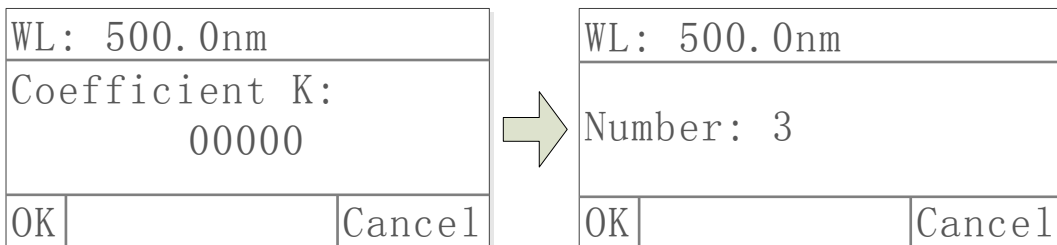

- 5) **Calibrate Standard Samples.** Put the corresponding standard samples in the light path as the screen indicates, press , to input the concentration, press (left) to confirm, to finish all the standard samples.

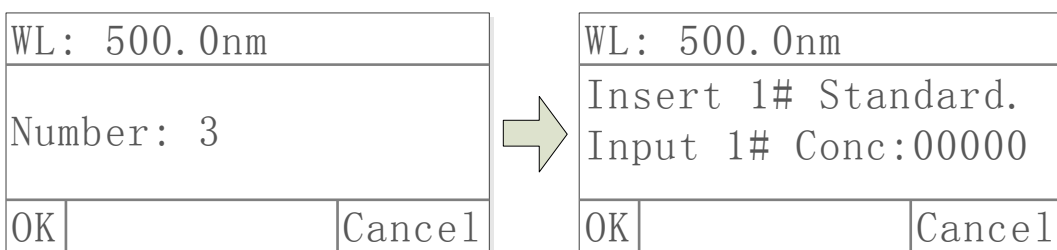

Load the Stored Curve

- Press , to choose "Load Curve", press , to choose the curve, press (left) to confirm.

<input type="radio"/> Create Curve
<input checked="" type="radio"/> Load Curve
<input type="radio"/> Clear Curve
OK
Cancel




C=KxA+B	WL.
C=1.000xA+0.2	500.0 <
C=0.02xA+0.32	470.0
OK	Cancel

Press (left) to enter the test mode after building or loading standard curve.

Step 3. Enter into Measuring Interface

Press (left) to enter into the Quantitation Measuring Interface.

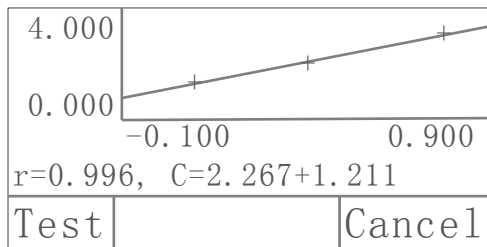

WL: 500.0nm	0.000A
No. WL	Abs. Conc.
Test	Cancel

Step 4. Blank

Put the Reference in the light path, press to do blank.

Step 5. Measure Samples


Put the sample to be tested in the light path, press (left) to measure. Then the test result will display in the data sheet. Repeat this step to finish measuring all the samples.

500.0nm	0.000A		
No. WL	Abs	Conc.	
1	500.0	0.039	0.078
2	500.0	0.042	0.084
3	500.0	0.041	0.082

3. Utility

Main Interface, press to go into utility setting.

WL: 500.0nm 0.000A	
100.0%T	
Basic	Quantitative




<input checked="" type="radio"/> Test Mode	
<input type="radio"/> D2 Lamp On	
<input type="radio"/> W Lamp On	
OK	Cancel

Test Mode

Press , to choose "Test Mode" , press (left) to enter ,press , to choose "Abs" , "%T" , "Energy" , press (left) to confirm.

<input checked="" type="radio"/> Test Mode	
<input type="radio"/> D2 Lamp On	
<input type="radio"/> W Lamp On	
OK	Cancel




<input checked="" type="radio"/> Abs	
<input type="radio"/> %T	
<input type="radio"/> Energy	
OK	Cancel

Turn On/Off D2 Lamp

Press , to choose "D2 Lamp" , then press (left) to enter into.Press , to choose "On" or "Off" , press (left) to turn on/off.


<input type="radio"/> Test Mode	
<input checked="" type="radio"/> D2 Lamp On	
<input type="radio"/> W Lamp On	
OK	Cancel



√D2 Lamp On	
<input checked="" type="radio"/> On	√
<input type="radio"/> Off	
OK	Cancel

Turn On/Off W Lamp


Press , to choose "W Lamp" , then press (left) to enter into.Press , to choose "On" or "Off" , press (left) to turn on/off.

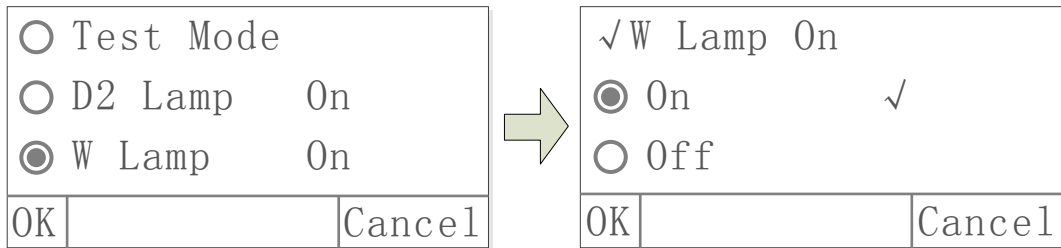

Get Dark Current


Keep the light path without anything blocking, press , to choose "Dark Current", then press (left) to resample Dark Current.

Note: During the course, open the lid of the compartment is prohibited.

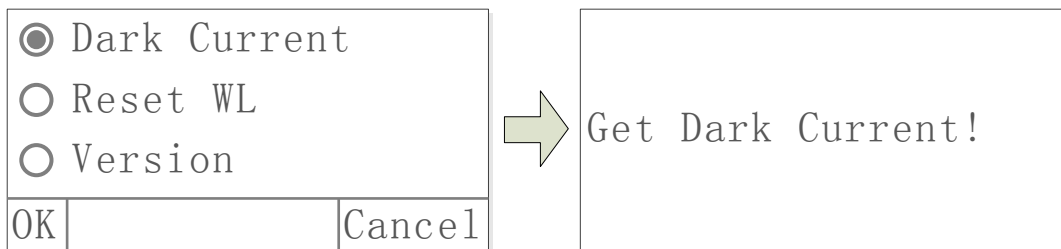


Reset Wavelength

Keep the light path without anything blocking, press , to choose "Reset WL", then press (left) to reset wavelength.

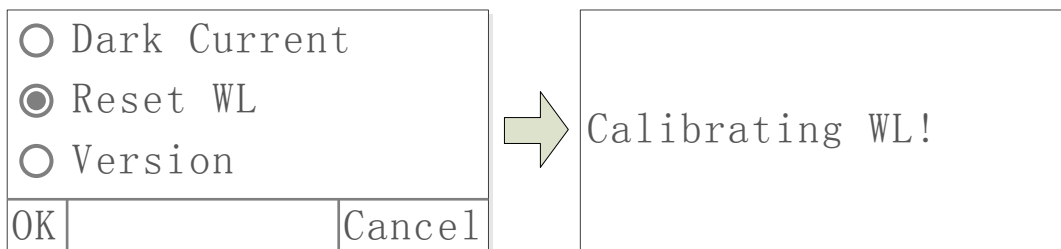

About Version

Press , to choose "Version", press (left) to view version information, press any key to return.

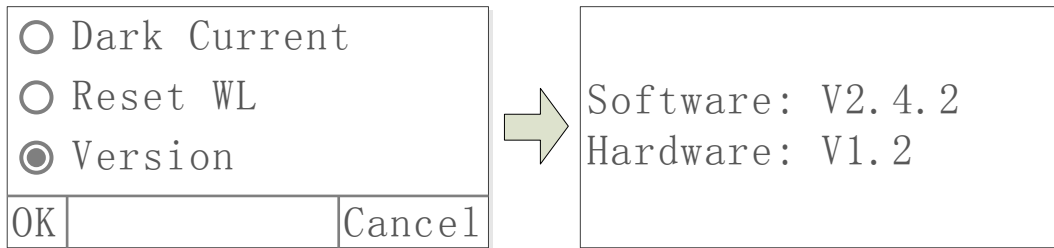

Troubleshooting

Review the information in the table below to troubleshoot operating problems.

Problem	Cause	Solution
Power on, no response	Power cord connection is not reliable	Improve connectivity
	Fuse burning	Replace fuse
Measurement uncertainty	Warm up is not enough	Warm up more time
	Sample is not Stable	Improve the sample
	The concentration of sample is too high	Diluted sample
	Power Supply Voltage Low or not Stable	Improve the Power Supply
	Lamp damage or lamp life maturity	Replace lamp
Dark Current Error when self-check	The lid of the compartment is open during self-check	Close the lid, restart
System Calibrate Failed	Something block the Light path	Remove it, calibrate again
Power on, back light is OK, but nothing display on the screen or display is not clear	Display Contrast problem	Adjust the contrast potentiometer
Measurements inaccurate	Cuvettes were contaminated	Clean cuvettes
	Samples were contaminated	Improve samples
	Worse matching of the cuvettes	Improve the matching of the cuvettes
	Dark current error	Resample dark current

Repair and Maintenance

1. Daily Maintain

Check the Compartment

After measurement, the cuvettes with sample solutions should be taken out of the compartment in time. Or the volatilization of the solution would make the mirror go moldy. Users must pay more attention to the corrosive sample and liquid easy to volatilize. Any solution remains in the compartment should be wiped off immediately.

Surface Clean

The cover of the instrument is with paint. Please use wet towel to wipe off the drips on the surface immediately. Organic solution is forbidden to be used to clean the cover. Please wipe off the dirt on the cover timely.

Clean the Cuvettes

After every test or after a solution change, the cuvettes should be cleaned carefully, or the remains on the surface would cause measuring error.

2. Spare Parts Replacement

Replace the Fuse



Danger! Be sure to switch off the power and unplug the socket before replacement!

Step 1. Tools preparation


Prepare a 3×75 Flat Blade screwdriver.

Step 2. Switch Off the power supply

Switch off the power supply, and unplug the socket.


Step 3. Take out the Fuse Seat

Take out the fuse seat by the screwdriver.

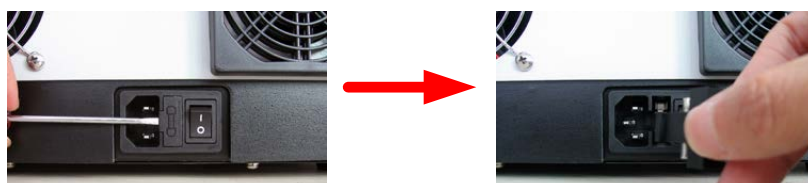

Step 4. Replace a new fuse

Pick out the spare fuse (3.15A/250V) and replace it to the working position.

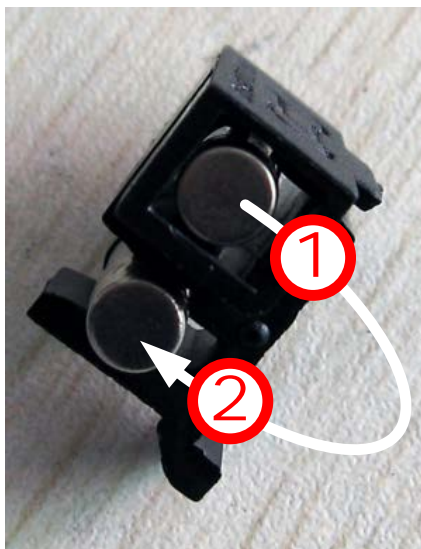

Step 5. Reset the fuse seat

Replace the fuse seat in the power socket.

Step 6. Switch on the power

Plug the socket and switch on the power.

Replace Lamps



Hot! Wait 20 minutes before open the lamp chamber after power off to avoid scald!

Step 1. Tools preparation


Prepare a 6×150mm Cross Blade screwdriver and a pair of glove.

Step 2. Power Off

Switch off the power supply and unplug the socket.


Step 3. Open the cover

Unscrew the 4 screws indicated(Each side with 2 screws)and remove the cover.

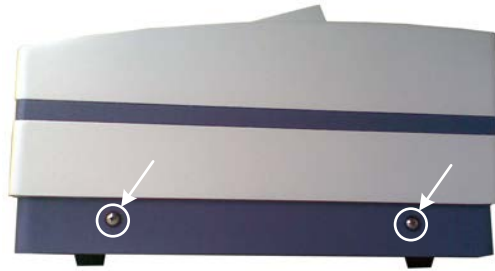


Step 4. Open the cover of the light chamber

Unscrew the 2 screws on the light chamber cover and remove it.

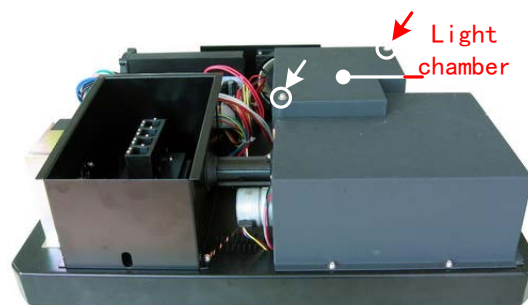

Step 5. Replace the D2 lamp


Unscrew the 2 screws on the D2 Flange (No.1), unplug the connector in the Power Board (No. 2) and remove the D2 lamp. Draw on the cotton glove and replace a new lamp. Fix the 2 screws and plug the connector again.

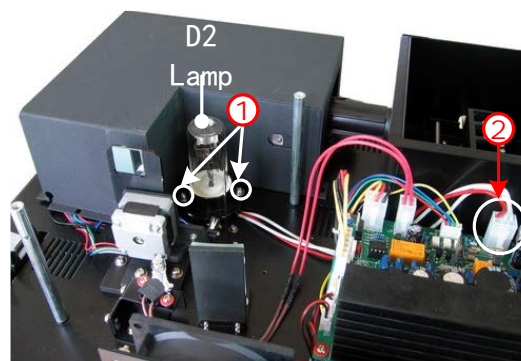

Step 6. Replace W lamp


Pull out the defected W lamp and draw on the cotton glove. Insert the new W lamp as deep as possible on the lamp seat. Be sure to keep the

filament in the same direction as the old one face.

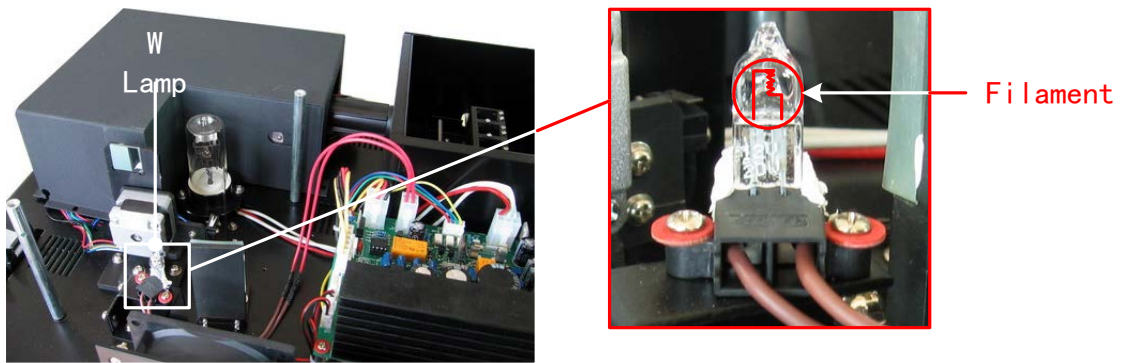

Adjust the position of the W lamp

Switch on the power (the Switch Mirror should be placed to the position as indicates). Observe the entrance facular, and it should in the center of the entrance hole. If the facular deviate to Left or Right, then loosen the No.1 screws in Fig. 5-8 and move the lamp seat to Left or Right until it focus on the center of the slot. Then fix the screws. If the facular deviate to Up and Down, then loosen the No.2 screws and move the lamp seat Up and Down until the facular focus on the center of the slot. Then fix the No. 2 screws again.

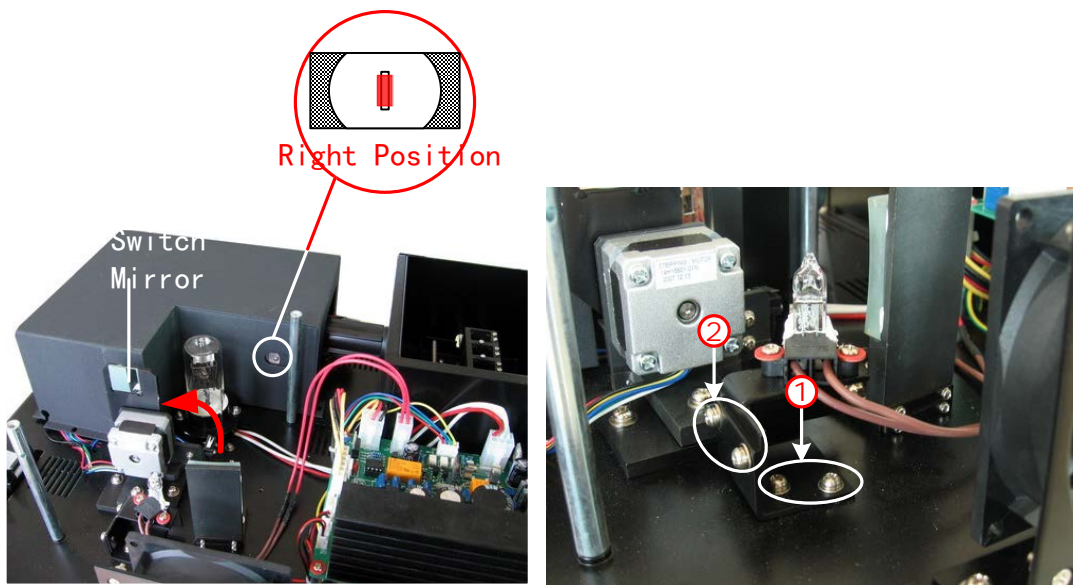

Step 7. Finish

Reset the cover of the light chamber and fix the screws. Reset the cover of the instrument and fix the screws. Recover the Pole in the

compartment, then the course finished.

Warranty

We warrant that this product will be free from defects in material and workmanship for a period of one (1) year from date of purchase. If a defect is present, we will, at its option, repair, replace, or refund the purchase price of this product at no charge to you, provided it is returned during the warranty period. This warranty does not apply if the product has been damaged by accident, abuse, misuse, or misapplication, or from ordinary wear and tear.

For your protection, items being returned must be insured against possible damage or loss. This warranty shall be limited to the replacement of defective products. IT IS EXPRESSLY AGREED THAT THIS WARRANTY WILL BE IN LIEU OF ALL WARRANTIES OF FITNESS AND IN LIEU OF THE WARRANTY OF MERCHANTABILITY.

Equipment Disposal



This equipment is marked with the crossed out wheeled bin symbol to indicate that this equipment must not be disposed of with unsorted waste.

Instead it's your responsibility to correctly dispose of your equipment at lifecycle -end by handling it over to an authorized facility for separate collection and recycling. It's also your responsibility to decontaminate the equipment in case of biological, chemical and/or radiological contamination, so as to protect from health hazards the persons involved in the disposal and recycling of the equipment.

For more information about where you can drop off your waste of equipment, please contact your local dealer from whom you originally purchased this

equipment.

By doing so, you will help to conserve natural and environmental resources and you will ensure that your equipment is recycled in a manner that protects human health.

Thank you!

