

# MM750B

## High Precision Benchtop Digital Multimeter



The Triplett MM750B is a 200000 count benchtop digital multimeter with high precision, multi-function and full-automatic measurements for various requirements.

### **Basic measurements:**

DC voltage measurement: 200mV, 2V, 20V, 200V, 1000V

DC current measurement: 200 $\mu$ A, 2mA, 20mA, 200mA, 2A, 10A

AC voltage measurement: RMS 200mV, 2V, 20V, 200V, 750V

AC current measurement: RMS 2mA, 20mA, 200mA, 2A, 10A

Resistance measurement: (2-wire, 4-wire) 200 $\Omega$ , 2k $\Omega$ , 20k $\Omega$ , 200k $\Omega$ , 2M $\Omega$ , 10M $\Omega$ , 100M $\Omega$

Capacitance measurement: 2nF, 20nF, 200nF, 2 $\mu$ F, 20 $\mu$ F, 200 $\mu$ F, 2mF

Continuity test: fixed 2k $\Omega$

Diode test: 0V-4V

Frequency measurement: 20Hz-1MHz

Cycle measurement: 1 $\mu$ s-0.05s

Temperature measurement: thermocouple and thermal resistance sensor supported

### **Mathematical functions:**

Maximum, minimum, average, standard deviation, relative measurement, bar chart, histogram, trend chart, dB/ dBm, Pass/Fail, etc.

### **Humanization design**

With easy-operating user interface and help system, Chinese & English menu, dual display and both U-disk and local storage supported.

### **Applications:**

Research and education

Research and development

Detection and maintenance

Calibration

Automated testing

## Features:

4.3-inch 480\*272 TFT-LCD

200000 count resolution

Up to 5k reading/s reading speed

True-RMS AC voltage/current measurement

1GB NAND Flash storage, mass storage system and test data

Built-in thermocouple cold junction compensation

Supports standard SCPI remote control command and software of upper computer, the latest mainstream multimeter command set compatible





Dual display, Chinese & English menu and built-in help system

Configuration interfaces: USB Device, USB Host, LAN, GPIB, RS-232C

Settings and the measured data can be record and read by VXI11, USBTMC and U-disk conveniently

## Design Features

Histogram, trend chart, bar chart、mathematical statistics function, dual display, hold function, dBm function, configuration interface

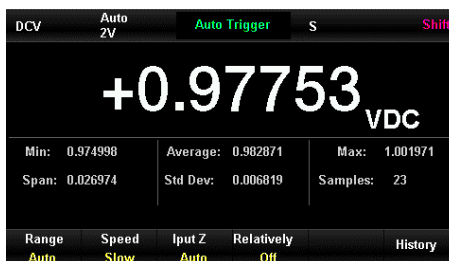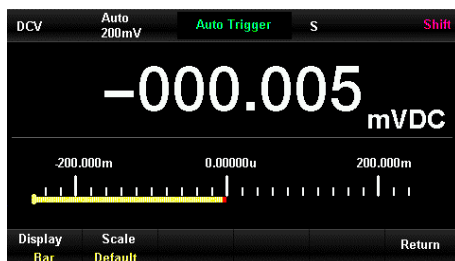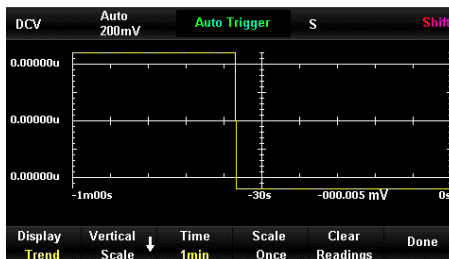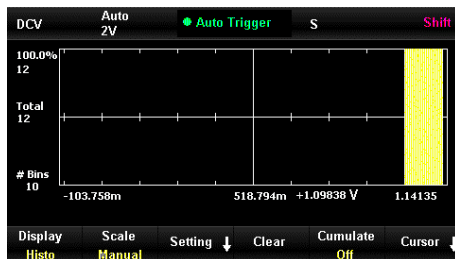



## Specification:

DC Characteristics				Accuracy $\pm$ (%reading + %range) <sup>[1]</sup>		
Function	Range <sup>[2]</sup>	Test current or load voltage	Input impedance	90-day accuracy 23°C±5°C	1-year accuracy 23°C±5°C	Temperature coefficient 0°C -18°C 28°C -50°C
DC voltage (DCV)	200.000mV		10MΩ or >10GΩ	0.008+0.004	0.01+0.004	0.0015+0.0005
	2.00000V		10MΩ or >10GΩ	0.008+0.003	0.01+0.003	0.0010+0.0005
	20.0000V		10MΩ or >10GΩ	0.008+0.004	0.01+0.004	0.0020+0.0005
	200.000V		10MΩ	0.012+0.003	0.015+0.003	0.0015+0.0005
	1000.00V <sup>[3]</sup>		10MΩ	0.012+0.003	0.015+0.003	0.0015+0.0005
DC current (DCI)	200.000μA	<30mV		0.050+0.005	0.055+0.005	0.003+0.001
	2.00000mA	<0.3V		0.050+0.005	0.055+0.005	0.002+0.001
	20.0000mA	<30mV		0.070+0.020	0.095+0.020	0.008+0.001
	200.000mA	<0.3V		0.060+0.008	0.070+0.008	0.005+0.001
	2.00000A	<0.1V		0.150+0.020	0.170+0.020	0.013+0.001
	10.0000A <sup>[4]</sup>	<0.3V		0.200+0.010	0.250+0.010	0.008+0.001
Resistance <sup>[5]</sup> (R)	200.0000Ω	1mA		0.012+0.005	0.030+0.005	0.003+0.0006
	2.00000kΩ	1mA		0.012+0.003	0.020+0.003	0.003+0.0005
	20.0000kΩ	100μA		0.012+0.003	0.020+0.003	0.003+0.0005

	200.000kΩ	10μA		0.012+0.004	0.020+0.004	0.003+0.0005
	2.00000MΩ	1μA		0.020+0.004	0.040+0.004	0.004+0.0005
	10.0000MΩ <sup>[6]</sup>	500nA		0.100+0.004	0.250+0.004	0.010+0.0005
	100.000MΩ	500nA    10MΩ		0.800+0.004	1.75+0.004	0.200+0.0005
Diode test	0~2.0000V <sup>[7]</sup>	1mA		0.05+0.03	0.05+0.03	0.005+0.005
	2.0000V~4.0000V	1mA		0.07+0.03	0.15+0.03	0.005+0.005
Continuity test	2000Ω	1mA		0.05+0.03	0.05+0.03	0.005+0.005

**Note:**

[1] The index is obtained after preheating for half an hour, uses slow speed measurement and the calibration temperature is 18°C~28°C.

[2] All scales except DCV 1000V and DCI 10A are allowed to exceed the range by 20%.

[3] Beyond ±500 VDC, error of 0.002 will be added every 1V exceeds.

[4] For continuous current > DC 7A or AC rms7A, it should be disconnected for 30s after connected 20s.

[5] For 4-wire resistance measurement or 2-wire mode with relative operation; ±0.2Ω additional error will be added in 2-wire resistance measurement without relative operation.

[6] The humidity requirement in scales of 10MΩ and 100MΩ is <60%.

[7] The accuracy is only for voltage measurement of input terminal, the typical value of test current is 1mA. The current source change will cause some variation in the voltage drop on the diode junction.

AC Characteristics			Accuracy ±(%reading + %range) <sup>[1]</sup>		
Function	Range <sup>[2]</sup>	Range of frequency	90-day accuracy 23°C±5°C	1-year accuracy 23°C±5°C	Temperature coefficient 0°C -18°C 28°C -50°C
True RMS AC voltage <sup>[3]</sup> (ACV)	200.000 mV	20Hz~45Hz	1.5+0.10	1.5+0.10	0.01+0.005
		45Hz~20kHz	0.19+0.05	0.2+0.05	0.01+0.005
		20kHz~50kHz	1.0+0.05	1.0+0.05	0.01+0.005
		50kHz~100kHz	3.0+0.05	3.0+0.05	0.05+0.010
	2..00000 V	20Hz~45Hz	1.5+0.10	1.5+0.10	0.01+0.005
		45Hz~20kHz	0.19+0.05	0.2+0.05	0.01+0.005
		20kHz~50kHz	1.0+0.05	1.0+0.05	0.01+0.005
		50kHz~100kHz	3.0+0.05	3.0+0.05	0.05+0.010
	20..0000 V	20Hz~45Hz	1.5+0.10	1.5+0.10	0.01+0.005
		45Hz~20kHz	0.19+0.05	0.2+0.05	0.01+0.005
		20kHz~50kHz	1.0+0.05	1.0+0.05	0.01+0.005
		50kHz~100kHz	3.0+0.05	3.0+0.05	0.05+0.010
	200..000 V	20Hz~45Hz	1.5+0.10	1.5+0.10	0.01+0.005
		45Hz~20kHz	0.19+0.05	0.2+0.05	0.01+0.005
		20kHz~50kHz	1.0+0.05	1.0+0.05	0.01+0.005
		50kHz~100kHz	3.0+0.05	3.0+0.05	0.05+0.010
750..000 V <sup>[4]</sup>	20Hz~45Hz	1.5+0.10	1.5+0.10	0.01+0.005	

		45Hz~20kHz	0.19+0.05	0.2+0.05	0.01+0.005
		20kHz~50kHz	1.0+0.05	1.0+0.05	0.01+0.005
		50kHz~100kHz	3.0+0.05	3.0+0.05	0.05+0.010
True RMS AC current <sup>[5]</sup> (ACI)	2.00000 mA	20Hz~45Hz	1.5+0.10	1.5+0.10	0.015+0.015
		45Hz~2kHz	0.5+0.10	0.5+0.10	0.015+0.006
		2kHz~10kHz	2.5+0.20	2.5+0.20	0.015+0.006
	20.0000 mA	20Hz~45Hz	1.5+0.10	1.5+0.10	0.015+0.005
		45Hz~2kHz	0.5+0.10	0.5+0.10	0.015+0.005
		2kHz~10kHz	2.5+0.20	2.5+0.20	0.015+0.005
	200.000 mA	20Hz~45Hz	1.5+0.10	1.5+0.10	0.015+0.005
		45Hz~2kHz	0.3+0.10	0.3+0.10	0.015+0.005
		2kHz~10kHz	2.5+0.20	2.5+0.20	0.015+0.005
	2.00000 A	20Hz~45Hz	1.5+0.20	1.5+0.20	0.015+0.005
		45Hz~2kHz	0.5+0.20	0.5+0.20	0.015+0.005
		2kHz~10kHz	2.5+0.20	2.5+0.20	0.015+0.005
10.0000 A <sup>[6]</sup>	20Hz~45Hz	1.5+0.15	1.5+0.15	0.015+0.005	
	45Hz~2kHz	0.5+0.15	0.5+0.15	0.015+0.005	
	2kHz~10kHz	2.5+0.20	2.5+0.20	0.015+0.005	

#### Additional crest factor error (Non-sine wave)<sup>[7]</sup>

Crest coefficient	Error(%range)
1-2	0.05
2-3	0.3

#### Note:

[1] The index is obtained after preheating for half an hour, uses slow speed measurement and the calibration temperature is 18°C~28°C.

[2] All scales except ACV 750V and ACI 10A are allowed to exceed the range by 20%.

[3] The index is obtained under the sinusoidal signal with amplitude of >5%; When the input is within 1%~5% and the frequency is <50kHz, the additional error, 0.1% of range is added.

[4] Beyond 400VAC, error of 0.025V will be added every 1V exceeds.

[5] The index is obtained under the sinusoidal signal with amplitude of >5%; When the input is within 1%~5%, the additional error, 0.1% of range is added.

[6] For continuous current > DC 7V or AC rms7A, it should be disconnected for 30s after connected 20s.

[7] when the frequency is < 100Hz

Frequency and Cycle Characteristics			Accuracy ±(%reading)		
Features	Range	Range of frequency	90-day accuracy 23°C±5°C	1-year accuracy 23°C±5°C	Temperature coefficient 0°C -18°C 28°C -50°C
Frequency and cycle	200mV~750V <sup>[2]</sup>	20Hz~2kHz	0.01+0.003	0.01+0.003	0.002+0.001
		2kHz~20kHz	0.01+0.003	0.01+0.003	0.002+0.001

	20kHz~200kHz	0.01+0.003	0.01+0.003	0.002+0.001
	200kHz~1MHz	0.01+0.005	0.01+0.006	0.002+0.002

Note:

[1] The index is obtained after preheating for half an hour.

[2] Besides especially marked, when the frequency is < 100kHz, the index is AC input voltage in 15%~120% scale, and when the frequency is > 100kHz, the index is applicable to scale of 30%~120%. The 750V scale is limited in 750Vrms, and the accuracy in 200mV scale is multiplied the % reading error by 10.

Capacitance Characteristics			Accuracy $\pm$ (%reading+%range) <sup>[1]</sup>		
Features	Range	Maximum test current	90-day accuracy 23°C $\pm$ 5°C	1-year accuracy 23°C $\pm$ 5°C	Temperature coefficient 0°C -18°C 28°C -50°C
Capacitance [2]	2.000nF	0.5 $\mu$ A	2.8+1.0	3+1.0	0.08+0.002
	20.00nF	1 $\mu$ A	1+0.5	1+0.5	0.02+0.001
	200.0nF	10 $\mu$ A	1+0.5	1+0.5	0.02+0.001
	2.000 $\mu$ F	100 $\mu$ A	1+0.5	1+0.5	0.02+0.001
	20.00 $\mu$ F	1mA	1+0.5	1+0.5	0.02+0.001
	200.0 $\mu$ F	1mA	1+0.5	1+0.5	0.02+0.001
	2.000mF	1mA	2+0.5	2+0.5	0.02+0.001

**Note:**

[1] The index is obtained after preheating for half an hour.

[2] The parameter is applicable to capacitance between 1%~120% in 2nF scale. In other scales, capacitance is between 10%~120%.

Temperature Characteristics			Accuracy $\pm$ (%reading+%range) <sup>[1]</sup>		
Function	Type of probe	Model of probe	Operating temperature	1-year accuracy 23°C $\pm$ 5°C	Temperature coefficient 0°C -18°C 28°C -50°C
Temperature	RTD <sup>[2]</sup>	$\alpha=0.00385$	-200°C~660°C	0.16°C	0.008+0.002
	Thermocouple <sup>[3]</sup>	B	0°C~1820°C	0.76°C	0.14°C
		E	-270°C~1000°C	0.5°C	0.02°C
		J	-210°C~1200°C	0.5°C	0.02°C
		K	-270°C~1370°C	0.5°C	0.03°C
		N	-270°C~1300°C	0.5°C	0.04°C
		R	-50°C~1760°C	0.5°C	0.09°C
		S	-50°C~1760°C	0.6°C	0.11°C
T	-270°C~400°C	0.5°C	0.03°C		

**Note:**

[1] The index is obtained after preheating for half an hour and the probe error is not contained.

[2] The index is suitable for 2-wire/4-wire relative measurement.

[3] Built-in cold junction compensation is near the rubber tip of test leads and its measuring error is  $\pm 2^{\circ}\text{C}$ .

Measuring methods and other features	
<b>DC voltage</b>	
Input resistance	10M $\Omega$ or > 10G $\Omega$ for scales of 200mV, 2V and 20V
	10M $\Omega$ $\pm 2\%$ for scale of 20V, 200V and 1000V
Input bias current	< 30 pA, 25 $^{\circ}\text{C}$ test
Input protection	1000 V for all ranges
Common mode rejection ratio	120dB (maximum $\pm 500$ VDC for 1k $\Omega$ balancing resistance of LO test lead)
Normal mode rejection ratio	60 dB (slow reading speed)
<b>Resistance</b>	
Measuring method	4-wire/2-wire resistance selectable
Input protection	1000 V for all ranges
<b>DC current</b>	
Current diverter	Sample resistance 100 $\Omega$ in 200 $\mu\text{A}$ and 2mA scale
	Sample resistance 1 $\Omega$ in 20mA and 200mA scale
	Sample resistance 8m $\Omega$ in 2A and 10A scale
Input protection	250mA, 250V replaceable fast fuse on rear panel
	Internal 10A, 250V slow fuse
<b>Continuity/diode test</b>	
Measuring method	Use constant flow source of 1mA $\pm 5\%$ measure resistance or voltage
Buzzer	Yes
Continuity threshold	Adjustable
Input protection	1000V
<b>True RMS AC voltage</b>	
Measuring method	AC coupling true RMS measurement, maximum 1000V offset in arbitrary range
Crest factor	Crest factor $\leq 3$ in full range



Input impedance	1M $\Omega$ $\pm$ 2% in all ranges with < 100 pF in parallel
AC filter bandwidth	20Hz~100kHz
Common mode rejection ratio	60 dB (for 1k $\Omega$ balancing resistance of LO test lead and < 60Hz, maximum $\pm$ 500 VDC)
<b>True RMS AC current</b>	
Measuring method	Coupling DC to shunt resistor, and coupling AC to true RMS measurement (measure input AC component)
Crest factor	Crest factor $\leq$ 3 in full range
Maximum input	RMS current < 10 A with DC component
Shunt resistor	0.008 $\Omega$ in 2A and 10A scale, 1 $\Omega$ in 20mA and 200mA scale, 100 $\Omega$ in 200 $\mu$ A and 2mA scale
Input protection	250mA, 250V replaceable fast fuse on rear panel Inter 10A, 250V slow fuse
<b>Cycle and frequency</b>	
Measuring method	Measure the time of signal cycle number and then calculate the frequency
Notice	Error will be introduced for low voltage and low frequency signal by all frequency meter
<b>Capacitance measurement</b>	
Measuring method	Charge the capacitance by constant current, and measure the average speed of voltage rising
Connecting method	2-wire
Input protection	All ranges 1000 V
<b>Arbitrary sensor measurement</b>	
Measuring method	Thermocouple, DCV, DCI, $\Omega$ (2-wire/4-wire), frequency output type sensor and built-in thermocouple cold junction compensation supported
Output polarity	Positive/negative selectable
Others	Preset conversions for ITS-90, Pt100 and Pt385 of B, E, J, K, N, R, S, T type thermocouple
<b>Frequency response</b>	
True RMS measurement	100kHz
<b>Sampling and trigger</b>	
Maximum measuring speed	5000rdgs/s (2.5 reading/s; 10 reading/s; 5k reading/s)

Trigger delay	6ms~10000ms optional	
External trigger input	Input level	TTL compatible
	Trigger condition	Rising edge/falling edge optional
	Input impedance	> 20k $\Omega$ /400pF (DC coupling)
	Minimum pulse width	500 $\mu$ s
VMC output	Level	TTL compatible (input $\geq$ 1k $\Omega$ load)
	Output polarity	Positive/negative selectable
	Output impedance	200 $\Omega$ (typical)
<b>History recording</b>		
Volatile memory	10k reading record	
Non-volatile memory	1GB NAND Flash storage, mass storage system and test data	
	6 sets of preset value configuration	
	External U-disk expansion is supported	
<b>Mathematical functions</b>		
Mathematical operations	Pass/Fail, Relative, min/max/average, standard deviation, dBm, dB, Hold, histogram, trend chart, bar chart	
<b>Interfaces</b>		
Interfaces type	USB Host, USB Device, LAN , RS-232C, GPIB(optional)	

## General characteristic:

### Power supply:

AC 90V ~ 110V, 45 ~ 440Hz

AC 110V ~ 132V, 45 ~ 440Hz

AC 200V ~ 240V, 45 ~ 66Hz

AC 216V ~ 264V, 45 ~ 66Hz

Power dissipation: MAX 20W

## Mechanical features:

Size: 260mm\*116mm\*332mm

Weight: 4.4kg

Color: off white and grey

## Other features:

**Accurate operating environment:** 0°C~28°C<90%; 28°C~40°C<75%; 40°C~55°C<50% (no condensation)

**Storage environment:** -20°C~70°C, <95%; the instrument needs to run continuously for at least 7 days after high humidity storage.

**Altitude:** ≤2000 m

**Vibration:** MIL-T-28800E, category III, class 5 (only for sine wave)

**Electromagnetic compatibility:** complies with low-voltage command (2004/108/EC) and standard EN61326-1:2013.

**Safety:** complies with low-voltage command (2006/95/EC), and standard EN61010 - 1:2010 (to be confirmed)

Remote interface 10 / 100Mbit LAN, USB Device, USB Host, RS-232C

**Programming language:** The latest mainstream multimeter SCPI command set compatible

**Preheat:** 30 minutes

## Package:

Three-core power line-----1  
Test leads-----1 pair  
USB connecting line-----1  
RS232 connecting line-----1  
Upper computer software-----1 set

### Warranty

Triplett / Jewell Instruments extends the following warranty to the original purchaser of these goods for use. Triplett warrants to the original purchaser for use that the products sold by it will be free from defects in workmanship and material for a period of (2) two years from the date of purchase. This warranty does not apply to any of our products which have been repaired or altered by unauthorized persons in any way or purchased from unauthorized distributors so as, in our sole judgment, to injure their stability or reliability, or which have been subject to misuse, abuse, misapplication, negligence, accident or which have had the serial numbers altered, defaced, or removed. Accessories, including batteries are not covered by this warranty.

Copyright © 2023 Triplett  
[www.triplett.com](http://www.triplett.com)