WÖHLER

The Wohler A 550 analyzer screen shows:

Fuel oil 2			
O₂:	5.0 %	Tₐ:	72.5 °F
CO₂:	11.7 %	Tғ:	280.7 °F
SL:	11.4 %	Eff:	88.6 %
CO:	109 ppm	Pr:	0.000
CO₂:	143 ppm	EA:	31 %
Dₚₜ:	116.9 °F	Cₐᵢᵣ:	-.----
GI: 0.0009			

THE EASY WAY OF DATA TRANSFER

Wohler A 550 Flue Gas Analyzer
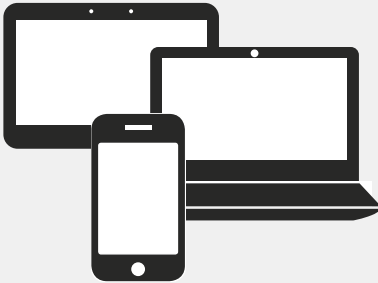
Online-Measurement

*The Measure of Technology*

Wohler A 550 Desktop Software

System requirements

Windows

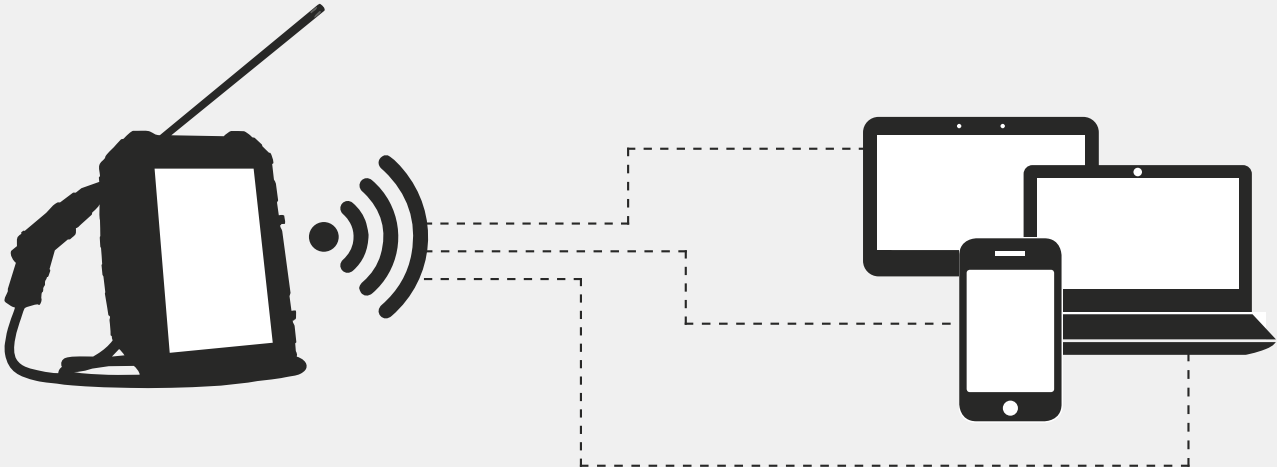· Data management software
  (computer interface necessary)

· Electronic devices:
  PC, Notebook

· Operating System: Windows 7, 8
  (without Windows RT) and 10, with
  current Service Pack

Synchronisation

Performing the online measurement

1. Step

· Open the data management software and start the online measurement

· Select interface, e.g. Bluetooth® and measurement instrument

2. Step

· Perform the Single Online Measurement with the Wohler A 550

· If necessary it is possible to perform various measurement consecutively

3. Step

· After the Single Online-Measurement is finished, the measurement data will be transfered to the data management software

Wohler A 550 Smartphone-App

Measurement App for Android devices for transfering the measurement data of the Wohler A 550 to an external software or for displaying and saving the data on the smartphone.

Application

· The Wohler A 550 App allows to exchange the measurement data of the Wohler A 550 with a software installed on a smartphone or tablet

System requirements

· Android , Version 4.1 and higher

· Bluetooth®-Interface

Measurement-App

· Download the Wohler A 550 App from the Google Play Store (free of charge)

WÖHLER

Wöhler USA Inc.

5 Hutchinson Drive · Danvers, MA 01923
Phone: +1 978 750 9876 · **Fax:** +1 978 750 9799
Email: info@wohlerusa.com

www.wohlerusa.com